

HIOKI CM3289

AC CLAMP METER

Instruction Manual

EN

Dec. 2025 Revised edition 2
CM3289A961-02



HIOKI

www.hioki.com/



All regional
contact
information

HIOKI E.E. CORPORATION

81 Koizumi, Ueda, Nagano 386-1192 Japan

2402 EN

Edited and published by HIOKI E.E. CORPORATION

Printed in Japan

- Contents subject to change without notice.
- This document contains copyrighted content.
- It is prohibited to copy, reproduce, or modify the content of this document without permission.
- Company names, product names, etc. mentioned in this document are trademarks or registered trademarks of their respective companies.

Europe only

• EU declaration of conformity can be downloaded from our website.

• Contact in Europe: HIOKI EUROPE GmbH

Helfmann-Park 2, 65760 Eschborn, Germany

hioki@hioki.eu

Warranty

Warranty malfunctions occurring under conditions of normal use in conformity with the Instruction Manual and Product Precautionary Markings will be repaired free of charge. This warranty is valid for a period of three (3) years from the date of purchase. Please contact the distributor from which you purchased the product for further information on warranty provisions.

Introduction

Thank you for purchasing the Hioki CM3289 AC Clamp Meter. This instrument is a clamp meter that can be perform true RMS measurement of current simply by clamping it around a circuit. To obtain maximum performance from the instrument, please read this manual first, and keep it handy for future reference.

Target audience

This manual has been written for use by individuals who use the product in question or who teach others to do so. It is assumed that the reader possesses basic electrical knowledge (equivalent to that of someone who graduated from the electrical program at a technical high school).

Information on download site

For details on the product application, the update file for the instrument, and the instruction manual, please check Hioki's website:

<https://cloud.gennect.net/dl>



Be sure to also read the separate document "Operating Precautions" before use.

Safety Notes

Symbols affixed to the device

	The instrument can be connected to or disconnected from a live conductor
	The flexible sensor can be connected to or disconnected from live conductors when appropriate protective insulation is used.
	The clamp meter and test leads can only be connected to or disconnected from insulated conductors suited to the voltage of the conductor under measurement.

! DANGER

- ⊘ To avoid electric shock, do not touch the portion beyond the protective barrier during use.

Do not subject the instrument to any voltages when the resistance measurement or continuity check function is selected. Doing so may damage the instrument and result in bodily injury. To avoid electrical accidents, turn off the circuit before measuring it.

! WARNING

- To avoid electric shock, short circuits and damage to the instrument, disconnect the test leads from the measurement object before switching the rotary switch.
- To prevent electric shock, when measuring the voltage of a power line use a test lead that satisfies the following criteria:
 - Conforms to safety standards IEC61010 or EN61010
 - Of measurement category III or IV
 - Its rated voltage is higher than the voltage to be measured
- The optional test leads for this instrument conform to the safety standard EN61010. Use a test lead in accordance with its defined measurement category and rated voltage.



- To prevent a short circuit accident, be sure to use the test leads with the sleeves attached when performing measurements in the CAT III measurement category. (For the measurement categories, see "Measurement categories" (Operating Precautions).)
- If the sleeves are removed during measurement, stop the measurement.
- To prevent an electric shock, do not exceed the every rating shown on either the instrument or each test lead, whichever is worse.
- Handle and dispose of batteries in accordance with local regulations.

! CAUTION

- ⊘ Do not place foreign objects between the jaw tips (or flexible loop couplings) or insert foreign objects into the gaps of the jaws (or flexible loop couplings). Doing so may worsen the performances of the sensor or interfere with clamping action.

- The **B** indicator is displayed when the remaining battery capacity is low. In this case, the accuracy of the instrument is not guaranteed. Replace the battery immediately.
- To avoid battery depletion, set the rotary switch in the **[OFF]** position after use. (Even when the automatic power-saving function is enabled, the instrument consumes a small amount of the battery power.)

Inspection Before Measurement

- Before using the instrument, check it and verify that it operates properly to make sure that it suffered no damage during storage or transportation.
- If damage is suspected, check the section below before contacting your authorized Hioki distributor or reseller.

- (1) **Check the test lead for breaks.**
If any, replace it with the new L9208 Test Lead.
- (2) **Check that the resistance measurement and continuity check operates normally.**
If any one of them does not operate normally, send the instrument for repair to the your authorized Hioki distributor or reseller. The instrument may have been subject to a voltage of greater than 600 V during resistance measurement or continuity check.
- (3) **Check that the battery weakens.**
If it weakens, replace the battery.

Functions

Automatic power-saving function

The instrument automatically turns off the LCD display after it is not operated for 30 minutes.

To restore the instrument from a non-displaying state

Set the rotary switch in the **[OFF]** position and then another one.

To cancel automatic power-saving function

- Set the rotary switch in a position other than **[OFF]** while holding down the **HOLD** key.
- The text **[APS]** and **[OFF]** are displayed in turn on the LCD display, and the automatic power-saving function is disabled. To enable the automatic power-saving function, set the rotary switch in the **[OFF]** position, and then another one.

Auto-range function

The instrument automatically selects the most appropriate measurement range.

The text **[AUTO]** is displayed on the LCD display.


To set the measurement range manually (Manual-range function)

1. Set the rotary switch in the **[OFF]** position and then set the rotary switch in a position other than **[OFF]** while holding down the **[HOLD]** key.
2. Press the **[HOLD]** key to switch the measurement range. (Any ranges can be set except for the continuity check.)

Overflow indication

If an input exceeds the measurement range, the text **[OF]** or **[-OF]** is displayed on the LCD display.

LCD Display With All Segments Turned On

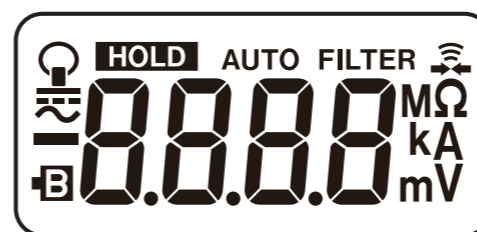


The segment **[FILTER]** is not used. The instrument screen displays the alphanumeric characters as follows.

A	B	C	D	E	F	G	H	I	J	K	L	M	N	O	P	Q	R	S	T	U	V	W	X	Y	Z
a	b	c	d	e	f	g	h	i	j	k	l	m	n	o	p	q	r	s	t	u	v	w	x	y	z
1	2	3	4	5	6	7	8	9	0																
1	2	3	4	5	6	7	8	9	0																

Parts Names

AC Clamp Meter

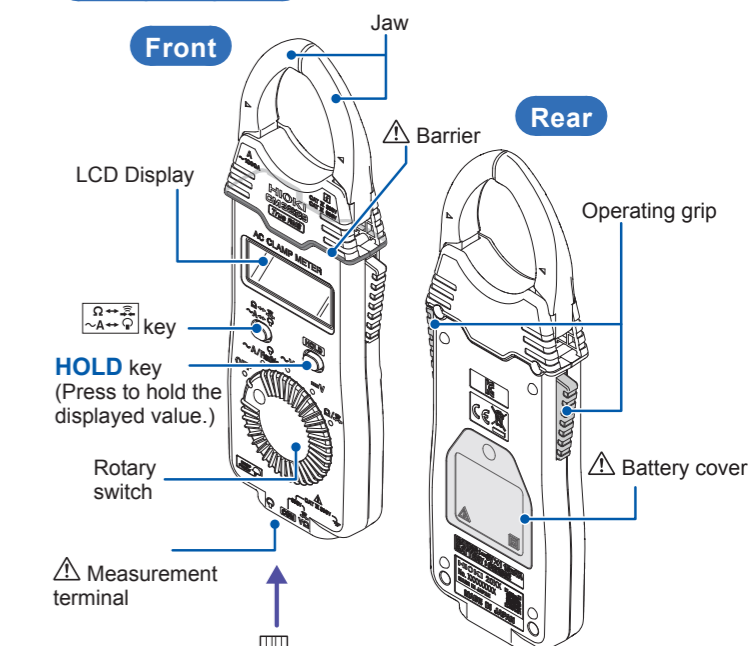


Test Leads Holder

* Optional
Replaceable with battery cover

Plug of test lead or flexible sensor

Test Lead



- With the sleeves attached: CAT IV 600 V / CAT III 1000 V, 10 A
- Without the sleeves attached: CAT II 1000 V, 10 A


Before attaching the L4933^{*1} or L4934^{*2} on test leads, bring the test leads into measurement category II rating (remove the sleeves when using the L9208).

*1: No measurement category,

Maximum rated voltage to earth: 30 V AC / 60 V DC

*2: CAT III 300 V / CAT II 600 V, 3 A

AC Flexible Current Sensor*

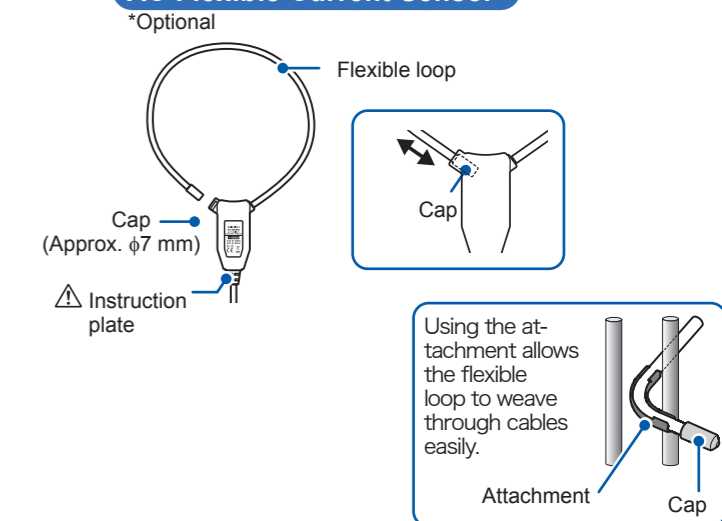


Using the attachment allows the flexible loop to weave through cables easily.



Measuring Methods

AC Current Measurement [~A/Flexible]

Measuring current with the instrument

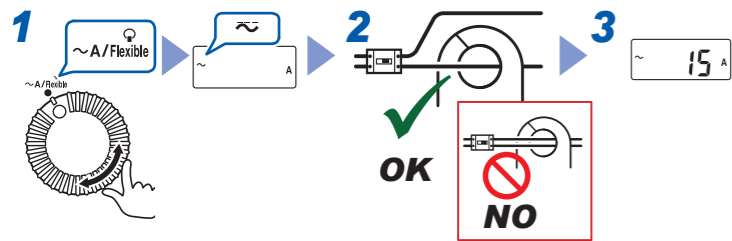


Measuring current with Model CT6280 AC Flexible Current Sensor (optional)

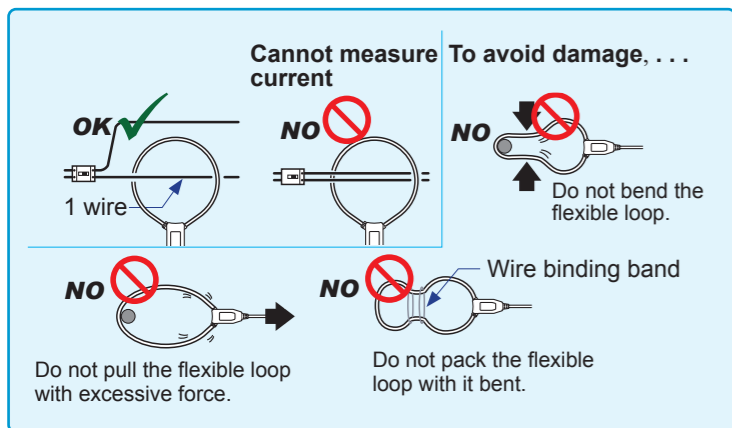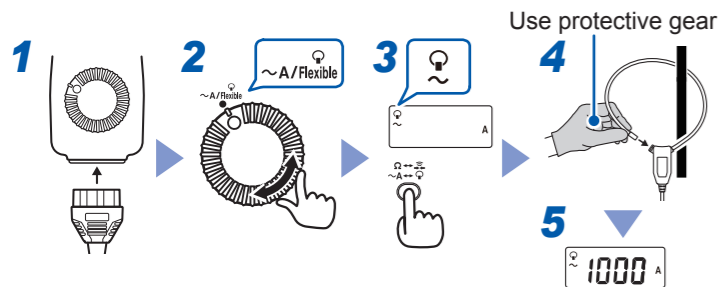


Voltage Measurement


AC Voltage Measurement [~V]

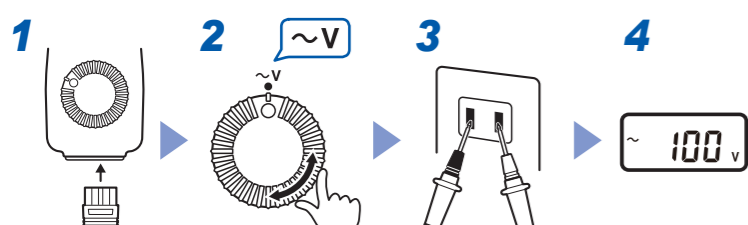


DC Voltage Measurement [=V]

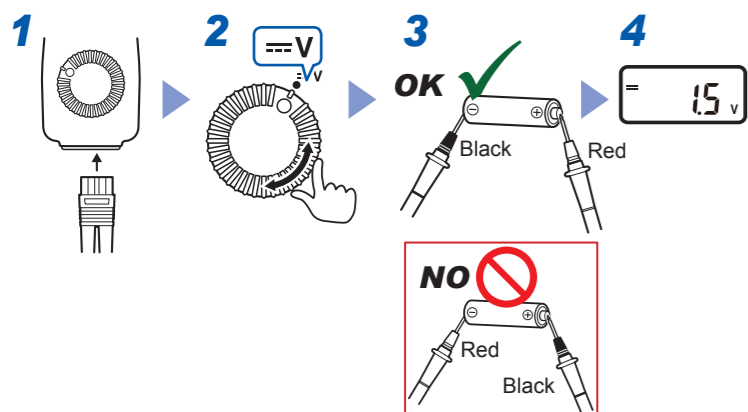

Resistance Measurement [Ω]

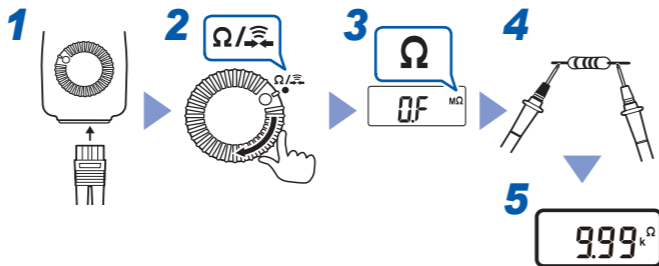

Continuity Check [~]

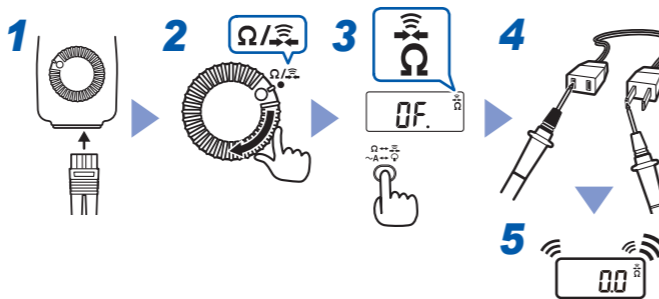


Cleaning / Replacing Battery

Cleaning

- Measurements are degraded by dirt on the mating surfaces of the jaw (or flexible loop coupling), so keep the surfaces clean by gently wiping with a soft, dry cloth.
- To clean the instrument, wipe it gently with a soft cloth moistened with water or mild detergent.
- Wipe the LCD display gently with a soft, dry cloth.

Replacing Battery

Necessary items: Phillips screwdriver (No.1) and Coin cell lithium battery (CR2032)

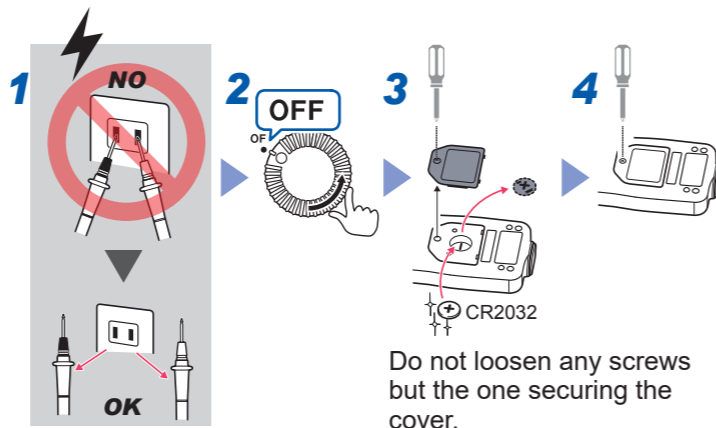

Do not turn any one of the three screws inside the battery case. Doing so will cause the instrument to report abnormal measured values.

CALIFORNIA, USA ONLY

This product contains a CR Coin Lithium Battery which contains Perchlorate Material - special handling may apply. See <https://dtsc.ca.gov/perchlorate/>

Specifications

General Specifications

Operating environment Indoors, pollution degree 2, altitude up to 2000 m (6562 ft.)

Operating temperature and humidity

Temperature	-25°C to 65°C (-13.0°F to 149.0°F) (For the 40 MΩ range: up to 40°C)
Humidity (no condensation)	Less than 40°C (104.0°F): 80% RH or less At least 40°C (104.0°F) but less than 45°C (113.0°F): 60% RH or less At least 45°C (113.0°F) but less than 50°C (122.0°F): 50% RH or less At least 50°C (122.0°F) but less than 55°C (131.0°F): 40% RH or less At least 55°C (131.0°F) but less than 60°C (140.0°F): 30% RH or less At least 60°C (140.0°F) but less than 65°C (149.0°F): 25% RH or less

Storage temperature and humidity -25°C to 65°C (-13°F to 149°F), 80% RH or less (no condensation)

Drop-proof Operate after a drop from 1 m on concrete

Standards Safety: EN61010
EMC: EN61326

Power supply Coin cell lithium battery CR2032 ×1 (3 V DC)
Rated power voltage: 3 V DC
Maximum rated power: 15 mVA

Continuous operating time Approx. 70 hours
(AC current measurement mode, continuous, unloaded)

Dimensions • CM3289: Approx. 57W×181H×16D mm (2.24"W × 7.13"H × 0.63"D)
• CT6280: Approx. 42W×65H×18D mm (1.65"W × 2.56"H × 0.71"D)
(excluding the flexible loop and output cable)

Dimensions (Jaw) Approx. 50W×11D mm (1.97"W × 0.43"D)

Mass • CM3289: Approx. 100 g (3.5 oz.) (including battery)
• CT6280: Approx. 71 g (2.5 oz.)

Product warranty period CM3289, CT6280: 3 years

Accessories • 9398 Carrying Case
• L9208 Test Lead
• Coin cell lithium battery CR2032 (Installed in Model CM3289, for LCD display)
• Instruction Manual
• Operating Precautions (0990A909)

Options • CT6280 AC Flexible Current Sensor (Attachment and C0205 are included)
• 9209 Test Leads Holder
• L4933 Contact Pin Set (Can be connected to the tip of the L9208, which comes with the instrument.)*
• L4934 Small Alligator Clip Set (Can be connected to the tip of the L9208, which comes with the instrument.)*
• C0205 Carrying Case (Models CT6280, L9208, and CM3289 can be stored.)
* Remove the sleeves to attach.

Basic Specifications

Maximum input current • Jaw (CM3289): 2000 A AC, continuous (45 Hz to 66 Hz)
• Flexible loop (CM3289+CT6280): 4200 A AC, continuous (50 Hz to 60 Hz)

Maximum input voltage 600 V AC/DC and 3×10⁶ V·Hz or less (ACV, DCV)

Overload protection 600 V AC/DC (ACV, DCV, Ω, continuity)

Maximum rated voltage to earth
Jaw, CT6280 600 V (Measurement category III), 300 V (Measurement category IV) (Anticipated transient overvoltage: 6000 V)

Voltage measurement terminal 300 V (Measurement category III) (Anticipated transient overvoltage: 4000 V)

AC measurement method True RMS measurement method

Display update rate 400 ms±25 ms

Noise rejection characteristics NMRR DCV -40 dB or more (50 Hz/60 Hz)
-100 dB or more (50 Hz/60 Hz, 1 kΩ unbalance)
CMRR DCV -60 dB or more (50 Hz/60 Hz, 1 kΩ unbalance)
ACV -45 dB or more for 600 V range.

Crest factor For 2500 counts or less, 2.5
Reduces linearly to 1.5 or less at 4200 counts

Zero-display range 5 counts (AC current measured with jaw or flexible loop)

Effects of conductor position • CM3289: within ±5.0% (Specified with a 11-mm-diameter cable)
• CT6280: within ±5.0% (At any positions, based on the center of sensor)

Maximum measurable conductor diameter • CM3289: φ33 mm or less
• CT6280: φ130 mm or less

Model CT6280 Cross-section diameter of sensor cable: Approx. φ5.0 mm
Sensor-tip cap diameter: Approx. φ7.0 mm
Output cable length: Approx. 800 mm

Accuracy Specifications

rdg. (reading or displayed value): The value currently being measured and indicated on the measuring instrument.

dgt. (resolution): The smallest displayable unit on a digital measuring instrument, i.e., the input value that causes the digital display to show a "1" as the least-significant digit.

Conditions of guaranteed accuracy

- Guaranteed accuracy period: 1 year (Number of jaw and flexible loop open/close cycles: 10,000 or less)
- Temperature and humidity for guaranteed accuracy: 23°C±5°C (73.0°F±9.0°F), 80% RH or less
- Temperature characteristic: Measurement accuracy × 0.1%/°C is added (excluding 23°C±5°C)

AC Current Measured With Jaw

Range	Accuracy range	Accuracy		
		40 Hz ≤ f < 45 Hz	45 Hz ≤ f ≤ 66 Hz	66 Hz < f ≤ 1 kHz
42.00 A	4.00 A to 41.99 A	±2.0% rdg. ±5 dgt.	±1.5% rdg. ±5 dgt.	±2.0% rdg. ±5 dgt.
420.0 A	40.0 A to 419.9 A	±2.0% rdg. ±5 dgt.	±1.5% rdg. ±5 dgt.	±2.0% rdg. ±5 dgt.
1000 A	100 A to 1000 A	±2.0% rdg. ±5 dgt.	±1.5% rdg. ±5 dgt.	±2.0% rdg. ±5 dgt.

Accuracy is not defined for currents of 3×10⁵ A·Hz or more.

AC Current Measured With Flexible loop

Range	Accuracy range	Accuracy		
		40 Hz ≤ f < 50 Hz	50 Hz ≤ f ≤ 60 Hz	60 Hz < f ≤ 1 kHz
420.0 A	40.0 A to 419.9 A	±3.5% rdg. ±5 dgt.*1,*2	±3.0% rdg. ±5 dgt.*1	±3.5% rdg. ±5 dgt.*1,*2
4200 A	400 A to 4199 A	±3.5% rdg. ±5 dgt.*1,*2	±3.0% rdg. ±5 dgt.*1	±3.5% rdg. ±5 dgt.*1,*2

*1: Includes accuracy of CT6280 AC Flexible Current Sensor, ±1.0% rdg.
*2: Accuracy is not defined for a current of 1000 A or more or that of 3×10⁵ A·Hz or more.

AC Voltage

Range	Accuracy range	Accuracy		Input impedance
		45 Hz ≤ f ≤ 66 Hz	66 Hz < f ≤ 500 Hz	
4.200 V	0.400 V to 4.199 V	±1.8% rdg. ±7 dgt.	±2.3% rdg. ±8 dgt.	11 MΩ±5%
42.00 V	4.00 V to 41.99 V	±1.8% rdg. ±7 dgt.	±2.3% rdg. ±8 dgt.	10 MΩ±5%
420.0 V	40.0 V to 419.9 V	±1.8% rdg. ±7 dgt.	±2.3% rdg. ±8 dgt.	10 MΩ±5%
600 V	400 V to 600 V	±1.8% rdg. ±7 dgt.	±2.3% rdg. ±8 dgt.	10 MΩ±5%

DC Voltage

Range	Accuracy range	Accuracy		Input impedance
		45 Hz ≤ f ≤ 66 Hz	66 Hz < f ≤ 500 Hz	
420.0 mV	40.0 mV to 419.9 mV	±2.5% rdg. ±5 dgt.	±2.5% rdg. ±5 dgt.	100 MΩ or more
4.200 V	0.400 V to 4.199 V	±1.0% rdg. ±3 dgt.	±1.0% rdg. ±3 dgt.	11 MΩ±5%
42.00 V	4.00 V to 41.99 V	±1.0% rdg. ±3 dgt.	±1.0% rdg. ±3 dgt.	10 MΩ±5%
420.0 V	40.0 V to 419.9 V	±1.0% rdg. ±3 dgt.	±1.0% rdg. ±3 dgt.	10 MΩ±5%
600 V	400 V to 600 V	±1.0% rdg. ±3 dgt.	±1.0% rdg. ±3 dgt.	10 MΩ±5%

Resistance

Range	Accuracy range	Accuracy	Open-circuit voltage
420.0 Ω	40.0 Ω to 419.9 Ω	±2.0% rdg. ±4 dgt.	3.4 V or less
4.200 kΩ	0.400 kΩ to 4.199 kΩ	±2.0% rdg. ±4 dgt.	
42.00 kΩ	4.00 kΩ to 41.99 kΩ	±2.0% rdg. ±4 dgt.	3.4 V or less
420.0 kΩ	40.0 kΩ to 419.9 kΩ	±2.0% rdg. ±4 dgt.	
4.200 MΩ	0.400 MΩ to 4.199 MΩ	±5.0% rdg. ±4 dgt.	3.4 V or less
42.00 MΩ	4.00 MΩ to 41.99 MΩ	±5.0% rdg. ±4 dgt.	

Continuity Check

Range	Accuracy	Threshold for buzzer sound	Open-circuit voltage
420.0 Ω	±2.0% rdg. ±4 dgt.	50 Ω±40 Ω or less	3.4 V or less

Function Specifications

Display Maximum count: 4199 counts

Battery indicator warning voltage The mark is displayed at a battery voltage of 2.3 V±0.15 V or less.