

Maximum accuracy of ±0.16% achieved with current sensors!

- Measure the primary and secondary sides of inverters
- □ Advanced motor analysis functions
- Measure inverter noise



V

A

kW

Large Assortment of Wide-band, High-Precision Feed-Through Current Sensors

4 Models

Effect of conductor position Effect of external electromagnetic field

Completely Minimized



200A CT6863



1000A CT6865

Current Sensor Method

Surpasses the Accuracy of Direct Connection Method



Power Analyzer 3390

When combined with the feed-through current sensors

Maximum accuracy of $\pm 0.16\%$





For Current Sensor specifications, please go to

page 15

Weight & Volume

A HIOKI proprietary engine

that takes advantage of the latest semi-conductor technologies

enables a much smaller footprint

than ever before (in comparison

with other HIOKI high

performance power meters)

Power Analyzing Control Engine **Technology processes**



Measurement data at high speeds

and with excellent accuracy

Feed-through current sensors

9709





CT6841



9272-10

Current sensor design allows for safe and efficient testing

- Choice of sensors include easy-to-measure AC and AC/DC clamp-on sensors and feed-through current sensors for highaccuracy measurements
- Immune to in-phase noise effects when measuring inverters

Basic accuracy of Model 3390: ±0.1%

Basic measurement range: DC, 0.5 Hz to 5 kHz

(Frequency bandwidth: DC, 0.5 Hz to 150 kHz)

Effective input range: 1% to 110%

- High accuracy, wide band, and wide dynamic range
- Also measure the secondary side of DC inverters in conjunction with a variety of HIOKI current sensors

All data updated at 50ms*

- 50ms data refresh rate for all measurements unaffected by settings restraints
- Synchronize the measurements of multiple 3390s Automatic update rate eliminates the need of switching for low-frequency measurements
- * 50ms data refresh rate does not apply to waveform and noise analysis

Meet the Needs of Alternative Energy and Inverter or Motor Evaluations

4-channel isolated input

Measure the primary and secondary sides of inverters simultaneously

- Choose wiring from single-phase two-wire to three-phase four-wire
- Synchronize the measurements of multiple 3390s



- Connect up to four **3390**s and synchronize their clocks and measurement timing for multiple-channel measurements (using the SYNC terminal and Connection Cable **9683**)
- Use dedicated application software to conduct synchronized operations for up to 4 units and obtain all the measurement data

CF card interface

& USB memory interface

Automatically save interval measurement data to a CF card (When saving manually, measured data and waveform data can

be saved directly to the CF card and USB memory)



Waveform Output and 16 Channel D/A output

- Use the **D/A OUTPUT OPTION 9792** to update data every 50ms and output up to 16 items in analog format
- Also output the voltage and current waveforms for each channel (using 1 to 8 channels)
 (Waveforms are output at 500 kS/s and sinusoidal waveforms can be represented accurately at up to 20 kHz)



Ideal for Motor Evaluation and Analysis

• Use of the **MOTOR TESTING OPTION 9791 (or 9793)** allows torque meter output and rotation input, and facilitates motor power measurement

For motor evaluation and analysis specifications, please go to pages 8 & 9

A Variety of Interfaces Standardly Equipped Includes 100Mbps Ethernet and USB 2.0 High Speed communications interfaces.




HTTP server function available with free dedicated PC software

- HTTP server function through web browser enables easy remote operation
- Free dedicated PC application can be downloaded from the HIOKI website

Collect data and operate the **3390** remotely by connecting it to a PC via LAN or USB






Extra-Large Screen Expands Possibilities

Capture measured data and waveforms at a glance utilizing a variety of display options

The 9" color LCD can display up to 32 data parameters

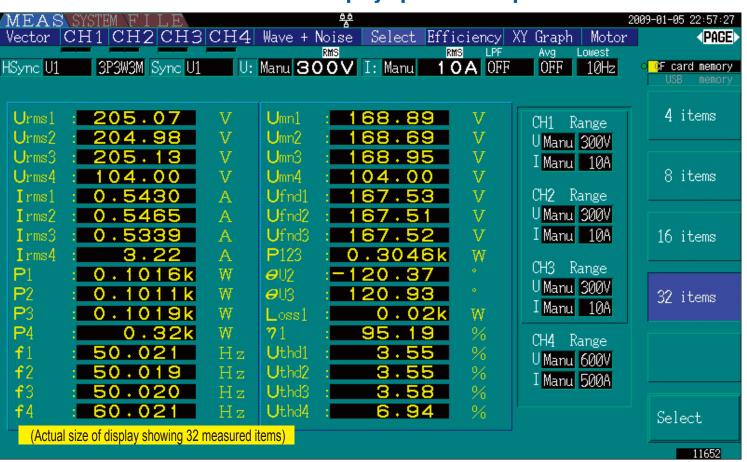




Wiring check function prevents connection errors


Display connection and vector diagrams on the Wiring screen

Improve efficiency and reliability while saving time in wiring even for three-phase measurements

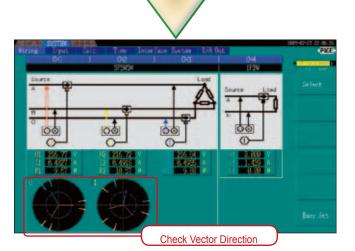

Display just the required data in an easy-to-read graphic interface on the Select screen Screen displaying 32, 16, 8, or 4 items

Display items can be set individually for each selected screen Read data quickly and easily by just switching between the screens

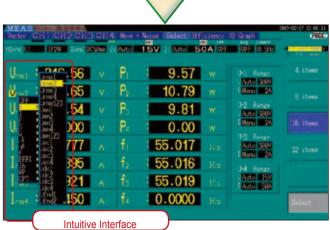


All data is processed in parallel simultaneously.

A wealth of data analysis functions all built-in and ready to use.

Channel display

RMS and MEAN values, and AC, DC, and fundamental waveform components can be measured and displayed simultaneously

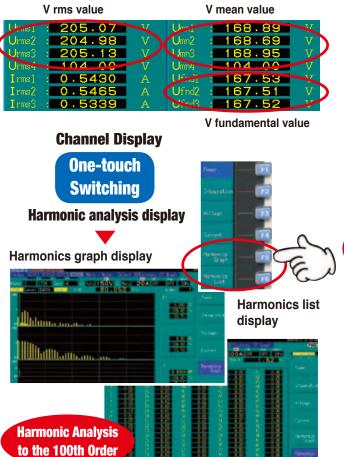



vectors

Vectors display


Measured voltage, current, and power on channels 1 to 4 as numerical values and as

Channel display

Fast

500kS/s

Measured power, voltage and current values, integration values, with access to harmonic graphs and lists for each channel.



Wave+Noise display

Ideal for frequency analysis of inverter noise (FFT nalysis)

Efficiency display

Simultaneously display efficiency and power loss

XY graph display

Power and torque display makes it easy to understand the motor I/O characteristics



Feed-through Current Sensor Enable Extremely Accurate Measurements

HIOKI's high-performance feed-through current sensors absolutely minimizes the effects of conductor position and external fields, making them exceptionally precise. Repeatability and stability are absolutely unmatched!











Feed-through current sensors meet a large variety of applications from electric or hybrid vehicle testing, inverter motor evaluations and solar power devices and fuel cell analysis to individual testing of electrical appliances and facilities equipment.

*For further information and specifications, please refer to page 15.

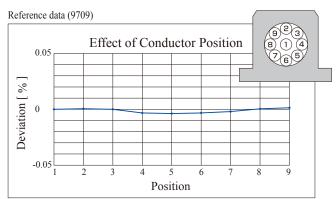



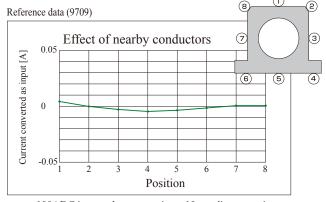

at 100ADC input, when measuring a 10mm diameter wire

Measure the primary and secondary sides of inverters (Performance evaluation of motors and inverters)


Accurately and easily measure the power of inverters and motors for a wide range of applications, from research and development to field tests

Advantages

- 1. Isolated input of voltage and current lets you measure the power on the primary and secondary sides of inverters simultaneously.
- 2. Using a non-invasive current sensor makes the connection simple and easy. A vector diagram display ensures connections are checked.

Proprietary HIOKI Technology

- 3. Accurately measure the fundamental wave voltage and current values related to the motor axis output with confidence
- 4. All data is measured simultaneously and updated every 50 ms.
- 5. In addition to the harmonic analysis required to evaluate the inverter control, noise components can also be measured at the same time ideal for determining the leakage of inverter noise
- 6. Use of a current sensor reduces the effect of in-phase noise from inverters when measuring the power

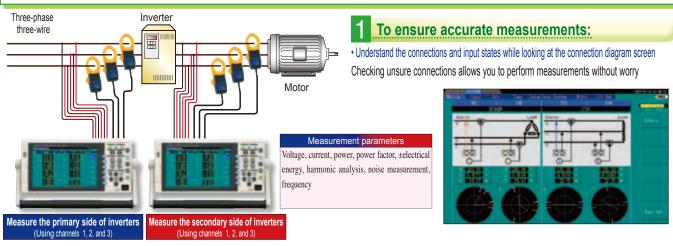


PC measurements and synchronizing multiple devices

 Dedicated application software allows you to perform PC measurements right out of the box

LAN and USB compatibility facilitates efficient data collection and remote operation. Bundled application software allows you to control up to 4 units.

Acquire all data even when multi-unit measurements are performed.
 Two units can be connected using the CONNECTION CABLE 9683 (option) to synchronize the internal clocks and control signals.

Interval measurements with the two units allow the acquisition of perfectly synchronized data, making it easy to collect completely harmonized data with a CF card without using a PC.

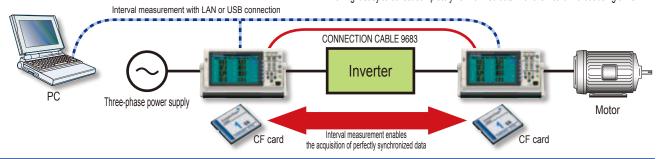

■ What's so special about inverter motors?

Inverter motors are indispensable as the power source of industrial equipment. The rotation of an induction motor depends on the input frequency, so if this input frequency can be made variable, the rotation can be controlled freely. Development of a frequency conversion technology called an inverter has made it possible to freely control the rotation of motors.

In recent years, the mainstream inverter control method is the PWM (Pulse-width Modulation) method.

• What is the PWM method?


A pseudo sinusoidal waveform (fundamental wave) resulting from the conversion of the fundamental wave frequency that determines the rotation of a motor to a pulse train called a carrier frequency (at about several kHz to 15 kHz) is effected, controlling the number of rotations.

Performance evaluation and electrical measurement of motor

The axis output of a motor is closely related to the fundamental wave frequency to be input, so an accurate measurement of this fundamental wave component is required to evaluate the input characteristics.

Conventional measurement method

Traditional methods use the average rectified RMS indication (Mean) in order to obtain a component value close to the fundamental wave frequency from a pseudo sinusoidal waveform (fundamental wave + carrier wave) to be input. To measure an accurate fundamental component, frequency analysis was required; however, the conventional processing method was not practical because it could barely perform real-time measurements with FFT as a result of the limited computing power.



• The 3390 is capable of measuring the fundamental wave component accurately.
The 3390 performs this frequency analysis using high-speed harmonic computation processing at an interval of 50 ms and displays the true fundamental wave component.

3 To make the best of inverter motor measurements:


• Parameters critical to the measurement of motor inputs (outputs on the secondary side of inverters) can be measured and displayed simultaneously.

Display item	Measurement details
rms value	RMS value of fundamental wave + carrier wave components
mn value	RMS value (mean value) close to the fundamental wave component
fnd value	True fundamental wave component
thd value	Displays the distortion factor of measured waveform
unb value	Displays the balance between phases
±pk value	Maximum positive/negative values of waveform that is being measured
dc value	Displays a DC component harmful to the motor
ac value	RMS value obtained by removing the DC component from the RMS value
f value	Frequency of each phase

4 Clearly display efficiency and loss of inverters

· Efficiency and loss measurement function built-in

The operating efficiency and power loss of an inverter can be displayed when measuring the inputs and outputs of the inverter simultaneously.




6 Harmonic measurement indispensable for inverter evaluation

 4-channel simultaneous harmonic analysis function built-in (Performed simultaneously with power measurement)

Harmonic analysis is essential for the development and evaluation of inverters Synchronized to the fundamental wave frequency from 0.5 Hz to 5 kHz Harmonic analysis up to the 100th order can be performed simultaneously with power measurement.




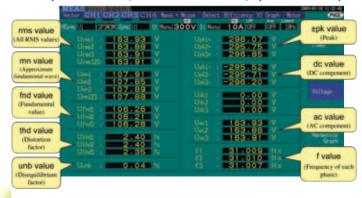

5 X-Y graph display lets you check the dynamic characteristics of inverters

• X-Y graph display function built-in (X-axis: 1 item, Y-axis: 2 items)


By simply specifying the voltage for the X-axis and the power consumption and efficiency for the Y-axis, you can display the dynamic characteristics of a motor in real time.



7 Evaluate of the troublesome noise of inverters

• Noise measurement function built-in (1-channel measurement: Performed simultaneously with power measurement and harmonic analysis)

Noise components at up to 100 kHz can be read while looking at the measured waveforms Simultaneously display the top 10 point frequency and voltage/current levels



8 Waveforms can be observed at 500 kS/s, and fundamental waves can also be checked

Waveform monitoring function fully supported

Display the voltage and current waveforms being measured

The carrier frequency components of an inverter are also displayed in real time

Filter function

A filter function is used to remove the carrier frequency components from the inverter, and fundamental wave frequency waveforms can be checked in the waveform display.

* The filter function is reflected in the measured values. Please be careful when you switch to the function during measurement.

Waveform monitoring of carrier frequency

When the 500 Hz filter is turned ON

Geared for the latest motor evaluation and analysis of Hybrid Electric Vehicles, Electric Vehicles and the like


Drive the research and development of three-phase inverter motors with high accuracy and high-speed measurements

Advantages

- 1. Use of the MOTOR TESTING OPTION 9791 (9793) lets you perform a total evaluation of inverter motors
- 2. The voltage, torque, rotation, frequency, slip, and motor power required for motor analysis can be measured with one unit
- 3. Current sensors make the connection simple. In addition, use of the AC/DC CURRENT SENSOR enables measurements with superior accuracy

Proprietary HIOKI Technology


- 4. All data is measured simultaneously and updated every 50 ms. Data collection and characteristics tests can be performed at the industry's fastest speed
- 5. Evolution of electrical angle measurements critical to motor analysis has made it possible to perform more accurate measurements using an incremental encoder
- 6. Harmonic analysis at 0.5 Hz to 5 kHz without the need for an external timing mechanism
- 7. Built-in digital anti-aliasing filter (AAF) lets you measure the broadband power on the secondary side of inverters to make accurate harmonic analyses

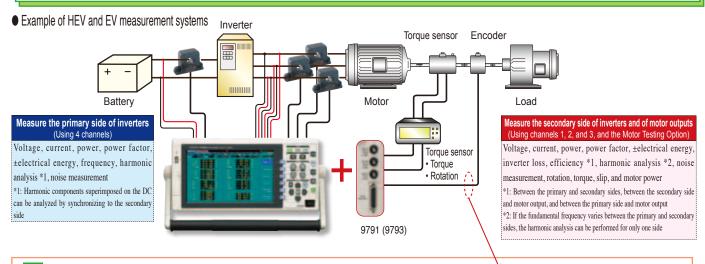

1 Evaluate high-performance vector control inverters:

- Measurements of fundamental wave voltage and current and their phases based on an accurate harmonic analysis are indispensable to motor analysis
- Support of an incremental encoder allows detecting synchronization signals from a motor easily and accurately

Electrical angle measurements are indispensable for dynamic characteristics analysis of motors. The 3390 can conduct FFT analyses synchronized to rotation pulses from the tachometer and the motor induced voltage, and the A-phase and Z-phase pulse inputs that allow measuring and detecting the origin of the motor more simply and accurately – fully meeting the needs of the latest motor analysis tests.



Encoder A-phase signal Encoder Z-phase signal Voltage / current waveform

■ Application 1: "Electrical angle measurement"

- \circ The voltage / current fundamental wave component " θ " from the machine angle origin can be calculated by performing harmonic analysis of motor input voltage / current by synchronizing to the A-phase signal and z-phase signal of an encoder.
- \circ A function to perform zero compensation for this phase angle when a motor induced voltage is generated can be used to measure the voltage and current phase (electrical angle) in real time based on the induced voltage when the motor is started.

■ The importance of measuring the electrical angle of synchronous motors

The key to the performance of high-performance low-fuel consumption vehicles represented by HEV and EV is the synchronous motor that is used as the power source. The synchronous motor is finely controlled by alternating signals generated by an inverter device (DC to AC conversion) using the electricity from batteries.

• What is a synchronous motor?

A synchronous motor rotates in synchronization with the AC frequency. Structurally, the motor is turned by the rotating force at the magnetic pole of the rotator (rotator magnetic pole), which is generated by the rotating magnetic field generated by applying an alternating current to the magnetic field (stator magnetic pole). The rotation speed is synchronized to the speed of the rotating magnetic field, so the

speed can be controlled by changing the speed of the rotating magnetic field (power supply frequency). In addition, high operating efficiency is one of the advantages of the synchronous motor.

• Why is electrical angle measurement necessary?

In the case of a synchronous motor, a phase shifting occurs between the stator magnetic pole and the rotator magnetic pole due to a change in the load torque. This shifted angle and the torque force that can be generated by a motor have a close relationship, so it is important to understand this shifted angle (electrical angle) in order to achieve high-efficiency motor control.

• The 3390 provides a more accurate measurement method

The 3390 supports the incremental encoder output in addition to the measurement methods of the HIOKI 3194 Power HiTESTER – enabling you to measure this electrical angle more easily and accurately.

2 Analyze harmonic signals from the low-speed rotation range of motors

• Harmonic analysis from a synchronization frequency of 0.5 Hz Accurate measurements can be performed in the low-speed rotation range of motors without the need of an external clock.

If the synchronization frequency is 45 Hz or more, analysis results are updated every 50 ms, so data analysis can be performed in real time.

Synchronization frequency range	Window wave number	Analysis order
0.5Hz to 40Hz	1	100th order
40Hz to 80Hz	1	100th order
80Hz to 160Hz	2	80th order
160Hz to 320Hz	4	40th order
320Hz to 640Hz	8	20th order
640Hz to 1.2kHz	16	10th order
1.2kHz to 2.5kHz	32	5th order
2.5kHz to 5.0kHz	64	3rd order

3 Vector display of electrical angles of motors


• Display vectors including that of the phase angle and electrical angle ($\varDelta\theta$) of fundamental wave voltage and current. The measured data can be used as parameters to calculate the Ld and Lq values.



5 X-Y graph display lets you check the dynamic characteristics of inverters

• X-Y graph display function built-in (X-axis: 1 item, Y-axis: 2 items)

By simply setting 2 items to the Y-axis as with a 6-axis graph used to evaluate motors, you can display the characteristics of a motor and similar devices in real time.



· Analyze up to the 100th order

Synchronized to the fundamental wave frequency of 0.5 Hz to 5 kHz Simultaneously perform analysis up to the 100th order harmonic along with power measurement



4 Clearly view the inverter efficiency/loss and motor power

• Output, efficiency, and loss of inverter motors can be measured with one single unit

Operating efficiency and power loss of the inverter and motor can be displayed when the inputs and outputs of the inverter are measured simultaneously.






■ Application 2: Electrical angle measurement using induced voltage of motors (The same measurements conducted with the HIOKI 3194 can also be performed)

Correct the rotation synchronization signal and induced voltage phase of motors as well as measure the phase of voltage and current for the induced voltage of a running motor as an electrical angle.

Step 1: Turn the motor from the load side, and measure the induced voltage of the motor




- Measure the fundamental wave's RMS value and the total RMS value of the induced voltage.
- Perform zero compensation for the phase between the rotation synchronization signal and the fundamental wave voltage of the induced voltage.

Other Advance Functionsmotor

- Frequency divider circuit (up to 1/60000 frequency dividing) helpful when the rotation synchronization signal consists of multiple pulses for one cycle of induced voltage.
- A-to-Y conversation function convert the line voltage to a phase voltage (virtual neutral reference) when three-phase three-wire (3P3W3M connection) measurements are performed.

Step 2: Measurement of a running motor



- Measure the fundamental wave component, harmonic component, and electrical angle of line voltage and current of a line to the motor. (The measured data can also be used as parameters for calculation of LplLq)
- \circ Simultaneously measure motor efficiency, inverter efficiency, total efficiency, and inverter loss while observing the motor control.

Evaluate new energies such as solar power, wind power, and fuel cells


Assess power conditioners that are indispensable for converting new energies to electrical power

Advantages

- 1. The input and output characteristics of a power conditioner can be measured simultaneously in combination with an AC/DC current sensor
- 2. Use of a current sensor makes the connection simple. Make accurate measurements in combination with the AC/DC CURRENT SENSOR
- 3. The sale and purchase of electrical energy of a power line connected to a power conditioner can also be measured with one unit

Proprietary HIOKI Technology

- 4. Measure DC mode integration, which responds quickly to changes in the input of sunlight and the like, and RMS mode integration, which handles the separate integration of the sale and purchase of electric energy, all at the same time
- 5. Ripple factor, efficiency and loss, which are required to evaluate power conditioners for solar power generation, can be measured with one single unit.

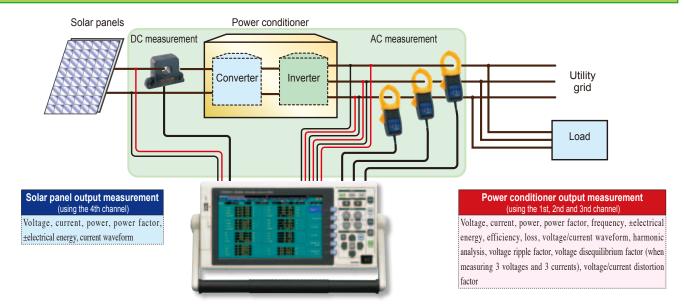

Conditioner-specific measurement items all measurable

 Power conditioner measurement-specific ripple factor and disequilibrium factor can also be measured and displayed simultaneously (up to 32 items can be displayed simultaneously), resulting in enhanced test efficiency

• • • • • • • • • • • • • • • • • • • •	
Display item	Measurement item
rms value	RMS (DC/AC voltage/current of input and output)
P, Q, S, λ values	Active power, reactive power, apparent power, power factor
Loss value	Input and output loss
η value	Efficiency
thd value	Distortion factor (voltage/current)
rf value	Ripple factor (for DC)
unb value	Disequilibrium
f value	Output frequency



■ Current trends in solar power generation

• Interconnected system of solar power generation and power conditioner Electrical energy generated from the solar power generation is DC electrical energy, so it needs to be converted to AC electrical energy to be used by connecting to the utility grid. The device to convert direct current to alternating current is the power conditioner. In particular, to sell electrical energy by connecting to the utility grid, the performance of the power conditioner is important, so the method to evaluate the performance is specified by the national standards.

IEC standard


IEC 61683:1999, Photovoltaic systems -Power conditioners- Procedure for measuring efficiency

Evaluation and measurement of power conditioners

The IEC standard stipulates detailed measurement items to evaluate the input and output characteristics of power conditioners such as harmonic level, ripple factor, voltage disequilibrium factor, and voltage/current waveform.


The 3390 supports a long list of measurement items including the specific ones required.

The 3390 can measure ripple factor and evaluate and analyze through simultaneous measurements.



The efficiency (loss) and the amount of electrical energy sold and purchased can be displayed clearly

 Not only the amount of electricity generated with solar cells and the efficiency (loss) of a conditioner but also the amount of electrical energy sold and purchased by connecting to the utility grid can be measured simultaneously with one single unit




4 Accurately measure harmonics that are important for connecting to the utility grid

• The harmonic component and distortion factor important for connecting a power conditioner to the utility grid can be measured simultaneously.


Synchronized to the fundamental frequency of 0.5 Hz to 5 kHz.

Analyze up to the 100th order of voltage, current, and voltage harmonic, and display the current direction



3 Check the input and output waveforms of a conditioner

• Simultaneously check the input and output waveforms of a conditioner at 500 kS/s The input and output waveforms required to evaluate power conditioners can be checked simultaneously with one unit.



5 Also measure the noise flow of a connected utility grid

• Noise measurement function (1-channel measurement: Performed simultaneously with power measurement and harmonic analysis)

Noise components at up to 100 kHz can be read while looking at the measured waveforms Frequency and voltage/current levels for the top 10 points can be displayed simultaneously.




Bundled software dedicated to the 3390 (free download from the HIOKI website)

♦ Features

- Connect the **3390** to a PC via LAN or USB for completely remote operation
- Save measured data to the PC in real time (interval saving is also available)
- Download data stored in the USB memory or CF card
- Connect up to four 3390 Power Analyzers using the free software for remote operation and simultaneous data collection

Delivery media	Download from the HIOKI website
Operating	Windows 2000, XP, Vista, 7 PC
environment	Pentium III 500 MHz or higher CPU, 128 MB or more RAM, and LAN or USB interface
	Java Runtime Environment (JRE) 1.5.0 or later required
Communication	Ethernet (TCP/IP), USB 1.1/2.0
method	For a USB connection, use the supplied dedicated driver (included with the software)
Number of simultaneously- connected units	4
oormootod driito	
= F	
■ Functions	
Remote operation function	Key operation and screen display on a PC
Download function	Downloads data stored on the media (Files in the USB memory or CF card)
Display function	Displays instantaneously measured values of the 3390 on the PC monitor
	Numerical display: Basic measurement items
	Waveform display: Instantaneous waveform data
	Bar graph: Harmonic
	Vector: Fundamental wave vector
Measured value	Saves the specified instantaneous value data to the PC
save function	Selects the item to save from the numerical value display items in the display function
Interval save function	Saves instantaneous value data to the PC at the specified interval
CSV conversion function	Saves the displayed waveform data in CSV format to the PC
BMP save function	Saves the displayed waveform and graph data in image format to the PC or copy images to the clipboa
Setting function	Sends the settings of the 3390 made on a PC to the 3390
Setting function	

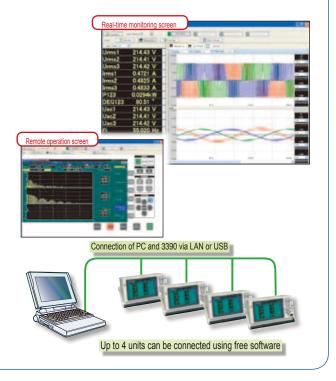

■3390 Specifications
(Accuracy guarantee conditions: 23°C ±3°C, 80%RH or less, warm-up time 30 minutes or more, sinusoidal wave input, power factor 1, voltage to ground 0 V, in the range where the fundamental wave meets the conditions of the synchronization source after zero adjustment)

Input				
Measurement line	Single-phase two- phase three-wire (3			
Connection setting	CH1	CH2	CH3	CH4
Pattern 1	1P2W	1P2W	1P2W	1P2W
Pattern 2	1P3	W	1P2W	1P2W
Pattern 3	3P3W	/2M	1P2W	1P2W
Pattern 4	1P3	W	1P:	3W
Pattern 5	3P3W	/2M	1P:	3W
Pattern 6	3P3W	/2M	3P3V	V2M
Pattern 7		3P3W3M		1P2W
Pattern 8		3P4W		1P2W
Number of input channels	Voltage: 4 channels Current: 4 channels			
Input terminals	Voltage: Plug-in ter Current: Dedicated	connector		
Input method	Voltage: Isolated in Current: Isolated in		tage dividing metho sensor (voltage outp	
Measurement range Voltage range Current range () indicates the sensor rating used	*400.00mA / *800.00 4.0000A / 8.0000A /2	60.000V / 150.00V 0mA / 2.0000A / 4.0 20.000A / 40.000A /	/ 300.00V / 600.00V 000A / 8.0000A / 20.	000A (20 A rating) 200 A rating)
Dower range	10.000A / 20.000A / 50.000A / 100.00A / 200.00A / 500.00A (500 A rating) * Only UNIVERSAL CLAMP ON CT CT6841 is applicable			
Power range Crest factor	Depends on combination of voltage and current range (6.0000 W to 2.2500 MW) 3 (voltage/current), 1.33 for 1500 V			
Input method	Voltage input part: 2 M Ω ±40 k Ω (Differential input and isolated input)			
(50/60Hz)	Voltage input part: 2 M Ω ±40 k Ω (Differential input and isolated input) Current sensor input part: 1 M Ω ±50 k Ω			
Maximum input voltage	* *			
Maximum rated voltage to ground	Voltage input terminal 1000 V (50/60 Hz) Measurement category III 600 V (Expected transient overvoltage 6000 V) Measurement category II 1000 V (Expected transient overvoltage 6000 V)			
Measurement method	Voltage and current simultaneous digital sampling and zero cross synchronization calculation method			
Sampling	500kHz / 16bit			
Frequency band	DC, 0.5 Hz to 150	kHz		
Synchronization frequency range	0.5Hz to 5kHz			
Synchronization source	U1 to U4 / I1 to I4 / Ext (with motor analysis option, CH B: when pulse is set) / DC (50 ms, 100 ms fixed) * Selectable for each connection (Zero cross auto follow-up by digital LPF when U / 1), Filter resistance two-stage switching (high / low), source input 30%f.s. or more when U / 1			
Data update rate	50ms			
LPF	OFF / 500 Hz / 5 kHz / 100 kHz (Selectable for each connection) When 500 Hz: Accuracy +0.1%f.s. specified at 60 Hz or less When 5 kHz: Accuracy specified at 500 Hz or less When 100 kHz: Accuracy specified at 20 kHz or less (1%rdg, is added at 10k Hz to 20 kHz			
Polarity determination	Voltage/current zero cross timing comparison method			
Polarity			(P), apparent power	
determination	(Q), power factor (λ), phase angle (φ), frequency (f), efficiency (η), loss (Loss)			
Measurement parameters	voltage ripple factor (Ufr), current ripple factor (Ifr), current integration (Ih) power integration (WP), voltage peak (Upk), current peak (Ipk)			
parameters	power integration (v	, 1 /, voltage peak (t	pr., current peak (I	μπ <i>)</i>

Accurate	Voltage, currency,	and active power m	easurements
Accuracy			
	Voltage (U)	Current (I)	Active power (P)
DC	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.
0.5Hz to 30Hz	±0.1%rdg.±0.2%f.s.	±0.1%rdg.±0.2%f.s.	±0.1%rdg.±0.2%f.s.
30Hz to 45Hz	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.
45Hz to 66Hz	±0.05%rdg.±0.05%f.s.	±0.05%rdg.±0.05%f.s.	±0.05%rdg.±0.05%f.s.
66Hz to 1kHz	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.
1kHz to 10kHz	±0.2%rdg.±0.1%f.s.	±0.2%rdg.±0.1%f.s.	±0.2%rdg.±0.1%f.s.
10kHz to 50kHz	±0.3%rdg.±0.2%f.s.	±0.3%rdg.±0.2%f.s.	±0.4%rdg.±0.3%f.s.
50kHz to 100kHz	±1.0%rdg.±0.3%f.s.	±1.0%rdg.±0.3%f.s.	±1.5%rdg.±0.5%f.s.
100kHz to 150kHz	±20%f.s.	±20%f.s.	±20%f.s.
	* Voltage and active power values * Voltage and active power values * Voltage and active power values * Voltage and active power values	wer values at 0.5 Hz to 10 Hz are ref more than 220 V at 10 Hz to 16 Hz; more than 750 V at 30 kHz to 100 k more than (22000/f [kHz]) V at 100 k more than 1000 V are reference valt wer values, add the accuracy of the ct	are reference values Hz are reference values Hz to 150 kHz are reference values ues
Accuracy guarantee period	6 months (One-year accuracy is the above accuracy × 1.5) (Post-adjustment accuracy guaranteed for 6 months)		
Temperature coefficient	±0.01%.f.s / °C (When D	OC: Add ±0.01%f.s./°C)	
Effect of common mode voltage	±0.01%f.s. or less (When input terminal and the ca	n applying 1000 V (50/60 se)	Hz) between the voltage
Effect of external magnetic field	±1.0%f.s. or less (in a ma	agnetic field at 400 A/m, D	OC, and 50/60 Hz)

Effect of power factor	$\pm 0.15\% f.s.$ or less (When power factor = 0.0 at 45 Hz to 66 Hz), add $\pm 0.45\% f.s.$ when LPF is 500 Hz
Effective measurement range	Voltage, current, and power: 1% to 110% of range
Display range	Voltage, current, and power: Range's zero suppress range setting to ±120%
Zero suppress range	Selects from OFF, 0.1%f.s., and 0.5%f.s. * When OFF is selected, a numerical value may be displayed even if zero is input
Zero adjustment	Voltage: ±10%f.s. Current: ±10%f.s. zero correction is performed for an input offset less than ±4 mV
Waveform peak measurement	Range: Within ±300% of respective voltage and current range Accuracy: Voltage and current respective display accuracy ±2%f.s.

	neasurement
Number of measurement channels	4 channels (f1, f2, f3, f4)
Measurement source	Selects from U / I for each input channel
Measurement method	Reciprocal method + zero cross sampling value correction
Measurement range	Within synchronization frequency range between 0.5 Hz and 5 kHz
Data update rate	50 ms (Depends on the frequency when 45 Hz or less)
Accuracy	±0.05%rdg.±1dgt. (When sinusoidal waveform is 30% or more relative to the measurement range of measurement source)
Display range	0.5000Hz to 9.9999Hz / 9.900Hz to 99.999Hz / 99.00Hz to 999.99Hz / 0.9900kHz to 5.0000kHz

Integration r	neasurement
Measurement mode	RMS / DC (Selectable for each connection, DC is only available when AC/DC sensor is used for 1P2W connections) RMS: Integrates the current RMS values and active power values, only the active values are integrated for each polarity
Measurement	DC: Integrates the current values and instantaneous power values for each polarity Current integration (Ih+, Ih-, Ih), active power integration (WP+, WP-, WP)
item	Ih+ and Ih- are available only in DC mode, and only Ih is available in RMS mode.
Measurement method	Digital calculation from each current and active power
Measurement interval	Data update rate of 50 ms
Display resolution	999999 (6 digits + decimal point)
Measurement range	0 to ±9999.99 TAh / TWh (Integration time is within 9999 h 59 m) If any integration value or integration time exceeds the above limit, integration stops.
Integration time accuracy	±50 ppm ±1 dgt. (0°C to 40°C)
Integration accuracy	±(Accuracy of current and active power) ± integration time accuracy
Backup function	If power fails during integration, integration resumes after power is restored

Integration time accuracy A channels (Harmonic measurement for another line at a different frequency cannot be performed) Harmonic voltage RMS value, harmonic voltage percentage, harmonic voltage phas angle, harmonic current RMS value, harmonic current percentage, harmonic current phase angle, harmonic active power, harmonic power percentage, harmonic current phase difference, total harmonic voltage distortion factor, total harmonic current distortion factor, voltage disequilibrium factor, current disequilibrium factor,	The same of the sa			
Accuracy cannot be performed) Harmonic voltage RMS value, harmonic voltage percentage, harmonic voltage phas angle, harmonic current RMS value, harmonic voltage phase angle, harmonic current phase angle, harmonic active power, harmonic power percentage, harmonic current phase angle, harmonic active power, harmonic voltage distortion factor, total harmonic voltage distortion factor, current diseoulle harmonic voltage distortion facto	Harmonic measurement			
Harmonic voltage RMS value, harmonic voltage percentage, harmonic voltage phangle, harmonic current RMS value, harmonic current percentage, harmonic current phase angle, harmonic active power, harmonic power percentage, harmonic voltage discording current phase angle, harmonic active power, harmonic power percentage, harmonic voltage discording current phase angle, harmonic active power, harmonic power percentage, harmonic voltage discording current phase angle, harmonic active power, harmonic power percentage, harmonic current phase angle, harmonic current RMS value, harmonic voltage discording to the phase angle, harmonic current discording voltage discording fustor, to voltage discording fustor, to voltage discording fustor, to voltage discording fustor, to voltage discording fustor, harmonic voltage pharmonic current processing during the voltage discording fustor, to voltage discording fustor, harmonic voltage harmonic current processing discording fustor, to voltage discording fustor, harmonic voltage pharmonic current processing discording fustor, voltage discording fustor, to voltage discording fustor, current discording fustor, voltage discording fustor, current discording fustor fustor, current discording fustor fustor fustor, current discording fustor fustor, voltage discording fustor, current discording fustor fustor, current discording fustor fustor fustor, current discording fustor, current dis	•			
angle, harmonic current RMS value, harmonic current percentage, harmonic curre phase angle, harmonic active power, harmonic power percentage, harmonic voltage current phase difference, total harmonic voltage distortion factor, total harmonic current distortion factor, voltage disequilibrium factor, current disequilibrium factor. Measurement method Zero cross synchronous calculation method (All channels same window) with ga Synchronization	accuracy	1 /		
Synchronization source FFT processing word length Anti-aliasing filter Window function Synchronization frequency range Data update rate Phase zero adjustment Maximum analysis order Maximum analysis order Maximum analysis order Zero cross synchronous calculation method (All channels same window) with gas ynchronization frequency method (C50 ms/100 ms) PFT processing word length Digital filter (Variable by the synchronization frequency) Rectangular O.5 Hz to 5 kHz Data update rate Synchronization frequency when less than 45 Hz) Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency range O.5Hz to 40Hz 1 100th order 40Hz to 80Hz 1 100th order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order	Measurement item	Harmonic voltage RMS value, harmonic voltage percentage, harmonic voltage phase angle, harmonic current RMS value, harmonic current percentage, harmonic current phase angle, harmonic active power, harmonic power percentage, harmonic voltage/ current phase difference, total harmonic voltage distortion factor, total harmonic current distortion factor, voltage disequilibrium factor, current disequilibrium factor		
Source DC (50 ms/100 ms) 32-bit Anti-aliasing filter Window function Rectangular O.5 Hz to 5 kHz Phase zero adjustment Maximum analysis order Maximum analysis order DC (50 ms/100 ms) 32-bit 32-bit 32-bit Oigital filter (Variable by the synchronization frequency) Rectangular O.5 Hz to 5 kHz Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency range Window wave number Analysis order 0.5Hz to 40Hz 1 100th order 40Hz to 80Hz 1 100th order 80Hz to 160Hz 2 80th order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order		Zero cross synchronous cal	culation method (All chann	nels same window) with gap
Maximum analysis order Manti-aliasing filter Anti-aliasing filter Digital filter (Variable by the synchronization frequency) Mindow function Synchronization Synchronization O.5 Hz to 5 kHz Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency when less than 45 Hz) Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency range Window wave number Analysis order 0.5Hz to 40Hz 1 100th order 40Hz to 80Hz 1 100th order 80Hz to 160Hz 2 80th order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order			otor analysis option included	I, CHB: when pulse is set) /
Window function Synchronization frequency range Data update rate Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency when less than 45 Hz) Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency range O.5Hz to 40Hz 1 100th order 40Hz to 80Hz 1 100th order 80Hz to 160Hz 2 80th order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order		32-bit		
Synchronization frequency range Data update rate 50 ms (Depends on the synchronization frequency when less than 45 Hz) Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency when less than 45 Hz) Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency range Window wave number Analysis order 0.5Hz to 40Hz 1 100th order 40Hz to 80Hz 1 100th order 80Hz to 160Hz 2 80th order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order	Anti-aliasing filter	Digital filter (Variable by the synchronization frequency)		
Data update rate 50 ms (Depends on the synchronization frequency when less than 45 Hz) Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency range Window wave number Analysis order 0.5Hz to 40Hz 1 100th order 40Hz to 80Hz 1 100th order 80Hz to 160Hz 2 80th order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order	Window function	Rectangular		
Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext) Synchronization frequency range Window wave number Analysis order	•	0.5 Hz to 5 kHz		
Synchronization source is Ext) Synchronization frequency range Window wave number Analysis order	Data update rate	50 ms (Depends on the synchronization frequency when less than 45 Hz)		
Maximum analysis order Maximum analysis order Maximum analysis order 0.5Hz to 40Hz		Phase zero adjustment is possible by key / communication command (only when the synchronization source is Ext)		
Maximum analysis order Maximum analysis order 0.5Hz to 40Hz		Synchronization frequency range	Window wave number	Analysis order
80Hz to 160Hz 2 80th order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order		0.5Hz to 40Hz	1	
Maximum analysis order 160Hz to 320Hz 4 40th order 320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order		40Hz to 80Hz	1	100th order
analysis order 160Hz to 320Hz		80Hz to 160Hz	2	80th order
320Hz to 640Hz 8 20th order 640Hz to 1.2kHz 16 10th order		160Hz to 320Hz	4	40th order
		320Hz to 640Hz	8	20th order
1 2kHz to 2 5kHz 32 5th order		640Hz to 1.2kHz	16	10th order
1.2Ki iz to 2.5Ki iz 32 Still older		1.2kHz to 2.5kHz	32	5th order
2.5kHz to 5.0kHz 64 3rd order		2.5kHz to 5.0kHz	64	3rd order

Accuracy	Frequency	Voltage (U) / current (I) / active power(P)
	0.5Hz to 30Hz	±0.4%rdg.±0.2%f.s.
	30Hz to 400Hz	±0.3%rdg.±0.1%f.s.
	400Hz to 1kHz	±0.4%rdg.±0.2%f.s.
	1kHz to 5kHz	±1.0%rdg.±0.5%f.s.
	5kHz to 10kHz	±2.0%rdg.±1.0%f.s.
	10kHz to 13kHz	±5.0%rdg.±1.0%f.s.
	* Not specified wh	en the synchronization frequency is 4.3 kHz or more
Noice mess	urement /EET press	noing)

	Not specified when the synchronization frequency is 4.5 kHz of friore
Noise measu	urement (FFT processing)
Number of channels	1 channel (Selects one channel from CH1 to CH4)
Measurement item	Voltage/current
Calculation type	RMS spectrum
Measurement method	500 kHz/s sampling (Decimation after digital anti-aliasing filtering)
FFT processing word length	32-bit
Number of FFT	1,000 points / 5,000 points / 10,000 points / 50,000 points (Linked to the
points	waveform display record length)
Anti-aliasing filter	Digital filter auto (Variable by the maximum analysis frequency)
Window function	Rectangular / Hanning / flat top
Data update rate	Within about 400 ms to 15 s depending on the number of FFT points, with gap
Maximum analysis frequency	100kHz / 50kHz / 20kHz / 10kHz / 5kHz / 2kHz
Frequency	0.2 Hz to 500 Hz (Determined by the number of FFT points and the
resolution	maximum analysis frequency)
Noise value	Calculates the levels and frequencies of voltage and current peaks
measurement	(maximum values) for the top 10 points

CH A: Analog DC input / frequency input (torque signal input)	MOTOR TES	TING OPTION (Applicable to the 9791 and 9793)				
Number of input channels CH A: Analog DC input / pulse input (rotation signal input) CH B: Analog DC input / pulse input (rotation signal input) Input terminal form input resistance (DC) Input method Isolation type BNC connector Input method Isolation type BNC connector Input method Isolated input and differential input (No isolation between CH B and CH Z) Measurement item Maximum input voltage Maximum rated voltage to ground Accuracy guarantee period 1. Analog DC input (CH A / CH B) Measurement range If to 110 / K S. Sampling In kHz / 16-bit Measurement method Synchronization Source and CH B) Accuracy ±0.1% fs. Temperature coefficient ±0.03% fs.β*C Temperature coefficient ±0.01% fs. or less when applying 50 V (DC 50/60 Hz) between the input terminal and the 3390 case Display range Display range 2-To radjustment 2-To requency input (only for CH A) Synchron leading 1 to 60000 Measurement range Band width IkHz to 100kHz Band width IkHz to 50 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) In 60000 Bassurement band IkHz to 50 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) Display range 2.5 μs or more descuracy 4.0.5 v or less, High: 2.0 V or more Measurement band IkHz to 1 k	O POIN I E					
channels $CH B: Analog DC input / pulse input (rotation signal input)$ Input terminal form Isolation type BNC connector Input resistance (DC) Input method Measurement item Voltage, torque, rotation, frequency, slip, motor output $\pm 20 \text{ V}$ (When analog / frequency / pulse) Maximum input voltage Maximum rated $\pm 20 \text{ V}$ (When analog / frequency / pulse) Maximum rated $\pm 20 \text{ V}$ (When analog / frequency / pulse) Maximum rated $\pm 20 \text{ V}$ (When analog / frequency / pulse) Maximum rated $\pm 20 \text{ V}$ (When analog / frequency / pulse) Maximum rated $\pm 20 \text{ V}$ (When analog / frequency / pulse) Maximum rated $\pm 20 \text{ V}$ (When analog / frequency / pulse) Maximum rated $\pm 20 \text{ V}$ (When analog DC input) Maximum rated $\pm 20 \text{ V}$ ($\pm 20 $	Number of input					
CH Z: Pulse input (Z-phase signal input) Input resistance (DC) Input method Measurement item Maximum input voltage, torque, rotation, frequency, slip, motor output ### ### ### ### ### ### ### ### ### #						
Input terminal form Input resistance (DC) In $\Omega \pm 100 \text{ k}\Omega$ Isolated input and differential input (No isolation between CH B and CH Z) Measurement Item Maximum input voltage BMAximum rated voltage to ground Accuracy Gmonths (One-year accuracy is the accuracy below x 1.5) (Post-adjustment accuracy guaranteed for 6 months) 1. Analog DC input (CH A / CH B) Measurement range $\pm 1 \text{ V} + 5 \text{ V} + 10 \text{ V}$ (When analog DC input) Effective input range $\pm 1 \text{ V} + 5 \text{ V} + 10 \text{ V}$ (When analog DC input) Simultaneous digital sampling and zero cross synchronization method (Zero cross averaging) Synchronization Same as the 3390 power measurement input specification (Common for CH A) and CH B) Accuracy $\pm 0.1\% f.s.$ Effect of common mode voltage to $\pm 0.01\% f.s.$ Effect of common mode voltage to $\pm 0.01\% f.s.$ or less when applying 50 V (DC 50/60 Hz) between the input terminal and the 3390 case Range's zero suppress range setting to $\pm 120\%$ Zero adjustment $\pm 0.01\% f.s.$ or less when applying $\pm 0.00\% f.s.$ or less $\pm 0.00\%$	onamicio					
Input resistance (DC) Input method Measurement item Maximum input voltage Maximum rated voltage to ground Accuracy guarantee period I. Analog DC input (CH A / CH B) Measurement range Holl-fire temperature coefficient Coefficient Effector for common Accuracy Biplay range Display range Display range Display range Display range Band width Accuracy Accuracy Sov (50 kg Hz) Samplifue Accuracy Accuracy Biplay range Display	Input terminal form					
Isolated input and differential input (No isolation between CH B and CH Z) Measurement item Maximum input voltage Maximum rated voltage to ground Accuracy guarantee period 1. Analog DC input (CH A / CH B) Measurement range Effective input range Symchronization Symchronization Symchronization Symchronization Same as the 3390 power measurement input specification (Common for CH A) Symchronization Same as the 3390 case Display range Display range Accuracy 2. Frequency input (only for CH A) Effective amplitude range Band width IkHz to 100kHz Band width IkHz to 100kHz Band width IkHz to 200 kHz (When duty ratio is 50%) Trequency divider setting range Measurement band Ith zo 200 kHz (When duty ratio is 50%) Trequency divider setting range Minimum Measurement lond IkHz to 1 kHz Maximum input voltage ±1 V / ±5 V / ±10 V (When analog DC input) Effective for month of the curracy guaranteed for 6 months) 1. Analog DC input (CH A / CH B) Measurement method Simultaneous digital sampling and zero cross synchronization calculation method (zero cross averaging) Some as the 3390 power measurement input specification (Common for CH A) Effect of common mode voltage Display range 1. 0.03%f.s./°C Effect of common mode voltage Display range Accuracy 1. 0.03%f.s./°C 2. Frequency input (only for CH A) Effective amplitude range ### Accuracy 1. 0.05%rdg.±3dgt. 1. 0.00kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement band 1. Hz to 5.0 kHz (Specified by the frequency at which the measurement frequency range Minimum detection width Accuracy 1. 0.05 vor less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 μs or more		7.1				
Measurement item Maximum input voltage Maximum rated voltage to ground Accuracy guarantee period 1. Analog DC input (CH A / CH B) Measurement range 41 V +5 V +10 V (When analog DC input) Measurement range 41 V +5 V +10 V (When analog DC input) Measurement method Synchronization Measurement method Synchronization Synchronization Synchronization Maximum rated voltage 40 method (zero cross averaging) Measurement method Maximum rated Minimum Maximum rated voltage ±1 V +5 V +10 V (When analog DC input) Measurement method Measurement method Measurement method Measurement Measurement Method Measurement Measureme						
Maximum input voltage #20 V (When analog / frequency / pulse) #30 V (50/60 Hz) #31 V (50 V (50/60 Hz) #32 V (50/60 Hz) #33 V (50 V (50/60 Hz) #34 V (50 V (50/60 Hz) #35 V (50/60 Hz) #36 V (50/60 Hz) #36 V (50/60 Hz) #36 V (50/60 Hz) #37 V (50/60 Hz) #38 V (50/60 Hz) #39 V (50/60 Hz) #30 V (50/60 Hz) #3						
Maximum rated voltage to ground Accuracy from the control of the		voltage, torque, rotation, frequency, snp, motor output				
voltage to ground Accuracy guarantee period (Post-adjustment accuracy is the accuracy below x 1.5) guarantee period (Post-adjustment accuracy guaranteed for 6 months) 1. Analog DC input (CH A / CH B) Measurement range	voltage	±20 V (When analog / frequency / pulse)				
Quarantee period Post-adjustment accuracy guaranteed for 6 months	Maximum rated voltage to ground	· · ·				
1. Analog DC input (CH A / CH B) Measurement range ±1 V / ±5 V / ±10 V (When analog DC input) Effective input range Synchronization method method (zero cross averaging) Synchronization source and CH B) Accuracy ±0.1%rdg, ±0.1%f.s. Temperature coefficient ±0.03%f.s./°C Effect of common mode voltage Display range Range's zero suppress range setting to ±120% Zero adjustment Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Measurement range Measurement range Band width IkHz to 100kHz Accuracy ±0.05%rdg,±3dgt. Display range 1.00wkHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement frequency divider setting range Measurement frequency divider setting range Measurement frequency range most side deby the set frequency dividing number) Minimum detection width Liz to 1 kHz Minimum detection width Liz to 1 kHz Minimum detection width Clark to 1 kHz Minimum detection width Clark to 1 kHz Minimum detection width Clark to 1 kHz Li v 1 kHz Li v 2.5 μs or more	Accuracy					
Measurement range Effective input range If to 110%f.s. Sampling If to 110%f.s. Sampling If to 110%f.s. Simultaneous digital sampling and zero cross synchronization calculation method method (zero cross averaging) Synchronization source Accuracy ±0.1%rdg.±0.1%f.s. Temperature coefficient ±0.03%f.s./°C Effect of common mode voltage Display range Range's zero suppress range setting to ±120% Zero adjustment Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Measurement range Measurement range Band width IkHz to 100kHz Accuracy ±0.05%rdg.±3dgt. Display range I to 60000 Synchronization Same as the 3390 power measurement input specification (Common for CH A) Effect of common terminal and the 3390 case ### 2016/f.s. ### 2016/	guarantee period	(Post-adjustment accuracy guaranteed for 6 months)				
Effective input range Sampling 10 kHz / 16-bit Measurement method Measurement method (zero cross averaging) Same as the 3390 power measurement input specification (Common for CH A and CH B) Accuracy ±0.1%rdg.±0.1%f.s. Temperature coefficient Effect of common mode voltage Display range Display range Paro adjustment Noltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Measurement range Measurement range Measurement range 100kHz Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement band Trequency divider setting range Measurement Measu	1. Analog DC in	put (CH A / CH B)				
Sampling 10 kHz / 16-bit	Measurement range	±1 V / ±5 V / ±10 V (When analog DC input)				
Sampling 10 kHz / 16-bit	Effective input range	1% to 110%f.s.				
Measurement method Simultaneous digital sampling and zero cross synchronization calculation method (zero cross averaging) Synchronization source and CH B) Accuracy ±0.1%rdg. ±0.1%f.s. Temperature coefficient ±0.03%f.s./*C Effect of common mode voltage Display range Range's zero suppress range setting to ±120% Zero adjustment Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Measurement range Band width 1kHz to 100kHz Accuracy ±0.05%rdg.±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement frequency grange Measurement frequency range Measurement frequency range Measurement frequency divider setting range Measurement frequency divider detection width 40.05%rdg. ±3dgt. 2.5 μs or more 40.05%rdg. ±3dgt. 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 40.01 kHz to 1 kHz 2.5 μs or more		10 kHz / 16-bit				
method method (zero cross averaging) Synchronization source and CH B) Accuracy ±0.1%rdg. ±0.1%f.s. Effect of common mode voltage bisplay range cardjustment voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range measurement input specification (Common for CH A) ±5V peak bisplay range 100kHz Band width 1kHz to 100kHz Accuracy ±0.05%rdg.±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Low: 0.5 V or less, High: 2.0 V or more 1 Hz to 200 kHz (When duty ratio is 50%) Has one of the decidence		Simultaneous digital sampling and zero cross synchronization calculation				
Synchronization source Accuracy Accuracy Display range Accuracy Effective amplitude range Measurement range Band width Accuracy 1000 kHz Bereating input (only for CH B) Detection level Accuracy 100 kHz (When duty ratio is 50%) Trequency divider range Measurement frequency at which the measurement frequency range Measurement frequency and the sid wided by the set frequency dividing number) Minimum detection level Low: 0.5 V or less, High: 2.0 V or more 2.5 µs or more 4. Pulse input (only for CH Z) Detection level Measurement band Minimum detection width Minimum detection width Alimimum detection width Minimum detection width Minimum detection width Minimum detection width Minimum detection width Accuracy 2.5 µs or more						
source and CH B) Accuracy ±0.1%rdg, ±0.1%f.s. Temperature coefficient ±0.03%f.s./*C Effect of common mode voltage terminal and the 3390 case Display range Range's zero suppress range setting to ±120% Zero adjustment Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range measurement range 100kHz Band width IkHz to 100kHz Accuracy ±0.05%rdg,±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band frequency divider grange Measurement the measurement frequency divider grange Measurement frequency divider side divided by the set frequency dividing number) Minimum detection level Low: 0.5 V or less, High: 2.0 V or more buse is divided by the set frequency dividing number) Measurement frequency divider side divided by the set frequency dividing number) More divided by the set frequency dividing number)						
Accuracy ±0.1%rdg. ±0.1%f.s. Temperature coefficient ±0.03%f.s.°C Effect of common mode voltage Display range Range's zero suppress range setting to ±120% Zero adjustment Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Measurement range Band width 1kHz to 100kHz Accuracy ±0.05%rdg.±3dgt. J.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement band Frequency divider setting range Measurement frange Measurement frange Measurement frange Measurement frange Measurement frange Now 1.5 V or less, High: 2.0 V or more 1 Hz to 200 kHz (When duty ratio is 50%) 1 to 60000 Now 1.5 V accuracy divider setting range Measurement frequency range Minimum Minimum Measurement band Now 1.5 V accuracy 1.005%rdg.±3dgt. 1.000kHz to 90.999kHz 2.5 μs or more 2.5 μs or more 2.5 μs or more Measurement band Minimum Metection width Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more Measurement band Now 1.5 V or less, High: 2.0 V or more	,					
Temperature coefficient #0.03%f.s./°C Effect of common mode voltage Display range Zero adjustment 2. Frequency input (only for CH A) Effective amplitude range Measurement range Band width 1kHz to 100kHz 3. Pulse input (only for CH B) Detection level Measurement frequency divider setting range Measurement frequency range Minimum detection level Measurement band Low: 0.5 V or less, High: 2.0 V or more 2.5 μs or more 2.5 μs or more Measurement band Minimum detection width Alia (2.5 μs or more 2.5 μs or more Measurement band Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width Alia (3.000 Hz to 1 kHz Minimum detection width)		*				
coefficient Effect of common mode voltage Display range Range's zero suppress range setting to ±120% Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Measurement range Band width 1kHz to 100kHz Accuracy 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement band Frequency divider setting range Measurement frange Measurement frange Measurement frange Measurement band Frequency divider setting range Measurement frange Minimum detection width Accuracy 4. Pulse input (only for CH Z) Detection level Measurement band O.1 Hz to 1 kHz Minimum detection width 2.5 μs or more						
mode voltage Display range Range's zero suppress range setting to ±120% Zero adjustment Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Measurement range Band width IkHz to 100kHz Accuracy ±0.05%rdg.±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement band Frequency divider setting range Measurement Measurement frequency divider range Measurement frequency divider setting range Measurement Measurement frequency range Minimum detection level Measurement Moltage	coefficient					
Display range Zero adjustment Voltage ±10%f.s. 2. Frequency input (only for CH A) Effective amplitude range Band width IkHz to 100kHz Accuracy ±0.05%rdg.±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement band 1 Hz to 200 kHz (When duty ratio is 50%) Frequency divider setting range Measurement frequency arge Measurement frequency arge Minimum detection level Measurement Measurement Measurement Molosymphoto 2.5 μs or more Measurement Measurement Measurement Molosymphoto Molo						
Zero adjustment 2. Frequency input (only for CH A) Effective amplitude range ±5V peak ### Measurement range Band width IkHz to 100kHz Accuracy ±0.05%rdg.±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Measurement band Ikz to 200 kHz (When duty ratio is 50%) 1 to 60000 Measurement frequency divider setting range Minimum detection width Accuracy 4. Pulse input (only for CH Z) Detection level Measurement band Minimum detection width Alignment Accuracy Measurement Band Minimum detection width						
2. Frequency input (only for CH A) Effective amplitude range Measurement range Band width Accuracy Display range 3. Pulse input (only for CH B) Detection level Measurement band Frequency divider setting range Measurement frequency range Minimum detection width Accuracy Detection level Low: 0.5 V or less, High: 2.0 V or more 1 to 60000 1 to 60000 2.5 µs or more 2.5 µs or more Measurement band O.1 Hz to 1 kHz Detection level Low: 0.5 V or less, High: 2.0 V or more 1 to 60000 1 to 60000 2.5 µs or more 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 2.5 µs or more						
Effective amplitude range Measurement range Band width Accuracy Display range 3. Pulse input (only for CH B) Detection level Measurement band Frequency divider setting range Measurement frequency range Minimum detection width Accuracy Detection level Low: 0.5 V a less, High: 2.0 V or more 1 to 60000 1 to 60000 2.5 µs or more 2.5 µs or more Measurement band O.1 Hz to 1 kHz Detection level Low: 0.5 V or less, High: 2.0 V or more 1 to 60000 1 to 60000 2.5 µs or more 2.5 µs or more Measurement band Minimum detection width Accuracy Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 2.5 µs or more		-				
amplitude range ±5 V peak Measurement range 100kHz Band width 1kHz to 100kHz Accuracy ±0.05%rdg,±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Low: 0.5 V or less, High: 2.0 V or more Measurement band 1 Hz to 200 kHz (When duty ratio is 50%) Frequency divider setting range 1 to 60000 Measurement frequency range 0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) Minimum detection width 2.5 μs or more 4. Pulse input (only for CH Z) Detection level Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 μs or more	2. Frequency in	put (only for CH A)				
Band width Accuracy Display range 1.000kHz to 99.999kHz 1.000kHz to 99.999kHz 1.000kHz to 99.999kHz 1.000kHz to 99.999kHz Low: 0.5 V or less, High: 2.0 V or more 1 Hz to 200 kHz (When duty ratio is 50%) 1 to 60000 Measurement frequency divider setting range Measurement frequency range Minimum detection width Accuracy 1.000kHz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) 2.5 µs or more 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 2.5 µs or more		±5Vpeak				
Band width		100kHz				
Accuracy ±0.05%rdg.±3dgt. Display range 1.000kHz to 99.999kHz 3. Pulse input (only for CH B) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 1 Hz to 200 kHz (When duty ratio is 50%) 1 to 60000 Measurement frequency divides the frequency at which the measurement pulse is divided by the set frequency dividing number) Minimum detection width Accuracy ±0.05%rdg. ±3dgt. 4. Pulse input (only for CH B) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 μs or more 2.5 μs or more	_					
Display range 3. Pulse input (only for CH B) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band d 1 to 60000 1 to 60000 0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) 2.5 μs or more ±0.05%rdg. ±3dgt. 4. Pulse input (only for CH Z) Detection level Measurement band Minimum detection width ΔCouracy 2.5 μs or more 2.5 μs or more 1 to 60000 2.5 μs or more 2.5 μs or more 1 to 60000 2.5 μs or more 2.5 μs or more 1 to 60000 2.5 μs or more 2.5 μs or more 2.5 μs or more						
3. Pulse input (only for CH B) Detection level Measurement band Frequency divider setting range Measurement frequency range Measurement frequency range Measurement band 0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) 2.5 µs or more 4. Pulse input (only for CH Z) Detection level Measurement band Minimum detection width 2.5 µs or more 2.5 µs or more Low: 0.5 V or less, High: 2.0 V or more 0.1 Hz to 1 kHz Minimum detection width 2.5 µs or more		0 0				
Detection level Measurement band Frequency divider setting range Measurement frequency range Measurement frequency range Minimum detection width Accuracy Measurement band Low: 0.5 V or less, High: 2.0 V or more 1 Hz to 200 kHz (When duty ratio is 50%) 1 to 60000 0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) 2.5 µs or more 4. Pulse input (only for CH Z) Detection level Measurement band Minimum detection width 2.5 µs or more 2.5 µs or more						
Measurement band 1 Hz to 200 kHz (When duty ratio is 50%) Frequency divider setting range 1 to 60000 Measurement frequency range 0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) Minimum detection width 2.5 μs or more 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 2.5 μs or more						
Frequency divider setting range Measurement frequency range Minimum detection width 1 to 60000 1 to 60000 0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) 2.5 µs or more 2.5 µs or more 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 2.5 µs or more						
Measurement frequency range Measurement frequency range Minimum detection width 1 to 60000 0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement pulse is divided by the set frequency dividing number) 2.5 μs or more 2.5 μs or more 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 2.5 μs or more		1 Hz to 200 kHz (When duty ratio is 50%)				
pulse is divided by the set frequency dividing number	setting range					
Minimum detection width 2.5 μs or more Accuracy ±0.05%rdg. ±3dgt. 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 μs or more	Measurement	0.5 Hz to 5.0 kHz (Specified by the frequency at which the measurement				
detection width Accuracy ±0.05%rdg. ±3dgt. 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 µs or more 2.5 µs or more	frequency range	pulse is divided by the set frequency dividing number)				
Accuracy ±0.05%rdg. ±3dgt. 4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band Minimum detection width 2.5 µs or more	Minimum	2.5 us or more				
4. Pulse input (only for CH Z) Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 µs or more	detection width	2.5 µs of more				
Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 µs or more	Accuracy	±0.05%rdg. ±3dgt.				
Detection level Low: 0.5 V or less, High: 2.0 V or more Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 µs or more	4. Pulse input (c	only for CH Z)				
Measurement band 0.1 Hz to 1 kHz Minimum detection width 2.5 µs or more						
Minimum detection width 2.5 μs or more		-				
detection width 2.5 μs or more						
OFF / ON (When ON, a frequency divider circuit of CH B is cleared by a rising edge)	detection width	'				
	Setting	OFF / ON (When ON, a frequency divider circuit of CH B is cleared by a rising edge)				

D/A OUTPUT	OPTION (Applicable to the 9792 and 9793)

Number of output channels 16 channels

Switchable between Waveform output / Analog output (selects from the measurement items) * Waveform output is only for CH 1 to CH 8
D-sub 25-pin connector × 1
16-bit (Polarity + 15-bit)
Analog: DC ±5 Vf.s. (Max. about DC ±12V) Waveform output: 2 Vrms f.s., crest factor: 2.5 or more
Analog output: Measurement accuracy $\pm 0.2\%$ f.s. (DC level) Waveform output: Measurement accuracy $\pm 0.5\%$ f.s. (at RMS level, in synchronization frequency range)
6 months (one-year accuracy is the above accuracy × 1.5) (Post-adjustment accuracy guaranteed for 6 months)
Analog output: 50 ms (As per the data update rate of the selected item) Waveform output: 500 kHz
100 Ω ±5 Ω
±0.05%f.s./°C

Display	
Display character	English / Japanese / Chinese (simplified characters)
Display	9-inch TFT color LCD display (800 × 480 pixels)
LCD backlight	ON / Auto OFF (1min / 5min / 10min / 30mim / 60min)
Display resolution	99999 counts (Integrated value: 999999 counts)
Display refresh rate	200 ms (Independent of internal data update rate; waveform and FFT depend on the screen)
Display screen	Measurement, Setting, File Manipulation screens

External inte	erfaces				
1. USB Interface	(Function)				
Connector	Series Mini-B receptacle				
Electrical specification	USB2.0 (Full Speed / High Speed)				
Number of ports	1				
Class	Vendor specific (USB488h)				
Destination	PC (Windows XP / Vista (32-bit version) / 7 (32-bit, 64-bit version))				
Function	Data transfer, remote operation, command control				
2. USB memory	interface				
Connector	USB type A connector				
Electrical specification	USB2.0				
Power supply	Up to 500 mA				
Number of ports	1				
Applicable USB memory	USB Mass Storage Class				
Recordable items	Setting file: Save/Load Measured value/recorded data: Copy (from the CF card data) Waveform data: Save, screen hard copy				
3. LAN interface					
Connector	RJ-45 connector × 1				
Electrical specification	IEEE802.3 compliant				
Transmission method	10BASE-T / 100BASE-TX auto recognition				
Protocol	TCP/IP				
Function	HTTP server (remote operation), dedicated port (port transfer, command control)				
4. CF card inter	face				
Slot	TYPE I × 1				
Usable card	Compact flash memory card (32 MB or more)				
Applicable memory capacity	Up to 2 GB				
Data format	MS-DOS format (FAT16 / FAT32)				
Recordable items	Setting file: Save / Load Measured value / automatically recorded data: Save (in CSV format) Waveform data: Save, screen hard copy				
5. RS-232C inter	rface				
Method	RS-232C, EIA RS-232D, CCITT V.24, JIS X5101 compliant				
Connector	D-sub 9-pin connector × 1				
Recordable items	Full duplex asynchronous method Data length: 8, parity: none, stop bit: 1, Flow control: Hard flow, delimiter: CR+LF				
Baud rate	9600, 19200, 38400 bps				
	ion control interface				
Terminal form	IN-side 9-pin round connector ×1, OUT-side 8-pin round connector x 1				
Signal	5 V (CMOS level)				
Maximum allowable input	±20V				
Signal delay	Up to 2 μs (Specified by the rising edge)				

Functions 1. Setting	
Rectification switching	rms / mean (Selectable for the voltage/current of each connection) rms: Displays the true RMS value (True RMS) mean: Displays the average-value rectified RMS value
Auto range	OFF / ON (Voltage and current range is selectable for each connection)

	OFF / 50 ms / 100 ms / 200 ms / 500 1 min / 5 min / 10 min / 15 min / 30		0 s / 15 s / 30 s /				
	* Maximum number of items to save can be specified by the setting (130 items/50						
	ms, up to 5000 items)						
	Interval time and maximum number Auto-save (When using a 512 MB card)						
Data save	of Items to be saved (When using a 512 MB card) Interval Number of items Number of items to save Maximum period						
interval	130 10 About 2 days						
	50ms (When 200 ms: 520)	40	About 14 hours				
	1s 2600	10	About 42 days				
	(5 s or more: 5000)	1000	About 11 hours About 416 days				
	1min 5000	4000	About 7 days				
	OFF / Timer / Actual time						
Time control	When using Timer: 10 s to 9999 h 59 When using Actual Time: Start time						
Scaling	VT ratio: OFF / 0.01 to 9999.99 CT ratio: OFF / 0.01 to 9999.99						
Averaging	Displays the averaged values of all in harmonic value	stantaneously me	asured values including				
	(Excluding the peak value, integrated	value, and noise	value)				
	* Averaged data applies to all data inc	luding the saved	data during averaging				
Method Response time	Exponential averaging (Applies to the OFF / 0.2s (FAST) / 1.0s (MID) / 5.0		te of 50 ms)				
Response une	(Time within which to fall in the accuracy ran	` /	anges to 0%f.s. to 100%f.s.)				
Efficiency/loss	Calculates the efficiency $\eta[\%]$ an	d loss [W] of a	active power for each				
calculation Calculated item	connection and channel. Active power value (P) for each channel.	el and connection	1				
Calculated Item	Motor power (Pm) when the 9791 and 9						
Calculation rate							
	* The latest data of calculation connections whose synchronization:						
Calculable factors	3 formats for the efficiency and loss, r						
Calculation algorithm	Calculated item is specified for Pin a		ormat below				
	η=100× Pout / Pin , Loss= Pin - Converts line voltage waveform t	· · · · · · · · · · · · · · · · · · ·	waveform using the				
Δ – Y calculation	virtual neutral point for 3P3W3M co	nnection					
_ r odlodiation	Uses a phase voltage to calculate all or voltage RMS value	voltage paramet	ers including harmonic				
Display hold	Stops and displays all displayed measure	d values and displa	y update of waveforms				
Data update	Updates data when the hold key						
Output data	reached, and when an external synchronization signal is detected D/A output, CF data save: Outputs the hold data (The waveform output continues,						
Output data	and the interval auto-save outputs data in						
Peak hold	Displays and updates the maximum va		measured data (without				
	waveform display and integrated value) (While averaging is performed, the many		applied to the measured				
	value after averaging. This cannot be used in conjunction with the Hold function)						
Data undata		Data is cleared when the hold key is manipulated, when the interval is					
Data update	Data is cleared when the hold key		, when the interval is				
	Data is cleared when the hold key reached, and when an external sync updated at an internal data update ra	chronization sign te of 50 ms)	, when the interval is				
Data update Output data	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rai D/A output, CF data save: Outputs the pe	chronization sign te of 50 ms) ak hold data	, when the interval is all is detected (Data is				
	Data is cleared when the hold key reached, and when an external sync updated at an internal data update ra	chronization sign te of 50 ms) ak hold data	, when the interval is all is detected (Data is				
Output data	Data is cleared when the hold key reached, and when an external sync updated at an internal data update ra D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared)	chronization sign te of 50 ms) ak hold data nd the interval	, when the interval is al is detected (Data is auto-save outputs data				
Output data 2. Display Connection	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and	chronization sign te of 50 ms) ak hold data and the interval	, when the interval is all is detected (Data is auto-save outputs data				
Output data	Data is cleared when the hold key reached, and when an external sync updated at an internal data update ra D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared)	chronization signate of 50 ms) also hold data and the interval and the voltage/curr vector diagram, so the	, when the interval is all is detected (Data is auto-save outputs data rent vector diagram to connection can be checked.				
Output data 2. Display Connection check screen Connection display screen	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and * The right connection range is displayed in the Displays measured power and harmo * The values are displayed for each measure	chronization signate of 50 ms) alk hold data and the interval and the voltage/curvector diagram, so the conic values on chement line pattern of	when the interval is all is detected (Data is auto-save outputs data rent vector diagram to connection can be checked. The combined connections				
Output data 2. Display Connection check screen Connection	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and * The right connection range is displayed in the Displays measured power and harmone	chronization sign te of 50 ms) ak hold data nd the interval : the voltage/cur vector diagram, so the mic values on che ment line pattern of tage Measuren	when the interval is all is detected (Data is auto-save outputs data rent vector diagram to connection can be checked. The combined connections				
Output data 2. Display Connection check screen Connection display screen	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmor *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Power Measurement screen, Vector start of the property	chronization sign te of 50 ms) ak hold data and the interval : all the voltage/curvector diagram, so the orici values on cho- ment line pattern of tage Measuren ement screen	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram e connection can be checked. annels 1 to 4 combined connections nent screen, Current				
Output data 2. Display Connection check screen Connection display screen DMM screen	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harma *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measur Bar Graph screen, List screen, Vector Selects and displays any 4, 8, 16, o	chronization sign te of 50 ms) ak hold data and the interval : all the voltage/curvector diagram, so the orici values on cho- ment line pattern of tage Measuren ement screen	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram e connection can be checked. annels 1 to 4 combined connections nent screen, Current				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmor *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Power Measurement screen, Vector start of the property	chronization sign te of 50 ms) ak hold data and the interval and the interval and the interval and the interval and the voltage/currector diagram, so the original and the voltage when the pattern of tage. Measuren ement screen coreen and the voltage and	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram to connection can be checked, annuels 1 to 4 frombined connections the screen, Current art items from all basic				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss	Data is cleared when the hold key reached, and when an external synupdated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and "The right connection range is displayed in the Displays measured power and harmor "The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Vector's Selects and displays any 4, 8, 16, of measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficie	chronization signate of 50 ms) ak hold data and the interval and the interval at the voltage/curvector diagram, so the onic values on channel line pattern of tage. Measuren ement screen ar 32 measurement and loss set in the street of the st	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram to connection can be checked. annuels 1 to 4 combined connections the screen, Current at items from all basic as (4 pattern switching)				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmore *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Vector's Selects and displays any 4, 8, 16, of measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficien Display pattern: 3 efficiency items, 3 lo	chronization signed of 50 ms) ak hold data and the interval and the voltage/curvector diagram, so the order of the comment line pattern of tage Measuren ement screen ar 32 measurement and loss set in tage the sitems.	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram e connection can be checked. annels 1 to 4 combined connections nent screen, Current at items from all basic as (4 pattern switching) the calculation algorithm				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harma *The values are displayed for each measure *Basic Measurement screen, Vol Measurement screen, Power Measur Bar Graph screen, List screen, Vectors Selects and displays any 4, 8, 16, o measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficiency items, 3 lo Displays the voltage/current waveforms *Displays the waveform and noise meas	chronization signer of 50 ms) alk hold data and the interval is the voltage/curvector diagram, so the original to the voltage when the pattern of tage Measuren ement screen creen ar 32 measurement and loss set in the signer. The voltage was a signer of the voltage when the voltage was a signer of the voltage when the voltage was a signer of the voltage when the voltage was a signer of the voltage was a signer of the voltage when the voltage was a signer of the voltage was a	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram e connection can be checked. annels 1 to 4 combined connections nent screen, Current at items from all basic as (4 pattern switching) he calculation algorithm z in a compressed screen				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harme *The values are displayed for each measure *Basic Measurement screen, Vol Measurement screen, Power Measur Bar Graph screen, List screen, Vector Selects and displays any 4, 8, 16, o measurement items Display apattern: 4 items, 8 items, 16 Displays the unmerical values of efficie bisplay pattern: 3 efficiency items, 3 lo Displays the voltage/current waveforms s * Displays the waveform and noise meas measurement is performed	chronization signate of 50 ms) ak hold data and the interval at the voltage/cur vector diagram, so the original to the voltage when the pattern of tage. Measuren ement screen ar 32 measurement items, or 32 item at and loss set in the sitems. The vector of the vector o	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram to connection can be checked. The same of the checked of combined connections and the same of the				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the pe (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harma *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measur Bar Graph screen, List screen, Vector Selects and displays any 4, 8, 16, o measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficie bisplay pattern: 3 efficiency items, 3 lo Displays the voltage/current waveforms s * Displays the waveform and noise meas measurement is performed Synchronization timing of harmonic	chronization signate of 50 ms) ak hold data ak hold data ak hold data the interval at the voltage/cur vector diagram, so th onic values on ch ement line pattern of tage Measuren ement screen r 32 measureme r 32 measureme items, or 32 item at and loss set in t ss items. sampled at 500 kH urement (FFT calc synchronization	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data rent vector diagram to connection can be checked. annuels 1 to 4 frombined connections the screen, Current output items from all basic as (4 pattern switching) the calculation algorithm is in a compressed screen ulation) result when noise source				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen	Data is cleared when the hold key reached, and when an external synupdated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and "The right connection range is displayed in the Displays measured power and harmor "The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measure Bar Graph screen, List screen, Vector's Selects and displays any 4, 8, 16, of measurement items Displays the numerical values of efficie Display pattern: 3 efficiency items, 3 to Displays the voltage/current waveforms s' Displays the voltage/current waveforms s' Splays the voltage/current waveforms s' Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 10,	thronization signate of 50 ms) ak hold data and the interval at the voltage/curvector diagram, so the solic values on chement line pattern of tage. Measuren ement screen ar 32 measurement and loss set in the sistems. Sampled at 500 kHz urement (FFI calcomposition) and the synchronization of 50,000 points × as the sistems.	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data arent vector diagram are connection can be checked. annels 1 to 4 combined connections nent screen, Current at items from all basic at (4 pattern switching) he calculation algorithm at in a compressed screen ulation) result when noise source				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmore. The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Power Measurement screen, Vector's Selects and displays any 4, 8, 16, of measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficie Display pattern: 3 efficiency items, 3 lo Displays the voltage/current waveforms s' Displays the waveform and noise meas measurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peakerording speed)	chronization signed of 50 ms) ak hold data and the interval and the voltage/curvector diagram, so the ment line pattern of tage Measuren ement screen ar 32 measurene ement screen items, or 32 item and 103s set in the sitems. The sitems of 32 items ampled at 500 kHzurement (FFT calcosynchronization / 50,000 points x a Peak compression and the sitems of the sitems o	when the interval is all is detected (Data is all is detected (Data is auto-save outputs data arent vector diagram e connection can be checked. annels 1 to 4 forobined connections nent screen, Current nt items from all basic as (4 pattern switching) the calculation algorithm is in a compressed screen ulation) result when noise source				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram an *The right connection range is displayed in the Displays measured power and harmor *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Vol Measurement screen, Power Measurement its screen, Vector Selects and displays any 4, 8, 16, o measurement items Displays the numerical values of efficie Display pattern: 3 efficiency items, 3 lo Displays the voltage/current waveforms s *Displays the waveform and noise meas measurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording length) Recording speed / Recording length	thronization signer of 50 ms) ak hold data ak hold data ak hold data ak the interval of the voltage/curr vector diagram, so the original of the voltage on channel line pattern of tage. Measuren ement screen ar 32 measurene at the voltage was the vector of the vector o	when the interval is all is detected (Data is auto-save outputs data auto-save outputs data arent vector diagram se connection can be checked. annels 1 to 4 combined connections nent screen, Current at items from all basic at (4 pattern switching) he calculation algorithm at in a compressed screen source all voltage/current channels on)				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per commendate of the waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmor *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Power Measurement screen, Vector Selects and displays any 4, 8, 16, o measurement items Displays the numerical values of efficiency pattern: 3 efficiency items, 3 to Displays the voltage/current waveforms s *Displays the wordern and noise measureasurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording speed / Recording speed / Recording length 1,000 points 5,000	thronization signed of 50 ms) ak hold data and the interval and the voltage/curvector diagram, so the monic values on charment line pattern of tage Measurenement screen r 32 measurement and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems. Sampled at 500 kH urement (FFT calcosynchronization / 50,000 points x and Peak compression points and points and points are peak compression points are peak compression points are peak compression points are peaked and peaked pe	when the interval is all is detected (Data is all is detected (Data is auto-save outputs data arent vector diagram se connection can be checked. annels 1 to 4 combined connections nent screen, Current at items from all basic as (4 pattern switching) he calculation algorithm is in a compressed screen aulation) result when noise source all voltage/current channels on points 50,000 points 100ms				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per commendate of the waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmon *The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Power Measurement screen, Vector selects and displays any 4, 8, 16, on measurement items Displays the voltage and tiems, 8 items, 16 Displays the numerical values of efficiency pattern: 3 efficiency items, 3 to Displays the voltage/current waveforms *Displays the wordern and noise meas measurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording speed / Recording speed / Recording length 1,000 points 5,000 points 5,000 points /	thronization signer of 50 ms) ak hold data nd the interval and the interval and the voltage/curvector diagram, so the ment line pattern of tage. Measurement screen ar 32 measurement screen ar 32 measurement and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 item and loss set in the sitems, or 32 items, or 3	when the interval is all is detected (Data is all is detected (Data is auto-save outputs data arent vector diagram as connection can be checked. Annels 1 to 4 combined connections nent screen, Current at items from all basic as (4 pattern switching) the calculation algorithm is in a compressed screen aulation) result when noise source all voltage/current channels and points 50,000 points and 100ms and 200ms				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmous *The values are displayed for each measure Basic Measurement screen, Power Measurement screen, Power Measurement screen, Power Measurement screen, Power Measurement items Bar Graph screen, List screen, Vector's Selects and displays any 4, 8, 16, of measurement items Displays the numerical values of efficiency pattern: 3 efficiency items, 3 to Displays the voltage/current waveforms s' Displays the vaveform and noise measurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording length 1,000 points 5,000 Recording speed / Recording length 1,000 points 5,000 SOOKS/S 2ms 1 250KS/S 4ms 22 100KS/S 10ms 5	thronization signer of 50 ms) ak hold data nd the interval and the voltage/curvector diagram, so the ment line pattern of tage. Measurement screen ar 32 measurement screen ar 32 measurement is sitems. Of 32 items and 100 set in the sitems of 32 items of the sitems of 32 items. Sampled at 500 kH. The surement (FFT calcosynchronization / 50,000 points x and Peak compression of the sitems of th	when the interval is all is detected (Data is all is detected (Data is auto-save outputs data arent vector diagram se connection can be checked. annels 1 to 4 combined connections nent screen, Current at items from all basic as (4 pattern switching) he calculation algorithm is in a compressed screen aulation) result when noise source all voltage/current channels on points 50,000 points 100ms				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmous *The values are displayed for each measure Basic Measurement screen, Power Measurement screen, Power Measurement screen, Power Measurement screen, Power Measurement items Bar Graph screen, List screen, Vector's Selects and displays any 4, 8, 16, of measurement items Displays the numerical values of efficiency pattern: 3 efficiency items, 3 to Displays the voltage/current waveforms so bisplays the voltage/current waveforms so bisplays the waveform and noise measurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording length 1,000 points 5,000 kS/s 2ms 1,000 kS/s 2ms 1,000 kS/s 20ms 1,000 kS	thronization signer of 50 ms) ak hold data and the interval and the voltage/curvector diagram, so the ment line pattern of tage. Measurement screen ar 32 measurement screen ar 32 measurement and loss set in the sitematic street. Signed the sitemati	when the interval is all is detected (Data is all is detected (Data is auto-save outputs data arent vector diagram as connection can be checked. Annels 1 to 4 combined connections nent screen, Current at items from all basic as (4 pattern switching) the calculation algorithm at a compressed screen ulation) result when noise source all voltage/current channels and points 50,000 points and 100ms area 200ms 500ms 500ms				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per CThe waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmous the values are displayed for each measure Basic Measurement screen, Power Measurement screen, Power Measurement screen, Power Measurement screen, Power Measurement items Bar Graph screen, List screen, Vector's Selects and displays any 4, 8, 16, of measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficiency pattern: 3 efficiency items, 3 to Displays the voltage/current waveforms is *Displays the waveform and noise measurement is performed Synchronization timing of harmonic 1,000 points /5,000 points /10,000 points /11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording length Recording length 1,000 points 5,000 points 5,000 points 5,000 points 5,000 points 1,000 points 5,000 points 1,000 points 5,000 points 5,000 points 1,000 points 5,000 points 5,000 points 1,000 points 5,000 points 1,000 points 5,000 points 1,000 points 5,000	thronization signer of 50 ms) ak hold data nd the interval signer of 50 ms) ak hold data and the interval signer of 50 ms) ak hold data nd the interval signer of 50 ms, ak hold data nd the interval signer of 50 ms, ak hold data nd the voltage/curvector diagram, so the ment line pattern of tage. Measuren ement screen creen ar 32 measurement ray a measurement and loss set in the signer of 50 ms, ampled at 500 kHz urement (FFT calconomic synchronization / 50,000 points x a Peak compression of 50,000 points x a Peak compression of 50,000 points x a 10,000 ms	when the interval is all is detected (Data is all is detected (Data is auto-save outputs data arent vector diagram e connection can be checked. annels 1 to 4 combined connections nent screen, Current at items from all basic as (4 pattern switching) the calculation algorithm is in a compressed screen all voltage/current channels are in a compressed screen all voltage/current channels are in a compressed screen all voltage/current channels are in a compressed screen are in a compressed screen are in a compressed screen all voltage/current channels are in a compressed screen all voltage are in a compressed scr				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per commendation of the per	chronization signer of 50 ms) ak hold data nd the interval signer of 50 ms) ak hold data and the interval signer of 50 ms) ak hold data nd the interval signer of 50 ms, ak hold data nd the interval signer of 50 ms, ak hold data nd the interval signer of 50 ms, ak hold data nd the vector of 60 ms ak hold data nd the v	when the interval is all is detected (Data is all is all is detected (Data is all is detected (Data is all is detected (Data is all is all is detected (Data is all is all is detected (Data is all is				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio Recording time	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmor at the values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Power Measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficie Display pattern: 3 efficiency items, 3 lo Displays the voltage/current waveforms * *Displays the voltage/current waveforms * *Displays the waveform and noise meas measurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording speed / Recording speed / Recording speed / Recording length	chronization signer of 50 ms) ak hold data nd the interval signer of 50 ms) ak hold data nd the interval signer of 50 ms) ak hold data nd the interval signer of 50 ms ak hold data nd the interval signer of 50 ms ak hold data nd the interval signer of 50 ms ak hold data nd the vector diagram, so the original signer of 50 ms ak hold data nd the vector of	when the interval is all is detected (Data is all is all is detected (Data is all is a				
Output data 2. Display Connection check screen Connection display screen DMM screen Harmonic screen Select/Display screen Efficiency/Loss screen Waveform & Noise Measurement screen Trigger Record Length Compression Ratio Recording time	Data is cleared when the hold key reached, and when an external sync updated at an internal data update rat D/A output, CF data save: Outputs the per (The waveform output continues, a immediately before it is cleared) Displays the connection diagram and *The right connection range is displayed in the Displays measured power and harmore. The values are displayed for each measure Basic Measurement screen, Vol Measurement screen, Power Measurement screen, Power Measurement items Display pattern: 4 items, 8 items, 16 Displays the numerical values of efficie Display pattern: 3 efficiency items, 3 lo Displays the voltage/current waveforms *Displays the voltage/current waveforms *Displays the waveform and noise meas measurement is performed Synchronization timing of harmonic 1,000 points / 5,000 points / 10,000 points / 11, 1/2, 1/5, 1/10, 1/25, 1/50 (Peak-Recording speed / Recording length 1,000 points 5,000 Recording length 5,000 Recording len	chronization signer of 50 ms) ak hold data and the interval at the voltage/curry vector diagram, so the office of the voltage on chement line pattern of tage. Measurement screen creen ar 32 measurement and loss set in the signer of the voltage of the vector of the vec	when the interval is all is detected (Data is all is all is detected (Data is all is a				

Motor screen	Displays the measured values of the MOTOR TESTING OPTION 9791 (9793) Display pattern: Displays the numerical values of 4 items				
3. Data save					
Auto data save	Saves each measured value to the CF card at each interval				
Save destination	OFF / CF card (cannot be saved to the USB memory), the save destination folder can be specified				
Save itemAuto	and peak value of the noise measurement function				
	CSV file format				
	Saves each measured value to each save destination when the SAVE key is pressed				
	USB memory / CF card, the save destination folder can be specified				
Save itemsave	Any item can be selected from all measured data, including harmonic value and peak value of the noise measurement function				
Data format	•				
Screen hard copy	Saves the display screen to the save destination when the COPY key is pressed				
Save destination	USB memory / CF card * The save destination folder can be specified when USB memory or CF card is specifie				
Data format	Compressed BMP format (256 colors)				
Setting data save	Setting information can be saved and loaded to and from the sav				
ŭ	destination as a setting file				
	(With the exception of language setting and communication setting)				
	USB memory / CF card (the save destination folder can be specified)				
	ected equipment				
Synchronized	The 3390 master and 3390 slaves can be connected with synchronization				
measurement	cables to perform synchronized measurements * If the interval setting is identical, synchronized measurements can be saved automatically				
Synchronized item	·				
	data reset, event Hold, manual save, screen copy				
Synchronization timing	Clock, data update rate, start/stop, data reset, event (During operation of the				
Synchronization unling	master by the key or via communication)				
Synchronization delay	Up to 5 μs per connection, up to +50 ms per event				
5. System					
Display language	English / Japanese / Chinese				
Clock function	Auto Calendar, Auto Leap Year Adjustment, 24 Hour Meter				
Clock setting	Year, Month, Day, Hour, Minute Setting, Zero Second Adjustment				
Real time accuracy	Within ±3 s / day (25°C)				
Beep tone	OFF / ON				
Screen color	COLOR1 / COLOR2 / COLOR3 / COLOR4 / MONO				
Start screen select	Connection screen / screen closed in the previous session (Measurement screen only				
LCD backlight	ON / 1min / 5min / 10min / 30min / 60min				
Sensor recognition	Automatically recognizes the current sensor connected				
Alarm display	Voltage/current peak over threshold detection, synchronization source nor				
	detection (Alarm mark on)				
Key lock	detection (Alarm mark on) ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on)				
Key lock System reset	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on)				
Key lock System reset	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting				
	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil				
System reset	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed)				
System reset File manipulation	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fit deletion, file copy between media				
System reset File manipulation General spe	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fit deletion, file copy between media cifications				
System reset File manipulation General spe Operating location	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fit deletion, file copy between media cifications				
System reset File manipulation General spe Operating location Storage temperature and humidity ranges	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation)				
System reset File manipulation	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) 0°C to 40°C, 80%RH or less (No dew condensation)				
System reset File manipulation General spe Operating location Storage temperature and humidity ranges Operating temperature	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fi deletion, file copy between media cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) 0°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fideletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fi deletion, file copy between media cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fit deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH B				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH ECH Z) and the unit case				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fi deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input reminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH I) CH Z) and the unit case Between CH A and CH B / CH Z				
System reset File manipulation General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges Withstand voltage	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH E CH Z) and the unit case Between CH A and CH B / CH Z Safety: EN61010				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges Withstand voltage Applicable standard Rated power	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input reminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH E) CH Z) and the unit case Between CH A and CH B / CH Z				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges Withstand voltage Applicable standard Rated power supply voltage	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH E CH Z) and the unit case Between CH A and CH B / CH Z Safety: EN61010 EMC: EN61326, EN61000-3-2, EN61000-3-3 100 to 240 VAC (expected transient overvoltage of 2500 V), 50/60 Hz				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges Withstand voltage Applicable standard Rated power	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH ECH Z) and the unit case Between CH A and CH B / CH Z Safety: EN61010 EMC: EN61326, EN61000-3-2, EN61000-3-3 100 to 240 VAC (expected transient overvoltage of 2500 V), 50/60 Hz				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges Withstand voltage Applicable standard Rated power supply voltage Maximum rated power	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fit deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH I CH Z) and the unit case Between CH A and CH B / CH Z Safety: EN61010 EMC: EN61326, EN61000-3-2, EN61000-3-3 100 to 240 VAC (expected transient overvoltage of 2500 V), 50/60 Hz 140VA 340 W × 170 H × 157 D mm (13.39" W × 6.69" H × 6.18" D)				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges Withstand voltage Applicable standard Rated power supply voltage Maximum rated power	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fit deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH I) CH Z) and the unit case Between CH A and CH B / CH Z Safety: EN61010 EMC: EN61326, EN61000-3-2, EN61000-3-3 100 to 240 VAC (expected transient overvoltage of 2500 V), 50/60 Hz				
General spe Operating location Storage temperature and humidity ranges Operating temperature and humidity ranges Withstand voltage Applicable standard Rated power supply voltage Maximum rated power Dimensions	ESC key: ON/OFF by holding down the key for 3 seconds (Key lock mark on) Sets the equipment to the default (factory) settings (Communication setting are not changed) Media data list display, media formatting, new folder creation, folder fil deletion, file copy between media Cifications Indoors, altitude up to 2000 m, contamination class 2 -10°C to 50°C, 80%RH or less (No dew condensation) O°C to 40°C, 80%RH or less (No dew condensation) For 1 minutes at 50/60 Hz AC5.312 kVrms: Between the voltage input terminal and the unit case AC3.32 kVrms: Between the voltage input terminal and the current input terminal / interface AC370 Vrms: Between the 9791 and 9793 input terminals (CH A, CH E CH Z) and the unit case Between CH A and CH B / CH Z Safety: EN61010 EMC: EN61326, EN61000-3-2, EN61000-3-3 100 to 240 VAC (expected transient overvoltage of 2500 V), 50/60 Hz 140VA 340 W × 170 H × 157 D mm (13.39" W × 6.69" H × 6.18" D) (excluding protrusions)				

Connection	1P2W	1P3W	3P3W2M	3P3W3M	3P4W				
Voltage and current	Xrms(i) =	Xrms12 or Xrms34 = Xrms123 =							
RMS value (True RMS value)	$\sqrt{\frac{1}{M}} \sum_{s=0}^{M-1} (X_{(i)s})^2$	$\frac{1}{2} \left(Xrms_{(i)} + Xrms_{(i+1)} \right) \qquad \frac{1}{3} \left(Xrms_1 + Xrms_2 + Xrms_3 \right)$				$\frac{1}{2} \left(Xrms_{(i)} + Xrms_{(i+1)} \right)$		$\frac{1}{1} \sum_{s=0}^{M-1} (X_{(i)s})^{2} = \frac{1}{2} (Xrms_{(i)} + Xrms_{(i+1)}) = \frac{1}{3} (Xrms_{1} + Xrms_{2} + Xrms_{3})$	
Voltage and current	Xmn(i)=	Xmn12 or Xmn34 = Xmn123 =				Xmn12 or Xmn34 =			
average rectified RMS indication value	$\left[\frac{p}{2\sqrt{2}} \frac{1}{M} \sum_{s=0}^{M-1} X_{(i)s} \right]$	$\frac{1}{2} \left(Xmn_{(i)} - \frac{1}{2} \right)$	$\frac{1}{2} \left(Xmn_{(i)} + Xmn_{(i+1)} \right) \qquad \frac{1}{3} \left(Xmn_1 + Xmn_2 + Xmn_3 \right)$						
Voltage and current alternating-current component		Xac(i) =	$\sqrt{\left(Xrms_{(i)}\right)^2}$ –	$(Xdc_{(i)})^2$					
Voltage and current mean value		$Xdc(i) = \frac{1}{1}$	$\frac{1}{M} \sum_{s=0}^{M-1} X_{(i)s}$						
Voltage and current fundamental wave component	Fundamenta	al wave value X	1(i) based on the	e harmonic calcu	lation result				
Voltage and current peak value	t Maximum value among X pk+(i) = X (i)s M Minimum value among X pk-(i) = X (i)s M								
Active power	$P(i) = \frac{1}{M} \sum_{s=0}^{M-1} (U_{(i)s} \times I_{(i)s})$	P12 = P34 =	P1+P2 P3+P4	P123 =P	1+P2+P3				
	• In the cases of 3P3W3M and 3P4W connections, phase voltage is used for the voltage waveform U (i)s. (3P3W3M-U1s = (U1s-U3s)3, U2s = (U2s-U1s)3, U3s = (U3s-U2s)2)) The polarity symbols of active power Pindicate the power direction when power is consumed (+P) and when power is regenerated (-P).								
Apparent power	S(i) = U(i)5I(i)	S12=S1+S2 S34=S3+S4	$S_{12} = \frac{\sqrt{3}}{2} (S_1 + S_2)$ $S_{34} = \frac{\sqrt{3}}{2} (S_3 + S_4)$	S123 =S	1+S2+S3				
	Selects rms or mn for U(i) and I(i) In the cases of 3P3W3M and 3P4W connections, phase voltage is used for the voltage U (i)								
	Q(i) =		Q1+Q2	O123 =O	1+O2+O3				
Reactive power	$\sin(\sqrt{3}) \sqrt{S_{(i)}^2 - P_{(i)}^2}$ Q34 =Q3+Q2								
neactive power	POWET - The polarity symbol si of reactive power Q indicates symbol [none]: lag and symbol [-]: lead The polarity symbol si(i) is determined by lag or lead of voltage waveform U (i)s and current waveform I (i)s for measurement channel (i), and in the cases of 3P3W3M and 3P4W connections, phase voltage is used for the vol waveform U (i)s.								
Power factor	$\lambda(i) = \frac{si_{(i)} \frac{P_{(i)}}{S_{(i)}}}$		$I_{34} = si_{34} \frac{P_{34}}{S_{34}}$	I ₁₂₃ = si	$\frac{P_{123}}{S_{123}}$				
i onto idoloi	13(1) 13(2) 13(2) 13(2) 13(2) 14(2) 15(2) 15(2) 16(2								

Connection Item	1P2W	1P3W	3P3W2M	3P3W3M	3P4W	
Phase angle	$ \begin{aligned} \phi(i) &= \\ \sin(\cos^{-1} I_{(i)} \end{aligned} $					
	The polarity symbol si(i) is determined by lead or lag of voltage waveform U (i)s and current waveform I (i)s for each measurement channel. si12, si24, and si123 are determined by the symbol of Q12, Q34, and Q123, respectively.					
(i): Measurement channel, M: Number of samples between synchronization timings, s: Sample point number						

Moto	analysis calcul	ation algor	ithm			
Item	Setting unit		Calculation algorithm			
	V (DV voltage)	$\frac{1}{M}\sum_{s=0}^{M-1}A_s$				
chA	N• m / mN• m / kN• m	When analog DC	A [V] × chA scaling setpoint			
	common (torque)	When frequency (Measurement frequency - fc setpoint) torque setpoint / fd setpoint				
	M: Number of samp	les between sync	hronization timings, s: Sample point number			
	V (DC voltage)	$\frac{1}{M}\sum_{s=0}^{M-1}B_s$				
	Hz (frequency)	When analog DC	B[V] × chB scaling setpoint			
chB		When pulse input	Pole number setpoint x pulse frequency / 2 × pulse number setpoint			
	r/min (rotation)	When analog DC	B[V] × chB scaling setpoint			
		When pulse input	$2 \times 60 \times$ frequency [Hz] / pole number setpoint			
	N• m (unit of chA)	(Indicated value	e of chA)×2× π × (indicated value of chB) / 60			
	mN• m (unit of chA)	(Indicated value of chA) $\times 2 \times \pi \times$ (indicated value of chB) / 60 / 1000				
Pm	kN• m (unit of chA) (Indicated value of chA) $\times 2 \times \pi \times (\text{indicated value of chB}) \times 1000 / 60$					
	Calculation cannot be performed when the unit of chA is other than the above, or the unit of chB is other than r/min.					
	Hz (unit of chB)	100 × input frequ	uency - indicated value of chB / input frequency			
Slip	r/min (unit of chB)	$100 \times 2 \times 60 \times$ input frequency – indicated value of chB × pole number setpoint / $2 \times \pi \times$ input frequency				
	Selects the input frequency from f1 to f4					

■ Current sensors specifications

Model	9272-10	CT6841	CT6843	9279-01
Rated current	AC 20A/200A	AC/DC 20A	AC/DC 200A	AC/DC 500A
Maximum continuous input range	50A/300A rms	40A rms	400A rms	650A rms
Accuracy (45 to 66 Hz, DC: DC compatible sensor)	±0.3%rdg.±0.01%f.s., ±0.2°	±0.3%rdg.±0.01%f.s. , ±0.1°		$\pm 0.5\% rdg. \pm 0.05\% f.s.$, $\pm 0.2^{\circ}$ (30 minutes after power is turned on and after magnetization)
Frequency characteristic	1Hz to 5Hz: ±2%rdg.±0.1%f.s. 1kHz to 5kHz: ±1%rdg.±0.05%f.s. 10kHz to 50kHz: ±5%rdg.±0.1%f.s.	DC to 500Hz: ±0.3%max. 500Hz To 10kHz: ±1.5%max. 10kHz to 100kHz: ±5.0%max.	DC to 500Hz: ±0.3%max. 500 to 10kHz: ±1.5%max. 10kHz to 50kHz: ±5.0%max.	DC to 1kHz: ±1.0% (±0.5°) 1 k to 10 kHz: ±2.5 % (±2.5°) 10 k to 20 kHz: ±5.0 % (±5.0°)
Effect of Notel conductor position	±0.2%rdg. or less (at 100A/55Hz input, using with the wire 10mm diameter)	Within ±0.1%rdg. (deviation from center)		±1.5%rdg. or less (DC,55Hz)
Effect of external electromagnetic field	100mA or less (in an AC electromagnetic field of 400 A/m, 60Hz)	50mA equivalent or less (400A/m, 60Hz)		Max. 2A (400 A/m, 55Hz and DC)
Operating temperature and	0°C to 50°C (-32°F to 122°F)	-40°C to 85°C (-40°F to 185°F)		0°C to 40°C (-32°F to 104°F)
humidity	80%RH or less (No condensation)	80%RH or less (No condensation)		80%RH or less (No condensation)
Measurable conductor diameter	φ 46mm (1.81")	φ 20mm (0.79")		φ 40mm (1.57")
Dimensions, mass	78W×188H×35Dmm(3.07"W×7.40"H×1.38"D), 430g(15.2 oz.)	153W(6.02")×67H(2.64")×25.5D(0.98")mm, 370g(12.3 oz.)		220W×103H×43.5Dmm(8.66"W×4.06"H×1.71"D), 470g(16.6 oz.)

Model	CT6862	CT6863	9709	CT6865
Rated current	AC/DC 50A	AC/DC 200A	AC/DC 500A	AC/DC 1000A
Maximum continuous input range	100A rms	400Arms	700A rms	1200A rms
Accuracy (45 to 66 Hz, DC: DC compatible sensor)	$\pm 0.05~\% rdg. \pm 0.01~\%~f.s.~, \pm 0.2^{\circ}$ (Right after power is turned on at DC and 16Hz to 400Hz)		± 0.05 %rdg. ± 0.01 % f.s. , $\pm 0.2^\circ$ (10 minutes after power is turned on)	±0.05 %rdg.±0.01 % f.s. , ±0.2°
Frequency characteristic	DC to 16 Hz: ±0.1%rdg.±0.02%f.s.(±0.3°) 5kHz to 10kHz: ±1%rdg.±0.02%f.s. (±1.0°)		DC to 45Hz: ±0.2%rdg.±0.02%f.s.(±0.3°) 5kHz to 10kHz: ±2%rdg.±0.1%f.s. (±2.0°)	DC to 16Hz: ±0.1%rdg.±0.02%f.s.(±0.3°) 500Hz to 10kHz: ±5%rdg.±0.05%f.s.
	$500kHz$ to 1M Hz: $\pm 30\% rdg. \pm 0.05\% f.s.$ Note2	300kHz to 500k Hz: ±30%rdg.±0.05%f.s. Note2	20kHz to 100kHz: ±30%rdg.±0.1%f.s. (±30°)	10kHz to 20kHz: ±30%rdg.±0.1%f.s.
Effect to conductor position	±0.01%rdg. or less (50A input, DC to	±0.01%rdg. or less (100A input, DC to	±0.05%rdg. or less (at 100ADC input,	$\pm 0.05\%$ rdg. or less (1000A input, 50/60Hz,
	100Hz, using with the wire 5mm diameter)	100Hz, using with the wire 10mm diameter)	using with the wire 10mm diameter)	using with the wire 20mm diameter)
Effect of external electromagnetic field	10mA or less	50mA or less	50mA or less	200mA or less
	Scaled value, in a DC or 60Hz magnetic field of 400 A/m			
Operating temperature and	CT6862/CT6863/CT6865: -30°C to 85°C (-22°F to 185°F), 9709: 0°C to 50°C (-32°F to 122°F)			
humidity	80%RH or less (No condensation)			
Measurable conductor diameter	φ 24mm (0.94")	φ 24mm (0.94")	φ 36mm (1.42")	φ 36mm(1.42")
Dimensions, mass	70W×100H×53Dmm (2.76"W×3.94"H×2.09"D), CT6862: 340g(12.0 oz.), CT6863: 350g(12.3oz.)		160W×112H×50Dmm (6.30"W×4.41"H×1.97"D), 9709: 850g(30.0oz.) CT9895: 1000g(35.3oz)	
VIIII I I I I VAVI				

Note1 : Includes derating characteristics Note2: No phase precision regulations

POWER ANALYZER




Order Code: 3390

Accessories: Instruction Manual × 1, Measurement Guide × 1, Power cord × 1, USB cable × 1, D-sub connector × 1 (when 9792 or 9793 is installed), Color label × 2

Ordering Information

Please purchase separately-sold voltage cord and current sensor for measurements A HIOKI-issued PC card is also necessary in order to save measured data. Factory options cannot be installed after delivery.



MOTOR TESTING & D/A OUTPUT OPTION

9793



Options for voltage measurements CAT III 1000V CAT IV 600V CAT IV 600V Voltage Cord L9438-50 Voltage Cord L1000 **Length**: 3m (9.84ft); Red x 1, yellow x 1, **Length**: 3m (9.84ft); Red x 1, black x 1 blue x 1, gray x 1, and black x 4 Indoor wiring in buildings and factories for measurements up to 1000 V; can also be used for internal voltage measurements of equipment up to 1000 V.



Grabber Clip 9243

Usage:

Attaches to the end of the Voltage Cord L1000 or L9438-50.




WIRING ADAPTER PW9000 For 3P3W WIRING





WIRING ADAPTER PW9001 For 3P4W WIRING

Usage:

Reduce voltage cords for easy wiring.







example When used with Model L1000

Note:

Dedicated PC application software and communication command manual are available for the 3390. Please download them from the HIOKI website.

Rack mounts available on special order. Please contact your local HIOKI office

When using the 3390 with a DC power supply as in the case of on-vehicle measurements, a separate DC-AC converter is required.

Required DC-AC converter output specification Sinusoid wave type, 50/60 Hz (60 Hz recommended) Output capacity: The maximum power consumption of the 3390 is 140VA. Select a rating more than the capacity.

Options for current measurements AC/DC CURRENT SENSOR CAT III 1000V CAT III 1000V CAT III 1000V CAT III 1000V CT6862 (AC/DC 50A) 9709 (AC/DC 500A) CT6865 (AC/DC 1000A) (AC/DC 200A) ■ CLAMP ON SENSOR ■ AC/DC CURRENT PROBE UNIVERSAL CLAMP ON CT CAT III 600V CE-marked 600 V insulated conductor



9272-10 (AC20/200A)



PC Card Precaution Use only PC Cards sold by HIOKI. Compatibility and performance are not guaranteed for PC cards made by other manufacturers. You may be unable to read from or save data to such cards.

CT6841 (AC/DC 20A)

PC Card 512M 9728 (Capacity: 512 MB) 9729 (Capacity: 1 GB) PC Card 1G PC Card 2G 9830 (Capacity: 2 GB)



CT6843 (AC/DC 200A)

CARRYING CASE 9794 Hard case dedicated to the 3390

448 W × 618 H ×295 D mm (17.64" W × 24.33" H × 11.61" D) (excluding protrusions)

9279-01

(AC/DC 500A)



CONNECTION CORD L9217 **Length**: 1.6 m (5.25 ft) length **Usage**: For input of the 9791 and




Usage: For synchronized



Length: 5 m (16.41 ft) supplied with straight to cross conversion cable

Combination example





POWER ANALYZER 3390 × 1



CODE









2. Inverter input and output evaluation and measurements (Three-phase there-wire (3P3W2M) two-circuit)







DISTRIBUTED BY







SENSOF L1000 × 1 9709 × 4 3. Motor evaluation and measurements

(DC input / three-phase motor evaluation (DC, 3P3W3M measurements))







 9709×4





PC CARD 1G (1GB) 9729 × 1

MOTOR TESTING & D/A OUTPUT OPTION 9793×1

Note: Company names and Product names appearing in this catalog are trademarks or registered trademarks of various companies

HIOKI E.E. CORPORATION

HEADQUARTERS

81 Koizumi, Ueda, Nagano, 386-1192, Japan TEL +81-268-28-0562 FAX +81-268-28-0568 http://www.hioki.com/ E-mail: os-com@hioki.co.jp

HIOKI USA CORPORATION TEL +1-609-409-9109 FAX +1-609-409-9108 http://www.hiokiusa.com / E-mail: hioki@hiokiusa.com

HIOKI (Shanghai) SALES & TRADING CO., LTD. TEL +86-21-63910090 FAX +86-21-63910360 http://www.hioki.cn / E-mail: info@hioki.com.cn

HIOKI INDIA PRIVATE LIMITED TEL +91-124-6590210 E-mail: hioki@hioki.in

HIOKI SINGAPORE PTE. LTD. TEL +65-6634-7677 FAX +65-6634-7477 E-mail: info-sg@hioki.com.sg

HIOKI KOREA CO., LTD.

TEL +82-2-2183-8847 FAX +82-2-2183-3360 E-mail: info-kr@hioki.co.jp