MR6000 MR6000-01



Instruction Manual

MEMORY HICORDER



Read carefully before use. Keep for future reference.

check for the latest edition and other language versions.





Nov. 2024 Revised edition 8 MR6000A966-08

Contents

3

Introduction	1
Notations	1
How to Use This Document	2

1 **Measurement Method**

1.1	Measurement Procedure	
1.2	Setting Measurement Conditions Sampling rate setting guideline	5 7
	Using the envelope	
1.3	Configuring the Input Channel	
	Settings	
	Analog channels	
1.4	Logic channels	
1.4	Configuring the Sheet Settings Switching sheets on the waveform	19
	screen	24
	Generating XY composite waveforms	
1.5	Starting/Stopping a Measurement	28
2	Operating the	
4	•	
	Waveform Screen and	
	Analyzing Data	29
2.1	Reading Measured Values	
	(Trace Cursors, Horizontal	
	Cursors)	30
2.2	Specifying the Waveform Range	
	(Section Cursor)	35
	Changing the display magnification of the waveforms while moving the section	
	cursor	36
2.3	Displaying Vertical Scales	
	(Gauge Function)	37
2.4	Scrolling Through Waveforms	
	Scrolling through waveforms	39
	Checking a position of waveforms with	40
2.5	the scroll bar Changing the Display Position	40
2.5	and Display Magnification of	
	Waveforms	41
	Differentiating a waveform display	
	position and display magnification from	
	those of other analog channels	
2.6	Operating the Rotary Knobs	45

	operating the Hotary Hitebe	
2.7	Enlarging a Part of the Waveform	
	(Zoom Function)	46
2.8	Generating XY Composite	
	Waveforms (XY Composite)	47
2.9	Displaying Measured Values	
2.10	Viewing Block Waveforms	51
	•	

3 Advanced Functions

3	Advanced Functions	53
3.1	Overlaying New Waveforms With	- 4
3.2	Previously Acquired Waveforms Converting Input Values	54
	(Scaling Function)	56
	When using Model U8969 Strain Unit	61
3.3	Adjusting the Waveform Display	~~~
3.4	Positions (Variable Function) Fine-Adjusting Input Values	62
5.4	(Vernier Function)	64
3.5	Inverting a Waveform	0+
0.0	(Invert Function)	65
3.6	Copying Settings (Copy Function)	
3.7	Configuring Measurement Module-	
	Specific Settings	67
	Configuring Model 8968 High Resolution	
	Unit settings	67
	Configuring Model 8967 Temp Unit	60
	settings Configuring Model U8969 Strain Unit	00
	settings	70
	Configuring Model 8970 Freq Unit	
	settings	72
	Configuring Model 8971 Current Unit	
	settings	75
	Configuring Model 8972 DC/RMS Unit settings	77
	Configuring Model MR8990 Digital	
	Voltmeter Unit settings	78
	Configuring Model U8974 High Voltage	
	Unit settings	80
	Configuring Model U8977 3CH Current	~ (
	Unit Settings	81
	Configure Model U8979 Charge Unit Settings	83
3.8	Configuring Generator Module-	00
0.0	Specific Settings	86
	Generating signals from Model MR8790	
	Waveform Generator Unit	86
	Configuring Model MR8790 Waveform	
	Generator Unit settings	88
	Generating signals from Model MR8791	00
	Pulse Generator Unit Configuring Model MR8791 Pulse	90
	Generator Unit settings	92
	Generating signals from Model U8793	
	Arbitrary Waveform Generator Unit	97
	Configuring Model U8793 Arbitrary	
	Waveform Generator Unit	99
	Registering arbitrary waveforms in the	
	U8793 Arbitrary Waveform Generator	100
	Unit	. 102

3

1

2

Editing arbitrary waveforms for Model	
U8793 Arbitrary Waveform Generator	
Unit	106
Editing programs of Model U8793	
Arbitrary Waveform Generator Unit	107
Installing Model SF8000 Wave Marker	
software	110

4 Saving/Loading Data and Managing Files 115

Data That Can Be Saved and	
Loaded	116
Saving Data	118
Saving types and setting procedure	118
Structure of the save destination	
folders	119
Automatically saving waveform data	120
Real-time saving	124
Freely choosing data items to be saved	1
and save files (SAVE key)	127
Loading Data	131
Data loading procedure	131
Loading waveform data in a batch	134
Automatically loading the settings	
(Automatic setup function)	135
Loading numerical calculation settings.	135
Managing Files	136
	Loaded Saving Data Saving types and setting procedure Structure of the save destination folders Automatically saving waveform data Real-time saving Freely choosing data items to be saved and save files (SAVE key) Loading Data Data loading procedure Loading waveform data in a batch

5 Configuring the Trigger Settings 137

5.1 5.2 5.3	Trigger Setting Procedure
	Setting140
5.4	Configuring the Pre-trigger and
	Post-trigger Settings142
	To observe an input waveform while the
	instrument is waiting for a trigger
5.5	Setting the Trigger Satisfaction
	Conditions (AND/OR Operation)
	Among Trigger Sources147
5.6	Triggering the Instrument Using
	Analog Signals (Analog Trigger)149
5.7	Triggering the Instrument Using
	Logic Signals (Logic Trigger)158
5.8	Triggering the Instrument at
	Regular Intervals
	(Interval Trigger)160
5.9	Externally Triggering the
	Instrument (External Trigger)162

5.10	Manually Triggering the Instrument	
	(Forcible Trigger)	162

5.11 Triggering the Instrument Using CAN Signals (CAN Trigger)163

6 Search Function 167

6.1	Searching For Peak Values	168
6.2	Searching For Positions Where a	
	Trigger Condition Is Satisfied	171
6.3	Searching For Differences from	
	a Fundamental Wave	
	(Memory HiConcierge)	176
6.4	Jumping to the Specified	
	Position	179

7 Numerical Calculation Function 181

7.1	Numerical Calculation Procedure	182
7.2	Configuring the Numerical	
	Calculation Settings	184
	Displaying numerical calculation	
	results	195
7.3	Evaluating Calculation Results on	
	a Pass/Fail Basis	197
	Displaying evaluation results and	
	externally outputting signals	200
7.4	Numerical Calculation Types and	
	Descriptions	201

8 Waveform Calculation Function 209

8.1 8.2	Waveform Calculation Procedure . Configuring the Waveform	211
	Calculation Settings	213
8.3	Defining Constants	220
8.4	Operators of the Waveform	
	Calculation and Calculation	
	Results	222
8.5	Examples of Configuring	
	Waveform Calculation Settings	230
	Obtaining an RMS waveform from an	
	instantaneous waveform	230
	FIR filter	233
	IIR filter	237
8.6	Explanations of Filter Calculation	242
	Filter type	
	Filter configuration	243
8.7	Setting Power Calculation	
	Conditions	244

	Detailed power calculation settings	244
	Wiring method settings	245
	Configuring zero-cross settings	247
	Low-pass filter settings	249
	Forced average time setting	250
	Δ-Y conversion setting	251
8.8	Types of Power Calculations and	
	Explanations	252
	U (voltage) and I (current)	253
	P (power)	254
	Others (efficiency, loss)	255

257

289

9 FFT Calculation Function

9.1 9.2	Operating Procedure Enabling the FFT Calculation	258
0.2	Settings	260
9.3	Setting FFT Calculation	
	Conditions	262
	Specifying the number of calculation	
	points	262
	Configuring the window function	
	settings	265
	Configuring the calculation result peak	267
	value settings	
	Averaging calculation results	
	FFT calculation advanced settings	272
9.4	Performing Calculations on the	
	Waveform Screen	276
	To specify a range before calculation	276
9.5	FFT Calculation Types	279
	Calculation types and display	
	examples	279
	Calculation types and internal	
	calculation formulas	288

10 Memory Division Function

10.1	1 Configuring the Memory Division		
	Settings	290	
10.2	Configuring the Display Settings	291	

11 Dual Sampling 295

11.1	Dual Sampling Procedure	296
11.2	Configuring Dual Sampling	
	Settings	297
11.3	Operating the Waveform Screen	
	for Analyzing Waveforms	301
11.4	Calculation Function	306
11.5	Files	308

12 CAN/LIN Measurement Function

	Function	311
12.1	CAN/LIN Measurement	
40.0	Procedure	
	Connecting CAN/LIN Interfaces Configuring the CAN/LIN Interface	
12.5	Settings	
12.4	Configuring the CAN/LIN Definition	
	Data Settings	325
40 5	Choosing CAN definition data	331
12.5	Configuring the Transmission Function Settings (Creating a	
	Transmission List)	333
12.6	Choosing Data Sets to Be	
	Displayed as Waveforms (When	
	Displaying Waveforms During	
107	Measurement) Choosing Data To Be Displayed	338
12.1	as Waveforms (When Using the	
	Waveform Calculation Function)	339
12.8	Saving Data	
12		
13	Configuring the System	
13	Configuring the System Environment Settings	343
13	Configuring the System Environment Settings	
	Environment Settings	
	Environment Settings Connecting the	
	Environment Settings Connecting the Instrument to	343
	Environment Settings Connecting the	
14	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and	343
14	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the	343 349
14	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network	343 349
14	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the	343 349 351
14 14.1	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network	343 349 351
14 14.1	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the instrument Managing Data in the Instrument With the FTP Server Function	343 349 351 351
14 14.1	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the instrument Managing Data in the Instrument With the FTP Server Function Configuring the FTP sever setting with	343 349 351 351 356
14 14.1	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the instrument Managing Data in the Instrument With the FTP Server Function Configuring the FTP sever setting with the instrument	343 349 351 351 356
14 14.1 14.2	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the instrument. Managing Data in the Instrument With the FTP Server Function Configuring the FTP sever setting with the instrument Operating the instrument with your computer (FTP server function)	343 349 351 351 356 357
14 14.1 14.2	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the instrument Managing Data in the Instrument With the FTP Server Function Configuring the FTP sever setting with the instrument Operating the instrument with your computer (FTP server function) Sending Data to a Computer With	343 349 351 351 356 357 358
14 14.1 14.2	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the instrument Managing Data in the Instrument With the FTP Server Function Configuring the FTP sever setting with the instrument Operating the instrument with your computer (FTP server function) Sending Data to a Computer With the FTP Client Function	343 349 351 351 356 357 358
14 14.1 14.2	Environment Settings Connecting the Instrument to Computers Configuring the LAN Settings and Connecting the Instrument to the Network Configuring the LAN settings with the instrument Managing Data in the Instrument With the FTP Server Function Configuring the FTP sever setting with the instrument Operating the instrument with your computer (FTP server function) Sending Data to a Computer With	343 349 351 351 356 357 358 359



13







8

9

10

Index

14.4	Configuring the FTP client setting with the instrument	
	instrument with a web browser	8
	Remotely operating the instrument	9
	Starting/Stopping measurement	
	Configuring the comment setting	
	Acquiring data from the instrument	
	Setting the clock	
	Handling files	
14.5	Sending Email messages	4
	Configuring the basic setting for sending	_
	email messages	5
	Configuring the email contents	~
	settings	О
	Configuring the authentication,	
	compression, and encryption settings	-
110	for email messages to be sent	1
14.0	Controlling the Instrument With	
	Command Communications	_
	(LAN)	
14.7	Connecting to a Network Drive	
	Host PC settings	
	MR6000 settings	3
_		

15 Externally Controlling the Instrument 385

15.1	External Input and Output	386
	External input (IN1), (IN2)	386
	External output (OUT1), (OUT2)	387
	Trigger output (TRIG.OUT)	389
	External trigger terminal (EXT.TRIG)	391
15.2	External Sampling (EXT.SMPL)	394

16 Appendix

395

16.1	Information for Reference Purposes	.395
	Waveform file size (values for reference	
	purposes) Maximum recordable time when the	.395
	real-time saving is enabled	
	(values for reference purposes)	.399
	Scaling method for strain gauges	.405
	Example of a waveform text file	.407
	File saving rates	
	(values for reference purposes)	.408
16.2	FFT Definitions	.409
16.3	Dual Sampling	.419
	Power Equations and Wiring	
	Specifications	.420

Power equation	420
Wiring specifications	421

Index 425

Introduction

Thank you for choosing the Hioki MR6000, MR6000-01 Memory HiCorder. Preserve this manual carefully and keep it handy to make full use of this instrument for a long time.

Model MR6000-01 Memory HiCorder is an upper model of Model MR6000, which is equipped with the following calculation functions:

- · Digital filter calculation
- Real-time waveform calculation

The latest edition of the instruction manual

The contents of this manual are subject to change, for example as a result of product improvements or changes to specifications.

The latest edition can be downloaded from Hioki's website.

https://www.hioki.com/global/support/download

Product registration

Register your product in order to receive important product information. <u>https://www.hioki.com/global/support/myhioki/registration/</u>



Туре	Contents	Printed	CD-stored file name
Operating Precautions	Information on the instrument for safe operation	~	_
Quick Start Manual	Basic instructions and specifications of the instrument	~	✓ MR6000A965-XX.pdf
Instruction Manual (this document)	Functions and instructions for the instrument	-	✓ MR6000A966-XX.pdf
MR6000-01 Dedicated Functions	Method to use functions including the calculation available with Model MR6000-01	_	✓ MR6000A968-XX.pdf
U8793, MR8790, MR8791 Instruction Manual	Functions, specifications, and instructions of Models U8793, MR8790, and MR8791	_	√ U8793A981-XX.pdf

Notations

*	Additional information is presented below.
	Indicates the initial setting values of the items. Initializing the instrument restores settings to each of these values.
(p.)	Indicates the location of reference information.
START (Bold-faced)	Names and keys on the screen are indicated in boldface.
[]	Menus, dialog boxes, buttons in a dialog box, and other names on the screen are indicated in blue brackets.
Windows	Unless otherwise specified, "Windows" represents Windows 7, Windows 8, and Windows 10.


Current sensor	Sensors measuring current are referred to as "current sensor."
S/s	The number of times per second the analog input signals are digitized by the instrument is expressed in terms of "samples per second (S/s)." Example: "20 MS/s" (20 megasamples per second) indicates that the signal is digitized 20 × 10 ⁶ times per second.

Accuracy

We define measurement tolerances in terms of f.s. (full scale), rdg. (reading), and setting values, with the following meanings:

f.s.	(maximum display value or scale length) The maximum displayable value or scale length.
rdg.	(displayed value) The value currently being measured and displayed on the measuring instrument.
Setting	(set value) Indicates the set value, such as voltage and current, that the instrument has been configured to output.

How to Use This Document

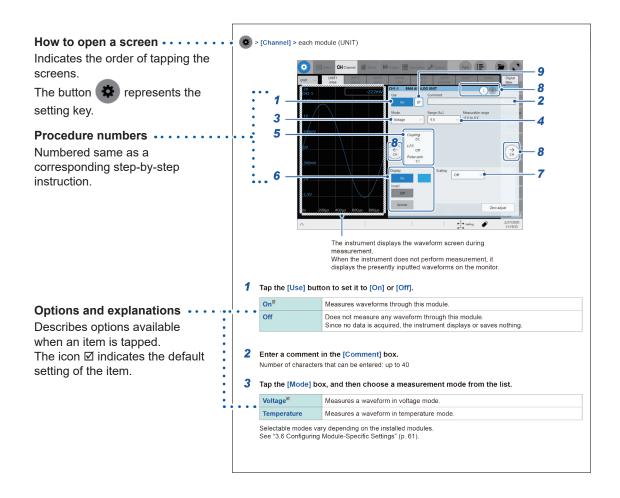

1

Measurement Method

1.1 Measurement Procedure

1

Inspecting the instrument before measurement

Configuring the basic settings for measurement

	Choose a sampling rate.	(p. 5)
	Choose a recording length.	(p. 6)
	Advanced settings "Using the envelope" "3.1 Overlaying New Waveforms With Previously Acquired Waveforms"	(p. 9) (p. 54)
Со	onfiguring the input channel settings	(p. 11)
	Configure the analog channel settings.	(p. 13)
	Specify the logic channel settings.	(p. 17)
	Advanced settings "3.2 Converting Input Values (Scaling Function)" "3.3 Adjusting the Waveform Display Positions (Variable Function)" "3.4 Fine-Adjusting Input Values (Vernier Function)" "3.5 Inverting a Waveform (Invert Function)"	(p. 56) (p. 62) (p. 64) (p. 65)
Со	onfiguring the sheet settings	
J	Choose a display format of waveforms.	(p. 19)
Co V	onfiguring the trigger settings	(p. 137)
	arting a measurement	(p. 28)
√ Fir	nishing the measurement	
	Advanced operation	
	"2.2 Specifying the Waveform Range (Section Cursor)" "Scrolling through waveforms"	(p. 35) (p. 39)

"7 Numerical Calculation Function"

(p. 181)

To configuring measurement settings automatically

Tapping **[Auto range]** on the waveform screen automatically specifies the sampling rate, measurement range, and zero position of the input waveform and start a measurement. See "3.7 Measuring Signals With the Auto-range Setting" in the Quick Start Manual.

To load settings registered previously

Load the settings file on the file screen. See "4.3 Loading Data" (p. 131).

To automatically load saved settings at the time of startup

Configure the setting for the instrument so as to load the file containing the instrument settings at the time of startup.

See "Automatically loading the settings (Automatic setup function)" (p. 135).

Initializing the instrument (Restoring the basic settings)


Select > [System] > [Initialize] to restore the instrument settings to the factory default.

The setting after the initialization is suitable for simple measurement. Initialize the instrument when you have found any unexpected or complicated operation. See "6.2 Initializing the Instrument" in the Quick Start Manual.

1.2 Setting Measurement Conditions

You have to set conditions required for measurement, such as the sampling rate ([Sampling]) and recording length ([Shot]).

> [Status] > [Condition]

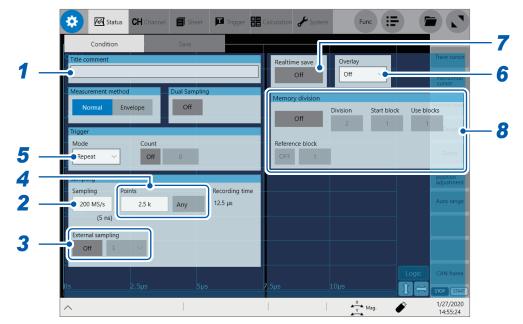

1 Enter a comment in the [Title comment] box.

Number of characters that can be entered: up to 40

2 Tap the [Sampling] box, and then choose a sampling rate from the list.

See "Sampling rate setting guideline" (p. 7).

200 MS/s^{II}, 100 MS/s, 50 MS/s, 20 MS/s, 10 MS/s, 5 MS/s, 2 MS/s, 1 MS/s, 500 kS/s, 200 kS/s, 100 kS/s, 50 kS/s, 20 kS/s, 10 kS/s, 5 kS/s, 2 kS/s, 1 kS/s, 500 S/s, 200 S/s, 100 S/s, 50 S/s, 20 S/s, 10 S/s, 5 S/s, 2 S/s, 1 S/s

The instrument can measure signals at a sampling rate of 200 MS/s even with several modules other than Model U8976 installed together. However, the data refresh rate does not exceed the maximum sampling rate of each module.

When the real-time waveform calculation (Model MR6000-01 only) is set to **[On]**, you cannot choose a sampling rate of 200 MS/s.

When the real-time saving is set to **[On]**, due to the combination of the number of channels to be used and save destinations, the maximum sampling rate that can be set varies as follows:

	Maximum sampling rate that can be chosen			
Number of channels to be used	SSD	HDD	USB flash drive SD Card FTP transmission	
1 channel to 2 channels	20 MS/s	10 MS/s	5 MS/s	
3 channel to 4 channels	10 MS/s	5 MS/s	2 MS/s	
5 channel to 8 channels	5 MS/s	2 MS/s	1 MS/s	
9 channel to 16 channels	2 MS/s	1 MS/s	500 kS/s	
17 channel to 32 channels	1 MS/s	500 kS/s	200 kS/s	

Only if the following Hioki-designated options are used, the real-time saving operation with the instrument is guaranteed:

- Model U8332 SSD Unit
 - Jnit Model U8333 HD Unit
- Model Z4006 USB Drive
 Model Z4001 and Model Z4003 SD Memory Card

3 Tap the [External sampling] button to set it to [On] or [Off].

The external sampling is cannot be set when the envelope is used.

Off	Disables the external sampling function.	
On	Choose this option to sample data at a sampling rate defined by a signal inputted into the external sampling terminal (EXT.SMPL).	

Ĺ	Samples data at rising edges of the input signal.
J¤	Samples data at falling edges of the input signal.
Ĵ&Ţ	Samples data at both rising and falling edges of the input signal.

4 Tap the [Points] box, and then from the list, choose an option for the number of points to be measured.

2.5 k[⊠], 5 k, 10 k, 20 k, 50 k, 100 k, 200 k, 500 k, 1 M, 2 M, 5 M, 10 M, 20 M, 50 M, 100 M, 200 M, 500 M, 1 G

Tap **[Any]** to enable it, and then tap **[Points]**, which allows you to enter the number of points in 100 increments.

When the real-time saving is set to **[On]**, you cannot specify the recording length in the **[Points]** box. Choose **[Save]**, and enter the recording length in the **[Recording time]** box. (p. 125)

The maximum recording length you can set varies depending on the number of channels to be measured.

5 Tap the [Mode] box, and then choose a recording mode from the list.

Single	Measures waveforms only once. Pressing the START key starts recording waveforms, and then stops when the specified recording length of the waveforms have been acquired.
Repeat [⊠]	Measures waveforms repeatedly. Pressing the STOP key stops the measurement in progress.

When you choose [Repeat] and set [Count] to [On], measurements repeat the number of times entered in the [Count] box.

When [Realtime save] is set to [On], you can choose [Single] mode only.

6 Configure the overlay setting.

See "3.1 Overlaying New Waveforms With Previously Acquired Waveforms" (p. 54).

7 Tap the [Realtime save] button to set it to [On].

The instrument can record data in an optional storage device while measuring waveforms. See "Real-time saving" (p. 124).

8 Configuring the memory division settings

The instrument can divide the internal memory into several blocks and store waveforms into them. See "10 Memory Division Function" (p. 289).


Sampling rate setting guideline

Maximum display frequency	Sampling rate	Maximum display frequency	Sampling rate
8 MHz	200 MS/s	400 Hz	10 kS/s
4 MHz	100 MS/s	200 Hz	5 kS/s
2 MHz	50 MS/s	80 Hz	2 kS/s
800 kHz	20 MS/s	40 Hz	1 kS/s
400 kHz	10 MS/s	20 Hz	500 S/s
200 kHz	5 MS/s	8 Hz	200 S/s
80 kHz	2 MS/s	4 Hz	100 S/s
40 kHz	1 MS/s	2 Hz	50 S/s
20 kHz	500 kS/s	0.8 Hz	20 S/s
8 kHz	200 kS/s	0.4 Hz	10 S/s
4 kHz	100 kS/s	0.2 Hz	5 S/s
2 kHz	50 kS/s	0.08 Hz	2 S/s
800 Hz	20 kS/s	0.04 Hz	1 S/s

Choose a sampling rate using the following table as a guideline.

If the instrument plots false waveforms (aliasing)

If a measured signal oscillates at a higher frequency compared to the sampling rate you chose, the instrument may plot false waveforms oscillating at a frequency lower than that of the actual signal once the signal frequency reaches a certain level. This phenomenon is called aliasing.

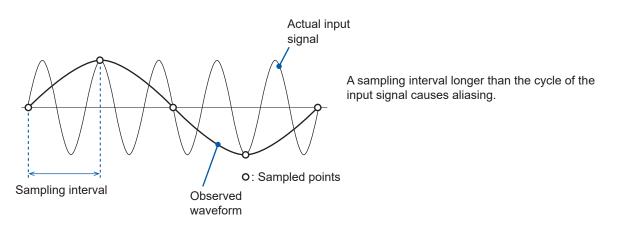

To plot a sign wave that allows you to observe the peaks without any aliasing, the instrument needs to sample the waveform at a minimum of 25 points per cycle.

To set the sampling rate automatically

See "3.7 Measuring Signals With the Auto-range Setting" in the Quick Start Manual.


Update rate of each module

The data refresh rate is not allowed to exceed the maximum sampling rate of each module. The instrument measures the same data until the data gets updated, causing the instrument to plot a stair-step waveform.

In addition, even though the instrument measures the same signal simultaneously, values may vary due to differences in the sampling rate, frequency range, and frequency characteristics of modules.

Modules	Maximum sampling rate or data update rate	Reference
Model 8966 Analog Unit	20 MS/s (50 ns)	-
Model 8967 Temp Unit	Depends on the data refresh setting.	p. 68
Model 8968 High Resolution Unit	1 MS/s (1 μs)	-
Model U8969 Strain Unit	200 kS/s (5 μs)	-
Model 8970 Freq Unit	Depends on the setting.	p. 72
Model 8971 Current Unit	1 MS/s (1 μs)	-
Model 8972 DC/RMS Unit	Depends on the response setting.	р. 77
Model 8973 Logic Unit	20 MS/s (50 ns)	-
MR8990 Digital Voltmeter Unit	Depends on the NPLC setting.	p. 78
Model U8974 High Voltage Unit	Depends on the response setting.	p. 80
Model U8975 4ch Analog Unit	5 MS/s (200 ns)	_
Model U8976 High Speed Analog Unit	200 MS/s (5 ns)	-
Model U8977 3CH Current Unit	5 MS/s (200 ns)	_
Model U8978 4CH Analog Unit	5 MS/s (200 ns)	-
U8979 Charge Unit	200 kS/s (5 μs)	_

Using the envelope

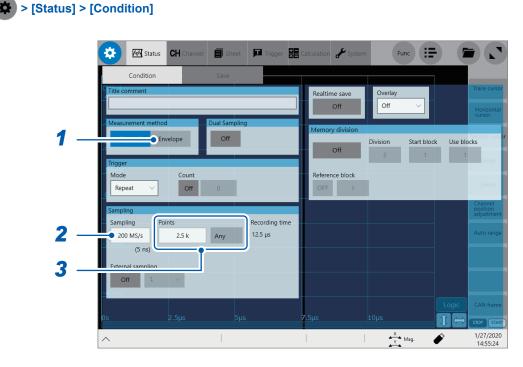

1 Under [Measurement method], tap [Envelope] to use the envelop.

Normal [∅]	Does not use the envelope.
Envelope	Uses the envelope.


• What is Normal?

The instrument records data at the specified sampling rate.

· What is Envelope?

At the specified recording interval, the instrument records the maximum and minimum values among data points sampled within each specified recording interval by sampling an input signal at an over-sampling rate* of 100 MS/s. Hence, even though a relatively longer recording interval is specified, peaks of fluctuations can be recorded without being missed.

- *: Over-sampled data (indicated by blue dots in the figure) are not saved.
- Values to be acquired using the envelope

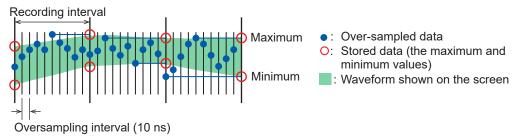

A set of sampled data acquired using the envelope consists of two values: the maximum value and the minimum value. These values are taken from the measured values acquired by sampling an input signal at an over-sampling rate during the recording interval chosen in the [Sampling] box. The screen displays a vertically wide waveform line. When saved in an external storage device, the data set that consists of the maximum and minimum values is stored for a single instance of measurement.

2 Tap the [Sampling] box, and then choose a sampling rate from the list.

The following are the sampling rates you can choose when the envelope is used.

10 MS/s^{II}, 5 MS/s, 2 MS/s, 1 MS/s, 500 kS/s, 200 kS/s, 100 kS/s, 50 kS/s, 20 kS/s, 10 kS/s, 5 kS/s, 2 kS/s, 1 kS/s, 500 S/s, 200 S/s, 100 S/s, 50 S/s, 20 S/s, 10 S/s, 5 S/s, 2 S/s, 1 S/s, 30 S/min, 12 S/min, 6 S/min, 2 S/min, 1 S/min

3 Tap the [Points] box, and then from the list, choose an option for the number of points to be measured.

2.5 k[⊠], 5 k, 10 k, 20 k, 50 k, 100 k, 200 k, 500 k, 1 M, 2 M, 5 M, 10 M, 20 M, 50 M, 100 M, 200 M, 500 M, 1 G

Tap **[Any]** to enable it, and then tap the **[Points]** box, which allows you to enter the number of points in 100 increments.


When the real-time saving is set to **[On]**, you cannot specify the recording length in the **[Points]** box. Choose **[Save]**, and enter the recording length in the **[Recording time]** box. (p. 125)

The maximum recording length you can specify varies depending on the number of channels to be measured.

1.3 Configuring the Input Channel Settings

Configure the settings of the analog and logic channels.


> [Channel]

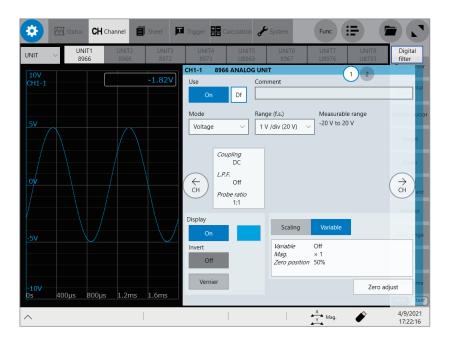

Operation available on the [Channel] screen


- Adding a comment to each channel
- Setting measurement conditions for each channel
- · Specifying the display method setting for waveforms
- · Converting measured values into physical quantities and displaying them

When a CAN/LIN interface is connected, you can toggle between **[UNIT]** and **[CAN/LIN]**. To configure the input channel settings, select **[UNIT]**.

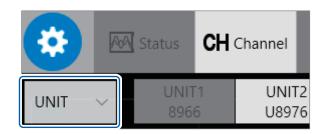


Channel setting procedure

Analog channels (CH1 through CH32) setting procedure

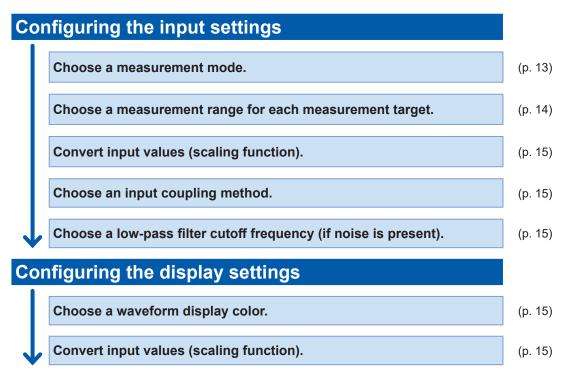

Logic channels (Model 8973 Logic Unit) setting procedure

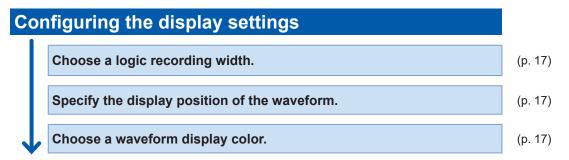


When the sheet display format is set to XY composite waveforms or FFT waveforms, no logic waveforms are displayed.

Analog channels

For details on configuring each module setting, refer to "3.7 Configuring Measurement Module-Specific Settings" (p. 67).



> [Channel] > each module (UNIT)

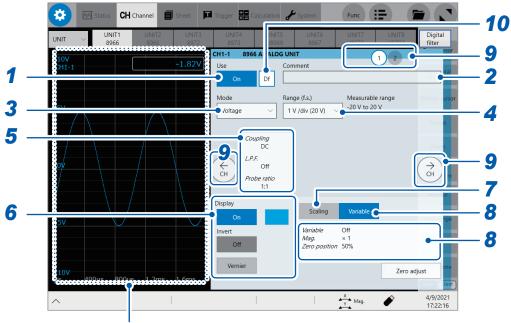

The instrument displays the waveform screen during measurement.

When the instrument does not perform measurement, it displays the presently inputted waveforms on the monitor.

1 Tap the [Use] button to set it to [On] or [Off].

On [⊠]	Measures waveforms through this module.
Off	Does not measure any waveform through this module. Since no data is acquired, the instrument displays or saves nothing.

2 Enter a comment in the [Comment] box.

Number of characters that can be entered: up to 40

3 Tap the [Mode] box, and then choose a measurement mode from the list.

Voltage [⊠]	Measures a waveform in voltage mode.
Temperature	Measures a waveform in temperature mode.

Selectable modes vary depending on the installed modules. See "3.7 Configuring Measurement Module-Specific Settings" (p. 67).

4 Tap the [Range (f.s.)] box, and then choose a measurement range from the list.

The value of the range represents its maximum displayable value (f.s.).

See the following table for the full-scale resolution of each module.

If the input voltage exceeds the measurable range (overrange occurs), change the measurement range to one with a lower sensitivity.


After changing measurement ranges, check values including level, upper, lower of the trigger, search, and numerical calculation functions.

Modules	Resolution (LSB)
Model 8966 Analog Unit, Model 8971 Current Unit, Model 8972 DC/RMS Unit	2,000
Model 8967 Temp Unit	20,000
Model 8968 High Resolution Unit, Model U8974 High Voltage Unit, Model U8975 4ch Analog Unit, Model U8977 3CH Current Unit, Model U8978 4CH Analog Unit	32,000
Model U8976 High Speed Analog Unit	1,600
Model U8969 Strain Unit, Model U8979 Charge Unit	25,000
Model 8970 Freq Unit (Power frequency mode)	2,000
Model 8970 Freq Unit (Count mode)	40,000
Model 8970 Freq Unit (Frequency mode, rotation speed mode, duty ratio mode, pulse width mode)	10,000
Model MR8990 Digital Voltmeter Unit	1,000,000

*: For the Model 8967 Temp Unit, the valid range varies depending on the thermocouples. For more information about resolution, refer to "Model 8967 Temp Unit" in "5.2 Specifications of the Options" in the Quick Start Manual.

5 Configure the input coupling, low-pass filter, and probe ratio settings.

Tapping the area that includes [Coupling] allows the setting dialog box to appear.

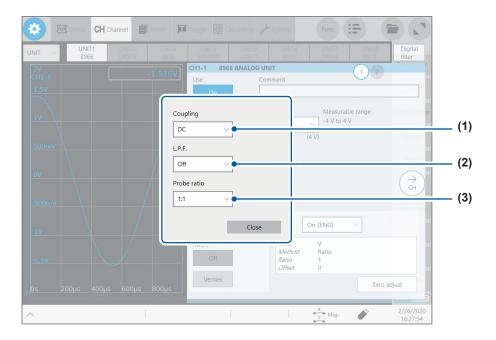

(1) Tap the [Coupling] box, and then choose a coupling method for an input signal from the list.

In general, use the DC coupling.

DC [⊠]	Measures both DC and AC components of an input signal.
AC	Measures an AC component only of an input signal. A DC component can be eliminated.
GND	Connects the input terminal to the ground (which allows you to check the zero position).

(2) Tap the [L.P.F] box, and then choose a cutoff frequency of the low-pass filter from the list.

Enabling the low-pass filter installed in the module can eliminate unwanted high-frequency components. Cutoff frequencies available vary depending on the module types. Choose an adequate cutoff frequency depending on the characteristics of an input signal.

Example: Model 8966 Analog Unit

Off[™], 5 Hz, 50 Hz, 500 Hz, 5 kHz, 50 kHz, 500 kHz

(3) Tap the [Probe ratio] box, and then choose a probe ratio from the list.

Choose any of the ratios when the measurement involves use of a connection cord or probe.

1:1 ^ℤ	Choose this ratio when using Model L9197, Model L9198, Model L9790, or Model L9217 Connection Cord.
1:10	Choose this ratio when using Model 9665 10:1 Probe.
1:100	Choose this ratio when using Model 9666 100:1 Probe, Model P9000-01 Differential Probe, or Model P9000-02 Differential Probe.
1:1000	Select this ratio when using Model 9322 Differential Probe, Model P9000-01 Differential Probe, or Model P9000-02 Differential Probe.

6 Tap the [Display] button to set it to [On] or [Off].

On ^ℤ	Displays the waveform on the waveform screen.		
	Color Allows you to choose a display waveform of each waveform. You can select the same color as other lines.		
(Off [∅] , On) inverted.		When the signs of displayed waveforms are reversed, the waveforms can be inverted. See "3.5 Inverting a Waveform (Invert Function)" (p. 65).	
	Vernier	Allows you to freely fine-adjust the input voltage on the waveform screen (display adjustment only). When recording physical values such as noise, temperature, and acceleration with sensors, you can adjust those amplitudes, facilitating calibration. See "3.4 Fine-Adjusting Input Values (Vernier Function)" (p. 64).	
Off	Does not display any waveform.		

7 Configure the scaling settings.

See "3.2 Converting Input Values (Scaling Function)" (p. 56).

8 Tap the [Variable] button to set it to [Off] or [On].

Off	Does not use the variable function but the [Magnification] box and the [Zero position button to adjust the waveform positions.	
On⊠	Uses the variable function. See "3.3 Adjusting the Waveform Display Positions (Variable Function)" (p. 62).	

You can use the **[Variable]** button when **[Fix grid]** is set to **[On]**. See "13 Configuring the System Environment Settings" (p. 343).

If [Variable] is set to [Off], tap the [Magnification] box, and then from the list, choose a magnification.

You can choose a magnification in the direction of the vertical axis (voltage axis).


×100, ×50, ×20, ×10, ×5, ×2, ×1[⊠], ×1/2, ×1/5, ×1/10


You can use the **[Magnification]** box when **[Fix grid]** is set to **[On]**. See "13 Configuring the System Environment Settings" (p. 343).

If [Variable] is set to [Off], tap the [Zero position] button, and then set the zero position.

You can specify where the zero-volt level is on the vertical axis.

Waveforms are magnified/demagnified with respect to the zero position. Although ranges of voltage shown on the waveform screen vary according to the magnification, the measurable ranges do not vary. Besides, input signals are not DC-biased but merely moved visually.





You can use the **[Variable]** button when **[Fix grid]** is set to **[On]**. See "13 Configuring the System Environment Settings" (p. 343).

9 Switch the channels.

Tap the corresponding location to switch the channels, and then set the measurement conditions by following the procedure described above.

10 Configuring the digital filter setting for each channel. (Model MR6000-01 only)


The **[Df]** setting is displayed for only channels with **[Digital filter]** set to **[On]**, allowing you to configure the digital filter setting for each channel.

For more information, refer to "Setting the Digital Filter Calculation" in MR6000-01 Dedicated Functions.

Logic channels

The logic sheet appears when the screen is in Single, Dual, Quad, Octa, or Hexadeca mode.

> [Channel]

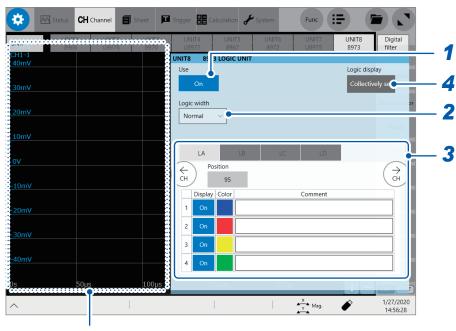

The instrument displays the waveform screen when a logic channel is chosen. You can check display positions of the logic signals.

1 Tap the [Use] button to set it to [On] or [Off].

On [⊠]	Measures a waveform through this module.
Off	Does not measure any waveform through this module. Since no data is acquired, the instrument displays or saves nothing.

2 Tap the [Logic width] box, and then choose a display width for logic waveforms from the list.

Making waveforms narrower can enhance the readability of a display that contains a large number of waveforms.

This setting is a cross-module for all logic modules installed in the instrument.

Wide	Increases the width of the waveforms.
Normal [⊠]	Displays the waveforms in normal width.
Narrow	Reduces the width of the waveforms.

3 Choose a display method for each probe (LA through LD).

Position	Allows you to specify a numeral that represents a logic waveforms position on the screen in one percent point increments. This setting is a cross-probe for all probes (LA through LD). You can display logic waveforms in a desired position.	
Display	Allows you to choose whether to display logic waveform.	
Color	Allows you to choose a display waveform of each waveform. You can also choose the same color as the lines acquired across other channels.	
Comment	Allows you to type a comment for each channel. Number of characters that can be entered: up to 40	

4 Under [Logic display], tap [Callectively set], and then from the list, select the logic waveform display setting.

All logic On	Displays all logic waveforms.	
All logic Off	Hides any logic waveforms.	
Unit On	Sets all the logic waveforms acquired with the enabled modules to display altogether.	
Unit Off	Sets all the logic waveforms acquired with the enabled modules to hide together.	
Probe On	Sets all the logic waveforms acquired with the chosen probes to display altogether.	
Probe Off	Sets all the logic waveforms acquired with the chosen probes to hide altogether.	


1.4 Configuring the Sheet Settings

You can define the display format of waveforms on the sheet. You can define different display formats for each of the 16 sheets. You can also switch sheets to be displayed on the waveform screen.

You can configure the XY composite waveform settings.

See "2.8 Generating XY Composite Waveforms (XY Composite)" (p. 47)

> [Sheet]

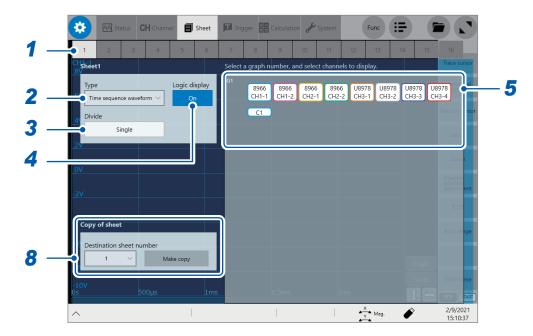

1 Choose a sheet.

2 Tap the [Type] box, and then choose a display format from the list.

Time sequence waveform [⊠]	Displays time-sequence waveforms.
XY composite waveform	Displays XY composite waveforms.
FFT waveform	Displays FFT-calculated waveforms.

1

3 Tap the [Divide] box, and then from the list, choose an option for the number of screens to be divided.

You can split the screen into multiple screens (graphs).

When you choose [Time sequence waveform] in the [Type] box

Single[⊠], Dual, Triangle, Quad, Hexagon, Octa, Nonagon, Hexadeca

When you choose [XY composite waveform] in the [Type] box

XY Single^Ø, XY Dual, XY Quad, Time sequence + XY Dual

When you choose [FFT waveform] in the [Type] box

FFT Single[⊠], FFT dual, FFT quad, Time sequence + FFT single, Time sequence + FFT dual, Time sequence + FFT quad

4 (When you choose [Time sequence waveform] in the [Type] box)Tap the [Logic display] button to set it to [On] or [Off].


Off	Does not display logic waveforms.
On ^ℤ	Displays logic waveforms.

5 Tap the display panel of each graph.


The [Select the channel] dialog box opens.

6 Choose channels to be displayed on the graph.

All channels are chosen in the default setting. Tapping a button deselects a channel (Tap it again to select it). Every time you tap [All], all waveform calculation channels is collectively selected or deselected.

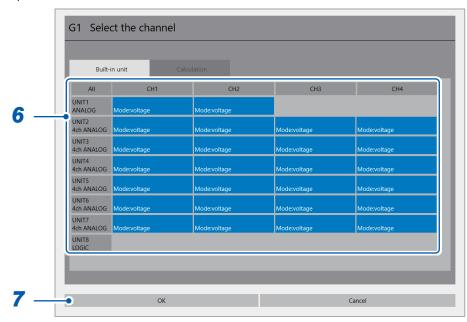

Example: Selection screen for time series waveforms

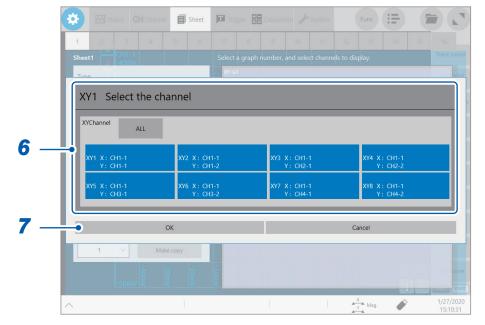

Example: Selection screen for XY composite waveforms

Example: Selection screen for FFT waveforms

	Sheet1 Type FFT1 Select the ch	5 6 7 8 Select a graph r G1 U8975	Calculation & System 9 10 11 12 umber, and select channels to di 18975 U8975 U8975	Func II- 13 13 14 15 isplay.	16 Trace cursor Portuge tal
6 -	FFT CalcChannel ALL FFT1 Linear spectrum FFT5 Linear spectrum			FFT4 1CHPhase spectrum FFT8 1CHPhase spectrum	
/ -	4 5 -200	MHz OMD		X Mag.	1/15/2019 15:38:47

7 Tap [OK].

Your selection is confirmed.


Tapping [Cancel] closes the dialog box without your selection confirmed.

When you choose [Time sequence waveform] or [FFT waveform] in the [Type] box) Tap [Destination sheet number] to choose a sheet number, and then tap the [Make copy] button.


The settings configured from steps **1** to **6** affect the copy destination sheet. The sheet settings have been finished.

(When you choose [XY composite waveform] in the [Type] box) Go on to step 9.

9 (When you choose [XY composite waveform] in the [Type] box) Tap the [X:/Y: Settings].

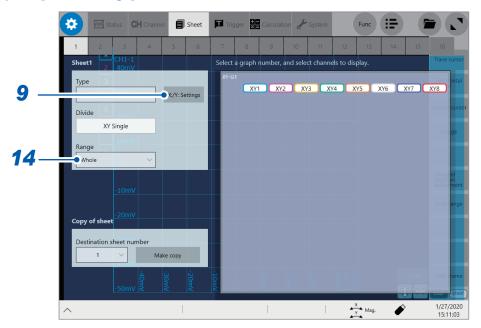

The [XY composite channel settings] dialog box is displayed.

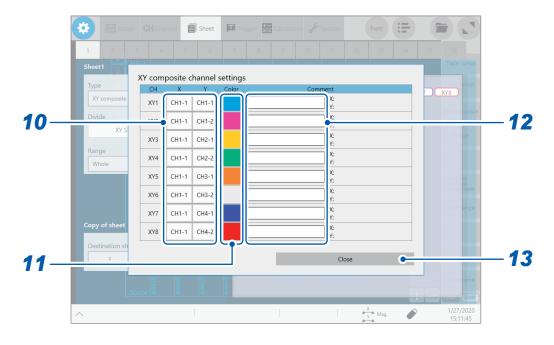

10 Tap a channel number button, and then from the list, choose channels to be assigned to the X and Y axes of the XY channel you chose.

11 Tap the color button, and then from the color pallet, choose a display color of the XY channel you chose.

You can choose the same color as lines acquired across other channels.

12 Enter a comment in the [Comment] box.

Number of characters that can be entered: up to 40

13 Tap [Close].


The [XY composite channel settings] dialog box closes.

14 Tap the [Range] box, and then from the list, choose an option for a range of waveforms to be used for generating XY composite waveforms.

Whole [∅]	Generates XY composite waveforms using waveforms spanning the whole range.
Segment 1	Generates XY composite waveforms using the waveforms of the scope specified as Segment 1.
Segment 2	Generates XY composite waveforms using the waveforms of the scope specified as Segment 2.

Switching sheets on the waveform screen



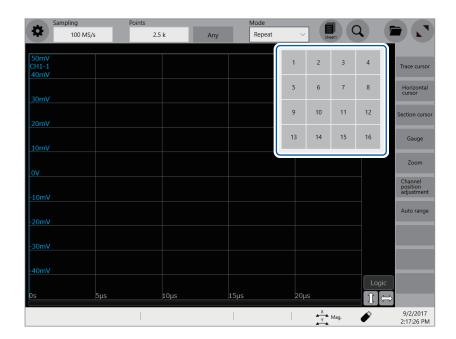


. .

Choose sheet numbers to be displayed.

Generating XY composite waveforms

During or after measurement, you can generate XY composite waveforms using waveform acquired across user-defined channels.



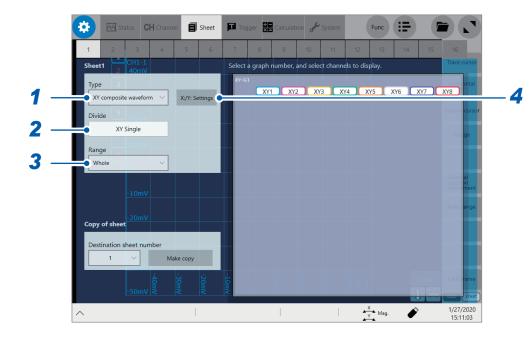

- **1** Tap the [Type] box, and then from the list, select [XY composite waveform].
- **2** Tap the [Divide] box, and then from the list, choose an option for the number of screens to be divided.


XY Single^Ø, XY Dual, XY Quad, Time sequence + XY Dual

3 Tap the [Range] box, and then from the list, choose an option for a range of waveforms to be used for generating XY composite waveforms.

Whole [⊠]	Generates XY composite waveforms using the whole waveforms.
Segment 1 Segment 2	Generates XY composite waveforms using the waveforms between the specified section cursors. How to specify section cursors See "2.2 Specifying the Waveform Range (Section Cursor)" (p. 35).

4 Tap the [X:/Y: setting].


The [XY composite channel settings] dialog box is displayed.

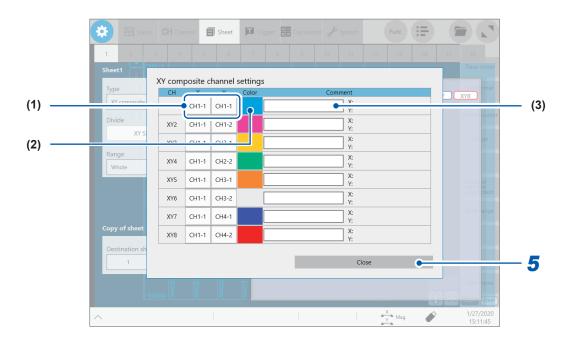

- (1) Tap a cell in the [X] and [Y] columns, and then from the list, choose channels to be used for generating XY composite waveforms. Up to eight XY composite waveforms can be generated.
- (2) Tap a color button in the [Color] column, and then choose a color for XY composite waveforms.
- (3) In the [Comment] box, enter a comment for the XY composite waveform.


5 Tap [Close].

The [XY composite channel settings] dialog box closes.

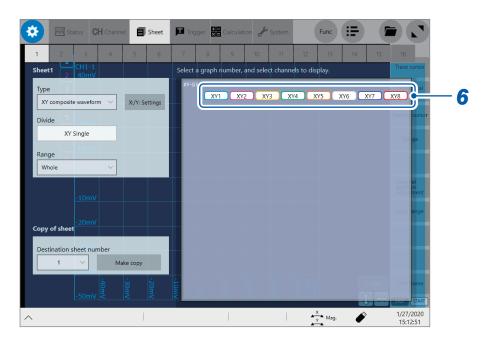

6 Tap the display panel of each graph.

The **[XY** Select the channel] dialog box is displayed.

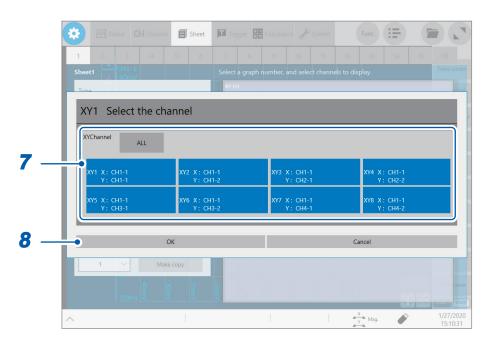

7 Tap the XY channel to be displayed.

- If you save a setting file, the settings for all the displayed sheet are saved.
- If you save a waveform file, the settings of the displayed sheet are saved as configured at the time of saving. Even when a waveform file is loaded, no sheets except the sheet displayed at the time of saving are loaded.

8 Tap [OK].

The **[XY** Select the channel] dialog box closes.

1.5 Starting/Stopping a Measurement

Starting a measurement

Pressing the **START** key starts a measurement.

- Waveforms shown on the screen are cleared once the measurement starts.
- You can also start a measurement by inputting a signal into the external control terminal.

See "15 Externally Controlling the Instrument" (p. 385).

Waveform display during measurement

In general, the waveforms appear after data with the specified recording length has been acquired. When the measurement speed is relatively slow, the instrument displays waveforms while it is acquiring the data.

However, even if a slow-speed range is set, the instrument may display waveforms after it has been acquired the data of the whole waveform, depending on the overlay or magnification setting.

To save data automatically during measurement

When waveforms of the specified recording have been acquired, the waveform data is automatically stored.

See "Automatically saving waveform data" (p. 120).

To save data during measurement in real time

The instrument can store data on a storage device during measurement in real time. See "Real-time saving" (p. 124).

Stopping the measurement

Pressing the **STOP** key once stops the measurement after the waveforms of the specified recording length have been acquired.

Pressing the **STOP** key twice stops the measurement immediately.


Operation on the waveform screen

When you operate a USB mouse connected to the instrument, the **[START]** and **[STOP]** buttons appear at the bottom right of the screen.

You can use the mouse in the same manner as the **START** and **STOP** keys on the instrument.



You can analyze measured data with various functions including trace cursor measurement of input waveforms and searches on the waveform screen. You can also change measurement conditions or other settings on this screen.

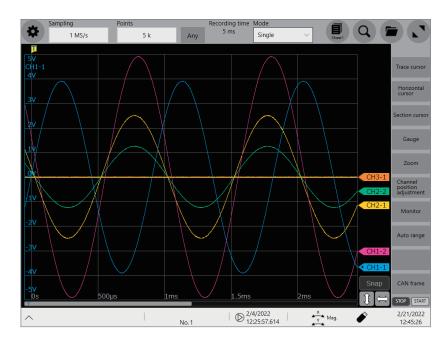

Operation available on the waveform screen

Using the trace cursors and horizontal cursors

• Reading measured values (p. 30)

Moving the waveform display position

- Dragging waveforms
- Moving waveforms with the scroll bar

Using the section cursors

• Specifying the waveform range (p. 35)

Changing the display magnification of waveforms


- Magnifying/demagnifying waveforms (p. 41)
- Magnifying a part of waveforms horizontally (p. 46)

Generating XY composite waveforms

Generating composite waveforms (p. 47)

2.1 Reading Measured Values (Trace Cursors, Horizontal Cursors)


You can read measured values (scaled values when the scaling is used) using trace cursors on the waveform screen. The instrument can simultaneously display up to eight trace cursors. You can read differences in times and measured values between any two cursors you choose from among all cursors. You can also read measured values of trace cursors on X-Y waveforms.

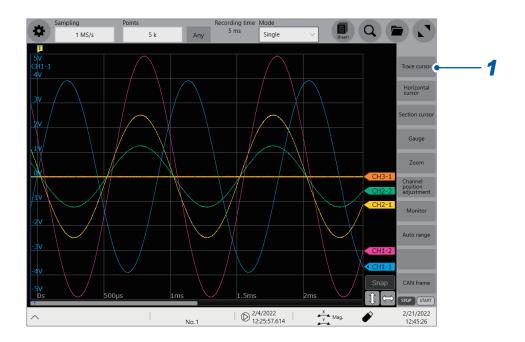

1 Tap [Trace cursor] on the wave screen.

2 Choose one or more cursors to be displayed from among [Trace cursor A] through [Trace cursor H] by tapping them.


The chosen trace cursors are displayed on the waveform screen. You can drag trace cursors on the time-series waveform screen.

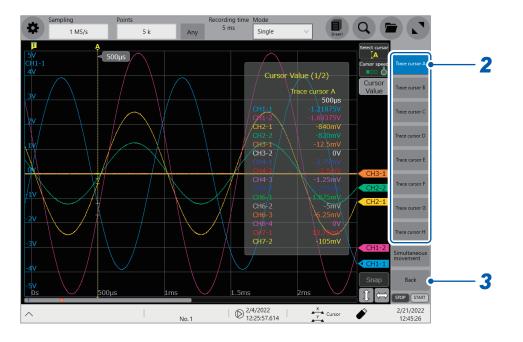

3 Tap [Back].

4 Tap [Cursor Value].

You can switch between on and off for the cursor value display every time you tap [Cursor Value].

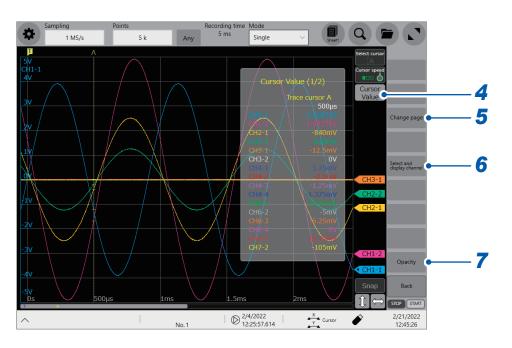


5 Tap [Change page].

When the instrument displays multiple channels, you can switch the pages to check cursor values of each channel.

Every time you tap it, the pages are switched.

6 Tap [Select and display channel].


The function buttons switch.

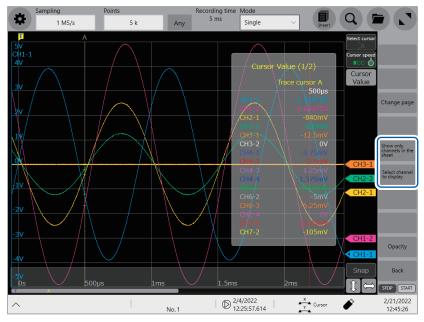

Tapping [Show only channels in the sheet] can only display channels in the present sheet. Tapping [Select channel to display] allows you to select channels of which you want to display cursor values.

7 Tap [Opacity].

The function buttons switch.

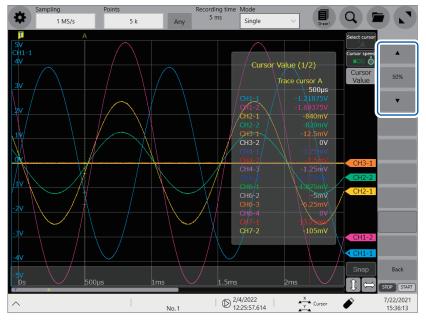


Tapping [▲] or [▼] allows you to change the opacity of the screen background between 0% and 100% in 10 percent points increments.

8 Tap [1: Trace cursor A] or [2: Trace cursor B].

The waveform screen has two areas where cursor values of trace cursors (trace cursor value 1 and Trace cursor value 2) appear.

Every time you tap [1: Trace cursor A], you can toggle the trace cursors displayed on the values of cursor values 1.

Every time you tap [2: Trace cursor B], you can toggle the trace cursors displayed on the values of cursor values 2.

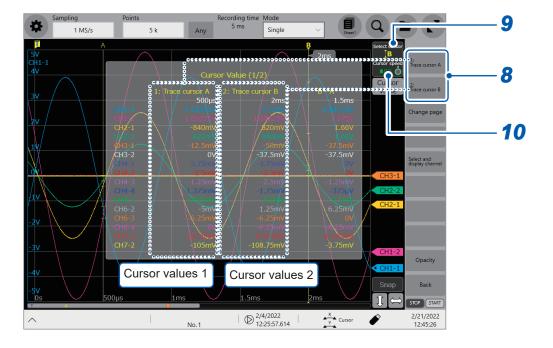

9 Tap [Select cursor].

Every time you tap it when the instrument displays multiple trace cursors, a cursor is activated one by one in sequence. In addition, you can activate any one of the cursors displayed on the screen by tapping it.

While you are operating the cursors on the waveform screen, the instrument may not displays [Cursor Value] and [Select cursor] depending on the screen operation. In this case, tap the waveform plotting field to redisplay the [Cursor Value] and [Select cursor] button.

10 Tap [Cursor speed].

You can switch the cursor moving speed on the rotary knob X on three levels every time you tap it.

Changing the display magnification of time-series waveforms while moving the trace cursor

Sliding your finger upward on the screen while dragging the trace cursor enlarges the time-series waveform display centered around the trace cursor in proportion to the dragging distance. Sliding your finger downward compresses the waveform display.

Once you have adjusted the display to a suitable size, move the trace cursor along the horizontal axis to change the display position.


Releasing your finger from the screen reverts the display to the original magnification.

To move the trace cursor using the rotary knob X

When **[Cursor]** is assigned to the rotary knob, you can move the active trace cursor with the rotary knob X.


Tapping **[Cursor speed]** allows you to switch the cursor moving distance on the rotary knob X on three levels.

The moving distance on the rotary knob Y is fixed at one.

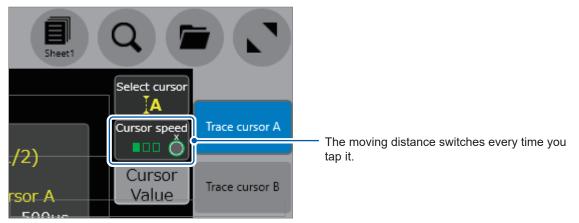

If no trace cursors appear on the screen even though the trace cursors are enabled

You can check the trace cursors positions on the scroll bar. (p. 40)

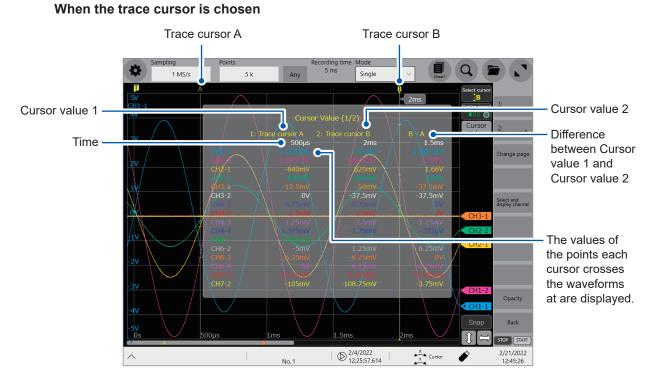

Reading measured values on the waveform screen

When the horizontal cursor is selected

The measured value at each cursor and the difference in the measured value between cursors.

The display of the cursor values varies depending on the chosen cursor type.

Cursor type	Cursor value
Trace cursor	When trace cursor A is assigned to cursor value 1; and trace cursor B, to cursor value 2. Time: A period of time from the trigger point or recording starting point until the trace cursor assigned to cursor value 1 or cursor value 2 B - A: Difference in measured values between trace cursor A and trace cursor B A B - A (Difference between measured values) B - A (Time lag)
Horizontal cursor	When horizontal cursor A is assigned to cursor value 1; and horizontal cursor B, to cursor value 2 Cursor value 1 or cursor value 2: Measured value at the specified cursor $B - A$: Difference in measured values between horizontal cursor A and horizontal cursor B A = A = B = A


When the external sampling is used, the time is represented in the number of samples.

2.2 Specifying the Waveform Range (Section Cursor)

You can specify the range using section cursors.

The specified range is applicable for saving files, making numerical calculation and searches and creating XY composite waveforms. The range selection remains unchanged even when you change the waveform display format.


1 Tap [Section cursor].

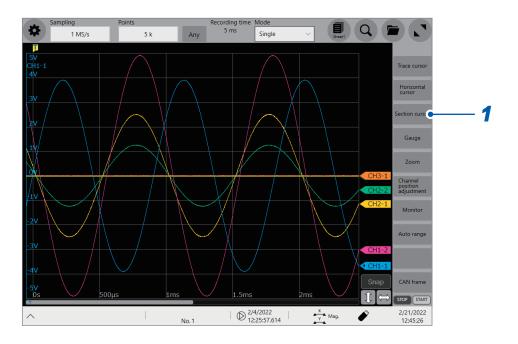

2 Tap [Section cursor 1] or [Section cursor 2].

The cursor is displayed on the left side of the screen. Drag the section cursors on the waveform screen. You can drag the section after tapping it to select.

Section cursor 1	Specifies the section with cursor 1A and cursor 1B.
Section cursor 2	Specifies the section with cursor 2A and cursor 2B.

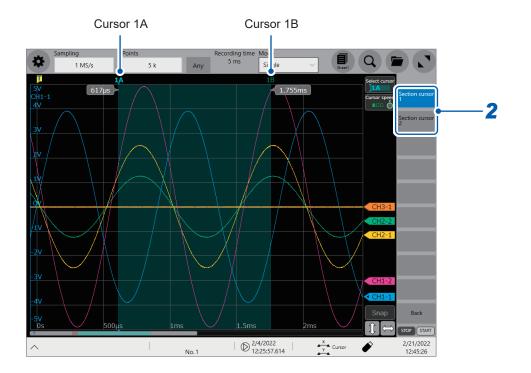

Changing the display magnification of the waveforms while moving the section cursor

Sliding your finger upward on the screen while dragging the section cursor enlarges the waveform display centered around the section cursor in proportion to the dragging distance (Sliding your finger downward compresses the waveform display.).


Once you have adjusted the display to a suitable size, move the section cursor along the horizontal axis to change the display position.

Releasing your finger from the screen reverts the display to the original magnification.

2.3 Displaying Vertical Scales (Gauge Function)


Using the gauge function enables the vertical scales (for convenience, hereafter referred to as "gauges") to be displayed overlapping waveforms.

1 Tap [Gauge].

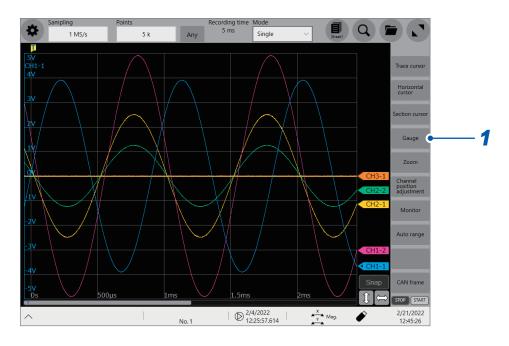


2 Choose gauges to be displayed from among [Gauge A] through [Gauge H]. The screen display the gauges at the left.

You can drag a gauge after tapping it to select.

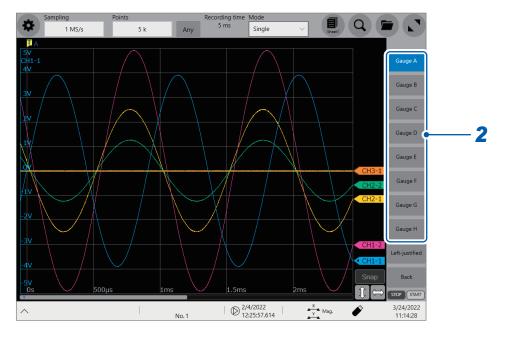

Tapping [Left-justified] aligns the gauges to the left.


3 Tap [CH \blacktriangle] or [CH \checkmark] to choose a channel to be displayed.

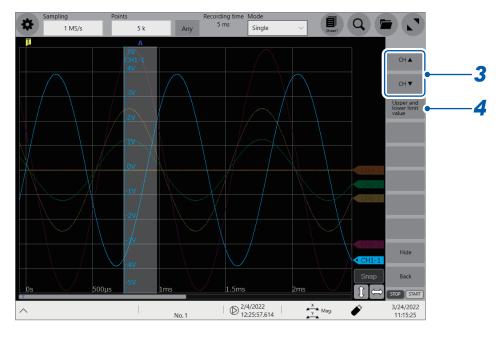

Tapping [Hide] hides the gauges.

4 Tap [Upper and lower limit value].

The setting dialog box appears. You can enter numbers that represent the display range of each channel. Enter an upper and lower values in the **[Upper]** and **[Lower]** boxes, respectively, and then tap **[OK]**.

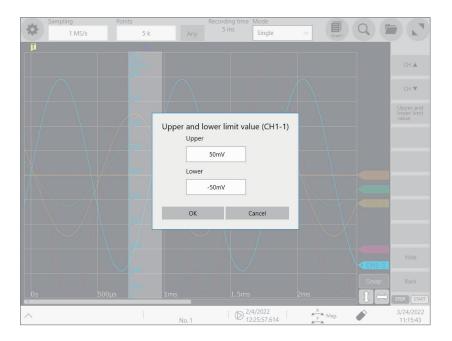


2.4 Scrolling Through Waveforms

Scrolling through waveforms

Dragging the waveform screen scrolls through waveforms that are being measured or existing waveforms.

Scrolling direction

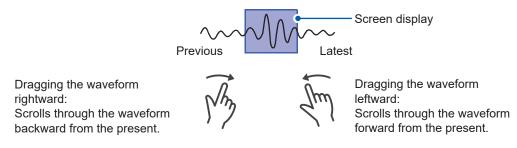


To quickly scroll waveforms sideways

When dragging the scroll bar, you can quickly scroll waveforms sideways. The longer distance you drag the scroll bar, the more quickly waveforms scroll through. Once you remove your finger from the screen, the scrolling waveforms stop.

To observe waveforms previously obtained during slow-speed measurement


When the waveforms are being displayed during a slow-speed measurement, dragging the waveform screen rightward allows you to observe waveforms previously obtained. To observe the waveforms being measured presently again, tap [>>>] on the screen.

To anchor the waveforms vertically



Tap the button to deselect it as the scroll direction.


To anchor the waveforms horizontally




-Tap the button to deselect it as the scroll direction.

Checking a position of waveforms with the scroll bar

The scroll bar provides the position and size of the displayed part of the waveforms relative to the entire recording length of the waveforms. It also shows the positions of the trigger point, trace cursors, and section cursors.

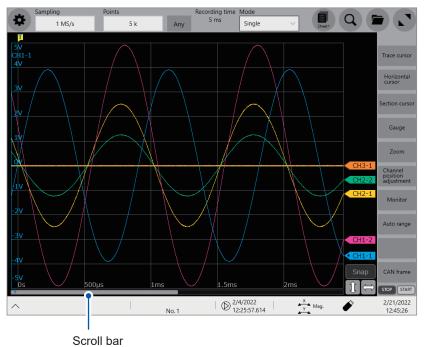

Checking the positions of the trigger point and cursors on the scroll bar

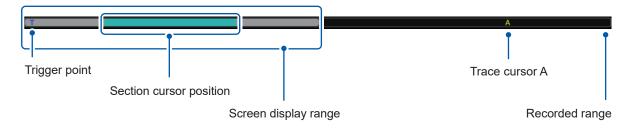

With the display zoomed in, the scroll bars are displayed at both the top and bottom.

To move the display position when [Memory division] is set to [On]

You can move a block by directly specifying a block number to be displayed.

2.5 Changing the Display Position and Display Magnification of Waveforms


Horizontally pinching in the waveform screen compresses waveforms horizontally, and pinching out enlarges.

Vertically pinching in the waveform screen compresses waveforms vertically, and pinching out enlarges.

1 Am	Pinch out	Zooms in the waveforms.
1 Mary	Pinch in	Zooms out the waveforms.

To toggle snap mode


When **[Snap]** has been enabled by tapping it, waveforms can scroll and enlarge/compress snapping the grid lines onto the edges.



Tap the button to select or deselect it.

To change the display position of logic channels in a batch


You can drag logic channels only after tapping **[Logic]** to select. When **[Logic]** is not chosen, you can drag analog channels only.




Tap the button to select or deselect it.

Differentiating a waveform display position and display magnification from those of other analog channels

1 Tap [Channel position adjustment].

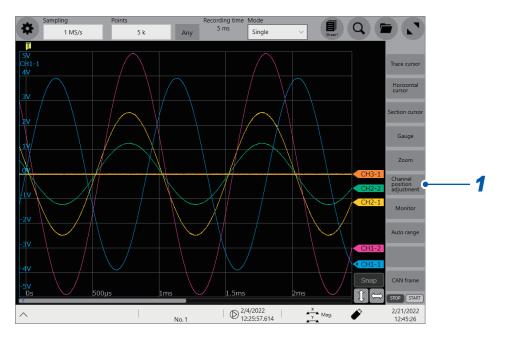

The channel position adjustment screen is displayed.

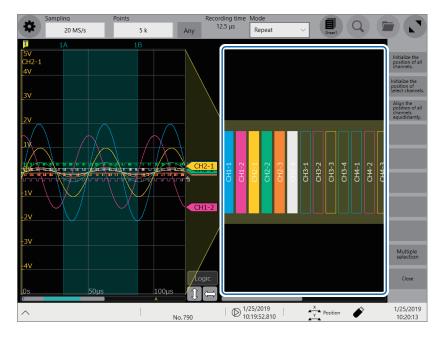

The yellow area shows the display range of the waveform screen.


2 Tap a channel number you want to move to choose and drag the chosen area.

The display position of the channel is moved.



3 Tap a channel number you want to magnify/demagnify to choose and pinch in/out the chosen area.

The channel is magnified/demagnified.

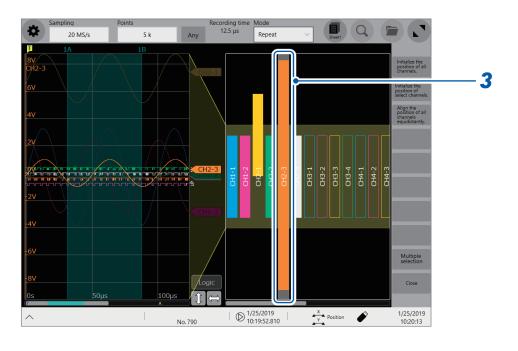

4 Adjust the display position and magnification.

The display can be adjusted as follows depending on the selected state.


Initialize the position of all channels.	Restores all the channels to the initial positions and displays them at the default magnifications.
Initialize the position of select channels.	Restores selected channels only to the initial positions and displays them at the default magnifications.
Align the position of all channels equidistantly.	Adjusts the display positions and magnifications of all channels such that they are aligned at the same intervals.
Multiple selection	Allows you to choose several channels to adjust the displays simultaneously.



2.6 Operating the Rotary Knobs

Push a rotary knob to choose an action and turn the knob to perform the action.


Operation of the rotary knob X



Each time you push the rotary knob X, the following actions are chosen one after another.

Magnification/ demagnification ratio	Changes the magnification/demagnification ratio of waveforms acquired across all channels in the horizontal axis direction.
Position	Changes the display position of waveforms acquired across all channels in the horizontal axis direction.
Cursor	Moves the chosen cursor.
Setting	Changes the sampling rate. This operation can be used on the waveform screen only.


Operation for the rotary knob Y



Each time you push the rotary knob X, the following actions are chosen one after another.


Magnification/ demagnification ratio	Changes the display magnification of the chosen channel in the vertical axis direction.
Position	Changes the display position of the chosen channel in the vertical axis direction.
Cursor	Moves the selected cursor by one sample.
Setting	Changes the measurement range. This operation can be used on the waveform screen only.

When you operate a rotary knob, the channel selection panel appears, which allows you to choose an channel to be operated by tapping the [\leftarrow] or [\rightarrow] button. In addition, you can directly choose an channel to be operated by tapping a channel marker.

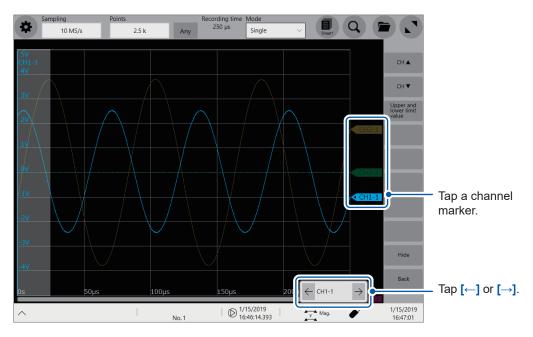

2.7 Enlarging a Part of the Waveform (Zoom Function)

Using the zoom function allows you to enlarge a part of waveforms.

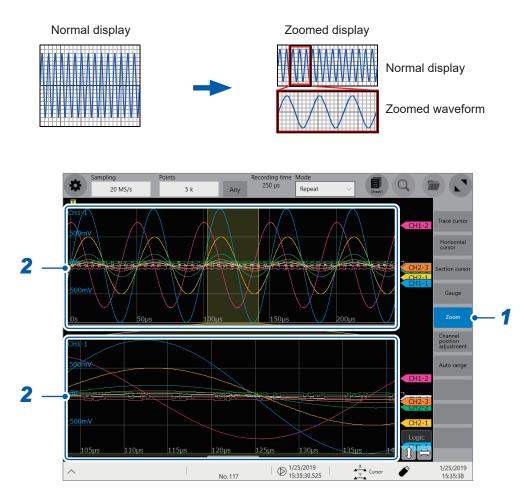

1 Tap [Zoom].

The screen splits into two, upper and lower, which enable the zoom function.

Upper screen: Displays the waveforms in the magnification specified before the zoom function was applied. The part of the waveforms enclosed by the yellow frame represents the zoomed display range

shown in the lower screen. Lower screen: Displays the zoomed-in waveform

2 Pinch in or out each screen to change the display magnification of waveforms on each screen.

3 Drag waveforms to scroll through them on each screen.

To cancel the zoomed display

Tap **[Zoom]** on the screen to cancel the zoomed display. When you cancel the zoomed display, the display (the upper screen) is restored to that with the normal magnification.

2.8 Generating XY Composite Waveforms (XY Composite)

During or after measurement, you can generate XY composite waveforms using waveforms acquired across user-defined channels.

Up to eight channels can be chosen from among analog channels, real-time calculation channels, and waveform calculation channels for generating XY composite waveforms.


No waveforms that have been acquired with the measurement method set to **[Envelope]** can be used for generating XY composite waveforms.

You can use the sheet setting screen to configure the display format, channels assigned to the X and Y axes, and the composite range settings.

To generate XY composite waveforms during measurement, you have to configure settings beforehand.

See "1.4 Configuring the Sheet Settings" (p. 19).

Operation on the waveform screen

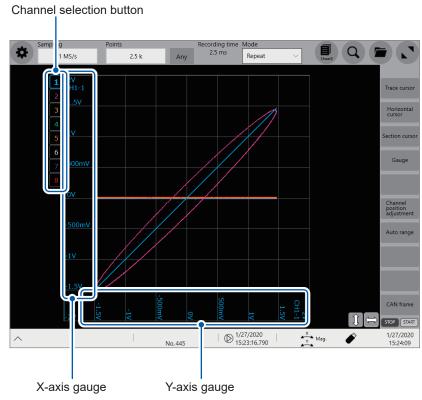

The X-axis and Y-axis gauges indicate the values of channels of each axis assigned to the chosen composite channel.

Dragging the waveform screen

Scrolls through displayed waveforms that are being measured or that have already existed.

Pinching in and out the waveform screen


Enlarges and compresses the waveforms.

Tapping the channel selection button

Switching the composite channels to be brought in front of others.

Generating XY composite waveforms using partial waveforms on the time sequence + XY dual mode screen

When the division setting is configured to **[Time sequence + XY Dual]** and the save range setting is configured to **[Segment 1]** or **[Segment 2]** on the sheet setting screen, you can directory specify the XY composite range by moving the section cursor on the time-series waveforms.

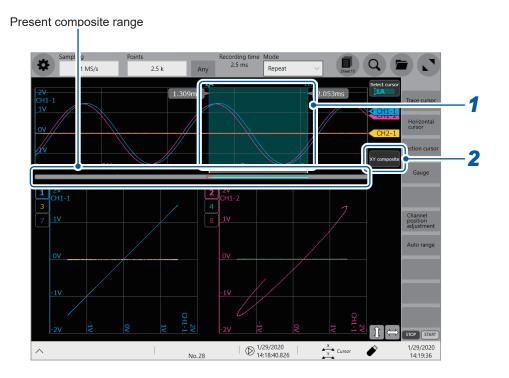


- **1** Drag the section cursor to specify the XY composite range.
- **2** Tap the [XY composite] button.

The XY composite waveforms are generated using the specified range.

2.9 Displaying Measured Values


This section explains how to configure the display settings to display measured values as well as waveforms.

While not performing measurement, the instrument will update the value of each channel every 0.5 s.

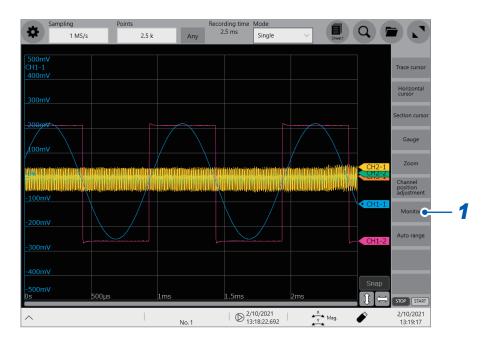

1 Tap [Monitor].

The numerical value display screen appears.

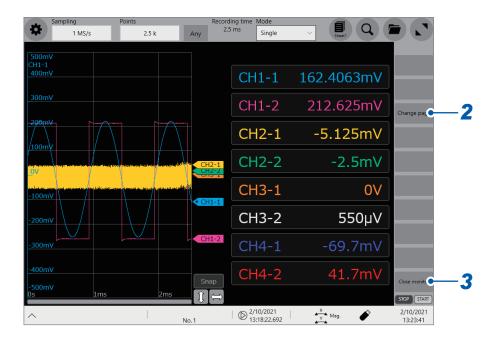


2 Tap [Change page].

If the instrument does not display some of the channels on a single screen, you can switch over the page. Every time you tap **[Change page]**, the page switches over to another.

3 Tap [Close waveform monitor].

The numerical value display screen closes.

While the instrument does not perform measurement, tapping a value can display the waveform acquired across its channel.

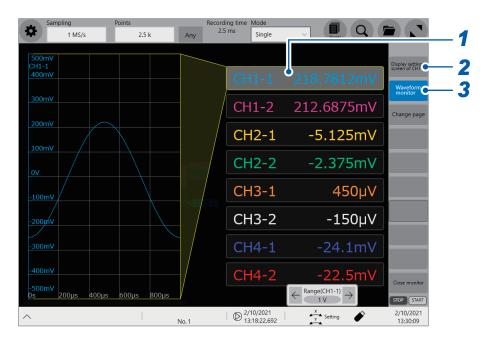

1 Tap the value of the channel whose waveform you wish to display.

2 Tap [Display setting screen of CH --].


The setting screen of the channel you chose in step **1** appears.

3 Tap [Waveform monitor].

Every time you tap [Waveform monitor], the waveform monitor appears or hides.

2.10 Viewing Block Waveforms


This section describes how to select blocks and view waveforms recorded using the instrument's memory division function.

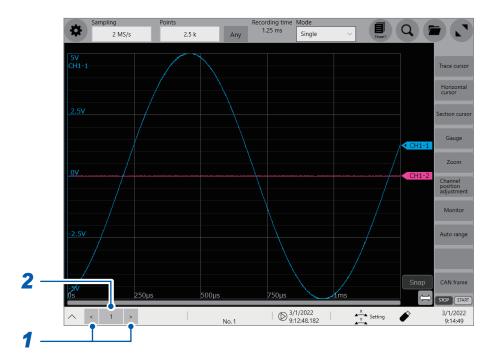

1 Tap the [<] and [>] keys to cycle through the block number shown on the waveform screen.

2 Tap the number box.

A window allowing you to change blocks will be displayed.

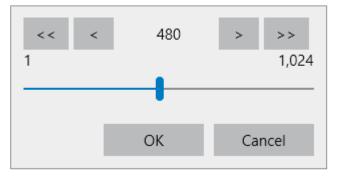

3 Select a block number using the arrow keys ([<] and [>]), the double-arrow keys ([<<] and [>>]), or the slider and tap [OK].

The waveform for the selected block will be displayed.

Viewing Block Waveforms

Advanced Functions Advanced measurements and settings

converting input values (scaling)			- · · · · · · · · · · · · · · · · · · ·
	(p. 56)	 Overlaying new waveforms with prev acquired waveforms (p. 54) 	iously
Adjusting the Waveform Display Po	ositions	Detailed module settings	(p. 6
(Variable Function)	(p. 64)	Anti-aliasing filter	
		Thermocouple type	
		 Reference junction compensation Wire break detection 	
Fine adjusting input values		Data refresh	
Fine-adjusting input values	(n, 64)	Executing automatic balancing	
	(p. 64)	Probe division ratio	
		Response time	
		Measurement mode	
Inverting a waveform			
	(p. 65)		
		, ,	
Copying a setting to another chann	nel		
	(p. 66)		

3

Converting input values (scaling)


(p. 67)

3.1 Overlaying New Waveforms With Previously Acquired Waveforms

New waveforms can be overlaid with the presently displayed waveforms.

- You can compare the new waveforms with those recorded before. (When [Mode] is set to [Repeat]) (p. 6)
- Two methods are available to overlay waveforms: the automatic overlaying during measurement and the manual overlaying.

> [Status] > [Condition]

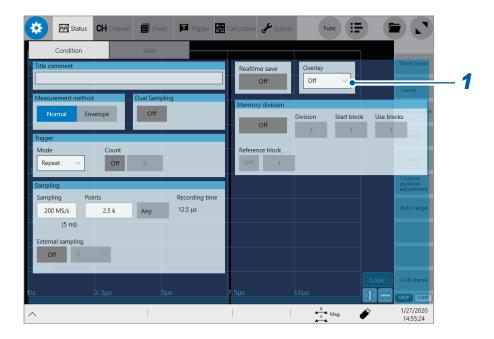


1 Tap the [Overlay] box, and then choose an overlaying method from the list.

Off	Does not overlay the waveforms.
Auto	Overlays waveforms newly acquired with the presently displayed waveforms every time the instrument acquires new ones. When [Mode] is set to [Repeat] , the instrument overlays the new waveforms with the presently displayed waveforms beginning from the start until the stop of the measurement.
Manual	Manually overlays the new waveforms with the presently displayed waveforms. See step 3 "Overlay the waveforms manually (leaving any waveforms to be displayed on the screen)." (p. 55).

See "When the overlay function is enabled (When [Overlay] is set to [Auto] or [Manual])" (p. 55).

2 Tap the button 🔅 to switch over the display to the waveform screen.

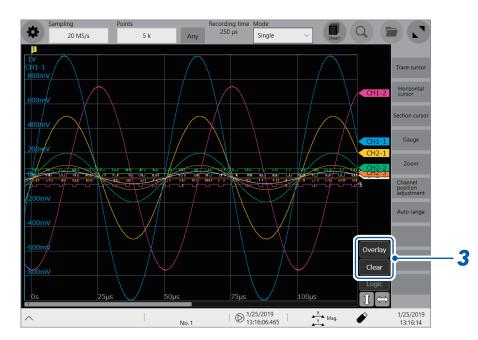

3 Overlay the waveforms manually (leaving any waveforms to be displayed on the screen). Tap the button on the right side of the waveform screen.

Overlay	Leaves the acquired waveforms displayed on the screen. The overlay setting continues to be available until the waveforms are cleared.
Clear	Clears all the overlaid waveforms displayed on the screen. No cleared waveforms can be displayed again.

When the overlay function is enabled (When [Overlay] is set to [Auto] or [Manual])

- The instrument displays the waveforms always after the data has been acquired.
- The trace cursors show the measured values of the waveforms most recently acquired.
- The following operation is not available on the waveform screen: Scrolling through waveforms, switching the zoom function between on and off, changing the magnification, and changing the zero position.
- The instrument leaves the waveforms most recently displayed only and clears the others in the following cases:
 - After selecting (> [Sheet] and changing its setting
 - After selecting > [Channel] and changing the waveform display settings (switching between on and off for the display setting or changing a waveform color)
 - After executing the search.


3.2 Converting Input Values (Scaling Function)

About the scaling function

The scaling function enables you to convert voltage outputted from measuring devices such as sensors into physical quantities of measurement targets.

Hereafter, the term "scale" refers to converting numerical values using the scaling function.

Gauge scales, scaled values (upper and lower limits of the vertical axis or voltage axis), and measured values using trace cursors are represented as scaled values in the specified units. You can configure different scale settings for each channel.

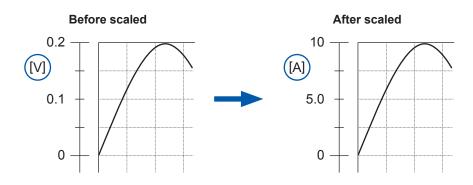


Scaling methods

The following six methods are available:

- · Specifying a conversion ratio and offset
- · Specifying two points
- · Choosing a model name of a connected current sensor or differential probe
- · Choosing an output rate
- · Specifying an input value in decibels and value after scaled
- Specifying a rated capacity and rated output according to an inspection record of a strain gauge converter (for Model U8969 Strain Unit only)

> [Channel]

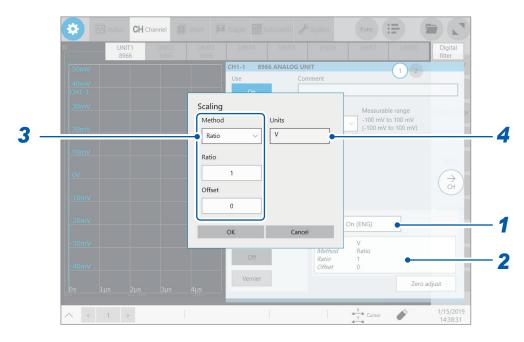

1 Tap the [Scaling] box, and then choose a scaling setting from the list.

Off [☑]	Does not scale any values.
On (ENG)	Displays values in decimal notation with a unit prefix (such as m and k).
On (SCI)	Displays values in scientific notation (as a power of 10).

2 Tap the setting items area.

The setting dialog box appears.

Ratio ^ℤ	Allows you to specify a conversion ratio and an offset.
2-Point	Allows you to specify two scaling-reference points.
Sensor	Allows you to choose a model name and measurement range of a connected current sensor or differential probe.
Output rate	Allows you to choose an output rate (ratio) of a current sensor or a division ratio of a voltage dividing probe.
dB	Allows you to specify an input value in decibels and value after scaled.
Rating	Allows you to specify a rated capacity and rated output according to an inspection record of a strain gauge converter to be used. (For Model U8969 Strain Unit only)

3 Tap the [Method] box, and then choose a setting method from the list.

When using [Ratio]

Enter a conversion ratio in the [Ratio] box.

-9.9999E+9 to 9.9999E+9

Enter an offset value in the [Offset] box.


-9.9999E+19 to 9.9999E+19


To convert inputted voltage values into current values

Specify a physical quantity per one volt of an inputted signal (conversion ratio: eu/V), an offset value, and a measurement unit to be used. The instrument converts (scales) measured values acquired in volts into that in the specified measurement unit. (eu: engineering unit)



Ratio: Change in amperes per volt; offset value: B Unit: A





When using [2-Point]

Enter a value in each of the following fields: [Input1], [Input2], [Scale1], [Scale2]. Enter two voltage values of an inputted signal in the [Input1] and [Input2] boxes. Enter each of two scaled value in the [Scale1] and [Scale2] boxes.


-9.9999E+29 to 9.9999E+29

The instrument converts (scales) measured values in volts into values in the specified measurement unit.

Example:

Input1, Input2	Scale1, Scale2
V _H : Higher potential point	A _H : Value for the higher potential point
V _∟ : Lower potential point	A _L : Value for the lower potential point

Scaling values using a conversion ratio and offset value, both of which are calculated using two points



When changing the value with the **[Ratio]** setting, the instrument does not change the values for V_L or V_H , but the values for A_L and A_H , all of which have been specified with **[Method]** set to **[2-Point]**.

When using [Sensor]

Tap the **[Sensor]** box, and then choose a model name of a current sensor or differential probe from the list.

Tap the [Range (f.s.)] box, and then choose a measurement range from the list.

Sensor	Measurement range
Model 3273-50	30 A
Model 3274	150 A
Model 3275	500 A
Model 3276	30 A
Model 3283 [⊠]	10 mA ^ℤ , 100 mA, 1 A, 10 A, 200 A
Model 3284	20 A ^ℤ , 200 A
Model 3285	200 A [⊠] , 2000 A
Model 9010-50	10 A [⊠] , 20 A, 50 A, 100 A, 200 A, 500 A
Model 9018-50	10 A [⊠] , 20 A, 50 A, 100 A, 200 A, 500 A
Model 9132-50	20 A ^ℤ , 50 A, 100 A, 200 A, 500 A, 1000 A
Model 9322	_
Model 9657-10	10 A
Model 9675	10 A
Model CT6700	5 A
Model CT6701	5 A
Model CT6710	500 mA, 5 A, 30 A
Model CT6711	500 mA, 5 A, 30 A

3 Advanced Functions

Setting example:

To display values measured with Model 9018-50 Clamp on Probe using the 10 A range as values in amperes (A) $\,$

Sensor: Model 9018-50

Range: 10 A Unit: A

When using [Output rate]

Tap the **[Output rate]** box, and then choose a current value per one volt outputted the current sensor from the list.

Otherwise, choose a voltage value per a one volt outputted from the differential probe.

10 mA^{II}, 100 mA, 1 A, 10 A, 20 A, 50 A, 100 A, 200 A, 250 A, 500 A, 1000 A, 2000 A, 2500 A, 5000 A, 1000 V

When using [dB]: Specify a physical quantity per input signal (ratio) in decibels.

Tap the **[Input dB]** box, and then enter an inputted signal value in decibels. Tap the **[Output dB]** box, and then enter an scaled value in decibels.

-200 to +200

You can specify values to five or less significant figures.

Setting example:

Converting (scaling) an input value of 40 dB into 60 dB

Input dB: 40

Output dB: 60

The instrument specifies a conversion ratio corresponding to inputted values in decibels. The offset value is set at zero.

When using [Rating]

(for Model U8969 Strain Unit only)

Tap the **[Capacity]** box, and then enter the rated capacity of a strain gauge converter to be used. Tap the **[Output]** box, and then enter a rated output of a strain gauge converter to be used.

+1.0000E-9 to +9.9999E+9

You can specify values to five or less significant figures.

Specify the parameters such that the quotient of the rated capacity divided by two times the rated output is less than or equal to 9.9999E+9.

For the rated capacity and rated output, see an inspection record of a strain gauge converter to be used.

Setting example: To display results measured with a strain gauge converter that has a rated capacity of 20 G and rated output of 1000 μ V/V as figures in gravities (G) Unit: G Rated capacity: 20 Rated output: 1000

The upper and lower display values of a waveform also automatically change according to the changes made in the scaling settings.

4 Tap the [Units] box, and then enter a unit used for scaled values.

(Number of characters: up to 7)

To copy the scaling setting to another channel

See "3.6 Copying Settings (Copy Function)" (p. 66).

When using Model U8969 Strain Unit

When an inspection record of a strain gauge converter provides a calibration factor

Example: To display waveform data measured with a strain gauge converter that has a calibration factor of 0.001442 G/1 × 10⁻⁶ strain* as figures in gravities (G)

(*: 10^{-6} strain = $\mu\epsilon$)

Scaling	On (ENG)
Method	Ratio
Units	G
Ratio	0.001442 [G] (Displayed as "1.4420 m")

When an inspection record of a strain gauge converter provides the rated capacity and rated output

See "When using the [Rating] setting" in "3.2 Converting Input Values (Scaling Function)" (p. 60).

When using a strain gauge that has a gauge factor of other than 2.0

Model U8969 Strain Unit measures outputs of the gauge supposing that the gauge factor stands at 2.0.

When a strain gauge that has a gauge factor of other than 2.0 is used, you need to convert its gauge factor into a conversion ratio.

For example, if the gauge factor stands at 2.1, the conversion ratio will be 0.952 (\approx 2 / 2.1).

Example: To display waveform data measured with a strain gauge (gauge factor: 2.1) as figures in gravities (G)

Converting output into physical quantities requires the two scaling (s) calculations: multiplying output by the gauge ratio and by a conversion ratio. In this case, enter the product of the conversion ratios of the gauge factor and the scaling conversion ratio as the conversion ratio.

Where the conversion ratio of the gauge factor is 0.952, and the conversion ratio to convert data into physical quantities is 0.001442^* . Conversion ratio = $0.952 \times 0.001442 = 0.0013728$

Enter [0.0013728] as the conversion ratio.


*: To convert values measured with a strain gauge into physical quantities, calculate the conversion ratio based on Young's modulus or Poisson's ratio of a measurement object. The conversion method varies depending on the conditions the strain gauge is used in.

See "Scaling method for strain gauges" (p. 405).

3.3 Adjusting the Waveform Display Positions (Variable Function)

This section describes how to adjust display ranges and waveform display positions in the direction of the vertical (voltage) axis, according to your preferences.


You can specify each waveform's upper and lower limit values for the vertical (voltage) axis to display the waveform enraging it to fill the screen.



Before using the variable function

- Make sure that the vertical-axis (voltage-axis) range is suitably set for the input signal.
- You can specify the upper and lower limit values when [Fix grid] is set to [On]. See "13 Configuring the System Environment Settings" (p. 343).




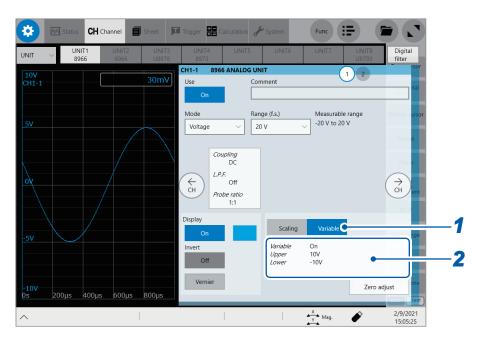

1 Tap [Variable].

2 Tap the variable setting item field.

The **[Variable]** dialog box appears.

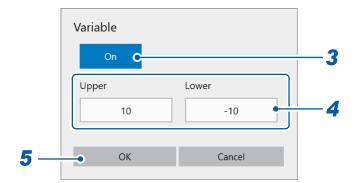

3 Tap [On].


If **[Variable]** is set to **[On]**, use the **[Magnification]** box and the **[Zero position]** button to adjust the waveform positions. (p. 16)

4 Tap the [Up] and [Low] boxes, and enter the value in each box.


5 Tap [OK].

3.4 Fine-Adjusting Input Values (Vernier Function)

You can freely fine-adjust input voltage on the waveform screen. When recording physical values, such as noise, temperature, and acceleration, with sensors, you can adjust those amplitudes, which facilitates calibration.

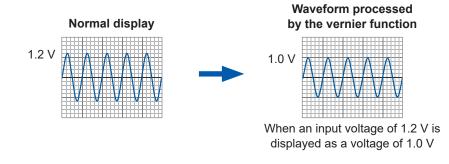

🌣 > [Channel]

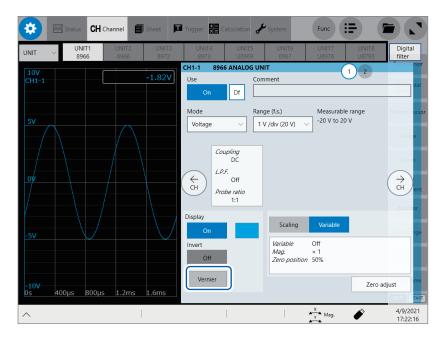

1 Tap [Vernier].

The adjustment keypad appears.

2 While observing the waveform, you can fine-adjust its amplitude by tapping [--], [-], [+], and [++].

Tap [C] to revert the fine -adjusted amplitude to its original.

- The adjustable range is from 50% to 250% of an original waveform.
- Using the vernier function turns the sides of [Vernier] blue.

 Waveform not processed by the vernier function
 Waveform processed by the vernier function

 Vernier
 Vernier

• Waveform data (data saved as files) is that adjusted by the vernier function.

3.5 Inverting a Waveform (Invert Function)


You can invert a waveform relative to the X axis. This function can be used for analog channels only.

Measured data saved in files is that inverted by the invert function.

Example:

- When a signal is inputted with spring-pulling force negative and spring-compressing force positive; however, you would like to display the results with spring-pulling force positive and spring-compressing force negative
- When a current sensor is clamped around a wire with its current direction mark mistakenly in the direction opposite to the current flow



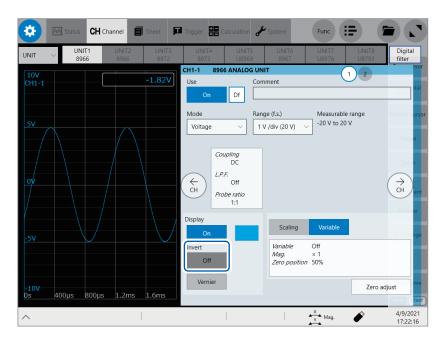

Tap the [Invert] button to set it to [On].

This setting is not available for Model 8967 Temp Unit, Model 8970 Freq Unit, and Model 8973 Logic Unit.


3.6 Copying Settings (Copy Function)

You can copy settings of other channels, as well as the trigger settings and the real-time waveform calculation settings (Model MR6000-01 only).

The following procedure explains how to copy settings of another channel.

> [Func] > [Copy] > [Channel]

The [Copy settings] dialog box appears.

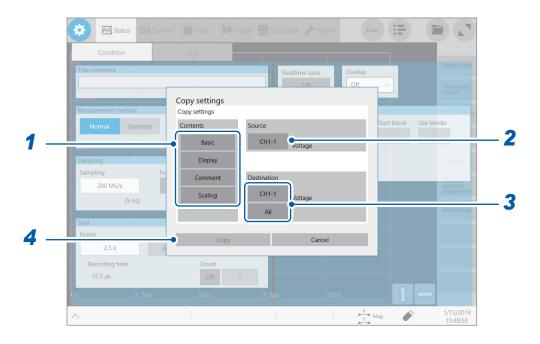

1 In the [Contents] area, tap one or more of items that you want to copy.

Depending on module types, some items may not be able to be copied.

Basic	Copies the mode, measurement range, coupling, L.P.F., division ratio, and module-specific settings.
Display	Copies the display setting (excluding comments).
Comment	Copies a comment.
Scaling	Copies the scaling setting.

2 Tap the [Source] box, and then choose a source channel from the list.

3 Tap the [Destination] box, and then choose a destination channel from the list. Otherwise, tap [All].

CH1-1 [⊠] (Channel selection)	Tap this option when you would like to copy the settings to any one of the channels, and then choose a destination channel from the list.
All	Copies settings to UNIT 1 through UNIT 8.

4 Tap [Copy].

After copying the settings, check that the measurement range, as well as setting values, such as the level, upper, and lower values, of the trigger function, the search function, and the numerical calculation function are appropriate.

3.7 Configuring Measurement Module-Specific Settings

You can configure advanced settings for each module.

Configuring Model 8968 High Resolution Unit settings

✿ > [Channel] > [8968]

CH Channel Func (III ÷ Т UNIT Digita filter UNIT Comment Mode Range (f.s.) Measurable range -1 V to 1 V Voltage 1 V A.A.F. Coupling DC Off L.P.F. ← сн Off → сн Probe ratio 1:1 Display Scaling Off Invert Vernie Zero adjust 600µs 2/27/2020 9:05:01 Y Po

1 Tap the area that includes [A.A.F].

The [A.A.F.] setting dialog box appears.

2 Tap the [A.A.F.] box, and then choose [On] or [Off] from the list for the anti-aliasing filter setting.

Enabling the anti-aliasing filter prevents aliasing distortion from influencing FFT calculations. The cutoff frequency automatically changes according to the sampling rate or frequency range (for the FFT function) settings.

Off	Disables the anti-aliasing filter.
On	Enables the anti-aliasing filter. (Disabled when the external sampling is used, or the sampling rate is set at 100 kS/s or faster)

3 Tap [Close].

The setting dialog box closes.

Configuring Model 8967 Temp Unit settings > [Channel] > [8967]



1 Tap the [Mode] box, and then choose a thermocouple type from the list.

Choose an option depending on the type of a thermocouple to be used.

Mode	Measurable range	Mode	Measurable range
K⊠	-200°C to 1350°C	R	0°C to 1700°C
J	−200°C to 1100°C	S	0°C to 1700°C
E	–200°C to 800°C	В	400°C to 1800°C
т	-200°C to 400°C	w	0°C to 2000°C
N	-200°C to 1300°C		

2 Tap the area that includes [RJC].

The setting dialog box appears.

3 Tap the [RJC] box, and then choose between [Int.] and [Ext.] from the list for reference junction compensation.

Int. [∞]	Execute the reference junction compensation inside the module. (Measurement accuracy: The sum of the accuracy of the temperature measurement and that of the reference junction compensation)
Ext.	Does not execute the reference junction compensation inside the module. (Measurement accuracy: The accuracy of the temperature measurement only)

When connecting a thermocouple directly to the module, choose [Int.]. When connecting a thermocouple via a reference junction device (e.g., zero-point bath), choose [Ext.].

4 Tap the [Burn out] box, and then choose between [On] and [Off] from the list for the wire break detection setting.

You can detect a broken thermocouple wire during temperature measurement. If a thermocouple wire breaks, measured values will fluctuate.

Off [⊠]	Does not check wires for a break.	
On	Check wires for a break by flowing about 100 nA of minuscule current through the thermocouple.	

If the thermocouple wires are long or have a relatively high resistance, set [Burn out] to [Off] to avoid measurement errors.

5 Tap the [Data update] box, and then choose a data update interval from the list.

Fast	Updates data about every 1.2 ms. Choose this option for a quicker response. However, choosing this option causes some increase in noise superimposed on input signals.
Normal [⊠]	Updates data about every 100 ms. Choosing this option eliminates noise, leading to stable measurement.
Slow	Updates data about every 500 ms. Choosing this option leads to stabler measurement.

6 Tap [Close].

The setting dialog box closes.

Configuring Model U8969 Strain Unit settings

Model U8969 Strain Unit can execute automatic balancing.


Executing automatic balancing regulates the reference output level of a transducer at the specified zero position. Automatic balancing is available for Model U8969 Strain Unit only.

You can use Model 8969 Strain Unit you own with this instrument. The instrument displays the model name of Model 8969 Strain Unit as **[U8969]**.

Before executing automatic balancing

- Turn on the instrument and leave it for 30 minutes to allow the internal temperature of the module to stabilize.
- After properly connecting a strain gauge converter to the module and a measuring object, execute automatic balancing without any input including distortion.
- You cannot execute automatic balancing during measurement.
- No key operation is accepted during automatic balancing.

To execute automatic balancing on the channel screen of each channel > [Channel] > [U8969]

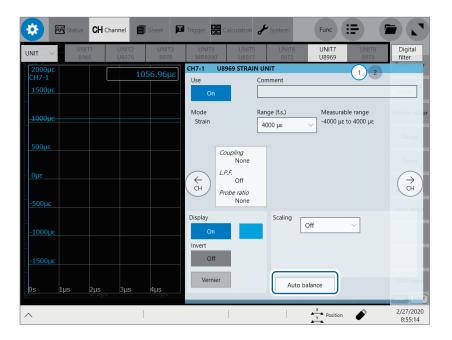

Tap [Auto balance], and then choose an automatic balancing setting from the list.

One channel onlyExecutes automatic balancing for only a channel displayed on the channelAllExecutes automatic balancing for all of the channels Model U8969 is insta		Executes automatic balancing for only a channel displayed on the channel screen.
		Executes automatic balancing for all of the channels Model U8969 is installed in.

To execute automatic balancing on the list screen

> [Channel] > []> [Operate] > [Auto balance]

Executes automatic balancing for all channels of Strain Units installed in the instrument.

In the following cases, execute automatic balancing again.

- After changing the vertical axis (strain axis) range
- · After replacing any modules
- After replacing the strain gauge converter
- · After cycling the instrument
- · After initializing the instrument
- · When the ambient temperature has changed significantly (the zero position may drift)


If automatic balancing fails

Check the following items, and re-execute automatic balancing.

- Is the strain gauge converter not subjected to any load?
- (Make sure that the strain gauge converter is not subjected to vibration, etc.)
- · Is the strain gauge converter connected to the measurement target properly?

Configuring Model 8970 Freq Unit settings




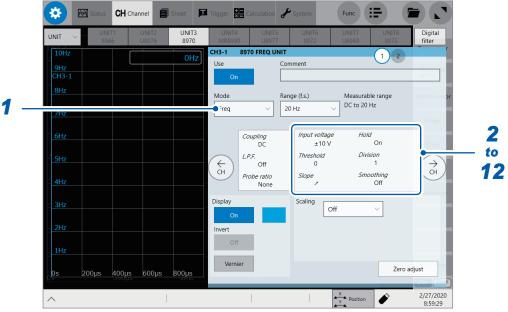

1 Tap the [Mode] box, and then choose a measurement mode from the list.

Freq [∅]	Measures frequency of a waveform (in hertz [Hz]).
Rotation speed	Measures the number of rotations of a measuring object (in rotations per minute [r/min]).
Power frequency	Measures power frequency fluctuation (in hertz [Hz]).
Count	Accumulates the number of input pulses.
Duty ratio	Measures duty ratios of a waveform to be measured (in percent [%]).
Pulse width Measures pulse widths (in second [s]).	

A pulse that rises during the dead time (during a calculation) cannot be measured (with a frequency of 25 kHz or higher).



2 Tap the area that includes [Input voltage].

The setting dialog box appears.

3 Tap the [Input voltage] box, and then choose an option for the maximum level of an input signal from the list.

±10 V^{II}, ±20 V, ±50 V, ±100 V, ±200 V, ±400 V

Tap the [Threshold] box, and then enter a threshold value.

- Measured values are acquired based on the following: the interval between the subsequent two points when measured waveform exceeds (or falls below) the threshold value, and the number of times when the waveform exceeds (or falls below) the threshold value.
- The upper and lower limits of the threshold value and the increment in the threshold value vary depending on the input voltage setting.

To prevent measurement errors due to noise, a hysteresis width of about 3% of the input voltage is tolerated for the threshold.

(When [Input voltage] is set to [±10 V], it stands at about ±0.3 V.)

Specify a threshold allowing for tolerance that exceeds the hysteresis width relative to a peak voltage.

5 Tap the [Slope] box, and then from the list, choose a signal direction to be detected.

	Detects a waveform when it exceeds the specified threshold value (while rising).
X	Detects a waveform when it falls below the specified threshold value (while falling).

5 Tap the [Division] box, and then enter a pulse count used for calculating frequency.

1 ^ℤ to 4,096	

Example: For an encoder that outputs 360 pulses per rotation, set [Division] at [360] to measure a frequency each rotation. When [Division] is not used, set it at [1].

7 Tap the [Timing] box, and then from the list, choose a condition used for starting a count. Only when [Mode] is set to [Count], this setting is available.

Start [⊠]	Starts a count when you press the START key.
Trigger	Starts a count when the instrument is triggered.

- With the **[Start]** setting, some internal processing time is required between the time when you press the **START** key and the start of measurement. Thus, the count value is not zero at the start point.
- With the **[Timing]** setting, an input that exceeds the trigger level does not trigger the instrument during pretrigger latency. Furthermore, the time for internal processing at the start and the trigger priority setting may not cause the instrument to trigger even when the input signal exceeds the specified trigger level.
- The memory division may cause the last data of the precious block to remain in the top of the block.

8 Tap the [Count over] box, and then from the list, choose an action to be performed when a count number is saturated.

Only when [Mode] is set to [Count], this setting is available.

Hold [⊠]	Counts pulses and stops counting when the pulse count reaches the upper limit (65 for the 40 k range).	
Back	Starts counting pulses and brings the count back to zero when the pulse count reaches 25 times of the range figure (50000 for the 40 k range).	

9 Tap the [Level] box, and then from the list, choose a side of the threshold level to be detected for pulse width measurement and duty ratio measurement.

Only when [Mode] is set to [Pulse width] or [Duty ratio], this setting is available.

High [⊠]	Detects pulses on the upper side of the threshold level.
Low	Detects pulses on the lower side of the threshold level.

10 Tap the [Smoothing] box, and then choose a scaling setting from the list.

Only when [Mode] is set to [Freq] or [Revolution], this setting is available.

Off	Records measured data without smoothing (resulting in a step-like waveform).
On	Interpolates measured data to smooth a waveform and outputs it. (Upper limit: 10 kHz; outputting data with this setting set to on lags behind that with this setting set to off)

11 Tap the [Hold] box, and then choose a measured-value retaining setting from the list.

Only when [Mode] is set to [Freq] or [Revolution], this setting is available.


Off (1 Hz), Off (0.5 Hz), Off (0.2 Hz), Off (0.1 Hz)	When the instrument cannot determine a measured value even when the frequency reaches a value in the brackets, the instrument determines the measurement to stop and regards the measured value as 0 Hz (0 rpm).
On [⊠]	Retains the value confirmed the last time.

12 Tap [Close].

The setting dialog box closes.

Configuring Model 8971 Current Unit settings



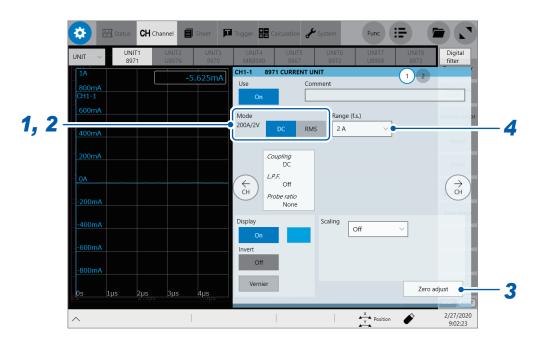

1 Confirm the output rate displayed in the [Mode] area.

The instrument automatically recognizes a current sensor connected to Model 8971 Current Unit and displays it as follows:

20A/2V [∅]	When one of the following current sensors is connected: Models 9272-10 (20 A range), 9277, and CT6841.
200A/2V	When one of the following current sensors is connected: Models 9272-10 (200 A range), 9278, CT6843, and CT6863.
50A/2V	When Model CT6862 AC/DC Current Sensor is connected
500A/2V	When one of the following current sensors is connected: Models 9279, 9709, CT6844, CT6845, CT6846*, and CT6865*.
None	When no current sensor is connected.

IMPORTANT

*: When Model CT6846 or Model CT6865 connects to Model 8971 Current Unit via Model 9318 Conversion Cable, the instrument recognizes the sensor as a 500 A AC/DC sensor. Set the conversion ratio at 2.00 in the scaling setting.

2 In the [Mode] area, tap the [DC] or [RMS] to choose a measurement mode.

DC [⊠]	For current measurement
RMS	For RMS measurement

3 (When you have changed the measurement mode) Tap [Zero adjust].

The instrument performs zero-adjustment. Execute zero-adjustment without any input.

4 Tap the [Range (f.s.)] box, and then choose a measurement range from the list.


You can choose a measurement range from among the options, which have been scaled for the current sensor detected automatically.

IMPORTANT

The figure of each measurement range name represents the maximum current that Model 8971 can measure using the range. However, the instrument cannot measure currents that exceed the rated current of a connected current sensor. Check the specifications of the current sensor used.

Configuring Model 8972 DC/RMS Unit settings



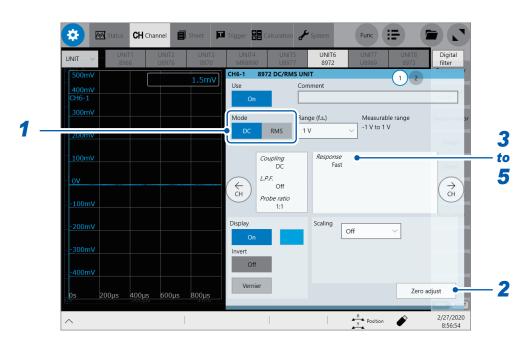

1 In the [Mode] area, tap the [DC] or [RMS] to choose a measurement mode.

DC ^ℤ	For voltage measurement
RMS	For RMS measurement

- 2 (When you have changed the measurement mode) Tap [Zero adjust]. The instrument performs zero-adjustment. Execute zero-adjustment without any input.
- **3** Tap the area that includes [Response]. The setting dialog box appears.

The setting dialog box appears.

4 Tap the [Response] box, and then from the list, choose a response time for RMS measurement.

Fast [⊠]	Sets the response time to about100 ms.
Normal	Sets the response time to about 800 ms.
Slow	Sets the response time to about 5 seconds.


Usually, choose [Fast]. Setting the response time to [Normal] or [Slow] can stabilize the measured values if the frequency is relatively low or the voltage fluctuates severely.

5 Tap [Close].

The setting dialog box closes.

Configuring Model MR8990 Digital Voltmeter Unit settings



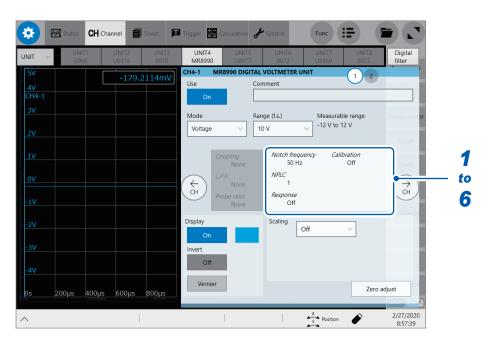

1 Tap the area that includes [Notch frequency].

The setting dialog box appears.

2 Tap the [Notch frequency] box, and then choose a power frequency from the list. Choose a power frequency of your region.

50 Hz [⊠]	Sets the period to 20 ms.
60 Hz	Sets the period to 16.67 ms.

An incorrect power frequency setting causes measured values to be unstable.

3 Tap the [NLPC] box, and then enter an integration time.

Define an integration time based on the power line cycle (PLC), which is the time equivalent to one period of the power frequency.

0.1 to 0.9, 1^{III}to 10, 20, 30, 40, 50, 60, 70, 80, 90, 100

Example: When the power frequency is 50 Hz and NPLC is set at 10, the integration time is calculated to be 200 ms (= 20 ms × 10).

The instrument updates waveform data every 200 ms.

4 Tap the [Response] box, and then choose a data update interval from the list.

Off [⊠]	Updates data at intervals of the integration time entered in the [NPLC] box.
On	Updates the data at high speed by calculating moving averages. • Updates data at intervals of 0.1 PLC when NPLC is set at 9 or less. • Updates data at intervals of 1 PLC when NPLC is set at 10 or more.

5 Tap the [Calibration] box, and then choose a calibration setting from the list.

Enabling this setting automatically calibrates the module or synchronizes the channels at the start of measurement. The synchronization between channels allows integration calculations to synchronize with each other.

Off [™]	Does not calibrate the module nor synchronize the channels.
On	Calibrates the instrument and synchronizes the channels.
Synchronization	Only synchronizes the channels.

- It takes about 150 ms to calibrate the module. The instrument cannot measure any input signals during calibration.
- If the channels are synchronized, the instrument sends a signal that interrupts the integration to each module at the start of measurement; thus, the instrument has to wait until the first integration finishes. The wait time required for this process stands at the sum of 10 ms and integration time*.
 - *: The integration time varies depending on the NPLC setting.

Even when synchronization is not performed, the wait time described above is required for measurement performed immediately after the settings of Model MR8990 Digital Voltmeter Unit has been changed. No wait time is required when the measurement is performed without any setting changes


• When [Calibration] is set to [Off] (default setting), execute calibration manually. See "2.12 Executing Calibration (For the Instrument With Model MR8990 Installed)" in the Quick Start Manual.

6 Tap [Close].

The setting dialog box closes.

Configuring Model U8974 High Voltage Unit settings



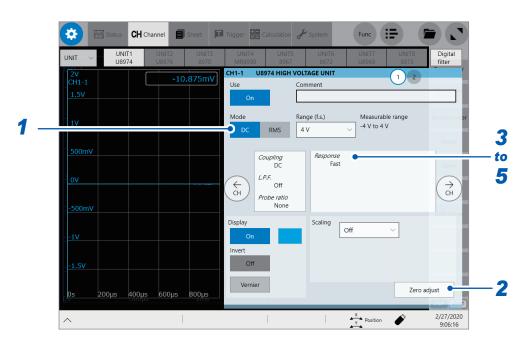

1 In the [Mode] area, tap the [DC] or [RMS] to choose a measurement mode.

DC [⊠]	For voltage measurement
RMS	For RMS measurement

- 2 (When you have changed the measurement mode) Tap [Zero adjust]. The instrument performs zero-adjustment. Execute zero-adjustment without any input.
- **3** Tap the area that includes [Response]. The setting dialog box appears.
- **4** Tap the [Response] box, and then from the list, choose a response time for RMS measurement.

Fast [⊠]	Sets the response time to 150 ms.
Normal	Sets the response time to 500 ms.
Slow	Sets the response time to 2.5 seconds.

Setting the response time to **[Slow]** can stabilize measured values if frequency is relatively low or voltage fluctuates severely.

5 Tap [Close].


The setting dialog box closes.

Configuring Model U8977 3CH Current Unit Settings

Each of Model 9709, Model CT6860 series, and Model CT6840 consists of a current sensor with the sub model-number "-05," which has a metal connector, and that without the sub model-number "-05," which has a black plastic connector.

You can directly connect a current sensor that has the sub model-number "-05," which has a metal connector, with Model U8977 3CH Current Unit. Using Model CT9900 Conversion Cable, you can connect a current sensor without the sub model-number "-05," which has a black plastic connector, to Model U8977 3CH Current Unit.

> [Channel] > [U8977]

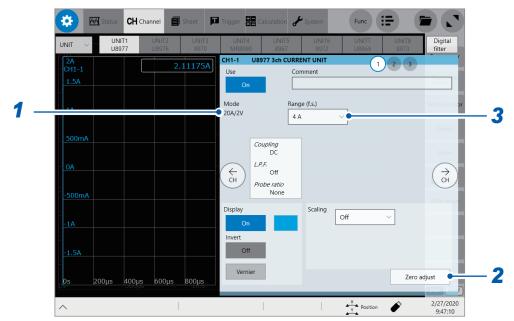

Current sensors to be connected determine whether the instrument automatically recognizes mode or whether you have to choose a current sensor setting.

1 (When the instrument automatically recognizes the sensors connected) Confirm the output rate displayed in the [Mode] area.

Available measurement ranges, which depend on automatically recognized output rates, are as follows:

2A/2V	200 mA, 400 mA, 1 A, 2 A, 4 A, 10 A
20A/2V	2 A, 4 A, 10 A, 20 A, 40 A, 100 A
50A/2V	4 A, 10 A, 20 A, 40 A, 100 A, 200 A
200A/2V	20 A, 40 A, 100 A, 200 A, 400 A, 1000 A
500A/2V*	40 A, 100 A, 200 A, 400 A, 1000 A, 2000 A
1000A/2V	100 A, 200 A, 400 A, 1000 A, 2000 A, 4000 A
2000A/2V	200 A, 400 A, 1000 A, 2000 A, 4000 A, 10000 A
None	When no current sensor is connected.

*: When Model CT6846 or Model CT6865 connects via Model CT9900 Conversion Cable, the instrument recognizes the sensor as a 500 A AC/DC sensor. Set the conversion ratio at 2.00 in the scaling setting.

(When you have to choose a current sensor setting) Tap the [Mode] box, and then choose a connected current sensor.

Available measurement ranges, which depend on chosen current sensors, are as follows:

CT7631/CT7731	200 A
CT7636/CT7736	200 A, 400 A, 1000 V
CT7642/CT7742	2000, 4000
CT7044/CT7045/ CT7046	2000, 4000, 10000
0.1mV/A	2000, 4000, 10000, 20000, 40000, 100000
1mV/A	200, 400, 1000, 2000, 4000, 10000
10mV/A	20, 40, 100, 200, 400, 1000
100mV/A	2, 4, 10, 20, 40, 100
1000mV/A	0.2, 0.4, 1, 2, 4, 10

IMPORTANT

When a current sensor included in Model CT6700 series connects via Model CT9920 Conversion Cable, set a current sensor model name or its output rate.

2 (When you have changed the measurement mode) Tap [Zero adjust].

The instrument performs zero-adjustment. Execute zero-adjustment without any input.

3 Tap the [Range (f.s.)] box, and then choose a measurement range from the list.

The instrument automatically configures the scaling setting for a measurement range according to a recognized current sensor.

IMPORTANT

The figure of each measurement range name represents the maximum current that Model U8977 can measure using the range. However, the instrument cannot measure currents that exceed the rated current of the connected current sensor. Check the specifications of the current sensor used.

Configure Model U8979 Charge Unit Settings

This setting allows you to choose between voltage measurement and acceleration measurement (charge-output or built-in pre-amplifier) for a channel.

[Voltage] mode and [Preamp] mode use BNC connectors, whereas [Charge] mode uses miniature connectors.

A channel can measure either one of them.

Model U8979 can automatically recognize TEDS-compliant* sensors.


*: Transducer electronic data sheet



1

Setting the measurement mode to [Preamp] allows Model U8979 Charge Unit to constantly provide power (3.0 mA, 22 V) to sensors. Set any measurement mode other than [Preamp] or tum off the instrument before connecting a sensor or probe with a BNC terminal to avoid an electric shock or damage to the measurement target.

> [Channel] > [U8979]

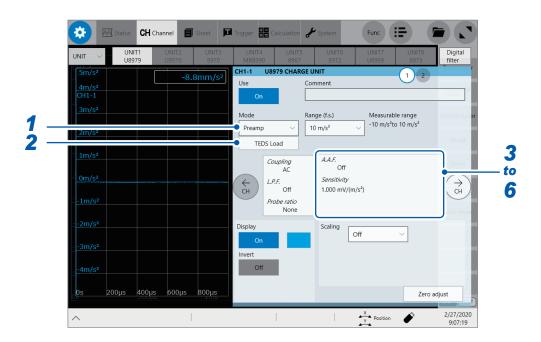

Tap the [Mode] box, and then choose a measurement mode from the list.

Mode	Measurement target	Measurement sensitivity
Voltage	Voltage	-
Charge [⊠]	Charge-output acceleration sensor	0.1 pC/(m/s ²) to 10 pC/(m/s ²)
Preamp	Acceleration sensor with a built-in pre- amplifier	0.1 mV/(m/s ²) to 10 mV/(m/s ²)

2 (When setting mode to [Preamp]) Tap [TEDS Load].

Acquires sensitivity of a connected sensor. However, the instrument can acquire sensitivity of TEDS-compliant acceleration sensors with a built-in pre-amplifier only.

When sensor sensitivity has been acquired, it is automatically set.

3 Tap the area that includes [A.A.F].

The setting dialog box appears.

4 Tap the [A.A.F.] box, and then choose a anti-aliasing filter setting from a list.

The anti-aliasing filter can prevent aliasing distortion that may be produced during FFT calculation. The cutoff frequency automatically changes according to the sampling rates or frequency range (for the FFT function) settings.

Off	Disables the anti-aliasing filter.
On	Enables the anti-aliasing filter. (Disabled when the external sampling is used, or the sampling rate is set at 100 kS/s or faster)

5 Tap [Sensitivity] box, and then enter sensor sensitivity.

You can enter sensor sensitivity to two decimal places. For a charge-output acceleration sensor or non-TEDScompliant sensor, enter its sensitivity marked on the sensor, which represents sensitivity per meter per second squared.

6 Tap [Close].

The setting dialog box closes.

Setting example for sensor sensitivity

Example 1

For a sensor with its sensor sensitivity per meter per second squared marked

Sensor sensitivity	(setting value)
1.08 pC/(m/s ²)	1.08

Example 2

For a sensor with its sensor sensitivity per gee (G) marked.

For a sensor with its sensitivity marked, enter a quotient of the marked sensitivity divided by 9.8 m/s^2 .

Sensor sensitivity	(setting value)
For sensor sensitivity of 64 pC/G 64.0 / 9.8 = 6.53061 pC/(m/s ²)	6.531 (to two decimal places)

To convert a unit from meter per second squared into gee (G)

The instrument measure charge quantities per meter per second squared. You can convert such charge quantities into those per gee (G) using the scaling function. See "3.2 Converting Input Values (Scaling Function)" (p. 56).

See 3.2 Converting input values (Scaling Function) (p.

Configure the scaling setting as follows;

Example 1

Specifying a conversion ratio

Ratio	0.1020E+00 (= 1/9.8)
Offset	0.0000E+00
Units	G

Example 2

Specifying two points

Input1	9.8000E+00	Scale1	1.0000E+00
Input2	0.0000E+00	Scale2	0.0000E+00
Units	G		

When using an out-of-setting-range current sensor

You can use an out-of-setting-range current sensor using the scaling function. See "Automatically saving waveform data" (p. 120).

1 Tap the area that includes [Sensitivity].

The setting dialog box appears.

2 Tap [Sensitivity] box, and then enter sensor sensitivity.

Multiply the sensor sensitivity of a sensor to be used by a certain value to allow a product to fall within the setting range (0.1 to 10), and enter the product.

3 Tap [Close].

The setting dialog box closes.

4 Tap the [Scaling] box, and then configure the scaling setting.

Configure the scaling setting so that a scaling ratio is the same value as the number you multiplied the sensor sensitivity by.

Example 1

For sensor sensitivity of 23.4 pC/(m/s²)

Specify 10 pC/(m/s²), which results from multiplying the sensor sensitivity by 1/2.34, as the sensor sensitivity. To display measured values after multiplying them by 1/2.34, configure the scaling setting as follows:

To configure the scaling setting using the conversion ratio method

Ratio	0.4274E+00 (= 10/23.4)
Offset	0.0000E+00
Units	m/s ²

To configure the scaling setting using the 2-point method

Input1	2.3400E+00	Scale1	1.0000E+00
Input2	0.0000E+00	Scale2	0.0000E+00
Units	m/s ²		

Example 2

For sensor sensitivity of 0.05 pC/(m/s²)

Specify 0.1 pC/(m/s²), which results from multiplying the sensor sensitivity by two, as the sensor sensitivity. To display measured values after multiplying them by two, configure the scaling setting as follows:

To configure the scaling setting using the conversion ratio method

Ratio	2.0000E+00 (= 0.1/0.05)
Offset	0.0000E+00
Units	m/s ²

To configure the scaling setting using the 2-point method

Input1	0.0500E+00	Scale1	1.0000E+00
Input2	0.0000E+00	Scale2	0.0000E+00
Units	m/s ²		

3.8 Configuring Generator Module-Specific Settings


This section describes how to configure settings related to the MR8790 Waveform Generator Unit, MR8791 Pulse Generator Unit, and U8793 Arbitrary Waveform Generator Unit.

Generating signals from Model MR8790 Waveform Generator Unit

For detailed information, see the Instruction Manual that came with the U8793, MR8790, and MR8791.

This section describes how to configure sync control and set the configuration method for signals generated by the MR8790 Waveform Generator Unit.

> [Channel] > [MR8790]

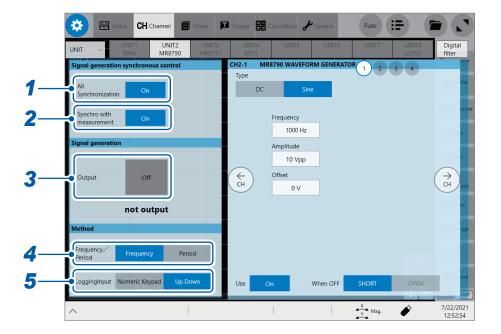

1 Tap the [All Synchronization] button and set it to [On] or [Off].

On	Controls signal generation for all units and channels simultaneously.
Off [∅]	Controls signal generation for channels set on this screen only.

2 Tap the [Synchro with measurement] button and set to [On] or [Off].

On	Synchronizes signal output with measurement start and stop events. Signal output will start when measurement starts and stop when measurement stops.	
Off [⊠]	Disables synchronization of signal output with measurement start and stop events. Signal generation must be controlled manually.	

3 Tap the [Output] button and set it to [On] or [Off].

On	Generates the signal.
Off [⊠]	Stops the signal.


4 Tap [Frequency] or [Period] and select the signal configuration method.

Frequency [™]	Use the frequency.
Period	Use the period.


5 Tap [Numeric Keypad] or [Up Down] to select how to enter values.

Numeric keypad [⊠]	Enter numerals using the numeric keypad.
Up Down	Enter numerals using the "Up" and "Down" buttons.

Numeric keypad




Up/down keys



Configuring Model MR8790 Waveform Generator Unit settings

This section describes how to configure MR8790 Waveform Generator Unit settings.



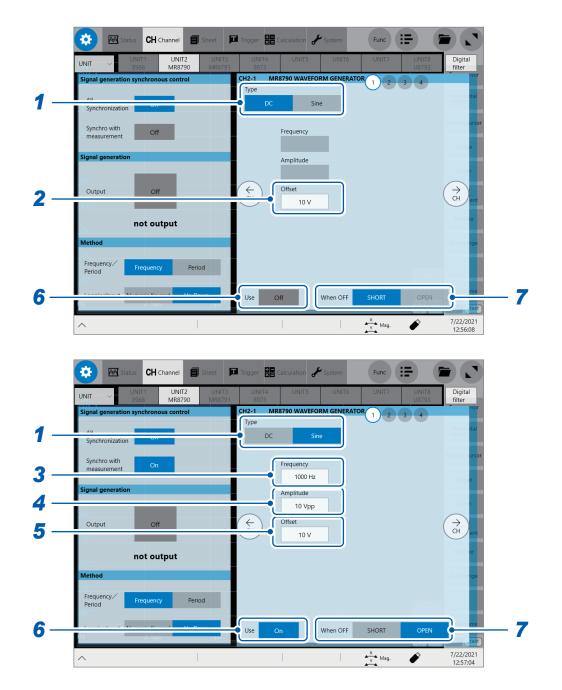

1 Tap the [Type] button and select the waveform type.

DC [⊠]	DC output
Sine wave	Sine wave output

2 (For DC output) Tap the [Offset] box and enter the output voltage.

-10.000 V to +10.000 V

3 (For sine wave output) Tap the [Frequency] box and enter the frequency.

0 Hz to 20000 Hz

4

(For sine wave output) Tap the [Amplitude] box and enter the amplitude.

Accuracy of output voltages (obtained by adding the offset to the amplitude) is guaranteed within the following range: -10 V to +10 V.

If the value obtained by adding the offset to the amplitude exceeds the accuracy guarantee range, output waveforms will be clamped to an upper limit of approximately +14 V and a lower limit of approximately -14 V.

0.000 Vpp to 20.000 Vpp

5 (For sine wave output) Tap the [Offset] box and enter the offset voltage.

Accuracy of output voltages (obtained by adding the offset to the amplitude) is guaranteed within the following range: -10 V to +10 V.


If the value obtained by adding the offset to the amplitude exceeds the accuracy guarantee range, output waveforms will be clamped to an upper limit of approximately +14 V and a lower limit of approximately -14 V.

-10.000 V to +10.000 V

6 (If [All Synchronization] is On) Tap the [Use] button to set output for each channel to [On] or [Off].

On	Generates output from this channel.
Off [∅]	Does not generate output from this channel.

7 Tap the [When OFF] button and select the pin state when not outputting a waveform.

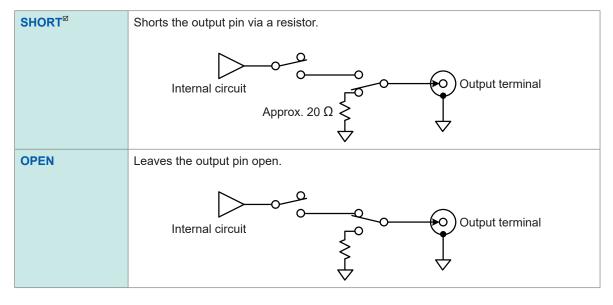


Generating signals from Model MR8791 Pulse Generator Unit

For detailed information, see the Instruction Manual that came with the U8793, MR8790, and MR8791.

This section describes how to configure sync control and set the configuration method for signals generated by the MR8791 Pulse Generator Unit.

> [Channel] > [MR8791]

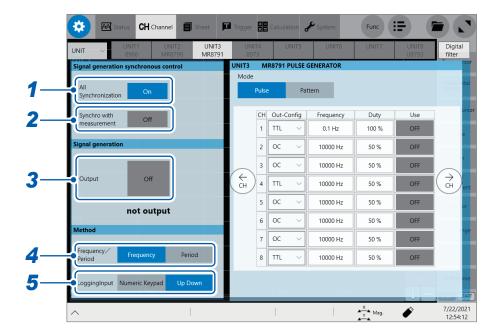

1 Tap the [All Synchronization] button and set it to [On] or [Off].

The MR8791 Pulse Generator Unit can be used by setting [All Synchronization] to On.

On	Controls signal generation for all units and channels simultaneously.
Off [∅]	Controls signal generation for channels set on this screen only.

2 Tap the [Synchro with measurement] button and set to [On] or [Off].

On	Synchronizes signal output with measurement start and stop events. Signal output will start when measurement starts and stop when measurement stops.
Off [⊠]	Disables synchronization of signal output with measurement start and stop events. Signal generation must be controlled manually.

3 Tap the [Output] button and set it to [On] or [Off].

On	Generates the signal.
Off [☑]	Stops the signal.


4 Tap [Frequency] or [Period] and select the signal configuration method.

Frequency [⊠]	Set by frequency.
Period	Set by period.


5 Tap [Numeric Keypad] or [Up Down] to select how to enter values.

Numeric keypad [⊠]	Enter numerals using the numeric keypad.
Up Down	Enter numerals using the "Up" and "Down" buttons.

Numeric keypad




Up/down keys



Configuring Model MR8791 Pulse Generator Unit settings

This section describes how to configure MR8791 Pulse Generator Unit settings.

> [Channel] > [MR8791]

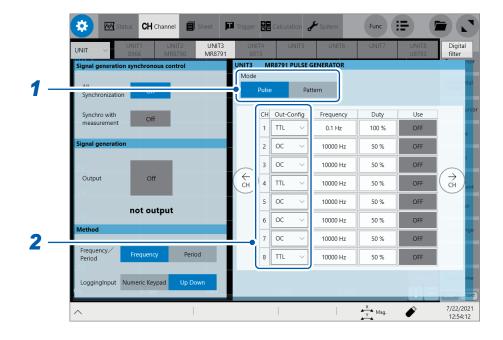

1 Tap the [Mode] button and select the output waveform type.

Pulse	Pulse output
Pattern [⊠]	Pattern output

2 Tap the [Out-Config] box and select the output configuration.

TTL	TTL (amplitude 0 to 5 V) output
OC⊠	Open collector output

Channels share the same ground and are not isolated.


When using open collector output

• Set the voltage applied between the collector and emitter to 50 V or less.

- Response time (10% to 90%): Max. approx. 5 μs (reference value: with a load capacitance of 1000 pF and pull-up resistance of 1 k $\Omega)$

Pulse output settings

If you set the output type to [Pulse], configure the following settings:

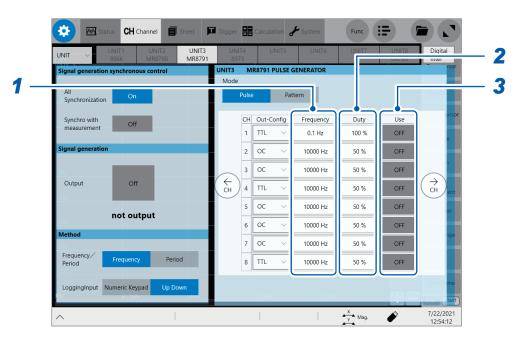

1 Tap the [Frequency] box and enter the frequency (in 0.1 Hz increments).

0 Hz to 20000 Hz

2 Tap the [Duty] box and enter the duty ratio (in 0.1% increments).


0% to 100%

- The output signal will be set to L level when set to 0% and to H level when set to 100%, causing no pulse to be output.
- When set to 100%, an H level signal will be output, even if the output setting is off.
- The pulse may disappear if the output pulse width is less than 1 µs as a result of the frequency and duty ratio settings.
- **3** Tap the [Use] button and set pulse output to [On] or [Off].

On	Outputs a pulse.
Off ^ℤ	Does not output a pulse.

Pattern output settings

If you set the output type to [Pattern], configure the following settings:

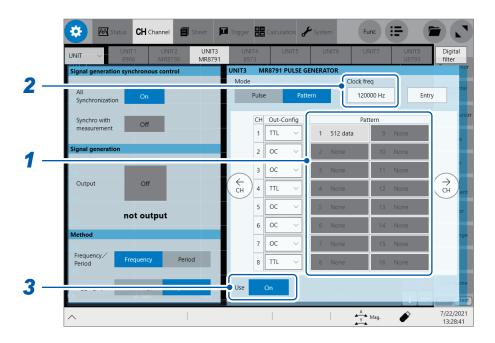

1 Tap the pattern you wish to use to select it.

If output is in the stopped state, the registered pattern's initial pattern will be output. Pattern data will be cleared when the instrument is turned off. Register pattern data again after turning the instrument on.

2 Tap the [Clock freq] box and enter the clock frequency (in 10 Hz increments).

0 Hz to 120000 Hz


3 (If [All Synchronization] is On) Tap the [Use] button to set output for each channel to [On] or [Off].

On	Generates output from this channel.			
Off [⊠]	Does not generate output from this channel.			

Pattern registration

Before performing this procedure, insert recording media containing the pattern data (with the extension .pls).

Up to 16 sets of pattern data can be registered.

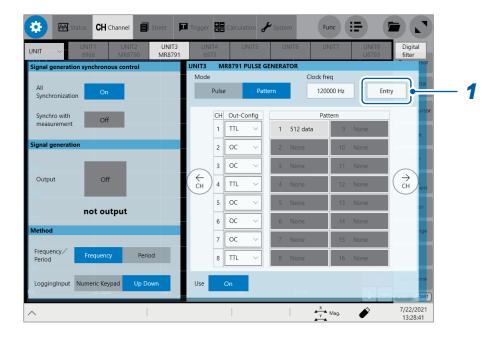

1 Tap [Entry].

A window will open allowing you to select a file.

	Open			×
	← → • ↑ <mark> </mark> «	HIOKI_MR6000 → GEN v Ö	Search GEN	Q
	Organize 👻 New fo			2
2—	This PC Desktop Documents Downloads Music Pictures	Name DAT1.pls DAT32.pls DAT512.pls DAT5048.pls	8/18/2021 1:04 PM 8/5/2021 12:58 PM 8/5/2021 1:01 PM	Type PLS File PLS File PLS File PLS File
	Videos Windows (C:) Volume (D:) USB Drive (E:) USB Drive (E:)			
		e <u>n</u> ame: v	All files (*.PLS) Open Canc	el

2 Select the file you wish to register.

The [Entry from File] dialog box will be displayed.

	Entry from File
	File name
	DAT2048.pls
2	Pattern No.
3-	Pattern2 None V
	Samples
	2048
4—	OK Cancel

- **3** Tap the [Pattern No.] box and select a pattern.
- **4** Tap [OK] to register the pattern.

Tap [Cancel] to close the dialog box without registering the pattern.

Generating signals from Model U8793 Arbitrary Waveform Generator Unit

For details, see the Instruction Manual that came with the U8793, MR8790, and MR8791. This section describes how to select the Arbitrary Waveform Generator Unit's output synchronization control and setting method.

> [Channel] > [U8793]



1 Tap the [All Synchronization] button to set it to [On] or [Off].

On	Controls the signal generation of all modules' all channels simultaneously.
Off [⊠]	Controls the signal generation of the channels only set on this screen.

2 Tap the [Synchro with measurement] button to set it to [On] or [Off].

On	Synchronizes signal outputting with the start/stop of measurements. The signals outputs and stops respectively in sync with the the start and stop of measurements.
Off [⊠]	Does not synchronize signal outputting with the start/stop of measurements. You can manually control signal outputting.

3 Tap the [Output] button to set it to [On] or [Off].

On	Outputs the signals.				
Off⊄	Stops outputting the signals.				


4 Tap [Frequency] or [Period] to set what parameter is used to set the oscillation speed.

Frequency [⊠]	Uses the frequency.
Period	Uses the period.


5 Tap [Numeric Keypad] or [Up Down] to choose a way of entering values.

Numeric Keypad [⊠]	Lets you use the numerical key pad.			
Up Down	Lets you use the Up Arrow and Down Arrow keys.			

Key pad



Up Arrow and Down Arrow keys



98

Configuring Model U8793 Arbitrary Waveform Generator Unit

This section describes how to configure the settings specific to the U8793 Arbitrary Waveform Generator Unit.



> [Channel] > [U8793]



List of parameters than can be displayed and set.

						✓: Displ	ayed, –: No	ot displayed
Туре	DC	Sine	Square	Pulse	Triangle	Ramp- Up	Ramp- Down	Arbitrary
Frequency or Period 0.00 to 100,000.00 (Hz) 0.00 to 100.00 (s)	_	~	~	~	~	~	~	_
Clock frequency or Clock period 0.00 to 20,000,000.00 (Hz) 0.00 to 100.00 (s)	_	_	_	_	_	_	_	~
Amplitude 0.000 to 20.000 (Vpp)	_	~	~	~	~	~	~	_
Amp. Adjust. 0.000× to 2.000×	-	_	_	_	-	_	_	~
Offset −10.000 to 15.000 (V)	\checkmark	~	~	~	~	~	~	~
Duty 0.1 to 99.9 (%)	_	_	_	~	_	_	_	-
Phase −360.0 to 360.0 (°)	_	~	~	~	~	~	~	_
Delay −250000 to 250000 (Can be set in the number of samples)	_	_	_	_	_	_	_	~

✓: Displayed, –: Not displayed

Туре	DC	Sine	Square	Pulse	Triangle	Ramp- Up	Ramp- Down	Arbitrary
Loop times 1 to 50000 (Infinity when set to zero)	_	_	_	_	_	-	-	~
Filter	_	-	_	-	_	-	-	~
Sweep (On/Off)	_	~	~	~	~	~	~	~
Sweep time 10 μ to 1000 (s)	_	\checkmark	\checkmark	\checkmark	~	\checkmark	\checkmark	~

• See "Editing programs of Model U8793 Arbitrary Waveform Generator Unit" for the [Program] settings.

• The least significant digit displayed in the valid setting range indicates the setting resolution.

Туре	Function
DC	Outputs a DC signal.
Sine	Outputs a sine wave.
Square	Outputs a square wave with a duty ratio of 50%.
Pulse	Outputs a pulse wave with a previously set duty ratio.
Triangle	Outputs a triangular wave.
RampUp	Outputs a ramp-up wave.
RampDown	Outputs a ramp-down wave.
Arbitrary	Outputs a created arbitrary wave. See "Registering arbitrary waveforms in the U8793 Arbitrary Waveform Generator Unit" (p. 102).
Program	Outputs a waveform according to a previously edited program. See "Editing programs of Model U8793 Arbitrary Waveform Generator Unit" (p. 107).

Parameter	Function		
Frequency	Allows you to enter the frequency or period of the output waveform.		
Clock frequency	Allows you to enter the frequency or period if you chose the arbitrary waveform setting.		
Amplitude	Allows you to enter the amplitude of the output waveform.		
Amp. Adjust.	Allows you to adjust the amplitude if you chose the arbitrary waveform setting.		
Offset	Allows you to enter the offset voltage of the output waveform. Allows you to enter the DC voltage if you chose the DC voltage setting.		
Duty	Allows you to enter the duty ratio if you chose the pulse wave setting.		
Phase	Allows you to enter the phase.		
Delay	Allows you to enter the delay time if you chose the arbitrary waveform setting.		
Loop times	Allows you to enter the number of looping times if you chose the arbitrary waveform setting. If you enter zero, the instrument displays the sign [∞] and continues outputting the signal repeatedly until you stop the output. The [Loop times] setting cannot be configured if the [Sweep] is set to [On].		
Filter	Allows you to choose the frequency used to filter the arbitrary waveform.		
	Off ^፼ , 50, 100, 200, 500, 1 k, 2 k, 5 k, 10 k, 20 k, 50 k, 100 k, 200 k, 500 k, 1M [Hz]		

Parameter	Function		
Sweep	Allows you to set the sweep function to on or off. You can set multiple parameters to on. However, either the frequency sweep or the duty ratio sweep, but not both, can be set to on.		
Sweep time	Allows you to set the sweeping time. Every parameter uses the common sweeping time.		
Use	This setting will appear when the [All Synchronization] has been set to [On].		
	On	Uses the channel as the output target.	
	Off [⊠]	Does not use the channel as the output target.	
When OFF	Allows you to choose an option used when the output is set to off.		
	SHORT ^I	Short-circuits the output terminal.	
	OPEN	Opens the output terminal.	

Registering arbitrary waveforms in the U8793 Arbitrary Waveform Generator Unit

. . .

This section describes how to register, display, and delete arbitrary waveform data.

> [Channel] > [U8793]




Display	Displays the arbitrary waveform data set chosen from among registered data sets. Tap to choose or check the registered arbitrary waveform data sets.		
Remove	Deletes the chosen arbitrary waveform data set. When the U8793 contains eight registered waveforms, delete any one of them before registering a waveform.		
Enty	Registers the arbitrary waveform in a vacant number (up to eight waveforms). It will take about 40 s to register a waveform consisting of 250,000 samples.		
	WAVE [∅]	Registers the waveform data the instrument has acquired. See "To resister the arbitrary waveform using measured data" (p. 103).	
	FILE	Reads the waveform data from a file and registers it. See "To resister the arbitrary waveform using a file" (p. 104).	
Save	Press the SAVE key to save arbitrary waveform data registered in the U8793 as files. See "Freely choosing data items to be saved and save files (SAVE key)" (p. 127).		

Initializing the instrument will not cause loss of registered waveform data.

To resister the arbitrary waveform using measured data


> [Channel] > [U8793]

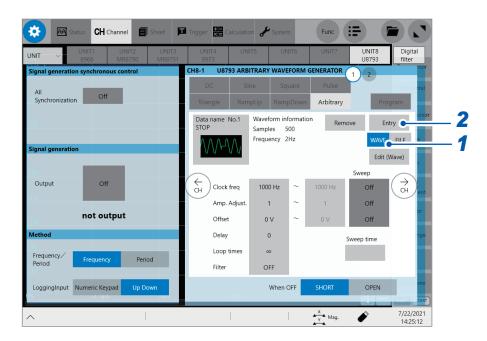

1 Tap [WAVE].

2 Tap [Entry].


The [Entry from Measured] dialog box appears.

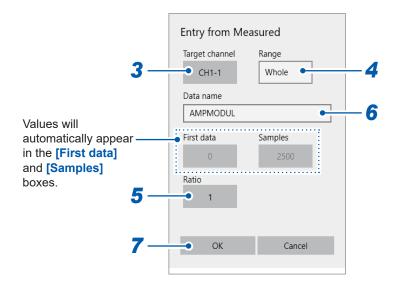

- **3 Tap the [Target channel] button to choose a channel you wish to register.** You can choose a channel to register from internal modules and waveform-calculation channels.
- **4** Tap the [Range] box, and then from the list, choose a registration range option.

Whole[⊠], Segment 1, Segment 2

Values will appear based on the specified range in [First data] and [Samples]. If you wish to register the measured data partly, specified the range to register by using [Section cursor]. See "2.2 Specifying the Waveform Range (Section Cursor)" (p. 35).




6 Enter a data name in the [Data name] box.

A data name can be up to 16 characters long. If you enter the name same as a registered data, the existing data will be overwritten.

7 Tap [OK].

To resister the arbitrary waveform using a file



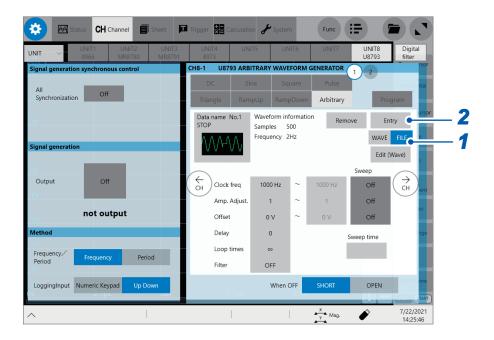

1 Tap [FILE].

2 Tap [Entry].

The file selection screen appears.

$\leftarrow \rightarrow \checkmark \uparrow$ $\blacksquare \Rightarrow$ (E:) \Rightarrow SF8000 \Rightarrow WFG $\checkmark \downarrow$	ි Search WFG 🔎
Organize 👻 New folder	III 🔻 🔟 📀
United Street Downloads	Date modified Type
Music HARMO49D.wfg	8/26/2020 9:30 AM WFG File
Videos isin.wfg Windows (C:) istep6.wfg Volume (D:) STOP.wfg	8/28/2015 6:05 PM WFG File 8/26/2020 9:29 AM WFG File 2/9/2021 10:08 AM WFG File
(E:) USB (F:)	
(E:) HIOKI_MR6000	
LOST.DIR	
SF8000 < <	>
File name:	All files (*.WFG;*.TFG)

3 Choose a file you wish to register (*.WFG, *.TFG, *.CSV, or *.TXT).

4 Tap [Open].

The [Enter from File] dialog box appears.

Values will automatically appear- in the [File name] and [Samples] boxes.	Entry from File File name HARMO49D.wfg Data name HARMO49D Samples		5
6 —	ок	Cancel	

5 Enter a data name in the [Data name] box.

A data name can be up to 16 characters long. If you enter the name same as a registered data, the existing data will be overwritten.




Editing arbitrary waveforms for Model U8793 Arbitrary Waveform Generator Unit

This section describes how to edit arbitrary waveforms using the SF8000 Waveform Maker software.

You must first install the SF8000 software.


See "Installing Model SF8000 Wave Marker software" (p. 110).

> [Channel] > [U8793]

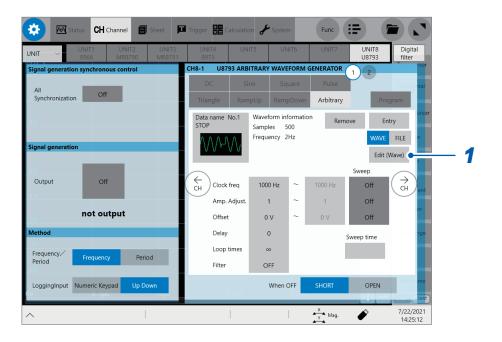

1 Tap [Edit (Wave)].

The SF8000 software will launch. Edit and save an arbitrary waveform. For more information about how to use the SF8000, see the Instruction Manual that came with the U8793, MR8790, and MR8791.

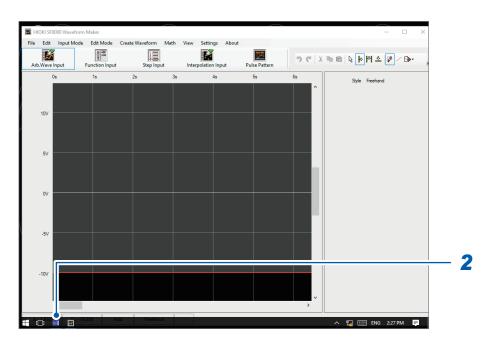

2 Tap the blue icon at the bottom left corner of the screen. The screen returns to the MR6000 software.


Editing programs of Model U8793 Arbitrary Waveform Generator Unit

You can use the program function to output a waveform generated by piecing up to 128 steps together.

Setting up the whole program list

This section describes how to load and edit a program list and configure the whole program list.

> [Channel] > [U8793]

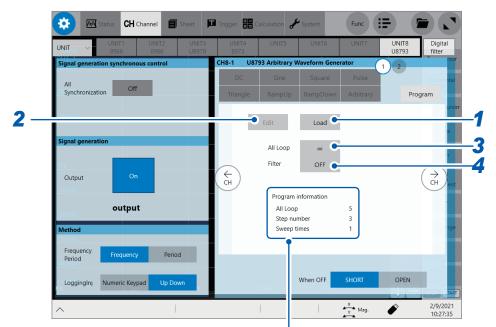

Displays the looping count, step number, and sweeping count of the still-in-progress process. When you have set the whole looping times to infinity, the instrument will show [∞] as the entire looping count of the still-in-progress process repeating more than 50,000 times.

- **1** Tap [Load] to load a program list into the instrument.
- **2** Tap [Edit] to edit the program list with the instrument. See "Editing the program list" (p. 108).
- **3** Tap the [All Loop] button to enter the number of repetitions the whole program is executed. If you enter zero, the instrument displays the sign [∞] and continues outputting the signal repeatedly until you stop the output.


1 to 50000, ∞[⊠]

4 Tap the [Filter] button to specify a filter frequency commonly used for every step.

OFF^{III}, 50, 100, 200, 500, 1 k, 2 k, 5 k, 10 k, 20 k, 50 k, 100 k, 200 k, 500 k, 1M [Hz]

Editing the program list

You can edit and display programs with up to 128 steps. Even if resetting the instrument, you cannot delete the program list.

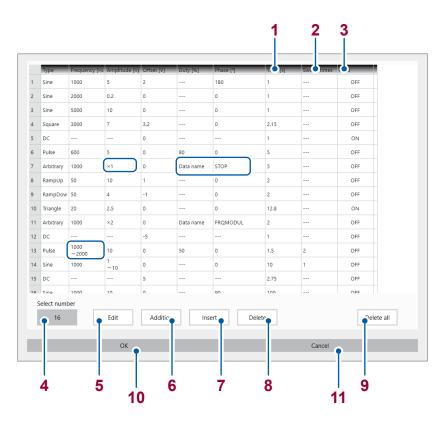

- When the [Type] is set to [Arbitrary], the clock frequency (Hz) will be displayed in the [Frequency [Hz]] column.
- When the [Type] is set to [Arbitrary], the amplitude adjustment factor, such as [×1], will be displayed in the [Amplitude [V]] column.
- When the [Type] is set to [Arbitrary], the data names, such as [Data name] and [STOP] respectively, will be displayed in the [Duty [%]] and [Phase [°]] columns.
- · Parameters whose sweep setting is set to [On] will be spread over two lines as follows:

[1000 to 2000]

No.	Element	Function
1	Time [s]	Allows you to set the generating time when the sweep is set to [Off].
		1 [™] to 1000
		Allows you to set the sweeping time when the sweep is set to [On].
		1 ^ℤ to 1000
2	Sweep times	Allows you to set the sweeping count when the sweep is set to [On].
		1 ^ℤ to 1000
3	Hold	When you set this column to [Off] , the instrument moves on to the next step after the time specified in the [Time [s]] column has elapsed. When you set this column to [On] , after the time specified in the [Time [s]] column has elapsed, the instrument continues outputting the signal while an IN signal of high level is being input into the U8793's external control terminal. It will move on to the next step when the IN signal of low level is input.

No.	Element	Function	
4	Select number	Displays the number you chose. The step will be used as the reference step to execute steps 5 through 8.	
5	Edit	Allows you to edit the chosen step.	
		Use the [Setting program step] dialog to enter parameters you wish to edit. Tap [OK] to confirm your entries by overwriting the existing step.	
		Setting program step Type Pulse Step No. 6	
		Sweep	
		Frequency 600 Hz ~ 600 Hz Off	
		Amplitude 5 Vpp \sim 10 Vpp Off Offset 0 V \sim 0 V Off	
		Duty 80 % ~ 50 % Off	
		Phase 0 *	
		Generat. Time 5 s	
		Sweep times Hold Off	
		OK Cancel	
		 When you set the [Sweep] column to [On], the dialog will display the string [Sweeping times]; when [Off], the string instead. The [Sweep times] setting cannot be configured if the [Sweep] column is set to [Off]. 	
6	Addition	Adds a step after the last step.	
7	Insert	Inserts a step before the chosen step.	
8	Delete	Deletes the chosen step.	
9	Delete all	Deletes all steps.	
10	ок	Registers the program list.	
11	Cancel	Does not update the program list. Your entry will be discarded.	

For information on other user-interface elements and their functions, see "Configuring Model U8793 Arbitrary Waveform Generator Unit" (p. 99).

Installing Model SF8000 Wave Marker software

1 Copy the SF8000 installer to a USB drive.


Copy the [setup] folder in [\SF8000\ENGLISH] on the included application disc to a USB drive.

📙 🛃 🔚 🖛 ENGLISH	I	_	
File Home Shar	e View		~ 🕐
← → ~ ↑ 📙 < SF		ch ENGLISH	
🚰 Quick access	Name	Date modified	Туре
	camnle	10/7/2021 8:57 PM	File folder
ineDrive 🍊 🗠	setup	10/7/2021 8:57 PM	File folder
This PC	08/93A981-04	10/7/2021 6:50 PM	PDF File
🥏 Network	<		•
3 items			


2 Turn on the instrument and connect the USB drive to the MR6000's USB connector.

3 Open Explorer.

- (1) Tap [Func].
- (2) Select [Explorer].

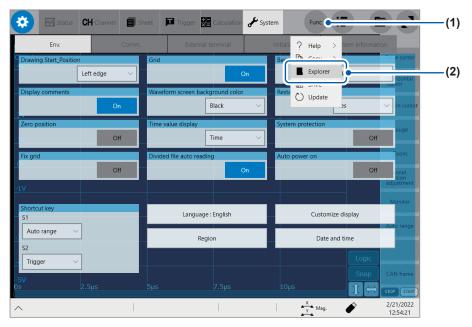

4 Execute [setup] inside the [setup] folder that you copied to the USB drive.

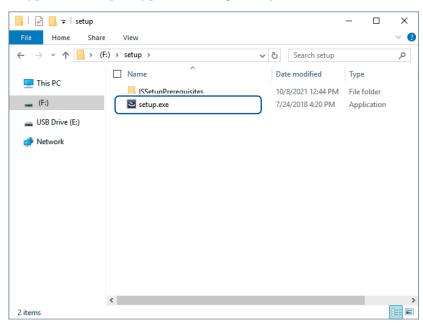

5 Tap [Next].

🖟 HIOKI SF8000 - InstallShield	Wizard X
2	Welcome to the InstallShield Wizard for HIOKI SF8000
	The InstallShield(R) Wizard will install HIOKI SF8000 on your computer. To continue, click Next.
	WARNING: This program is protected by copyright law and
	international treaties.
	< Back Next > Cancel

6 Accept the License Agreement and tap [Next].

😸 HIOKI SF8000 - InstallShield Wizard	×
License Agreement	
Please read the following license agreement carefully.	
User's License Agreement	^
Important	
Please read the following agreement carefully. This user's license agreement (hereafter referred to as Agreement) is a legal contract between the software user (individual or institution) and HIOKI E. E. CORPORATION (hereafter referred to as HIOKI). The term "software" includes any related electronic documentation and computer software and media, as well as any printed matter (such as the Instruction Manual). By installing, reproducing, or using the software, you, the Licensee, agree to	~
I accept the terms in the license agreement	
○ I do not accept the terms in the license agreement	
InstallShield	
< Back Next > Cancel	


7 Leaving the destination folder unchanged, tap [Next].

🖟 HIOKI SI	F8000 - InstallShield Wizard X
	ion Folder xt to install to this folder, or click Change to install to a different folder.
	Install HIOKI SF8000 to: C:¥Program Files (x86)¥HIOKI ¥HIOKI SF8000¥
InstallShield -	< Back Cancel

8 Tap [Install].

🖟 HIOKI SF8000 - InstallShield Wizard	×
Ready to Install the Program	
The wizard is ready to begin installation.	
If you want to review or change any of your installation settings, click Back. Click Cancel to exit the wizard.	
Current Settings:	
Setup Type:	
Typical	
Destination Folder:	
C:¥Program Files (x86)¥HIOKI¥HIOKI SF8000¥	
User Information:	
Name:	
Company:	
InstallShield	
< Back Cancel	

9 Tap [Finish].

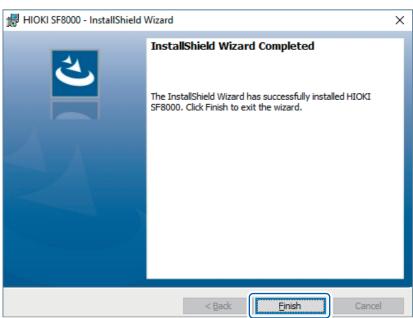

The installation is complete.

10 Tap the blue icon at the lower-left corner of the screen.

The screen goes back to the MR6000's screen.

Configuring Generator Module-Specific Settings

Saving/Loading Data and Managing Files

This chapter explains how to save and load data and manage files.

Before saving data, select [Status] > [Save], and configure the save setting.


The file screen allows you to load data.

Explorer allows you to manage files.

You can use Explorer to control filing, including copying and moving files, and to check files not supported by the instrument.

See "4.4 Managing Files" (p. 136).

> [Status] > [Save]

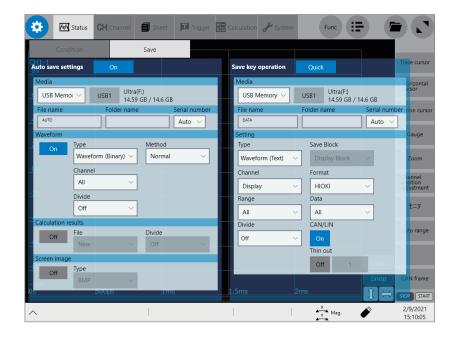

Operation available on the [Save] screen

Automatic saving

Configuring the automatic saving method settings for measured data (p. 120)

Real-time saving

Setting the method of saving waveform data in real time (p. 124)

SAVE key operation

- Setting the operation implemented when the SAVE key is pressed (p. 127)
- Specifying contents to be saved when [Quick] is selected (p. 127)

4

4.1 Data That Can Be Saved and Loaded

Data saved with another instrument cannot be loaded onto the instrument.

File Saving					✓: Enable,		
File type	format	File extension and description		Auto	Manual	Loading	Loading on a PC
Setting data*1	Binary	SET	Setting data (measurement conditions)	-	~	~	-
		MEM	Normal waveform data	✓	~	✓	- * ³
		REC	Envelope waveform data	~	~	✓	- * ³
Waveform data* ²	Binary	FLT	Waveform data in floating- point format	~	~	_	_
Data of whole waveforms acquired in	Dinary	MDF	MDF format waveform data (MDF 3.0 format)	~	~	~	~
the instrument or a part of waveforms within the range between the		MF4	MDF format waveform data (MDF 4.0 format)	~	~	~	~
section cursors	Text	CSV, TXT* ⁶	Text data	~	~	_	~
	TEXL	CFG, DAT	COMTRADE data	~	~	_	~
		IDX	Index data of the division save	~	~	~	-
Waveform managing data ^{*4} (When division save, memory division save, dual-sampling save, or CAN frame data save	(Index	SEQ	Index data of the memory division save (automatically created at a batch save)	~	~	~	_
		R_M	Index data of dual-sampling batch save	~	~	~	_
is used)		IXC	Index data when CAN frame data saved	~	~	~	-
	BMP* ⁵	BMP	Image data	~	~	_	~
Screenshot, waveform image	PNG*⁵	PNG	Image data (PNG format)	~	~	_	~
waveloini iniage	JPEG* ⁵	JPEG	Image data (JPEG format)	~	\checkmark	_	~
Numerical calculation result	Text	CSV, TXT* ⁶	Text data	~	√	-	~
CAN frame data	Binary	CLG	Saves waveform file and index file toghther.	~	~	~	_
	Text	CSV, TXT	Text data	-	~	_	~
	Binary	WFG	Arbitrary waveform data (for U8973)	-	~	~	-
Waveform generation data		TFG, CSV, TXT	Arbitrary waveform data (for U8973)	_	_	~	~
	Program	FGP	Waveform generating program data (for U8973)	-	~	~	_

116

- *1: The instrument automatically loads data at the time of startup. (p. 135)
- *2: To load data with the instrument: Save the data in binary format. Waveform data and a part of measurement settings data are saved.
 - To load data on your computer: Save the data in text format. (p. 118)

To save a part of waveforms: Specify the saving range with section cursors. (p. 30, p. 35)

*3: Data can be loaded with Wave Viewer (Wv).

*4: To load all blocks when the memory division is used Save waveform data using [All block]. The instrument automatically creates a directory, waveform data of each block, and index data (SEQ). To load waveform data of each block, load this index data. To load divided waveform data, load the index data (IDX).

*5: BMP format: This is one of the standard Windows[®] image file format. Various graphics programs can open these files.

PNG format: Internationally standardized image file format conforming to ISO/IEC15948


JPEG format: Internationally standardized image format conforming to ISO/IEC10918

*6: When you choose a separator other than [Comma ,] in [Region], files are saved with the .TXT extension. (p. 348)

4.2 Saving Data

Saving types and setting procedure

Three ways are available to save data.

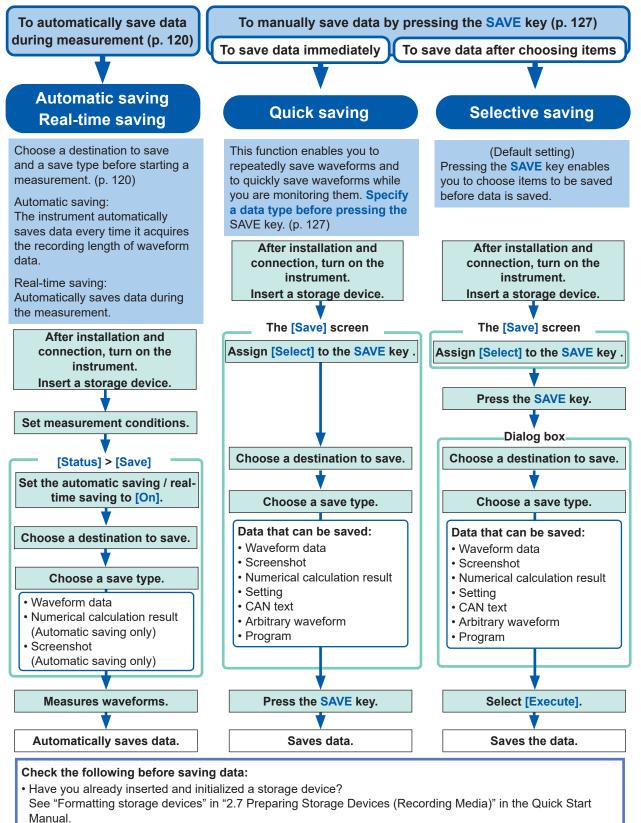


- Is the save destination specified correctly?
- When the automatic saving is used, is [Auto save settings] set to [On]?

Structure of the save destination folders

The instrument will automatically create the HIOKI_MR6000 folder immediately under the storage device and sub-folders according to saving type.

When you specified a save destination folder, the instrument will save files in the folder regardless of the file type.


Folder name	File type
WAVE	Waveform (binary), waveform (text), waveform (MDF), waveform (float), CAN text
CONFIG	Setting
MEASURE	Numerical calculation result
PICT	Sceenshots
GEN	Arbitrary waveform, program
User-definable folder	Destination location to save when specified

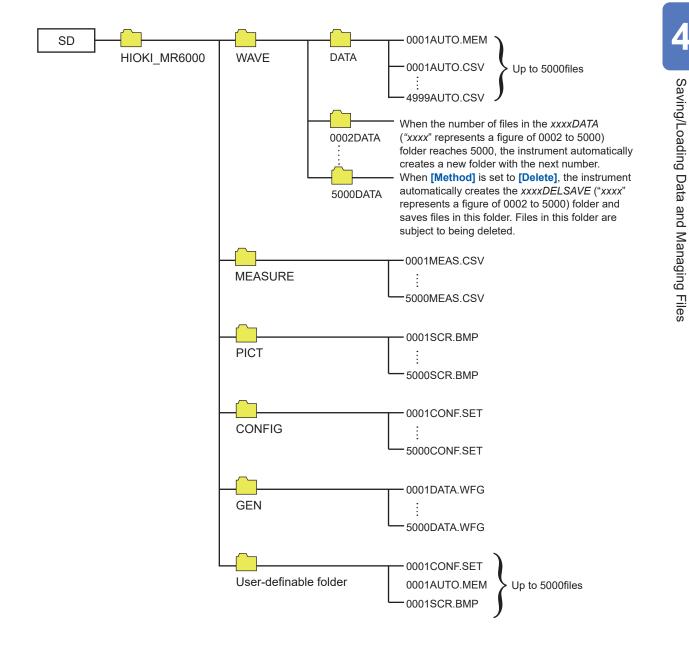

Automatically saving waveform data

The instrument automatically saves data every time it acquires a recording length of waveform data. Specify a save destination and items to be saved before starting a measurement.

> [Status] > [Save]

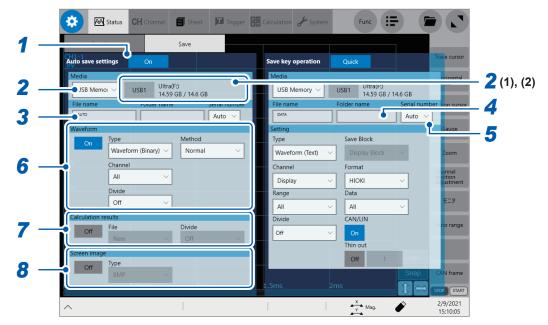

1 Tap the [Auto save settings] button to set it to [On].

2 Tap the [Media] box, and then from the list, choose a destination to save.

SSD/HDD	Saves data onto the built-in drive.
SD Card	Saves data on an SD memory card.
USB Memory [⊠]	Saves data on a USB flash drive.
Mail	Sends email messages with waveform data attached to computers in your network or to remote computers.
FTP	Sends waveform data to a computer connected to your network
Network	Saves data in a shared folder of a Windows [®] -based computer connected to your local network.

- (1) When you choose a save destination, the state of the storage device such as its drive letter and capacity appears on the right of the [Media] box. If no storage device is inserted, the string [None] appears.
- (2) When you choose [USB Memory] as the save destination, choose a USB flash drive you would like to use as a save destination from among all attached USB flash drives.
- If selecting [Network], [Mail], or [FTP], you can set a backup-file saving destination used for communication failure. When a backup is enabled, choose from SSD/HDD, SD card, and USB flash drive for the destination to save.



- If selecting [Network], configure the shared folder and network drive settings.
- See "14.7 Connecting to a Network Drive" (p. 381).When you choose [FTP], configure the LAN and FTP client function settings.
- See "Configuring the LAN settings with the instrument" (p. 351) and "14.3 Sending Data to a Computer With the FTP Client Function" (p. 359).
- For protecting data, use the following Hioki's options: Model U8332 SSD Unit, Model U8333 HD Unit, Model Z4006 USB Drive, Model Z4001 SD Memory Card (2 GB), and Z4003 SD Memory Card (8 GB).

3 Enter the file name in the [File name] box.

- Number of characters for a file name: Up to 100 characters
- The maximum length of a file name that includes its path: Up to 255 characters

4 Enter a folder name in the [Folder name] box.

If you wish to choose a destination folder, enter a folder name. If you leave the box blank, the instrument will sort files into folders based on the file type.

Folder name: up to 32 characters

5 Tap the [Serial number], and then from the list, choose a format of sequential number to be added to folder/file names.

Previous [™]	Prefixes a sequential number to each folder/file name.
Tail	Suffixes a sequential number to each folder/file name.
Auto	Saves folders/files without sequential numbers. Suffixes a sequential number to each folder/file name if a folder/file with the same name has already existed.

6 In the [Waveform] area, tap [On] or [Off] to configure the waveform save setting.

Off	Does not save any waveforms.
On	Saves waveforms.

Tap the [Type] box, and then choose a save format from the list.

Waveform (Binary) [⊠]	Saves waveform data in binary format. (Only data saved in binary format can be loaded onto the instrument)
Waveform (Text)	Saves waveform data in text format. (The instrument decimates the data and saves the remaining data as a file. The files can be opened with editors and spreadsheet software installed in computers; however, they cannot be loaded onto the instrument.)
Waveform (MDF)	Saves waveform data in MDF format. (You can use an MDF-capable waveform viewer installed in a computer to load MDF waveform data.)

Tap the [Method] box, and then from the list, choose an action to be taken if the size of waveform data to be saved exceeds the capacity of the storage device.

Normal [∅]	Stops the automatic saving if the storage device is full.
Delete	Deletes older files and continues the automatic saving even when the storage device is full (waveform files only). The instrument deletes files only created after the measurement has started. It does not delete previously existing files.

Tap the [Channel] box, and then from the list, choose an option for channels to be saved.

All	Saves data acquired across all measured channels (channels with measurement set to [On]). The instrument also saves data acquired across channels with the waveform display set to [Off].
Display	Saves data acquired across channels with the waveform display set to [On] on all sheets.

(When you choose [Waveform (Binary)] in the [Type] box) Tap the [Divide] box, and then from the list, choose a size of each file.

Off		Saves a file without dividing it.
16 MB, 32 MB, 64 MB	3	Choose this option to divide a large file into several files and save them. A file is divided into several files each of which has the specified size. The instrument creates a folder with the specified name, divides a file into several files, and then saves them in the folder.

Even if the **[Divide]** has been set to **[Off]**, the instrument automatically divides files more than 512 MB in size, which can be generated in some measurement conditions. When the instrument needs to divide a file, it automatically creates a folder to save divided files and an index file with the extension .INX. Loading the IDX file allows the waveform files to be loaded in a batch.

When using the memory division function, you cannot use the division save function.

See "Loads divided files in a batch." (p. 134) and "10 Memory Division Function" (p. 289).

(When you choose **[Waveform (Text)]** in the **[Type]** box) Tap the **[Divide]** box, and then from the list, choose an option for the number of lines of each file.

Off [∅]	Saves a file without dividing it.
60,000 data, 1,000,000 Data	Divides a file according to data points (row) you specify.

Even if the **[Divide]** has been set to **[Off]**, the instrument automatically divides files more than 512 MB in size, which can be generated in some measurement conditions.

When using the memory division function, you cannot use the division save function.

See "10 Memory Division Function" (p. 289).

(When you choose [Waveform (Text)] in the [Type] box) Tap the [Thin out] button to set it to [On] or [Off].

When you choose [On], tap the number box on the right, and then enter the number of samples out of which a data point is retained

Storing files in text format requires a lot of storage space. Data decimation can reduce file sizes.

Off [⊄]	No data is decimated.
	Allows you to enter the decimation number. The instrument retains one data point out of the specified number of data points.

Example

When you enter [3], the instrument retains one data point out of three consecutive data points: it decimates the two other points. The number of samples is reduced by one third of the original number.

7 In the [Calculation result] area, tap [On] or [Off] to configure the numerical calculation result setting.

Off [⊠]	Does not any save numerical calculation results.
On	Saves numerical calculation results.

Tap the [File] box, and then from the list, choose an option for saving data to files.

New [∅]	Creates a new file for each measurement and saves it.
Append	Appends data to an existing file and saves it.

Tap the [Divide] box, and then choose a file division setting from the list.

Off [∅]	Does not divide any files.
Split by Calc. No.	Creates a file for each calculation number.

8 In the [Screen image] area, tap [On] or [Off] to configure the display image saving setting.

Off [⊠]	Does not save any screenshot.
On	Saves a screenshot.

Tap the [Type] box, and then choose a save format of images from the list.

BMP^{II}, PNG, JPEG

When you choose data in text format or numerical calculation results to be saved

Characters or display items used on the instrument are converted as follows:

Character used on the instrument	Saved character
2	^2
3	^3
μ	ĩu
Ω	~o
з	~е
0	~c
±	~+

Waveform data

The instrument automatically divides large-size waveform data files (.MEM or .REC) before saving.

Real-time saving

Since setting the real-time saving to **[On]** allows data to be saved in a storage device simultaneously with measurement, the instrument can perform measurement for a long period of time regardless of the capacity of the internal memory.

The measurement condition settings are different between setting the real-time saving to **[On]** and **[Off]**.

- When setting the real-time saving to **[On]**, you cannot use the following functions: Automatic saving, trigger function, waveform calculation function, and memory division function.
- No storage device can be removed or replaced during the real-time saving.
- If displaying the message, Error No. 235 [Real-time saving could not be completed within available time.], the instrument may record abnormal data in a waveform file saved in a storage device.
- The operation may be automatically restricted if there is a risk that saving data cannot be completed in time during the real-time saving.
- When any numerical calculation is set, only manual calculation can be executed.
 After the measurement has been complete, select > [Calculation] > [Numerical calculation], and then tap [Execute].
- Configuring the waveform display setting with the higher vertical compression ratio may cause saving data not to be completed in time during the real-time saving. Lower the compression ratio such a case.
- For real-time saving, use the following Hioki's options: Model U8332 SSD Unit, Model U8333 HD Unit, and Model Z4006 USB Drive Model Z4001 SD Memory Card (2 GB), Model Z4003 SD Memory Card (8 GB)
- When using Model Z4006 USB Drive for real-time saving, connect the drive to the USB 3.0 connector on the right side of the instrument. Connecting the drive to the USB 2.0 connector cannot deliver the real-time saving speed specified in the product specifications.

Maximum recording time

- When the real-time saving is set to **[On]**, the maximum recording time is determined based on the recording interval, the remaining capacity of a storage device, and the number of channels to be used.
- When the sampling rate is set at a slow rate, the recording time is set to a long period of time (one year or more) depending on a condition. The operation cannot be guaranteed because the warranty period or product life may disturb it.
- When the external sampling is used, the instrument calculates the maximum recording time assuming a recording interval of 10 MS/s.

See "Maximum recordable time when the real-time saving is enabled (values for reference purposes)" (p. 399).

Waveform data


When recording waveforms with the real-time saving set to **[On]**, the instrument directly saves measured waveform data (.MEM or .REC) onto a storage device. If the file size is large, the instrument automatically divides the file into several files each of which has 512 MB and saves them.

Deleting and saving files when saving data in real time

- If the capacity of the storage device becomes full while the instrument is storing files, it automatically deletes waveform files created after the measurement has started beginning from the oldest, securing free space in the storage device. However, when free space in a storage device is less than the sum of the created file size and 512 MB before starting a measurement, the instrument cannot overwrite any new files over the older files. Use a storage device with as much free space as possible.
- The instrument does not delete waveform files saved in the past.

• When [Method] is set to [Delete], the recording length can be set at 10000 days at a maximum; however, data the instrument retains after the measurement is limited to a free space size of a storage device at the start of recording (recording time of the normal saving).

> [Status] > [Save]

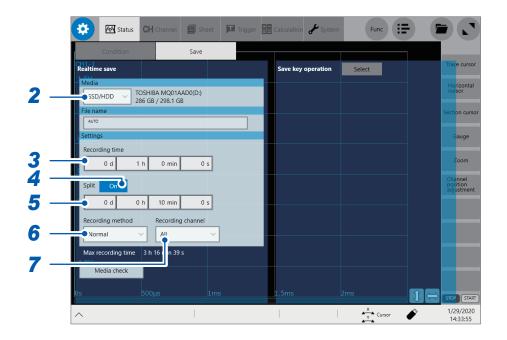

1 On the [Condition] screen, configure the realtime save and sampling settings. See "1.2 Setting Measurement Conditions" (p. 5).

2 Tap the [Media] box, and then choose a destination to save from the list.

When selecting **[FTP]** as the destination to save, you can specify another backup destination used if the communication fails.

When a backup is enabled, choose from SSD/HDD, SD card, and USB flash drive for the destination to save.

3 Tap the [Recording time] box, and then enter a recording time.

d	0 to 10000 (days)
h	0 to 23 (hours)
min	0 to 59 (minutes)
S	0 to 59 (seconds)

4 Tap the [Split] button to specify whether to divide a file before it is saved.

Off [⊮]	Does not divide a file.
On	Divides a file.

Δ

5 (When the [Split] button is set to [On])

Tap the time entry boxes under [Split] to enter the length of time each divided file has.

d	0 to 100 (days)
h	0 to 23 (h)
min	0 to 59 (min.)
S	0 to 59 (s)

If the file size exceeds 512 MB before the set division time has elapsed, the file is divided at the time, and 512 MB of the recorded data is saved.

6 Tap the [Method] box, and then from the list, choose a way to handle if a space of a storage device is insufficient.

Normal ^ℤ	Stops the real-time saving and measurement if the storage device is full.
Delete	Deletes older files and saves files in real time if the storage device is full (waveform files only). The instrument deletes files only created after the measurement has started. It does not delete previously existing files.

Setting [Media] to [FTP] forces this setting into [Normal].

7 Tap the [Recording channel] box, and then choose a channel to be saved.

	AII [∅]	Saves data acquired across all the channels that have performed measurement (whose measurement settings are [On]).
	Display	Saves data acquired across all the channels whose display settings are [On].

8 Check settings that include the input channel settings, and then press the START key to start a measurement.

The instrument saves data onto a storage device in real time during measurement.

Freely choosing data items to be saved and save files (SAVE key)


You can configure saving action setting the instrument performs when you press the SAVE key.

Selective save: After you press the **SAVE** key, the instrument allows you to configure the save settings before saving data.

You can save the following types of data:

- Waveform data
- Screenshot
- Numerical calculation result
- Setting
- CAN text
- · Arbitrary waveforms
- Program

> [Status] > [Save]

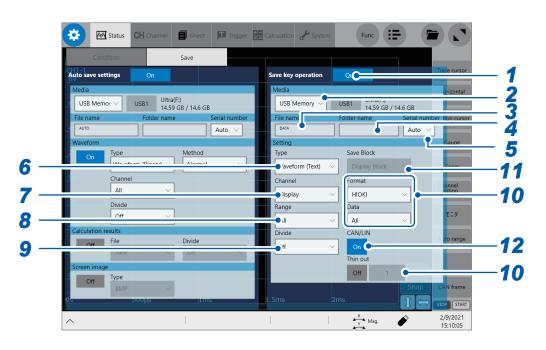

1 Tap the [Save key operation] button, and then choose a save method adopted when you press the SAVE key.

Select [⊠]	Displays the dialog box to allow you to choose items to be saved and saves them. The instrument displays the dialog box when you press the SAVE key to start a measurement, which allows you to configure subsequent settings. This operation cannot be executed if another dialog box is open. See "Selective saving" (p. 118).
Quick	Immediately saves data consisting of pre-specified items. See "Quick saving" (p. 118).

2 Tap the [Media] box, and then choose a destination to save from the list. (See p. 120.)

3 Tap the [File name] box, and then enter a file name.

- Number of characters for a file name: Up to 100 characters
- The maximum length of a file name that includes its path: Up to 255 characters

Δ

Quick save: Pressing the **SAVE** key causes the instrument to save data that consists of prespecified items.

4 Enter a folder name in the [Folder name] box.

If you wish to choose a destination folder, enter a folder name. If you leave the box blank, the instrument will sort files into folders based on the file type.

Folder name: up to 32 characters

5 Tap the [Serial number], and then from the list, choose a format of sequential number to be added to folder/file names.

Previous [⊠]	Prefixes a sequential number to each folder/file name.
Tail	Suffixes a sequential number to each folder/file name.
Auto	Saves folders/files without sequential numbers. Suffixes a sequential number to each folder/file name if a folder/file with the same name has already existed.

6 Tap the [Type] box, and then choose a save format from the list.

Waveform (Binary) [⊠]	Saves waveform data in binary format. Choose this option to reload the waveforms into the instrument.
Waveform (Text)	Saves waveform data in text format. Choose this option to load the waveforms with a computer.
Waveform (MDF)	Saves waveform data in MDF format. Choose this option to load the data using an MDF-capable waveform viewer installed in a computer.
Waveform (Float)	Saves waveform data in binary format (32-bit floating point). Choose this option to load the waveforms with a computer.
Screen image	Saves screenshots. The data saved can be viewed on a computer with image viewing software.
Numerical calculation result	Saves numerical calculation results.
Setting	Saves the present measurement conditions.
Arbitrary waveform	Saves arbitrary waveform data.
Program	Saves a waveform generation program.
CAN text	Saves CAN frame data in text format.

7 Tap the [Channel] box, and then choose an option for channels to be saved.

When [Type] is set to [Waveform (Binary)] or [Waveform (Text)]

All	Saves data acquired across all measured channels (channels with measurement set to [On]). Saves the data acquired across the channels with the display setting set to [Off].
Display [⊠]	Saves data acquired across the channels with the display setting set to [On] on all sheets.

8 Tap the [Range] box, and then choose an option for the save range from the list. When [Type] is set to [Waveform (Binary)] or [Waveform (Text)]

AII	Saves all data written in the memory.
Segment 1	Saves data in the section between section cursors [1A] and [1B].
Segment 2	Saves data in the section between section cursors [2A] and [2B].

The instrument saves data acquired across the channels displayed on the screen.

See "2.2 Specifying the Waveform Range (Section Cursor)" (p. 35). When no target section cursors are set, whole data is saved regardless of the [Segment 1] or [Segment 2] setting.

9 Tap the [Divide] box, and then from the list, choose an option for a file size of each file. When [Type] is set to [Waveform (Binary)].

Off	Saves a file without dividing it.
16 MB, 32 MB	Choose this option to divide a large file into several files and save them. A file is divided into several files each of which has the specified size. The instrument creates a folder with the specified name, divides a file into several files, and then saves them in the folder.

Even if the **[Divide]** has been set to **[Off]**, the instrument automatically divides files more than 512 MB in size, which can be generated in some measurement conditions. When the instrument needs to divide a file, it automatically creates a folder to save divided files and an index file with the extension .INX. Loading the IDX file allows the waveform files to be loaded in a batch.

When using the memory division function, you cannot use the division save function.

See "Loads divided files in a batch." (p. 134) and "10 Memory Division Function" (p. 289).

When [Type] is set to [Waveform (Text)].

Off [∅]	Saves a file without dividing it.
60,000 Data 1,000,000 Data	The instrument divides a file into several files each of which contains the specified number of data points.

Even if the **[Divide]** has been set to **[Off]**, the instrument automatically divides files more than 512 MB in size, which can be generated in some measurement conditions.

When using the memory division function, you cannot use the division save function. See "10 Memory Division Function" (p. 289).

10 Configure advanced save settings according to the [Type] box setting.

Saving format	S	etting	Description
Waveform (Text)	Format	HIOKI [⊠]	Saves data in commonly used text format.
		COMTRDE	Saves data in COMTRADE-compliant format.
	Data	AII [∅]	Saves all data in .
		Event	Saves only the data points at event marks.
	Thin out	Off [⊌] , On (2 to 1,000)	A large amount of space is required to save files in text format. Decimating data points before saving a file can reduce the file size. This setting allows you to specify the decimation number (the instrument retains a data point out of the decimation number of data points). Example:When you specify [10] , the instrument saves one out of every 10 consecutive data points and disregards nine others. The number of samples is reduced to one-tenth of the original amount.
Screen image (screenshot)	Туре	BMP [∅] , PNG, JPEG	Allows you to choose a type for saving image files.
Numerical calculation result	File designation	New [∅]	Saves files with a new file name each time. The instrument allocates sequence numbers when the same name is given.
		Append	Appends data to the same file and saves it.
	File division	Off [⊠]	Saves all calculations in a single file.
		Split by Calc. No.	Creates a new folder, divides a file into several files according to calculation number, and save them in the folder. The instrument appends the string "_K + sequential number" following each file name.

Saving/Loading Data and Managing Files

4

Saving format	Set	ting	Description
Arbitrary	Channel Data name		Select a channel number of the measured waveform to be saved or that of the U8793 with the arbitrary waveform registered.
			Allows you to enter a data name to be saved (for measured waveforms) or that of an arbitrary waveform data name to be saved (for the U8793).
Program	Channel		Allows you to choose the channel number of the U8793 where the program you wish to save has been registered.
Waveform (MDF)	Format	MDF3.0	Saves data in MDF 3.0 format with the MDF extension.
		MDF4.0	Saves data in MDF 4.0 format with the MF4 extension.

11 (When using the memory division function or the dual sampling function)Tap [Save Block] box, and then from the list, choose an option for blocks to be saved.

Display block [⊠]	Saves waveforms included in displayed blocks.
All block	(When using the memory division function) Saves all blocks specified by the "use blocks" setting, starting with the start block.
	(When using the dual sampling function) Saves all trend and instantaneous waveform blocks.

12 (When CAN signals are recorded)

Tap the [CAN/LIN] button to configure the simultaneous-save setting of the waveform file and the CAN binary file.

Off⊄	Saves the waveform file only.
On	Saves the CAN log file and index file as well as the waveform file.


Whenever you press the SAVE key, the instrument saves data that consists of specified items.

File division

The instrument automatically divides a large-size data file into several files each of which is 512 MB in size before saving.

Performing the SAVE key operation using the screen

You can use the screen to perform the **SAVE** key operation.

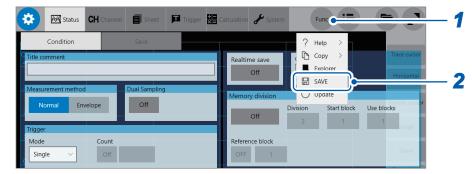

- **1** Tap [Func].
- **2** Select [SAVE].

4.3 Loading Data

You can load data saved in a storage device or written in the internal memory of the instrument.


Data loading procedure

Before attempting to load the data, make sure that a storage device is inserted, and the save destination is correctly specified.

Open the file screen, choose a storage device, and double-tap a file you want to load.

Waveform and settings files saved in waveform (binary) format can be loaded on the instrument. The instrument displays only loadable files on the file screen.

You can use Explorer to check files not supported by the instrument, including those in text and BMP formats.

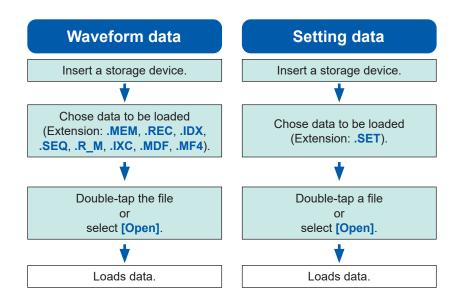



To display the file screen

IMPORTANT

The file screen lets you to choose files to load. It will not display files the instrument cannot load. You can use Explorer to control files, including copying and moving them, and to check files not supported by the instrument.

See "4.4 Managing Files" (p. 136).

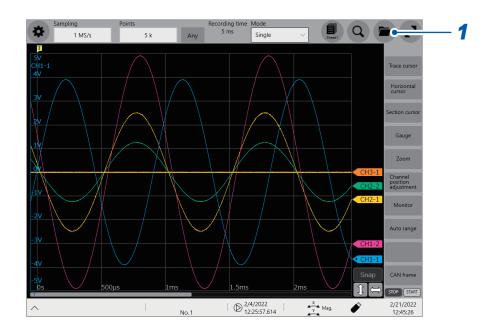

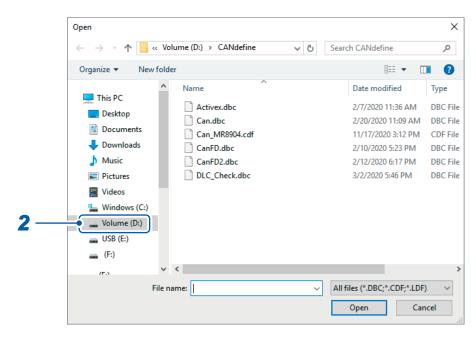

1 Tap 🔎 on the waveform screen.

A window will open allowing you to select a file.

2 Choose a storage device to be operated.

When loading data from a storage device

Insert a storage device before choosing it.

Others

- The MR6000 can load data saved with the MR6000, MR8847, MR8827, MR8740, and MR8741 Memory HiCorder. Data saved with other recorders cannot be loaded onto the MR6000.
- The MR6000 cannot load some settings when loading data saved with the MR8847, MR8827, MR8740, and MR8741.
- Loading a waveform file changes the settings of the instrument to those when the waveform file was saved. When a measurement starts with this state, the instrument measures waveforms with the settings of the loaded waveform file; however, the settings of the modules are restored to those set before the waveform file was loaded. To discard the module settings of the loaded waveform file, execute **[Initialize waveform data]** (See "6.2 Initializing the Instrument" in the Quick Start Manual.).
- Loading a waveform file suspends the waveform monitor until one of the following actions is performed:
 - Start a measurement.
 - Initializing the instrument by executing [Initialize waveform data], [Initialize Settings], or [Initialize all]
 - · Loading a setting file

Loading waveform data in a batch

Loading one of the following index files allows waveform data to be loaded in a batch. Configuring the following settings allows the instrument to create an index files and waveform file together.

Extension	Content
IDX	Loads divided files in a batch. The instrument with the file division setting creates an index file (the file division setting is included in the automatic saving or the SAVE key operation settings). However, when [Type] is set to any type other than [Waveform (Binary)], the instrument does not create any index file. See "Automatically saving waveform data" (p. 120) and "Freely choosing data items to be saved and save files (SAVE key)" (p. 127).
SEQ	(When using the memory division function) The instrument loads waveforms of all blocks at a time. The instrument creates an index file when the instrument with the memory division function enabled automatically save data or you press the SAVE key to save data of all blocks (p. 130). See "Freely choosing data items to be saved and save files (SAVE key)" (p. 127) and "Automatic saving for the memory division setting" (p. 293).
R_M	(When using the dual sampling function) Loads all trend and instantaneous waveform files at once. Index files are created when saving data automatically during dual sampling measurement and when saving all blocks with the SAVE key. See "Freely choosing data items to be saved and save files (SAVE key)" (p. 127) and "11.5 Files" (p. 308).
IXC	(When using CAN/LIN channels) Loads waveforms and CAN frame data at once. Index files are created when automatically saving data while using CAN/LIN channels and when saving CAN binary files simultaneously with the SAVE key. See "Freely choosing data items to be saved and save files (SAVE key)" (p. 127) and "12.8 Saving Data" (p. 342).

Loading waveform generating data (registration)

The instrument can load data for signal generating modules. The signal generating screen in the channel screen can be used to load such data. See the Instruction Manual that came with the U8793, MR8790, and MR8791.

Extension	Content
WFG, TFG, CSV, TXT	Loads waveform generator data to the specified channel of the arbitrary waveform generator module. (registration) The instrument will output the signal of the loaded (registered) waveform data from the U8793 Arbitrary Waveform Generator Unit. See "Registering arbitrary waveforms in the U8793 Arbitrary Waveform Generator Unit" (p. 102). Only CSV and TXT files that include one generator data value per line in text format are valid.
PLS	Loads pulse pattern data to the specified channel of the pulse generator module. (loading) The instrument will output a pulse pattern waveform of the loaded pulse pattern data from the MR8791 Pulse Generator Unit. See "Configuring Model MR8791 Pulse Generator Unit settings" (p. 92).
FGP	Loads an FGP waveform generator program file to the specified channel of the arbitrary waveform generator module. (registration) See "Editing programs of Model U8793 Arbitrary Waveform Generator Unit" (p. 107).

Automatically loading the settings (Automatic setup function)

The instrument can load a setting file with the file name "STARTUP" in the [CONFIG] folder in the [HIOKI_MR6000] folder at the time of startup.

The instrument searches the drives beginning from drive D in alphabetical order for the file "STARTUP.SET," loading the file found first.

Loading numerical calculation settings

When loading a waveform file during the numerical calculation setting enabled, you can choose whether to overwrite the existing numerical calculation settings with those of the waveform file.

Read waveform file	
Do you want to overwrite the numerical with the settings in the waveform file?	calculation settings
Yes Overwrite and read the waveform	No Read the waveform without overwriting


4.4 Managing Files

Opening Explorer allows you to manage data saved in storage devices.

Operation available on Explorer

Changing storage devices	Storage devices can be changed.
Sorting files	Files on a file list can be sorted based on the chosen basis.
Moving files to a folder	Files can be moved to a folder of your choice.
Copying files	Files can be copied to a specified folder. When you choose folders to be copied, the chosen folders are copied to the specified folder.
Creating a folder	A new folder can be created.
Renaming a file	A file or folder can be renamed.
Deleting files	Files and folders can be deleted.
Format	A storage device can be formatted.

To open the explorer

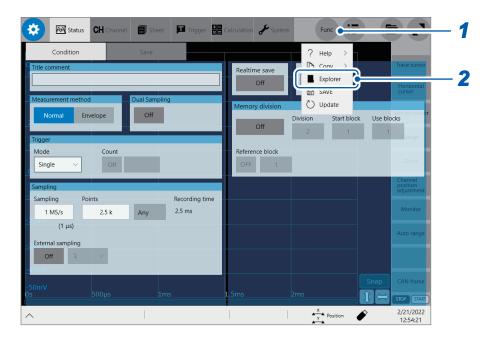

1 Tap [Func].

2 Select [Explorer].

Explorer appears. Choose a storage device to be operated.


5 Configuring the Trigger Settings

The trigger function allows you to start and stop measurement using specific signals. When recording is started or stopped by specific signals, it is called "The instrument is triggered." When the real-time saving is set to **[On]**, you cannot use the trigger function.


In this chapter, the mark $\overline{\mathbf{p}}$ represents the point the start trigger is activated; the mark $\overline{\mathbf{p}}$ represents the point the stop trigger is activated.

In the descriptions of each trigger source, the mark $\mathbf{\overline{p}}$ represents a point each trigger condition is satisfied and a point each trigger is generated.

> [Trigger] > [Common]

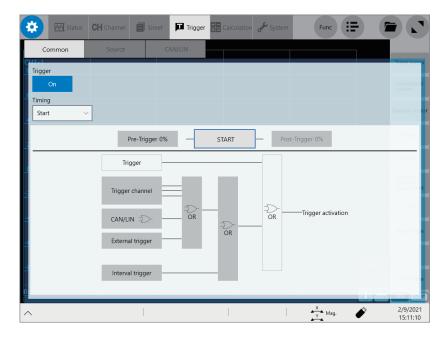

Operation available on the [Trigger] screen

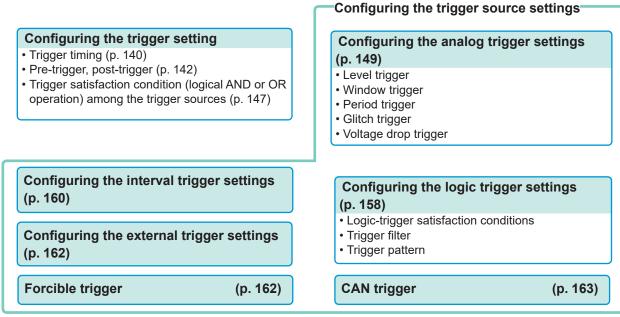


You can configure the trigger setting so that the instrument can output an signal from the external control terminals when the trigger activates.

See "External trigger terminal (EXT.TRIG)" (p. 391).

5.1 Trigger Setting Procedure

- The instrument is triggered based on trigger satisfaction conditions (logical AND or OR operation) among trigger sources except for the forcible trigger. (p. 147)
- When triggered, the instrument outputs the TRIG.OUT signal from the external control terminal. (p. 389)

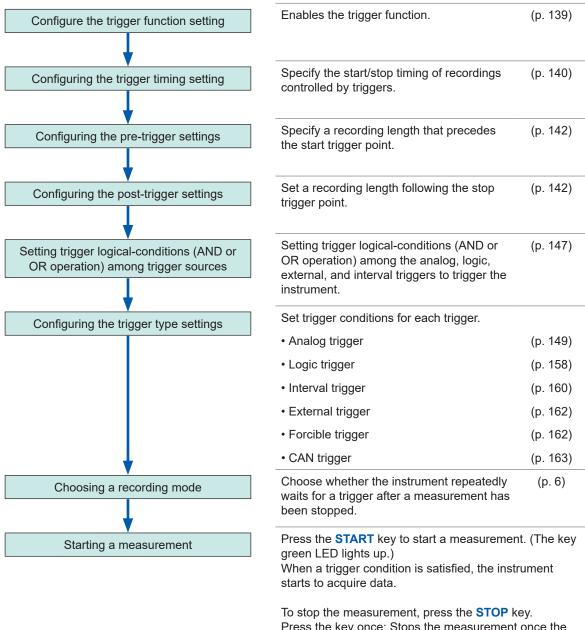


Press the key once: Stops the measurement once the instrument has acquired the specified recording length of data.

Press the key twice: Stops the recording immediately.

5.2 Enabling the Trigger Function

> [Trigger] > [Common]

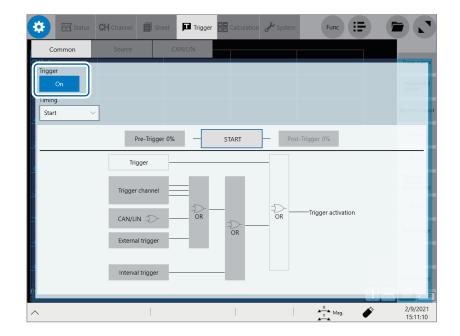

Tap the [Trigger] button to set it to [On].

Off [∅]	Disables the trigger function.
On	Enables the trigger function.

To copy settings to other channels

You can copy settings on the analog trigger setting screen. See "3.6 Copying Settings (Copy Function)" (p. 66).

5.3 Configuring the Trigger Timing Setting

Configure the waveform recording settings the instrument follows when it is triggered.

> [Trigger] > [Common]

Status	CH Channel	Sheet Trigger	Calculatio	n 🥜 System	Func	
Common	Source	CAN/LIN				
Chil-1 § Trigger On Timing Start						Horizontal cursor Section cursor
2	Pre-Tri	gger 0% —	START	- Post-	Trigger 0%	Gauge
0	Trigger					Zeom
-2	Trigger chan			5		Channe position signaturet
4	CAN/LIN 🗐	> OR			-Trigger activation	
-6	External trigg	er	OR			e
-8 -1 0:	Interval trigg	er	-		115	
^					Y Mag.	2/9/2021 15:11:10


1 Tap the [Timing] box, and then choose a trigger recording method from the list.

Start [⊠]	Starts recording when the instrument is triggered, and stops the recording after the instrument has acquired the recording length of waveforms.
Stop	Starts recording when you press the START key, and stops the recording when the instrument is triggered.
Start/Stop	Starts recording when a start trigger is activated and records data until a stop trigger is activated.

When Model U8975 4ch Analog Unit or MR8990 Digital Voltmeter Unit or both are included in the measurement modules, the displayed trigger point may lag behind the actual trigger point by one sample.

Trigger timing


Behavior varies depending on the recording mode.

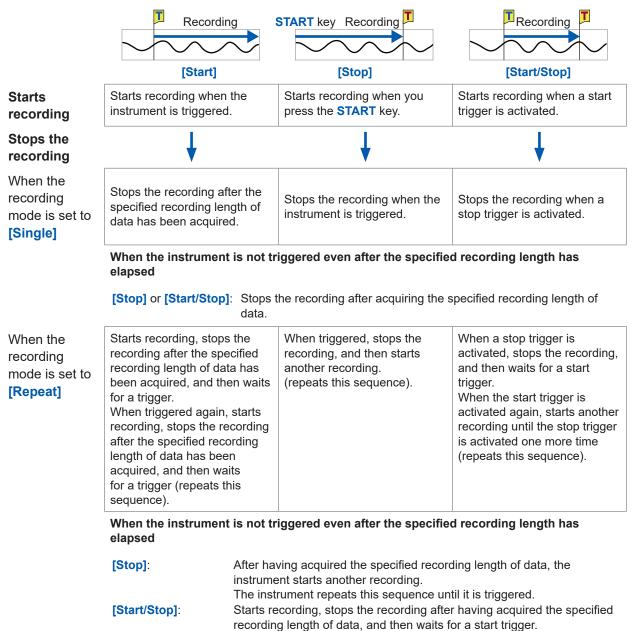


Example of trigger timing

When the trigger type is set to the level trigger; level, level, at 0.000 V; and slope, to positive [/]





Records the specified recording length of data.



Starts recording when you press the **START** key. Continues the recording until a stop trigger is activated.

[Start/Stop]

Starts recording when a start trigger is activated. Continues the recording until a stop trigger is activated.

The above processes are repeated when the recording mode is set to [Repeat].

5.4 Configuring the Pre-trigger and Post-trigger Settings


Pre-Trigger	You can record not only waveforms that appear after a start trigger has been activated, but also those that appear before the trigger is activated. Setting of timing: [Start], [Start/Stop]	Also records data before the start trigger.		
Post-Trigger	You can also record waveforms that appear after the specified recording length elapses from the stop trigger point. Setting of timing: [Stop], [Start/Stop]	Also records data after the stop trigger.		

The pre-trigger and post-trigger are expressed as a percentage of the recording length (unit: percent).

- Setting all the trigger sources (including analog and interval triggers) to [Off] disables pre-trigger and post-trigger settings.
- The setting of the recording length or the recording time is prioritized over the post-trigger setting. Example


When the recording length is set at10,000 points and the post-trigger length at 30%, and the stop trigger is activated after the instrument measures 8000 points of waveforms, the instrument records only 2000 points of the waveforms after the stop trigger has been activated.

> [Trigger] > [Common]

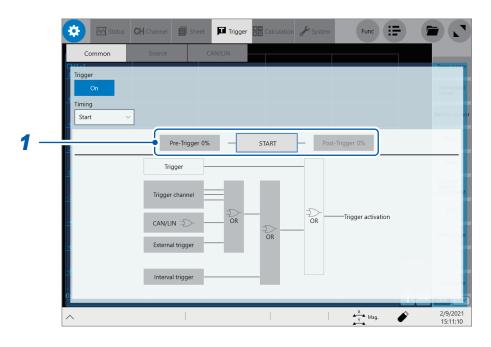

1 Tap [Pre-Trigger 0%] or [Post-Trigger 0%].

The setting dialog box appears.

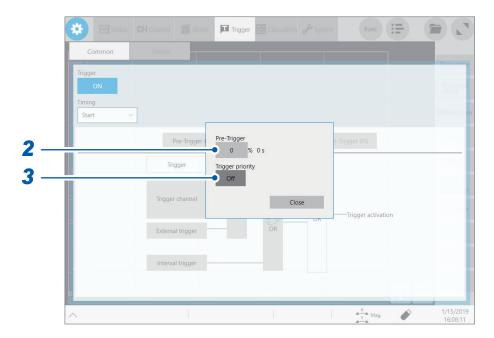

2 Tap the [Pre-trigger] or [Post-trigger] boxes, and then enter a pre- or post-trigger length.

Pre-Trigger	0% ^ℤ to 100%
Post-Trigger	0% [™] to 40%

See "For saving data acquired without using the envelope on Model U8333 HD Unit" (p. 400). When setting both [Pre-Trigger] and [Post-Trigger] in combination, make sure that the total percentage points of [Pre-Trigger] and [Post-Trigger] is 80% or less.

5 co

Difference between [Waiting for Pre-Trigger] and [Waiting for Trigger]

When starting a measurement, the instrument starts filling the pre-trigger memory. During this period, the instrument displays the message **[Waiting for Pre-Trigger]**. After having filled the pre-trigger memory, the instrument displays the message **[Waiting for Trigger]** until it is triggered. While displaying **[Waiting for Pre-Trigger]**, the instrument is not triggered even when a trigger condition is satisfied.

Pre-trigger, post-trigger, and recording range


· Using the pre-trigger along with the start trigger setting


When the pre-trigger length is set at 95%: Records the recording length of waveforms, 95% of which appear before the start trigger point.

When the pre-trigger length is set at 50% Records the recording length of waveforms, 50% of which appear before the start trigger point.

• Using the post-trigger along with the stop trigger setting


When the post-trigger length is set at 20%: Also records data after the stop trigger.





Period of time shorter than the specified recording length or recording time

· Using the pre-trigger and post-trigger along with the Start/Stop triggers setting



Records 30% of the recording length of waveforms that appear before the start trigger point.

Also records 20% of the recording length of waveforms that appear after the stop trigger point.


3 Tap the [Trigger priority] button to choose a way to handle triggers activated while the instrument is filling the pre-trigger memory.

You can choose whether the instrument is triggered when the trigger conditions are satisfied while the instrument is filling the pre-trigger memory.

Off [⊄]	Ignores triggers while filling the pre-trigger memory.	
On	Accepts a trigger while filling the pre-trigger memory.	

When the trigger conditions are satisfied while the message [Waiting for Pre-Trigger] is being displayed

Example: When the pre-trigger length is set to 50%

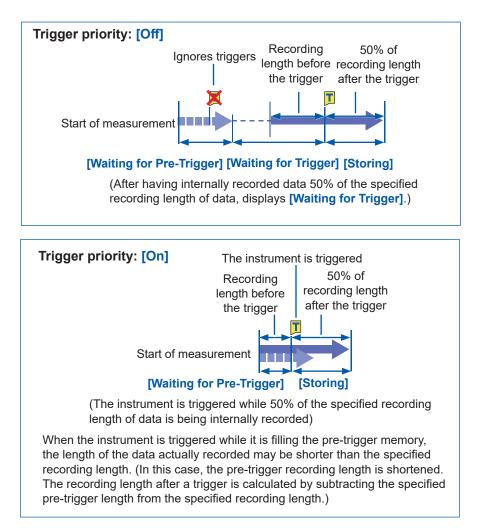


To observe an input waveform while the instrument is waiting for a trigger


...

1 Tap [Waveform monitor].

A waveform acquired across one of any channels is displayed.

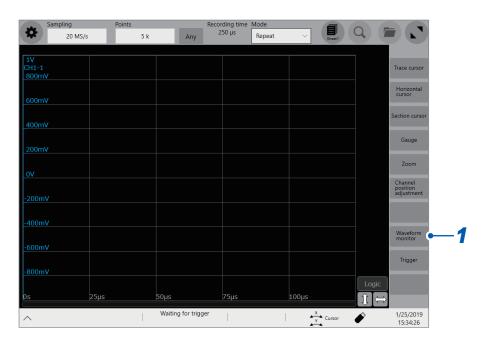

2 Tap [CH ▲] or [CH ▼] to choose a channel to be displayed.

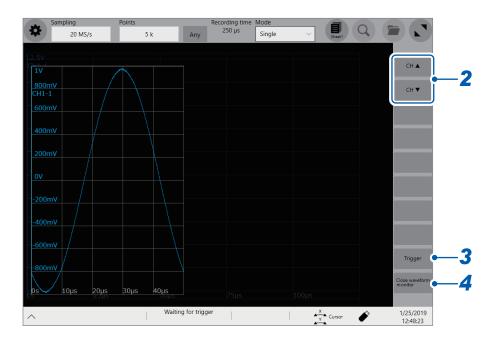

3 Tap [Trigger].

You can forcibly trigger the instrument.

4 Tap [Close waveform monitor].


The screen restores to the waveform screen.

5.5 Setting the Trigger Satisfaction Conditions (AND/OR Operation) Among Trigger Sources

Set the trigger satisfaction conditions among the analog, logic, CAN, external, and interval triggers by choosing between logical AND or OR operation.

The forcible trigger triggers the instrument regardless of the trigger satisfaction conditions setting. If all trigger sources are set to off (i.e., with no trigger setting), recording starts immediately (free run).

> [Trigger] > [Common]

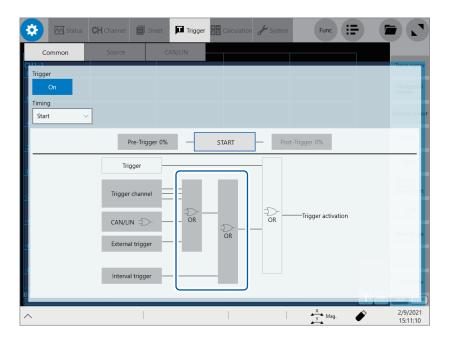

Tap [AND] or [OR], whichever is displayed, to switch to the other.

OR [∅]	When any one of the specified trigger conditions changes from not being satisfied to being satisfied (at a changing point), the instrument is triggered. Thus, even though a trigger condition has been already satisfied at the start of waiting for a trigger, the instrument is not triggered until a changing point is detected.	
AND	Only when all of the specified trigger conditions are satisfied, the instrument is triggered. Thus, if all the specified trigger conditions have been already satisfied at the start of waiting for a trigger, the instrument is immediately triggered.	

Setting example: To trigger the instrument when a waveform crosses the zero-volt level while rising $([\nearrow]^*)$

The instrument is triggered based on whether the trigger satisfaction condition is set to AND or OR operation in the following ways:

Channel	Trigger	Level	Slope	Filter
CH1, CH2	Level	0.00 V	*	Off
Ŧ	Start		Start	
	[AND]			[OR]
	One waveform is above 0 V, and the other is also above 0 V.			form crosses 0 V


When the trigger timing is set to **[Start/Stop]**, the instrument determines that a logical AND or OR operation is satisfied in a set of trigger sources assigned to the start trigger or those assigned to the stop trigger.

*: With the [AND] setting, the slope setting item appears as [HIGH].

5.6 Triggering the Instrument Using Analog Signals (Analog Trigger)


This section explains how to configure the analog trigger settings and types of the analog triggers.

> [Trigger] > [Source]

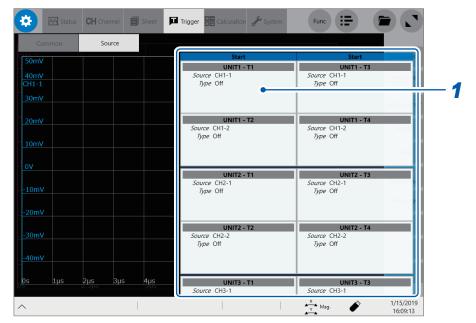

1 Tap a trigger source to be set.

The setting dialog box appears.

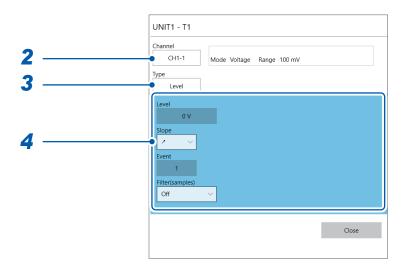

2 Tap the [Channel] box, and then from the list, choose a channel you want to set a trigger condition for.

See "Settable channels for each trigger source" (p. 150).

3 Tap the [Type] box, and then choose a trigger type from the list.

Off^ℤ, Level, In, Out, Voltage drop, Period-in, Period-out, Glitch


4 Configure each trigger-type-specific setting.

Trigger source	Module (UNIT) channel	Calculation channel
UNIT1 – T1, T3	Channels of UNIT1	W1
UNIT1 – T2, T4		W2
UNIT2 – T1, T3	Channels of UNIT2	W3
UNIT2 – T2, T4	Channels of UNIT2	W4
UNIT3 – T1, T3		W5
UNIT3 – T2, T4	Channels of UNIT3	W6
UNIT4 – T1, T3		W7
UNIT4 – T2, T4	Channels of UNIT4	W8
UNIT5 – T1, T3		W9
UNIT5 – T2, T4	Channels of UNIT5	W10
UNIT6 – T1, T3		W11
UNIT6 – T2, T4	Channels of UNIT6	W12
UNIT7 – T1, T3	Channels of UNIT7	W13
UNIT7 – T2, T4		W14
UNIT8 – T1, T3	Channels of UNIT8	W15
UNIT8 – T2, T4		W16

Settable channels for each trigger source

1. [Level] trigger

When an input signal crosses the specified level in the positive or negative direction, an analog trigger is generated.




Slope: [/]

Setting			Description
Level -f.s. to +f.s. Default: 0 [⊠]			Allows you to enter a level of the level trigger.
Slope With OR		, ✓	The level-trigger condition is satisfied when a waveform crosses the threshold value (level) while rising.
		X	The level-trigger condition is satisfied when a waveform crosses the threshold value (level) while falling.
With AND	HIGH [∅]	The level-trigger condition is satisfied when a waveform is higher than the threshold value (level).	
		LOW	The level-trigger condition is satisfied when a waveform is lower than the threshold value (level).
Event With OR 1 ¹² to 4,000		1 [⊠] to 4,000	Allows you to enter the number of events. The instrument counts the number of times the level-trigger condition is satisfied. An analog trigger is generated when the count reaches the specified number of events.
	With AND		Not available
Filter	Filter Off [⊠] , 10 to 10,000		Allows you to enter a filter width in the number of samples. Only after the level-trigger condition is continuously satisfied during the specified period, an analog trigger is generated. Specifying this option prevents the instrument from being unintentionally triggered due to noise.
Off [⊠] , 1 ms, 10 ms		10 ms	Allows you to enter a filter width in milliseconds when the envelope is used.

With the [Filter] setting

Specifying the filter width prevents analog triggers from being unintentionally generated due to noise, allowing it to be generated only after the level-trigger condition is continuously satisfied during the specified width or longer.




Noise does not generate any analog trigger.

With the [Event] setting


If the trigger condition is repeatedly satisfied, setting the number of events prevents an analog trigger from being generated until the number of times the level-trigger condition is satisfied reaches the specified number of counts.

Example: When the number of events is set to [4] (Slope: [7]).



2. [In] trigger, [Out] trigger

When an input signal falls within (**[In]**) or exits of a range (**[Out]**), which is determined by specifying upper and lower values, an analog trigger is generated. These triggers are disabled when the sampling rate is set at 200 MS/s.

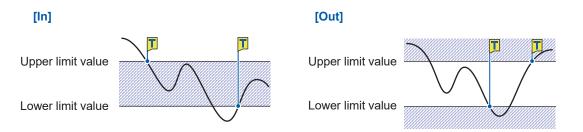

Setting			Description
Event	With OR	With OR1 ^{III} to 4,000Allows you to enter the number of events. The instrument counts the number of times the window- condition is satisfied. Only after the count reaches the si number of events, an analog trigger is generated.	
	With AND		Not available
Filter	Off ^፼ , 10 to 10,000		Allows you to enter a filter width in the number of samples. Only after the window-trigger condition is continuously satisfied during the specified period, the analog trigger is generated. Specifying this option prevents the instrument from being unintentionally triggered due to noise.
	Off [⊠] , 1 ms, 10 ms		Allows you to enter a filter width in milliseconds when the envelope is used.
Upper	-f.s. to +f.s.		Allows you to enter an upper limit value.
Lower	-f.s. to +f.s.		Allows you to enter a lower limit value.


Behavior with the in trigger and out trigger settings varies depending on the trigger satisfaction conditions (AND and OR operations).

	1		
With OR	In	The window-trigger condition is satisfied when an input signal crosses the upper or lower limit value of the threshold (level) and thereby falls within the range, which is specified by the upper and lower limit values of the threshold (level).	
Out		The window-trigger condition is satisfied when an input signal crosses the upper or lower limit value of the threshold (level) and thereby exits the range, which is specified by the upper and lower limit values of the threshold (level).	
With AND	In	The window-trigger condition is satisfied when an input signal is inside the range, which is specified by the upper and lower limit values of the threshold (level).	
	Out	The window-trigger condition is satisfied when an input signal is outside the range, which is specified by the upper and lower limit values of the threshold (level).	

3. [Voltage drop] trigger

When a voltage peak is continuously lower than a specified level for a time of half a period or more, the voltage-drop-trigger condition is satisfied. The sampling rate can be set at a figure in the range of 2 kS/s to 100 MS/s.

The external sampling is cannot be set when the envelope is used. These triggers cannot be set either when Model MR8990 or Model 8970 is used.



Settir	Setting		Description
Level	0 to +f.s. (100 V [⊠])		Allows you to enter a level to be used to check for voltage drops.
Frequency	50 Hz [⊠] , 60 Hz		Allows you to choose the frequency of the power to be measured.
RMS (root- mean-square value)	Varies in conjunction with the level settings		Displays a rough indication of the RMS value.
Event	With OR 1 ² to 4,000		Allows you to enter the number of events. The instrument counts the number of times the voltage- drop-trigger condition is satisfied. Only after the count reaches the specified number of events, an analog trigger is generated.
	With AND		Not available

Behavior of the voltage drop trigger varies depending on the trigger satisfaction conditions (AND and OR operations).

With OR	As soon as the instrument determines that a voltage peak became lower than a specified level for a time of half a period or more, the voltage-drop-trigger condition is satisfied.
With AND	While a voltage peak is lower than a specified level for a time of half a period or more, the voltage-drop-trigger condition is continuously satisfied.


4. [Period-in] trigger and [Period-out] trigger

The instrument measures periods of an input waveform, which are time lags between consecutive two points at which an input voltage crosses the specified level in the positive or negative direction. The period-trigger condition is satisfied when a period is inside the specified range (In) or outside the specified range (Out).

An trigger point lags behind the actual trigger point by one sample. These triggers are disabled when the sampling rate is set at 200 MS/s.

The external sampling is cannot be set when the envelope is used. These triggers cannot be set either when Model MR8990 and Model 8970 is used.

See "Setting of the period range" and "[Period-out] trigger" (p. 156).



	Setting		Description				
Level	-f.s. to +f.s. Default: 0 [⊠]		Allows you to enter a level for detecting the rising or falling slopes of a signal.				
Slope	, , ,		Allows you to choose which of the following points to use to calculate periods: two consecutive points at which a signal crosses the specified level while rising; or those while falling.				
Period lower limit*	Zero or 5 times the or more	e sampling period	The lower limit of periods cannot be set to a value higher than that in the [Period upper limit] box. When the lower limit of periods is set to [0] , the instrument ignores the value in the [Period lower limit] box, and the period-trigger condition is satisfied using the value in the [Period upper limit] box only.				
Period upper limit*	20,000 times or les period	s of the sampling	The higher limit of periods cannot be set to a value lower than that in the [Period lower limit] box.				
Event	With OR	1 [⊠] to 4,000	Allows you to enter the number of events. The instrument counts the number of times the period-trigger condition is satisfied. Only after the count reaches the specified number of events, an analog trigger is generated.				
	With AND	·	Not available				
Filter	Off [≌] , 10 to 10,000		Allows you to enter a filter width in the number of samples. Only after the period-trigger condition is continuously satisfied during the specified period, an analog trigger is generated. Specifying this option prevents the instrument from being unintentionally triggered due to noise.				

*: Configurable ranges of the period lower limit and period upper limit vary according to the sampling rates (periods).

Setting of the period range

The period range settings of the period trigger vary depending on the sampling periods (sampling rates).

(The setting value of the period range also changes in conjunction with the sampling period **[sampling rate]** setting.)

Select [Status] > [Condition] > [Sampling] and check the sampling rate setting.

To set the period-trigger condition such that it is satisfied when an input frequency exceeds the upper limit value (when the period becomes shorter)

Set **[Type]** to **[Period-in]** and set **[Period lower limit]** at **[0]**. The instrument ignores a value in the **[Period lower limit]** box, and the period-trigger condition is satisfied when an input frequency exceeds a value in the **[Period upper limit]** box.

To set the period-trigger condition such that only when an input frequency falls below the upper limit value (when the period becomes longer):


Set **[Type]** to **[Period-out]** and set **[Period lower limit]** at **[0]**. The instrument ignores a value in the **[Period lower limit]** box, and the period-trigger condition is satisfied when an input frequency falls below a value in the **[Period upper limit]** box.

[Period-out] trigger

The instrument calculates periods by monitoring times when an input signal crosses the specified level in the positive or negative direction, and the period-trigger condition is satisfied when a period exits the specified period range.


Points at which the period-trigger condition is satisfied varies depending on the specified period range and the period of a measuring object.

When an input signal period is shorter than the specified lower limit of periods (with the slope set to positive $[\nearrow]$).



The period-trigger condition is satisfied when a rising slope of an input signal crosses the specified level before the lower limit of periods elapses.

When an input signal period is longer than the specified upper limit of periods (with the slope set to positive [7])




The period-trigger condition is satisfied when the upper limit of periods elapses before a rising slope of an input signal crosses the reference voltage level.

Thus, points at which the period-out-trigger condition is satisfied varies depending on the upper limit of a period range.

5. [Glitch] trigger

The glitch-trigger condition is satisfied when a pulse width of an input signal that has crossed the specified level is shorter than the specified width. These triggers are disabled when the sampling rate is set at 200 MS/s.

The external sampling is cannot be set when the envelope is used. This trigger cannot be set when Model MR8990 is used.






	Setting		Description		
Level	-f.s. to +f.s. Default: 0 [⊠]				
Slope	", ∖		Allows you to choose which of the following points to use to detect glitches: two consecutive points at which a signal crosses the specified level while rising; or those while falling.		
Event	EventWith OR1 [™] to 4,000With ANDWidth2 times to 4000 times of the sampling period		Allows you to enter the number of events. The instrument counts the number of times the glitch-trigger condition is satisfied. An analog trigger is generated only after the count reaches the specified number of events.		
			Not available		
Width			Allows you to enter a pulse width (time), which is used to determine a glitch. The glitch-trigger condition is satisfied when a pulse width is shorter than the specified width. (The available setting range varies depending on the sampling periods. Lower limit: 2 times sampling period or more; Upper limit: 4000 times sampling period or less)		

5.7 Triggering the Instrument Using Logic Signals (Logic Trigger)

The section explains the logic trigger function.

- Input signals acquired across the logic channels serve as a trigger source.
- You can set a trigger pattern and trigger satisfaction condition by choosing between logical AND and OR operations. When the logic-trigger conditions are satisfied, a logic trigger is generated.
- With the trigger filter setting, no logic triggers are generated until the logic-trigger condition is continuously satisfied during the specified filter.

> [Trigger] > [Source]

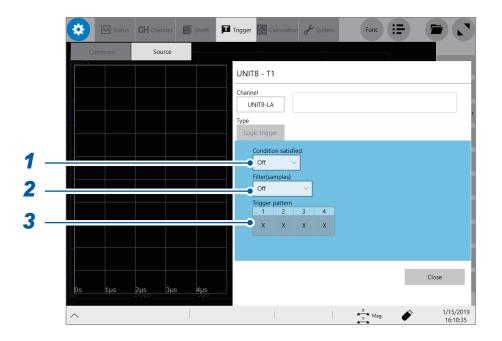

1 Tap the [Condition satisfied] box, and then choose a logic-trigger satisfaction condition from the list.

Off [∅]	Disables the logic trigger.
OR	The logic-trigger condition is satisfied when any one of logic input signals matches the trigger pattern.
AND	The logic-trigger condition is satisfied when all logic input signals match the trigger pattern.

2 Tap the [Filter] box, and then choose a sampling count of the filter from the list.

Only after the level-trigger condition is continuously satisfied during the specified period, an analog trigger is generated.

Configuring the trigger filter setting prevents a logic trigger from being unintentionally generated due to noise. (p. 151)

Off ^፼	Disables the trigger filter.
10 to 10000	Enables the trigger filter. Allows you to enter a filter width in the number of samples.

When the envelope is used


Off	Disables the trigger filter.
1 ms, 10 ms	Enables the trigger filter.

X	Ignores a signal.
0	The logic-trigger condition for each logic signal is satisfied when the signal is at a low level.
1	The logic-trigger condition for each logic signal is satisfied when the signal is at a high level.


3 Tap each of the signals under [Trigger pattern] to set a logic-trigger pattern.

Setting example

The logic-trigger conditions differ depending on the combination of the **[Condition satisfied]** setting (logical OR or AND operation) and the **[Trigger pattern]** setting as follows:

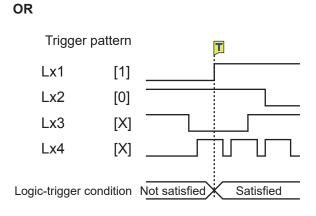

AND

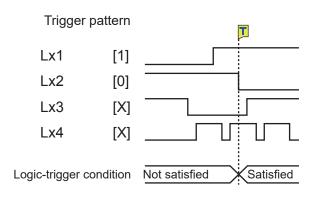


5.8 Triggering the Instrument at Regular Intervals (Interval Trigger)

Start triggers can be activated at specified intervals. Setting the recording mode to **[Repeat]** allows the instrument to record waveforms at regular intervals.

- When using the pre-trigger, the instrument starts monitoring interval-trigger times after the first pre-trigger time elapses since the start of measurement.
- No start triggers are activated by any interval triggers while the instrument is filling the pre-trigger memory. An interval trigger triggers the instrument while the instrument is waiting for a trigger after the instrument has filled the pre-trigger memory.
- Since the clock is internally corrected, displayed trigger times may not synchronize with the intervals of the interval trigger.


> [Trigger] > [Common]

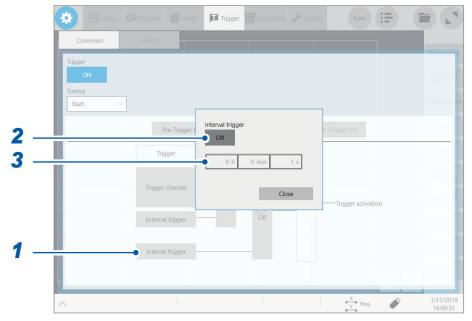

- **1** Tap [Interval trigger].
- **2** Tap [Interval trigger] to set it to [On].
- **3** Tap the [h], [min], and [s] boxes, and then enter a period of time for interval triggers. An internal trigger is generated at the start of measurement, and triggers are repeatedly generated at the specified intervals.

Acquiring data at regular intervals (relation between a time interval and a recording length or recording time)

The instrument is not triggered until having acquired data that has the specified recording length or recording interval.

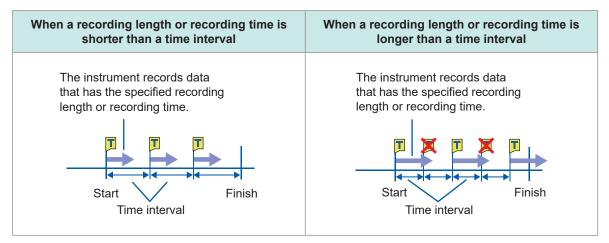


5.9 Externally Triggering the Instrument (External Trigger)

External signals applied to the external control terminals can serve as trigger sources. External signals can also be used to operate multiple instruments in synchronization with each other.

See "External trigger terminal (EXT.TRIG)" (p. 391).

5.10 Manually Triggering the Instrument (Forcible Trigger)

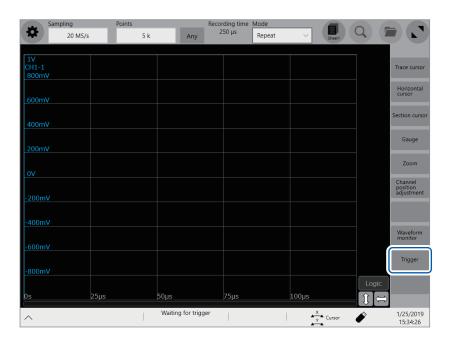

Tapping **[Trigger]** on the right side of the waveform screen allows you to manually trigger the instrument while the instrument is waiting for a trigger.

The forcible trigger triggers the instrument regardless of other trigger source settings.

To stop the recording, press the STOP key.

Press the key once: Stops the measurement once the instrument has acquired the specified recording length of data.


Press the key twice: Stops the recording immediately.

5.11 Triggering the Instrument Using CAN Signals (CAN Trigger)

The instrument can be triggered using CAN signals as a trigger source.


The instrument is triggered when the CAN signal that meets the set type and ID is inputted.

> [Trigger] > [CAN]

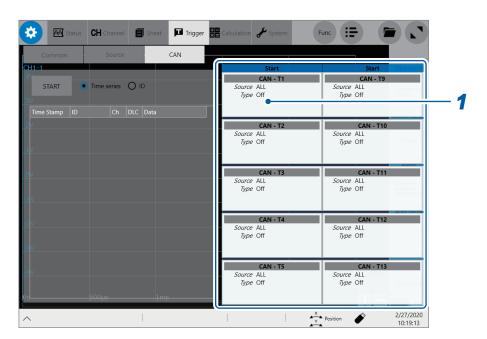

1 Tap a trigger source area you wish to configure.

The setting dialog box is displayed.

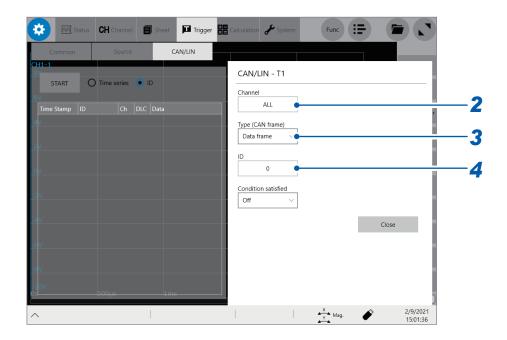

2 Tap the [Channel] box, and then from the list, choose a channel of which you wish to configure trigger conditions.

When [ALL] is selected, CAN signals inputted across any channels can trigger the instrument.

3 Tap the [Type] box, and then from the list, choose a trigger type.


Off[™], Data frame, Error frame, Remote frame

4 (When [Data frame] or [Remote frame] is set in the [Type] box) In the [ID(HEX)] box, enter a message ID set as the trigger source in hexadecimal.

Hexadecimal is a positional system that represents numbers using a base of 16. In addition to the ten numbers, 0 to 9, it uses the alphabets, A to F to represent values ten to fifteen, respectively.

Decimal	0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	
Hexadecimal	0	1	2	3	4	5	6	7	8	9	А	В	С	D	Е	F	10	

5 (When you choose [Data frame] in the [Type] box)

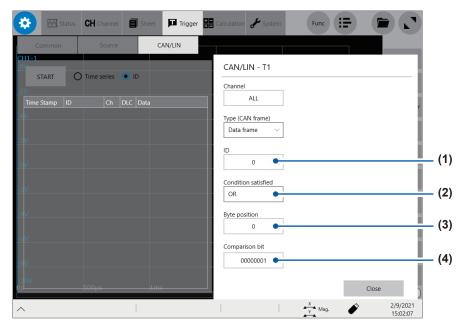

(1) Tap the [ID] box, and then set the message ID you wish to use as the trigger source. Use hexadecimal notation.

(2) Tap the [Condition satisfied] box, and then from the list, choose a CAN-trigger satisfaction condition.

Off [⊠]	Does not use the trigger pattern. The CAN-trigger condition is satisfied when a signal of the specified ID is input.
OR	The CAN-trigger condition is satisfied when any one of CAN input signals matches the trigger pattern.
AND	The CAN-trigger condition is satisfied when all CAN input signals match the trigger pattern.

(3) Tap the [Byte position] box, and then specify the byte location you wish to use as the trigger source.

0 to 63

X	Ignores a signal.
0	The CAN-trigger condition for each CAN signal is satisfied when the signal is at a low level.
1	The CAN-trigger condition for each CAN signal is satisfied when the signal is at a high level.

(4) Tap the [Comparison bit] box, and then set the CAN-trigger pattern.

The CAN-trigger conditions are defined, as with the logic-trigger conditions, depending on the combination of the condition setting of satisfaction and the trigger pattern setting. See "5.7 Triggering the Instrument Using Logic Signals (Logic Trigger)" (p. 158).

You can monitor CAN bus states by tapping [START] on the CAN trigger setting screen.

*	Kal Status	H Channel	Sheet Trigger	Calculation	✔ System	Func	
CAN	✓ C1	C2	C3 C4	C1	Sign	nal setting Send setti	ng
	START O TI	ime series 🛛 💿	D	Use On	Comment	Exec	Listics tal Cursor
Ti	me Stamp ID	Ch DLC	Data	Mode	Baudrate		
27	228477064	3 C1 2	FB 58	CAN	~ 50	0 kBaud	
1V-	228319778	2 C1 2	18 F9				Gauge
	228193621	1 C1 2	E9 E9				Zoom
ov	228626159	4 C1 2	E9 E9		cceptance Filter		
-17	128166024	5 C1 2	A3 52	$\left(\begin{array}{c} \leftarrow \\ Prev \end{array} \right)$	XXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXX	<i>iilter</i> (XXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXX	
-2V -3V				ACK Normal	~		
-4V				Driv	er		
05 -	050-0	500	750	1.25us			CAN frame
		_	> >				
						Cursor	3/13/2020 9:53:00


See "Monitor the state of the CAN/LIN bus." (p. 323).

Triggering the Instrument Using CAN Signals (CAN Trigger)

6 Search Function

Using the search function allows you to search measured data for positions where user-defined search conditions have been satisfied and displays search results.



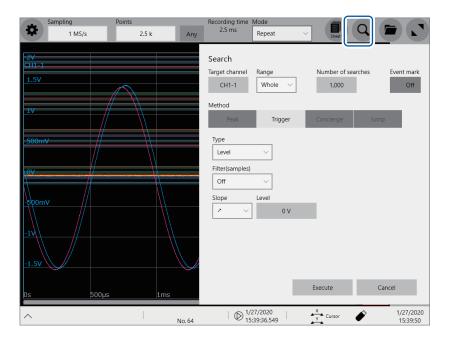

Operation available on the search screen

Peak search

You can choose from the maximum, minimum, local maximum (maximal), and local minimum (minimal) value to search for it. (p. 168)

Trigger search

You can set a trigger condition to search for positions where the condition is satisfied. (p. 171)

Memory HiConcierge

You can specify a fundamental wave to automatically detect differences from the fundamental wave based on a histogram or standard deviation. (p. 176)


Jump

You can jump to the specified time, trace cursor position, section cursor position, event number, trigger point, or search mark. (p. 179)

6.1 Searching For Peak Values

You can choose any one of the maximum, minimum, maximal, and minimal values and search measured data for it.



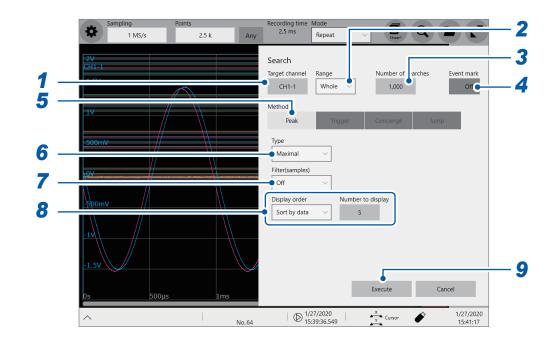

- **1** Tap the [Target channel] box, and then from the channel setting dialog box, choose a channels to be searched for values.
- **2** Tap the [Range] box, and then choose an option for the search range from the list.

Whole [⊠]	Searches whole waveform for values.
Segment 1, Segment 2	Search a range specified as Segment 1 or Segment 2 for values.

See "2.2 Specifying the Waveform Range (Section Cursor)" (p. 35).

- **3** Tap the [Number of searches] box, and then enter the number of search results.
- **4** Tap the [Event mark] box to set whether to display event marks at positions where userdefined search conditions have been satisfied.

On ^ℤ	Displays event marks.	
Off	Does not display event marks.	

5 In the [Method] area, tap [Peak] to choose a search method for searching for peak values.

6 Tap the [Type] box, and then from the list, choose a value type to be searched for.

Maximum [⊠]	Allows you to search for the maximum value.	
Minimum	llows you to search for the minimum value.	
Maximal	Allows you to search for maximal values. When the envelope is used, the instrument searches maximum value data for maximal values.	
Minimal	Allows you to search for minimal values. When the envelope is used, the instrument searches minimum value data for minimal values.	

• If search results have two or more maximum or minimum values, the instrument displays any one of them as a representative value among the search results.

· Search results have multiple maximal or minimal values

7 (When you choose [Maximal] or [Minimal] in the [Type] box)

Tap the [Filter(samples)] box, and then from the list, choose a decision condition for maximal or minimal values.

Off [⊠]	Regards a value as a maximal value when it is larger than the values found one point before and after, and a minimal value when it is smaller.
10 to 10,000	Regards a value as a maximal value when it is larger than any other value in the range between the specified points before and after, and a minimal value when it is smaller.

8 (When you choose [Maximal] or [Minimal] in the [Type] box)

Tap the [Display order] box, and then from the list, choose a sequence to sort.

Sort by time [⊠]	Displays the search results in chronological order. You cannot set the [Number to display] box. The instrument handles up to 1000 search results. The instrument stops the search if it retrieves more than 1000 results.
Sort by data	With the [Maximal] setting, displays search results the number of which is specified in the [Number to display] box in descending order. With the [Minimal] setting, displays them in ascending order.

(When you choose [Sort by data] in the [Display order] box)

Tap the [Number to display] box, and then enter the number of search results to be displayed.

9 Tap [Execute].

The instrument puts search marks ([S]) on positions where the search condition is satisfied. The [Search Pos.] switching panel appears on the waveform screen.

To stop the search

Press the **STOP** key.

6

10 Change retrieved positions using the [Search Pos.] switching panel and check the search results.

You can change retrieved positions by tapping [<] or [>]. The display order follows the setting in the [Display order] box.




[Trace cursor]

Set to [On] to move the trace cursor H to the retrieved positions.

[Event mark]

Set to [On] to place event marks () to the retrieved positions.

Tapping **[Next]** executes another search beginning from the next point of the retrieved position presently displayed. The instrument discards a previous search result.

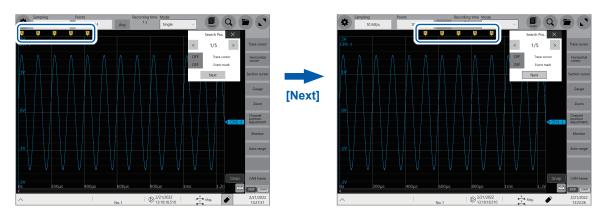

To specify a retrieved position and jump there


As described in "6.4 Jumping to the Specified Position" (p. 179), choose **[Search number]** in the **[Type]** box, and then tap **[Execute]**.

6.2 Searching For Positions Where a Trigger Condition Is Satisfied


Setting a trigger condition allows you to search measured data for positions where the trigger condition is satisfied.




1 Tap the [Target channel] box, and then from the channel setting dialog box, choose a channel to be searched for positions where a trigger condition is satisfied.

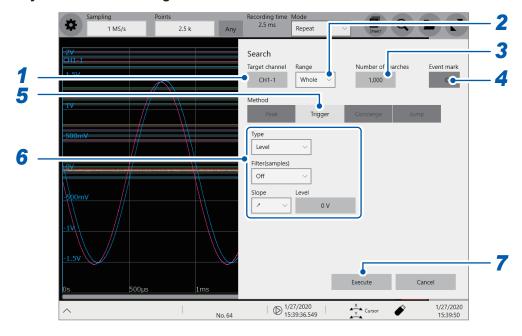

When you choose an analog channel



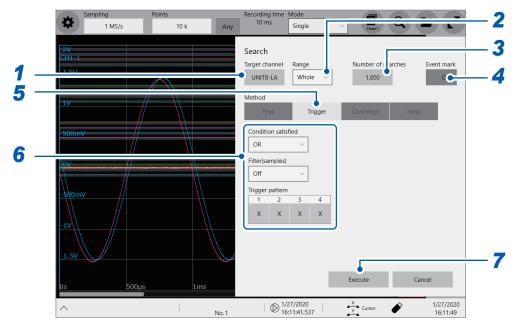

2 Tap the [Range] box, and then from the list, choose an option for a range to be searched for positions where a trigger condition is satisfied

Whole [⊠]	Allows you to search whole waveform.	
Segment 1, Segment 2	Allows you to search the scope specified as Segment 1 or Segment 2.	

- **3** Tap the [Number of searches] box, and then enter the number of search results.
- **4** Tap the [Event mark] box to set whether to display event marks at positions where userdefined search conditions have been satisfied.

On [⊠]	Displays event marks.	
Off	Does not display event marks.	

5 In the [Method] area, tap [Trigger] to choose a search method for searching for triggers.

6 Set a search condition.

-1. When you choose an analog channel under [Target channel] Tap the [Type] box, and then from the list, choose a trigger type to be searched for.


Level [∅]	Allows you to enter a level and search for positions where a waveform crosses the level.
In	Allows you to enter an upper and lower limit values to specify a range and search for positions where a waveform falls within the range.
Out	Allows you to enter an upper and lower limit values to specify a range and search for positions where a waveform exits the range.

Setting a search condition.

Items to be set may vary depending on trigger types.

(1) When you choose [Level]

Measurement method: [Normal]




The point where the max. crosses the level The point where the min. crosses the level

172

Setting		Description
Filter	Off [€] , 10 to 10,000	Allows you to enter a filter width in terms of the number of samples. Positions where a search condition is continuously satisfied during the specified period are determined to be the retrieved positions.
Slope	, , ,	Allows you to choose which of the following points to search for, points at which a signal crosses the specified level while rising or those while falling.
Level	-3.4028E+38 to 3.4028E+38 Default: 0 [⊠]	Allows you to enter a threshold (level) to be searched for.

(2) With the [In] or [Out] setting

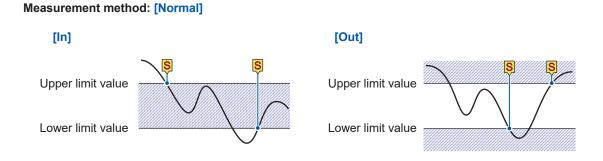


[Out]

Upper limit value

Lower limit value

Measurement method: [Envelope]



The points where either the max. or min. value falls within the range.

The points where either the max. or min. value gets outside the range.


Maximum

Minimum

Setting		Description
Filter	Off ^ℤ , 10 to 10,000	Allows you to enter a filter width in terms of the number of samples. Positions where a search condition is continuously satisfied during the specified period are determined to be the retrieved positions.
Upper limit value	-3.4028E+38 to 3.4028E+38 Default: 0.2 [⊠]	Allows you to enter an upper limit value.
Lower limit value	-3.4028E+38 to 3.4028E+38 Default: -0.2 [⊻]	Allows you to enter a lower limit value.

-2. When you choose a logic channel under [Target channel]

The instrument searches for positions where signals match the specified pattern. You cannot use this function when the envelope function is used.



Setting		Description
Condition satisfied	OR [⊠]	Positions where any one of the signals matches the specified search patterns are determined to be retrieved positions.
	AND	Positions where all signals match the specified patterns are determined to be retrieved positions.
Filter	Off [⊠] , 10 to 10,000	Allows you to enter a filter width in the number of samples. Positions where a search condition is continuously satisfied during the specified period are determined to be the retrieved positions.
Trigger pattern	X	Ignores data.
	0	Searches for low-level positions.
	1	Searches for high-level positions.

For the logic search, a retrieved position is a point where a condition that has not been satisfied changes to being satisfied. Thus, even if signals match a search pattern at the start of a search, it is not regarded as a retrieved position.

7 Tap [Execute].

The instrument puts search marks ([S]) at positions where a search condition is satisfied. Up to 1000 positions can be retrieved. The instrument stops the search if it finds more than 1000 positions. The retrieved position switching panel appears on the waveform screen.

To stop the search

Press the **STOP** key.

8 Change retrieved positions using the [Search Pos.] switching panel to check search results.

You can change retrieved positions by tapping [<] or [>]. The display order follows the setting in [Display order].




[Trace cursor]

Set to [On] to move the trace cursor H to the retrieved positions.

[Event mark]

Set to **[On]** to place event marks (**E**) to the retrieved positions.

Tapping **[Next]** executes another search beginning from the next point of the retrieved position presently displayed. The previous search result is discarded.

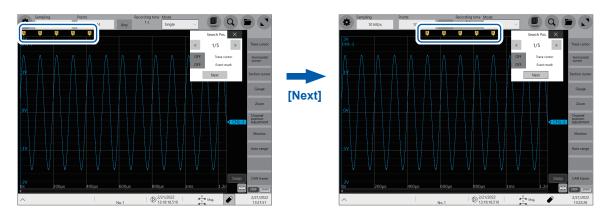

To jump to a specified retrieved position


As described in "6.4 Jumping to the Specified Position" (p. 179), choose [Search number] in the [Type] box, and then tap [Execute].

6.3 Searching For Differences from a Fundamental Wave (Memory HiConcierge)

You cannot use this function when the envelope function is used.

Using Memory HiConcierge allows you to detect differences from the specified fundamental waveform based on a histogram or standard deviation.



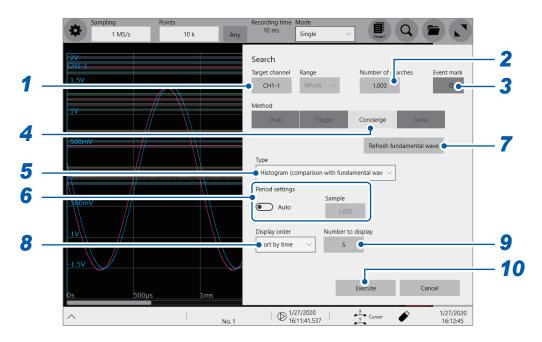

- **1** Tap the [Target channel] box, and then from the channel setting dialog box, choose a channel to be searched for differences.
- 2 Tap the [Number of searches] box, and then enter the number of search results.
- **3** Tap the [Event mark] box to set whether to display event marks at positions where userdefined search conditions have been satisfied.

On [⊠]	Displays event marks.		
Off	Does not display event marks.		

4 In the [Method] area, tap [Concierge] to set the search method to Concierge.

5 Tap the [Mode] box, and then from the list, choose a type to be searched for.

Histogram (comparison with fundamental wave) [⊠]	Searches for differences from the specified fundamental wave based on a histogram.
Histogram (comparison with previous waveform)	Searches for differences from the previous waveform based on a histogram.
Standard deviation (comparison with fundamental wave)	Searches for differences from the specified fundamental wave based on a standard deviation.
Standard deviation (Compared with previous waveform)	Search for differences from the previous waveform based on a standard deviation.

Memory HiConcierge searches a whole measured waveform for differences. You cannot specify a segment to be searched.

6 Use the [Period settings] toggle switch to choose a period setting used for searches.

Auto [⊠]	Automatically detects the period.
Any	Allows you to tap the [Sample] box to enter the number of samples, which specifies a period.

With the **[Auto]** setting, the instrument may not be able to determine a period depending on measured waveforms. If a fundamental wave have an unintended form, change this setting to **[Any]** and specify a period in terms of the number of samples in the **[Sample]** box.

7 Tap [Refresh fundamental wave] to display a fundamental wave.

The instrument extracts a fundamental wave from the specified period and displays the wave on the screen.

8 Tap the [Display order] list and choose a display order from the list.

Sort by time [⊠]	Displays retrieved positions in chronological order.		
Sort by data	Displays retrieved positions in order of decreasing difference from a comparison target (fundamental wave or previous waveform).		

9 Tap [Number to display] box and enter the number of retrieved points to be displayed.

10 Tap [Execute].


The instrument puts search marks (\mathbb{S}) at positions where a search condition is satisfied. The retrieved position switching panel appear on the waveform screen.

To stop the searching

Press the STOP key.

11 Change retrieved positions using the [Search Pos.] switching panel to check search results.

You can change the retrieved positions by tapping [<] or [>]. The display order follows the setting in [Display order].




[Trace cursor]

Set to [On] to move the trace cursor H to the retrieved positions.

[Event mark]

Set to [On] to place event marks () to the retrieved positions.

Tapping **[Next]** executes another search beginning from the next point of the search result. The previous search result is discarded.

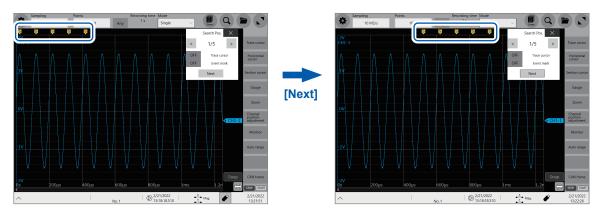


To jump to a specified retrieved position

As described in "6.4 Jumping to the Specified Position" (p. 179), choose [Search number] in the [Type] box, and then tap [Execute].

6.4 Jumping to the Specified Position

You can jump to the specified time, trace cursor position, section cursor position, event number, trigger point, or search mark.



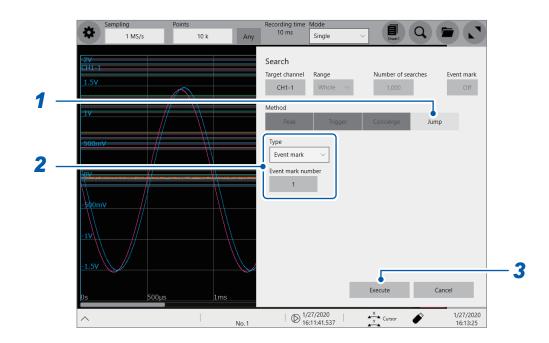

1 In the [Method] area, tap [Jump] to set the search method to the jump method.


2 Tap the [Type] box, and then from the list, choose a type to jump to.

Event mark [⊠]	Allows you to enter an event number to jump to in the [Event mark number] box.		
Cursor	Allows you to choose a position, at which a trace cursor or section cursor is specified, to jump to.		
Time	Time	Allows you to enter an absolute time to jump to when ([System] > [Env.] >) [Time value display] is set to [Date].	
	Time from trigger point	Allows you to enter a time relative to the trigger point to jump to when ([System] > [Env.] >) [Time value display] is set to [Time] or [Mod 60].	
	Points	Allows you to enter the number of points to jump to in the [Points] box when measurement is performed using the external sampling or when ([System] > [Env.] >) [Time value display] is set to [Samples].	
Trigger	Jumps to the start or stop trigger point.		
Search number	Allows you to enter a search number to jump to in the [Search number] box.		

3 Tap [Execute].

The instrument put search marks ([S]) at positions where the search condition is satisfied. When **[Type]** is set to **[Event mark]**, you can jump to an event mark ([E]) position. When **[Type]** is set to **[Search number]**, you can jump to a search mark ([S]) position. The jump-destination switching panel appears on the waveform screen.

4 Change jump destinations using the [Search Pos.] switching panel to check jump results. You can change the retrieved positions by tapping [<] or [>].



[Trace cursor]

Set to [On] to move the trace cursor H to the retrieved positions.

[Event mark]

Set to [On] to place event marks to the retrieved positions.

Numerical Calculation Function

The instrument performs calculations using acquired waveform data to numerically displays calculation results on the waveform screen. The instrument can evaluate these calculation results on a pass/fail basis.

No numerical calculation is available when the envelope is used.

> [Calculation] > [Numerical calculation]

	AA Status	CH Channel	Sheet Trigger	Calculation 🖋 Sy	stem Func		
		Real-time waveform calculation	Waveform calculation	FFT calculation			-
	erical calculation	n Judge stop condi PASS & FAIL				Numeri E Calculation	xecute
No.1	Type Off					Execute Calculation	Section curse
No.2	Type Off						Gauge
No.3	Type Off						Zoom
No.4	Type Off						Channel position adjustment
-20mV -2 No.5	Type Period Area Whole Stat.	Judge On V Up Low	Target channel UNIT1 12 UNIT2 12 UNIT3 12 UNIT4 123	UNITS 1234 UNITE 1234 UNITE 1234 UNITE 12 UNITE 12	RealTime 12346 Calc.	678	Auto range
-40mV	Тор	 ✓ -1 	Level S 0	lope Filter(samples)	~		
0 No.6	Type	Sus	10µs	15µs	20µs	$1 \Leftrightarrow$	
^					Y Mag.	ø	1/15/2019 15:42:28

Operation available on the [Numerical calculation] screen

Numerical calculation		
Average	Pulse width	Angle of XY waveform
• RMS	Duty ratio	CAN statistics
• P-P	Pulse count	(33 types in total)
Maximum	 Arithmetic operations 	
Time to maximum	Time difference	 Calculation using data between
Minimum	Phase contrast	section cursors
Time to minimum	High level	Numerical calculations can be
Period	Low level	performed for data within the
Frequency	 Intermediate value 	range specified with section
Rise time	Amplitude cursors.	
Fall time	Overshoot	
 Standard deviation 	Undershoot	For details on arithmetic
• Area	• +Width	expressions, refer to "Calculation
• X-Y area	• –Width	target channels and setting contents
Time to level	Burst width	of calculation conditions for each
Level at time	Accumulation	calculation type" (p. 187).

Evaluating numerical calculation results on a pass/fail basis(p. 197)

Evaluating numerical calculation results by comparing them with specified reference ranges, giving pass or fail judgments.


The instrument can simultaneously execute up to 32 types of numerical calculations. When the scaling function is enabled, the instrument performs calculations using scaled values.

7.1 Numerical Calculation Procedure


The following two methods are available:

c	Automatically performing calculations after neasurement	The numerical calculation settings must be configured before starting a measurement (not available when the real-time saving is set to on).		
	Performing calculations using existing data	The instrument can perform calculations using waveform data that has already been acquired and that saved on storage devices.		

Performing calculation during measurement

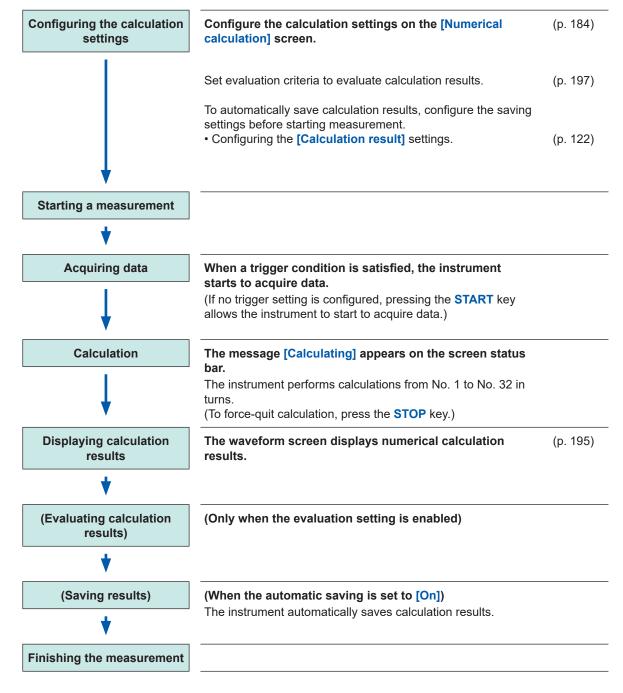

Performing calculations using existing data

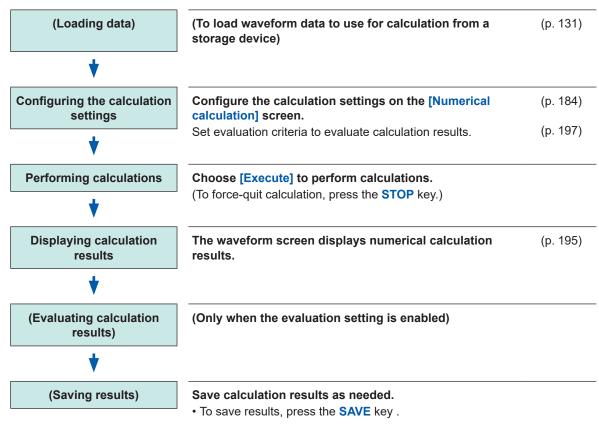


To specify a calculation range and perform calculation

Before performing calculation, specify a calculation range using section cursors on the waveform screen. Set **[Area]** to **[Segment 1]** or **[Segment 2]** on the **[Numerical calculation]** screen. See "2.2 Specifying the Waveform Range (Section Cursor)" (p. 35) and "7.2 Configuring the Numerical Calculation Settings" (p. 184)

7.2 Configuring the Numerical Calculation Settings

> [Calculation] > [Numerical calculation]

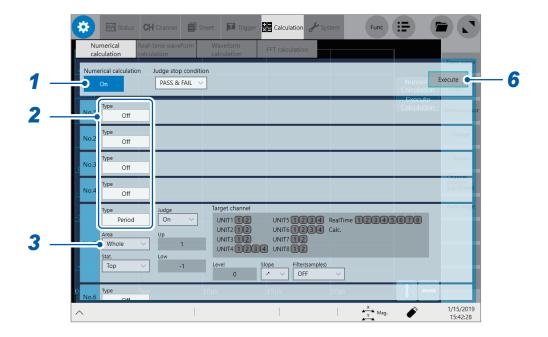

1 Tap the [Numerical calculation] button to set it to [On].

2 Tap the [Type] box, and then choose a calculation type from the list.

Off [⊮]	The instrument does not perform any calculation.		
Average	Average value of waveform data		
RMS	RMS value of waveform data		
P-P	Peak-to-peak value of waveform data		
Maximum	Maximum value of waveform data		
Time to maximum	Period of time elapsed from a trigger point to the time of the maximum value		
Minimum	Minimum value of waveform data		
Time to minimum	Period of time elapsed from a trigger point to the time of the minimum value		
Period* ²	Period of waveform data		
Frequency* ²	Frequency of waveform data		
Rise time*1	Rise time of waveform data		
Fall time*1	Fall time of waveform data		
Standard deviation	Standard deviation of waveform data		
Area	Area enclosed by the horizontal axis and waveform data		
X-Y area	Area enclosed by an XY composite curve		
Time to level*2	Period of time elapsed from a trigger point to the time when waveform data reached the specified level		
Level at time* ²	Measured value when the specified time has elapsed from a trigger point		
Pulse width*2	Pulse width of waveform data		
Duty ratio*2	Duty ratio of waveform data		
Pulse count*2	Pulse count of waveform data		
Arithmetic operations	Four arithmetic operations of numerical calculation results		
Time difference*2	Time lag between phenomena A and B		
Phase contrast* ²	Time lag between phenomena A and B represented as a phase difference		
High level ^{*1}	High level of waveform data		
Low level*1	Low level of waveform data		
Intermediate value	Intermediate value of waveform data		
Amplitude*1	Amplitude value of waveform data		
Overshoot*1	Overshoot value of waveform data		
Undershoot*1	Undershoot value of waveform data		
+Width* ¹	Time value above the intermediate level		
-Width*1	Time value below the intermediate level		
Burst width*2	Burst width of waveform data		
Accumulation	Accumulated value of waveform data		
Angle of XY waveform	Slope angle of a regression line on an XY composite curve		
CAN statistics	Average, minimum, and maximum values of CAN signals' arrival time intervals		

*1: Unable to perform any calculations using data acquired across the measurement channels of Model MR8990 Digital Voltmeter Unit.

*2: The settings can also be configured for the logic channels.

See "Calculation target channels and setting contents of calculation conditions for each calculation type" (p. 187).

3 Tap the [Area] box, and then from the list, choose an option for a save range.

You can specify a calculation range for each calculation.

Whole [⊠]	Performs calculations using whole waveforms.		
Segment 1	Performs calculations using waveforms between cursors of Segment 1.		
Segment 2	Performs calculations using waveforms between cursors of Segment 2.		
After Trigger	Performs calculations using waveforms obtained after the trigger.		

When choosing [Segment 1] or [Segment 2], specify a calculation range with section cursors on the waveform screen.

See "2.2 Specifying the Waveform Range (Section Cursor)" (p. 35).

When the instrument does not acquire any waveforms, perform another measurement and specify a range. Doing so allows you to perform calculations using data acquired within the specified range from the next measurement.

4 Tap a calculation target channel.

The channel selection screen appears. See "Calculation target channels and setting contents of calculation conditions for each calculation type" (p. 187).

5 Set calculation conditions.

See "Calculation target channels and setting contents of calculation conditions for each calculation type" (p. 187).

6 (To perform calculation using existing data)

Tap [Execute].

(To automatically perform calculation using acquired data after measurement) Press the START key.

Calculation target channels and setting contents of calculation conditions for each calculation type

Туре	Setting	Description	Sample screen
Average RMS P-P Maximum Time to maximum Minimum	Target channel (Analog, real-time calculation, waveform calculation)	Allows you to specify calculation target channels.	
Time to minimum Standard deviation Area High level Low level Intermediate value Amplitude Overshoot Undershoot Accumulation	With the [Area] or [Accumulation] setting, set [Method] . (Total [⊠] , Absolute value, Positive, Negative)	Calculates an area or accumulation according to the method you specify here.	Type Judge Target channel Average Off V UNITS 1234 Avea UNITS 1236 UNITS 1234 Whole V UNITS 1236 UNITS UNITS 1236 UNITS UNITS 1236 UNITS

Туре	5	Setting		Description	Sample screen
Period Frequency Pulse width Duty ratio	Target channel (Analog, logic, real-time calculation, waveform calculation)			Allows you to specify channels as calculation targets.	
	Level*			The instrument performs calculations using values based on a period of time when a waveform crossed the level specified here. No setting is available for logic channels.	
	Slope No slope c be specifie	d for	, ∞	Performs calculations using values based on a period of time when a waveform crossed the specified level while rising.	
	calculating the duty ratio.	the	X	Performs calculations using values based on a period of time when a waveform crossed the specified level while falling.	
	Filter(samples) (Off [⊠] , 10 to 10,00	10)	Allows you to enter duration used to determine that a waveform crosses the specified level. Only after a waveform has crossed the level and has never crossed the level again during the specified filter duration, the instrument determines that the waveform has crossed the level. This is useful to eliminate false level-crossing events caused by noise.	Type Judge Target channel Period Off UNIT1 12 UNIT5 12 3 d Minole UNIT1 12 3 d UNIT5 12 3 d Whole UNIT2 12 3 d UNIT5 12 3 d Stat: UNIT5 12 3 d UNIT5 10 3 d Top Iterval Stope 0 Iterval OFF	
	Stat. Top [⊠]			Detects a value obtained first from the beginning within the specified range.	
	N	Average Max Min		Calculates the average, maximum, or minimum value for each parameter within the specified range.	
	Times		Calculates the value when the number of times a waveform crosses the level reaches the specified number from the beginning within the specified range.		

Туре		Setting	Description	Sample screen
Rise time Fall time			Allows you to specify calculation target channels.	
			Allows you to specify which part of a waveform between the upper and lower limits is used for calculating the rise time (or fall time). A rise time (or fall time) is calculated based on the percentage, which is specified here, of the range between the upper and lower limit values.	Type Target channel Rise time Off V UNT11 12 UNTS 12 2 4 Mras UNT2 12 3 4 UNT2 12 3 4 UNT3 12 3 4 13 4 13 12 14 14 12 14 12 14 12 14 12 12 12 14 12
	Stat.	Тор [⊠]	Detects the value obtained first from the beginning within the specified range.	Stat: UNIX4 (JAZ/JAJA) UNIX8 Top ✓ Time 5 % → 95 %
		Average	Calculates the average,	
		Мах	maximum, or minimum value for each parameter within the	
		Min	specified range.	
	Times		Calculates the value when the number of times a waveform crosses the level reaches the specified number from the beginning within the specified range.	
X-Y area Angle of XY waveform			Allows you to assign channels to the X- and Y-axis.	Type Judge Target channel Angle of XY Off V X Waveform X CH(1, 1)
			Calculates an XY area according to a calculation method.	Arra CH(1, 1)

Туре	Se	tting	Description	Sample screen
Time to level Pulse count	Target chan (Analog, logi calculation, v calculation)	c, real-time	Allows you to specify calculation target channels.	
	Times (Phase contr	ast only)	Detects the time when the number of times a waveform crossed the specified level reaches the specified number.	
	Level*		Detects the time when a waveform crossed the level specified here or a pulse count that crossed the level. No setting is available for logic channels.	
	Slope	¥ ∅	Detects a time when a waveform crossed the level specified here while rising or a pulse count that crossed the level while rising.	Type Judge Target channel Time to level Off UNIT1 12 UNIT5 12/3/4 Area UNIT2 12/3/4 UNIT6 12/3/4 UNIT6 12/3/4 Whole UNIT4 12/3/4 UNIT6 11/2/3/4 UNIT6 11/2/3/4
			Detects the time when a waveform crossed the level specified here while falling or a pulse count that crossed the level while falling.	0 2 OFF
	Filter(samples) (Off [⊠] , 10 to 10,000)		Allows you to enter duration used to determine that a waveform crosses the specified level. Only after a waveform has crossed the level and does not cross the level again within the specified filter duration, the waveform is considered to have crossed the level. This is useful to eliminate false level-crossing events caused by noise.	
Level at time	Target channel (Analog, logic, real-time calculation, waveform calculation)		Allows you to specify calculation target channels.	
	Method		Allows you to set the time- specifying method.	
	Time [⊭]	Time	Allows you to enter a time for obtaining a measured value with the trigger point position fixed at zero.	Type Judge Target channel Level at time Off UNIT1 1/2 UNIT5 1/2/3/4 Vrss UNIT2 1/2/3/4 UNIT5 1/2/3/4 UNIT2 1/2/3/4 UNIT5 1/2/3/4
	Calc. No. Calculation No.		Allows you to choose a calculation number when you use numerical calculation results. You cannot specify any number equal to or more than the calculation number you specified. Specifying a range using Segment 1 and Segment 2 is not available.	Whole UNIT 1 2 3 4 UNIT UNIT 1 2 3 4 UNIT 1 UNIT 1 2 3 4 UNIT 1 1 1 1 2 3 4 UNIT 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1

Туре		Setting	Description	Sample screen
+Width -Width	(Analog	channel g, real-time tion, waveform tion)	Allows you to specify calculation target channels.	
		samples) 10 to 10,000)	Allows you to enter duration used to determine that a waveform crosses the specified level. Only after a waveform has crossed the level and does not cross the level again within the specified filter duration, the waveform is considered to have crossed the level. This is useful to eliminate false level-crossing events caused by noise.	Target channel UNITS [] 2 3 4 +Width Off UNITS [] 2 3 4 Mras UNITS [] 2 3 4 UNITS [] 2 3 4 Whole UNITS [] 2 3 4 UNITS [] 2 3 4 Stat Fillertamples) Fillertamples)
	Stat.	Тор [⊠]	Detects the value obtained first from the beginning within the specified range.	
		Average	Calculates the average,	
		Max	maximum, or minimum value	
		Min	for each parameter within the specified range.	
	Times		Calculates the value when the number of times a waveform crosses the level reaches the specified number from the beginning within the specified range.	

Туре	5	Setting		Description	Sample screen
Burst width	(Analog, logic, real-time calculation, waveform calculation)			Allows you to specify calculation target channels.	
	Slope (Logic char only)	(Logic channels		Detects rising edges and calculates a burst width. Detects falling edges and calculates a burst width.	-
	Filter(samples) (Off [⊠] , 10 to 10,000)			Allows you to enter duration used to determine that a waveform crosses the specified level. Only after a waveform has crossed the level and does not cross the level again within the specified filter duration, the waveform is considered to have crossed the level. This is useful to eliminate false level-crossing events caused by noise.	Type Judge Target channel Burst width Off UNIT1 12 UNIT5 12 (34) Area UNIT2 11 (23) (4) UNIT6 12 (34) UNIT3 12 (32) (32) (4) UNIT6 12 (34)
	Burst end filter(samples) (Off [⊠] , 10 to 10,000)			Allows you to set duration used to determine whether a waveform is a burst signal. If a waveform falls within the window level range and remains in the range longer than the specified filter duration, the instrument determines the detected period to be a burst duration.	Whole UNI3 12 23 44 UNI7 Stat. UNI4 12 34 UNI8 11 Top Fiber(sample) Burst end fiber(samples) OFF OFF OFF
	Window-level range* (Up , Low)			Allows you to enter an upper and lower limit values used to determine whether a waveform is a burst signal.	
	Stat. 1	Гор		Detects the value obtained first from the beginning within the specified range.	
	4	Average		Calculates the average,	
		Max Min		maximum, or minimum value for each parameter within the specified range.	
	Times			Calculates the value when the number of times a waveform crosses the level reaches the specified number from the beginning within the specified range.	

Туре		Setting	Description	Sample screen
Time difference Phase contrast	channel		Allows you to specify the reference channel and the target channel.	
	Level*		The instrument calculates values based on times when a waveform crossed the level specified here. This setting is not available for logic channels.	
	Slope		Performs calculations using values based on a period of time when a waveform crossed the specified level while rising.	
		×	Performs calculations using values based on a period of time when a waveform crossed the specified level while falling.	
	Filter(samples) (Off [⊠] , 10 to 10,000)		Allows you to enter duration used to determine that a waveform crosses the specified level. Only after a waveform has crossed the level and does not cross the level again within the specified filter duration, the waveform is considered to have crossed the level. This is useful to eliminate false level-crossing events caused by noise.	Type Judge Reference channel Level Stope Area Off CH(1, 1) 0 Z Whole V Target channel UNITS 12.3.4 UNITS 12.3.4 Stat UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 Top UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 Level State State State UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4 UNITS 17.2.3.4
	Method (Phase contrast only)	0° to 360°	Displays phase difference using the angle range of 0° to 360°.	
		–180° to 180°	Displays phase difference using the angle range of –180° to 180°.	
	Stat. T	Top [⊮]	Detects the value obtained first from the beginning within the specified range.	
		Average	Calculates the average,	
		Мах	maximum, or minimum value	
		Min	for each parameter within the specified range.	
	Times			

7

Туре	Setting	Description	Sample screen	
Arithmetic operations	Calculation number 1, Calculation number 2 (No. 1 to No. 15)	Allows you to specify two numerical calculation numbers to use for calculations.		
	Target channel	Allows you to specify a target channel that has a numerical calculation number to use for calculations.	Dype Judge Calculation number 1 Channel Arithmetic operations Off V No.1 CH(1, 1) +	
	Operator (+, -, ×, ÷)	Allows you to choose among the four basic arithmetic operations.	-	
CAN stat.	Target channel (C1 to C4)	Allows you to specify a CAN channel used as the calculation target.	Type Judge larget Channel CAN stat. Off ✓ C1	
	ID (0 to 1FFFFFF)	Allows you to specify a CAN channels as calculation targets in hexadecimal notation.	Whole V D 0	

- With the [Period], [Frequency], [Rise time], and [Fall time] calculations, the instrument may not be able to perform calculations depending on the condition of waveform data.
- With the **[Period]** and **[Frequency]** calculation, correct measurement results may not be obtained if the filter setting is close to half the period (an integer multiple of an actual period may be calculated).
- When the scaling is enabled, the instrument scales waveform data before calculation. Units for parameter values are those set in the scaling function.
- If a waveform across a calculation target channel exceeds the measurable range (overrange waveform), the instrument substitutes the upper or lower measurement limit for values that exceed the measurable range before calculation.

See "3.2 Converting Input Values (Scaling Function)" (p. 56).

Settings: Calculations for which [Stat.] can be set


Period, frequency, rise time, fall time, pulse width, duty ratio, time lag, phase contrast, +Width, -Width, and burst width

Top [⊠]	Performs calculations within the calculation range in the initial condition.
Average	Calculates the average value of calculation results for data within the calculation range.
Мах	Calculates the maximum value of calculation results for data within the calculation range.
Min	Calculates the minimum value of calculation results for data within the calculation range.
Times	Calculates the value when the number of times a waveform crosses the level reaches the specified number for data within the calculation range.

Displaying numerical calculation results

This section describes how to check calculation results on the waveform screen.



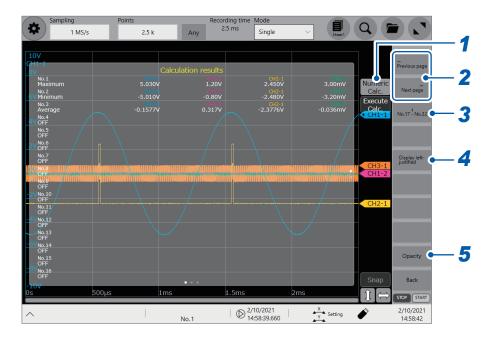

1 Tap [Numerical calculation].

Every time you tap it, the numerical calculation result screen appears or hides. If the instrument cannot calculate the periods or discontinue the calculations, results are expressed as the string [******].

The results of channels not set as calculation targets are expressed as the sign [-].

2 Tap [Previous page] or [Next page].

If the instrument cannot display some of the results of all channels' numerical calculations on a single screen, you can switch over the page.

3 Tap [No.1 – No.16] or [No.17 – No.32].

A single screen can display 16 types of numerical calculation results. Every time you tap either, the the numerical calculation results switches between those for Nos. 1 through 16 and those for Nos. 17 through 32.

4 Tap [Align the columns of channels] or [Display left-justified].


Every time you tap either, alignment of numerical calculation results is switched.

If you choose [Align the columns of channels], the results including those of channels not set as calculation targets are displayed as well.

If you choose **[Display left-justified]**, results of channels only set as calculation targets are displayed in left alignment.

5 Tap [Opacity].

The function keys switch over to those for opacity adjustment of the numerical calculation result screen's background.

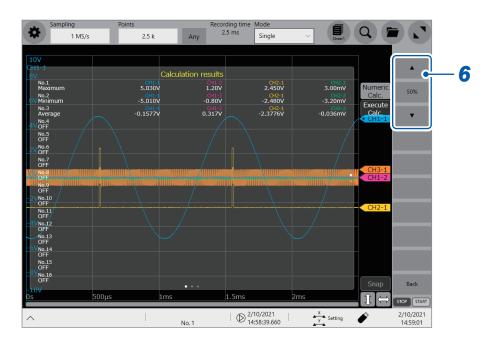

6 Tap [▲] or [▼].

Pressing either key can adjust the opacity of the numerical calculation result screen's background between 0% and 100% in step of 10 percent points.

To save the calculation results after the measurement


See "Freely choosing data items to be saved and save files (SAVE key)" (p. 127).

7.3 Evaluating Calculation Results on a Pass/Fail Basis

You can specify evaluation criteria ([Up] and [Low]) to evaluate numerical calculation results on a pass/fail basis.

Each numerical calculation can has different evaluation criteria.

The waveform acquisition process varies depending on the recording mode setting ([Single] or [Repeat]) and the stop condition specified to stop measurement according to an evaluation ([PASS], [FAIL], or [PASS & FAIL]).

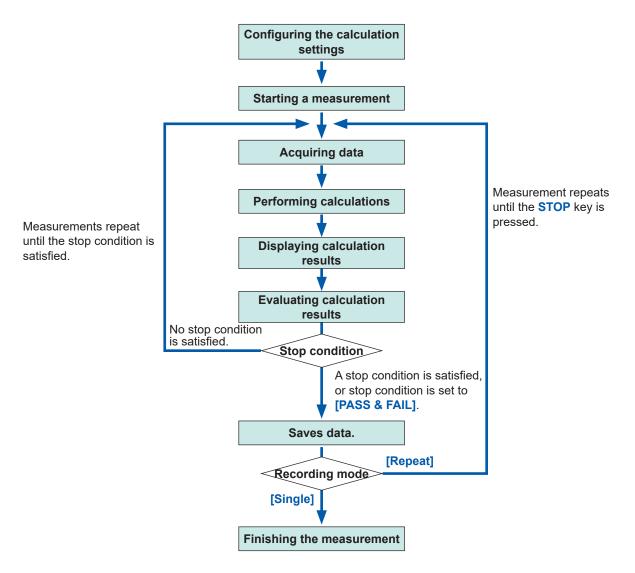

Automatic saving is not carried out until the stop condition is satisfied at the end of calculation evaluation.

> [Calculation] > [Numerical calculation]

*	A Status	CH Channel	Sheet Trigger	Calculation	System Func		
	lumerical alculation	Real-time waveform calculation	Waveform calculation	FFT calculation			
4 Nur	nerical calculatic	n Judge stop cond PASS & FAIL				Numeri E Calculation	execute
No. 20m	1 Type Off					Calculation	Section cursor
	2 Type Off						Gauge
No.	3 Type Off						Zoom
_ No.	4 Type Off						position adjustment
-20m -21No.	Type Period Area Whole Stat.	Judge On Up 1	Target channel UNIT1 (12) UNIT2 (12) UNIT3 (12) UNIT4 (12) (3)	UNIT6 1234 UNIT7 12) RealTime (1)(2)(3)(4)() Calc.	5678	Auto range
-40m	Тор	~ _1	Level 0	Slope Filter(sample	s) 		
0s No.	Type	5us	10µs	15µs	20µs		
^					Y Mag.	ø	1/15/2019 15:42:28

1 Tap the [Judge stop condition] box, and then from the list, choose a stopping condition applied according to judgments.

PASS	Stops measurement when a calculation result falls within a criteria range (pass judgment).
FAIL	Stops measurement when a calculation result is outside a criteria range (fail judgment).
PASS & FAIL ^Ø	Stops measurement regardless whether a pass or fail judgment is given.

2 Tap the [Judge] box, and then from the list, choose whether or not to evaluate calculation results.

Off⊄	Evaluates calculation results.
On	Yields a FAIL judgment if a result is outside a criteria range. Calculated values in a channel with the FAIL judgment are highlighted in red.

3 Tap the [Up] and [Low] boxes in turn, and then enter evaluation criteria values in each of them.

Enterable range: -9.9999E+29 to -1.0000E29, 0, +1.0000E29 to +9.9999E+29

4 (To evaluate existing data) Tap [Execute].

(To automatically execute evaluation after measurement) START key

About upper and lower limit values

You cannot specify an upper limit value lower than a lower limit value. Neither can you specify a lower limit value higher than a upper limit value.

To record all calculation results

Choose [PASS & FAIL] for the stopping condition.


Judging method of CAN statistics

The instrument makes CAN statistics judgments by comparing the following values:

- The maximum value of the CAN statistics with the upper limit of the evaluation criterion
- The minimum value of the CAN statistics with the lower limit of the evaluation criterion .

Displaying evaluation results and externally outputting signals

The numerical calculation result screen of the waveform screen displays numerical calculation evaluation results.

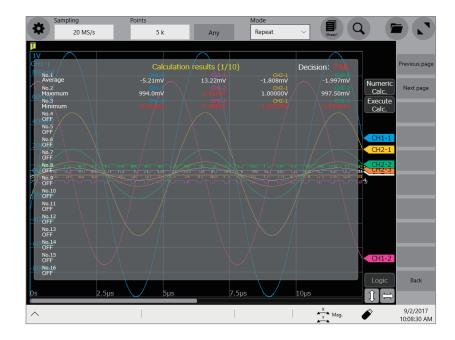

Values that fall within an evaluation criteria range: Pass judgment Values outside an evaluation criteria range: Fail judgment (highlighted in red)

When a pass judgment is given

When the external output terminals (OUT 1, OUT 2) are set to **[Judge(Pass)]**, a PASS signal is output from the external output terminals (OUT 1, OUT 2).

When a fail judgment is given


When the external output terminals (OUT 1, OUT 2) are set to **[Judge(Fail)]**, a FAIL signal is output from the external output terminals (OUT 1, OUT 2). A fail judgment is given when any one of the channels is judged to be a fail.

7.4 Numerical Calculation Types and Descriptions

Calculation type	Dese	cription				
Average	Calculates an average value of waveform data. $AVE = \frac{1}{n} \sum_{i=1}^{n} di$ $AVE:$ Average n: Number of data points di: <i>i</i> th-point data acquired across a channel					
RMS	Calculates an RMS value of waveform data. When the scaling is enabled, the instrument scales waveform data before calculation. $RMS = \sqrt{\frac{1}{n}\sum_{i=1}^{n} di^2} \begin{array}{l} RMS: \text{Root-mean-square value} \\ n: \text{Number of data points} \\ di: ith-point data acquired across a \\ channel \end{array}$					
P-P	Calculates a difference (peak-to-peak value) between the maximum and minimum values of waveform data.	Maximum Minimum				
Maximum	Calculates the maximum value of waveform data.	Maximum				
Time to maximum	Calculates a period of time (unit: s) from a trigger point to the maximum value. When waveform has two or more points of the maximum value, the instrument determines the first of them in the waveform used for a calculation to be the maximum value.	Maximum				
Minimum	Calculates the minimum value of waveform data.	Minimum				
Time to minimum	Calculates a period of time (unit: s) from a trigger point to the minimum value. When waveform has two or more points of the minimum value, the instrument determines the first of them in the waveform used for a calculation to be the minimum value.	Minimum				
Period Frequency	Displays a period (unit: s) and frequency (unit: Hz) of a signal waveform. Calculates a period and frequency based on a time lag between the time when a waveform crossed the specified level in the positive (or negative) direction the first time and the time when it next crossed the specified level. Settings: Level, Slope, Filter, Stat.	Level				

Calculation type	Description					
Rise time Fall time	Calculates a A%-to-B% rise time (or a B%- to-A% fall time; unit: s) based on the 0% and 100% levels based on a histogram (frequency distribution) of acquired waveform data. The instrument calculates a rise time (or fall time) of the first rising (or falling) slope that appears in acquired waveform data. When a range is specified with section cursors, the instrument calculates a rise time (or fall time) of the first rising (or falling) slope that appears between cursors. You can specify values of A and B in percent. The values of A and B varies along with each other. When the value of A is 5%, the value of B is specified at 95%; when the value of A is 30%, the value of B is specified at 70%. Settings: Rise time (A% to B%) and Fall time (B% to A%) values in percent, Stat.					
Standard deviation	Calculates a standard deviation of waveform data. $\sigma = \sqrt{\frac{1}{n} \sum_{i=1}^{n} (di - AVE)^2} \begin{array}{l} \sigma: \text{ Standard deviation} \\ AVE: \text{ Average} \\ n: \text{ Number of data points} \\ di: ith-point acquired across a channel} \end{array}$					
Area Method: Total	Calculates an area by subtracting an area (unit: V·s) enclosed by the zero-level (zero-potential) line and the negative-amplitude part of a signal waveform from an area (unit: V·s) enclosed by the zero-level (zero-potential) line and the positive-amplitude part of the signal waveform. When a calculation range is specified with section cursors, the instrument calculates an area between the cursors. $S: \text{ Area}$ $n: \text{ Number of data points}$ $S = \sum_{i=1}^{n} di \cdot h di: ith-point data acquired across a channel h = \Deltat: Sampling interval S = \sum_{i=1}^{n} di \cdot h di: ith-point data acquired across$					
Area Method: Absolute value	Calculates an area value (unit: V·s) enclosed by the zero-level (zero-potential) line and a signal waveform. When a calculation range is specified with section cursors, the instrument calculates an area between the cursors. $S = \sum_{i=1}^{n} di \cdot h \xrightarrow{S: \text{ Area}}_{\substack{n: \text{ Number of data points}\\di: ith-point data acquired acrosss}\\a \text{ channel}\\h = \Delta t: \text{ Sampling interval}}$					

Calculation	Description						
type							
Area Method: Positive (Only the positive- amplitude part)	Calculates an area enclosed by the zero (zero-potential) line and the positive-ampart of a signal waveform. When a range is specified with section of the instrument calculates an area betwee cursors. $S: \text{Area}$ $n: \text{Number of data point}$ $S = \sum_{i = 1, di > 0}^{n} di: i\text{th-point data acquire}$ $a \text{ channel}$ $h = \Delta t: \text{ Sampling interval}$	plitude sursors, en the s ed across $S = S_1$					
Area Method: Negative (Only the negative- amplitude part)	Calculates an area enclosed by the zero-level (zero-potential) line and the negative-amplitude part of a signal waveform. When a calculation range is specified with section cursors, the instrument calculates an area between the cursors. $S = \sum_{i=1, di < 0}^{n} \frac{S: \text{ Area}}{\substack{n: \text{ Number of data points}\\di: ith-point data acquired across}\\a \text{ channel}\\h = \Delta t: \text{ Sampling interval}}$						
X-Y area Method: Coordinate method	Calculates an area (unit: V^2) enclosed by calculates an area enclosed by the lines even when no XY composite curve is dis You can specify a calculation range on a channel using section cursors. The instr curve within the specified range (you ca using section cursors).	y an XY composite curve. The instrument as illustrated below. An area can be calculated					

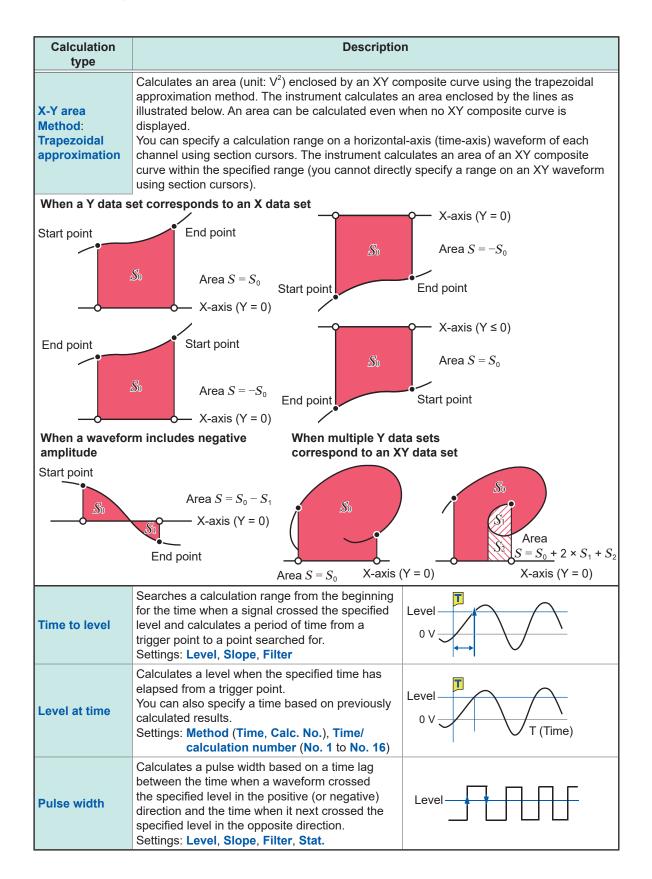

Calculation type	Description					
Duty ratio	Calculates a duty ratio based on a time lag between the time when a waveform crossed the specified level while rising and the time when it next crossed the specified level in the opposite direction, and a time lag between the time when the waveform crossed the specified level while falling and the time when it next crossed the specified level while rising. Duty ratio = $\frac{T_{u-d}}{T_{u-d} + T_{d-u}} \times 100 [\%]$ T_{u-d} : Time from rising edge to falling edge (unit: s) T_{d-u} : Time from falling edge to rising edge (unit: s) Settings: Level, Filter, Stat.	Level T_{u-d} T_{d-u}				
Pulse count	Counts the number of pulses that crossed the specified level in the positive (or negative) direction. For the pulse counts, it is considered as one count that a period between the point when a pulse crossed the level while rising and the point when the pulse crossed the level while falling (otherwise, between that while falling and while rising). Settings: Level, Slope, Filter					
Arithmetic operations	Allows you to freely choose numerical calculation results and the instrument performs arithmetic operations of the results of your choice. Settings: Calculation number 1, Arithmetic operations $(+, -, \times, \div)$, Calculation number 2					
Time difference	Calculates a time lag T (unit: s) between the time when waveform A crossed the specified level in the positive (or negative) direction and the time when waveform B crossed it in the same direction. (Time lag T) = (Time when waveform B crossed the level) – (Time when waveform A crossed the level) Settings: Waveform A (Reference channel, Level, Slope, Filter); Waveform B (Target channel, Level, Slope, Filter)					
Phase contrast	Calculates a phase difference (unit: degree) with reference to waveform A based on a time lag between the time when waveform A crossed the specified level in the positive (or negative) direction and the time when waveform B crossed it in the same direction. Phase difference = $\frac{\text{Waveform A and B}(T)}{\text{Period of waveform A}} \times 360 [°]$ Settings: Waveform A (Reference channel, Level, Slope, Filter); Waveform B (Target channel, Level, Slope, Filter)	Level				
High level Low level	Calculates a low and high levels letting 0% and 100% of acquired waveform data be them, respectively, based on a histogram (frequency distribution).					
Intermediate value	Calculates the average of the maximum and minimum values of waveform data. [(Maximum value) + (Minimum value)] / 2	Maximum Minimum				

Calculation type	Description					
Amplitude	Calculates a value (amplitude) between a low and high levels letting 0% and 100% of acquired waveform data be them, respectively, based on a histogram (frequency distribution). (High level) – (Low level)	Number of data points 100%				
Overshoot Undershoot	Calculates a ratio of a difference between the maximum (or minimum) value and a high (or low) level to a difference between a high and low levels, which are calculated letting 0% and 100% of acquired waveform data be them, respectively, based on a histogram (frequency distribution). [(Maximum value) – (High level)] / [(High level) – (Low level)] × 100 [(Low level) – (Minimum value)] / [(High level) – (Low level)] × 100	Overshoot Number of data points 100% With High level 0% Low level Undershoot				
+Width (Period during which a waveform is above the intermediate level) -Width (Period during which a waveform is below the intermediate level)	Calculates a time lag between the time when a waveform crossed the intermediate line level (50%) in the positive (or negative) direction and the time when it next crossed the intermediate level in the opposite direction. Settings: Filter, Stat.	100% ++WidthWidth 50%				
Burst width	Calculates a time during which a burst signal is outputted. Settings: Filter, Burst end filter, Window (Up, Low), Stat.	Window-level range				
Accumulation Method: Total	Calculates an accumulation by subtracting an accumulation (V) enclosed by the zero-level (zero-potential) line and the negative-amplitude part of a signal waveform from an accumulation (unit: V) enclosed by the zero-level (zero-potential) line and the positive-amplitude part of a signal waveform. When a calculation range is specified with section cursors, the instrument calculates an accumulation between the cursors. $S = \sum_{i=1}^{n} di \qquad \begin{array}{c} \text{S: Accumulation} \\ n: \text{Number of data points} \\ di: ith-point data acquired across a channel \end{array}$	S1 S1 Cursor A $S = S_1 - S_2$ S2 Cursor B				

Calculation type	Description						
Accumulation Method: Absolute value	Calculates an accumulation (unit: V) enclosed by the zero-level (zero-potential) line and a signal waveform. When a calculation range is specified with section cursors, the instrument calculates an accumulation between the cursors. $S = \sum_{i=1}^{n} di \qquad S: Accumulation n: Number of data pointsdi: ith-point data acquiredacross a channel$	S_1 S_2 $Cursor A$ $S = S_1 + S_2$ $Cursor B$					
Accumulation Method: Positive (Only the positive- amplitude part)	Calculates an accumulation (unit: V) enclosed by the zero-level (zero-potential) line and the positive-amplitude part of a signal waveform. When a calculation range is specified with section cursors, the instrument calculates an accumulation between the cursors. $S = \sum_{i=1, di > 0}^{n} \frac{S: Accumulation}{di: ith-point data acquired}$ Cursor A $S = S_{1}$						
Accumulation Method: Negative (Only the negative- amplitude part)	Calculates an accumulation (unit: V) enclosed by the zero-level (zero-potential) line and the negative-amplitude part of a signal waveform. When a calculation range is specified with section cursors, the instrument calculates an accumulation between the cursors. $S = \sum_{i=1, di < 0}^{n} \frac{S: \text{Accumulation}}{i: \text{ith-point data acquired}}$ Cursor A $S = -S_2$						
Angle of XY waveform	Calculates a regression line of an XY composite curve, and then a slope angle. $SLOPE = \frac{\sum_{i=1}^{n} (x_i - \overline{x}) \cdot (y_i - \overline{y})}{\sum_{i=1}^{n} (x_i - \overline{x})^2}$ $\theta = \arctan(SLOPE) \cdot \frac{180}{\pi} [^{\circ}]$ $xi: ith-point data acquired across theX-axis channelyi: ith-point data acquired across theY-axis channel\overline{x}: Average value of the X-axis channel\overline{y}: Average value of the Y-axis channel$	Regression line					
CAN statistics	Calculates average, maximum, and minimum values of CAN signals' arrival time intervals.	CAN frame					

Numerical Calculation Types and Descriptions

8 Waveform Calculation Function

The instrument performs calculations using acquired waveform data and pre-defined arithmetic expressions to numerically display calculation results on the waveform screen. Up to 16 calculations are simultaneously available.

No waveform calculation is available when the envelope is used.

- · When the envelope is used
- When the real-time saving is set to [On]

Calculation] > [Waveform calculation]

*	100	tatus CH	Channel	Sheet	Trigger	Calc	ulation of Syste	m Func	
	merical ulation		-time wavefor Ilation		iveform culation	FFT ca	culation		1
Calcula		Area Whole	~				Power calculation :	setting Constant	Execute Cursor
Z1 On	Pwr. Calc	Comment Formula					Units	Display On	Scale
Z2 On	Pwr. Calc.	Comment Formula					Units	Display On	Scale
CZ3 On	Pwr. Calc.	Comment Param	A - Urms1				Units	Display On	Scale Channel position
Z4 On	Pwr. Calc	Comment Param	η	IN	A - P1	С	Units	Display On	Scale Monito
Z5 Off	Pwr. Calc.	Comment Formula]		Auto ran
Z6 Off	Pwr. Calc	Comment Formula]		
Z7 Off	Pwr. Calc.	Comment Formula					Is	200µs	
^								Y Mag.	2/21/20 13:35:2

Operation available on the [Waveform calculation] screen

Waveform Calculation

- Four arithmetic operations
- Addition (+), subtraction (-), multiplication (×), division (÷)
- Basic

Absolute value, exponent, common logarithm, moving average, differential, integral, square root, cubic root, parallel move

Waveform parameter

Average, maximum value, minimum value, level at time

- Averaging
- Simple average, exponential average
- Period

Half-wave average, half-wave period, half-wave frequency, half-wave RMS value, full-wave average, full-wave period, full-wave frequency, full-wave RMS value, polarity, encoder, resolver, reminder

• FIR filter, IIR filter

Low-pass, high-pass, band-pass, band-stop, binarization

Trigonometric function

Sine, cosine, tangent, arc sine, arc cosine, arc tangent

• CAN

CAN conversion

Power calculation

Voltage, current

RMS value, average value, simple average value

- Power
- Effective power, apparent power, reactive power, power factor, power phase angle
- Others
- Efficiency, loss
- For details on arithmetic expressions, see "8.4 Operators of the Waveform Calculation and Calculation Results" (p. 222).
- For details on power calculation expressions, see "16.4 Power Equations and Wiring Specifications" (p. 420).
- Section-cursor range calculation: You can perform calculations using waveforms within a range specified with section cursors.
- When the scaling function is enabled, the instrument performs calculations using scaled values.
- You can enter each value of numerical calculation results in arithmetic calculations of waveform parameter.
- Up to 16 operations (Z1 to Z16) can be performed simultaneously; only one waveform or power operation can be performed per one operation among Z1 to Z16.

The power calculation results may not match those of other measuring instruments such as wattmeters. This is due to differences in measurement principles, accuracy, and frequency characteristics.


See "8.8 Types of Power Calculations and Explanations" (p. 252) for more information on each calculation.

8.1 Waveform Calculation Procedure


The following two methods are available:

Performing calculation during measurement	You have to configure the waveform calculation settings before starting measurement.		
Performing calculations using existing data	The instrument can perform calculations using waveform data that has already been acquired and that saved on storage devices.		

Performing calculation during measurement

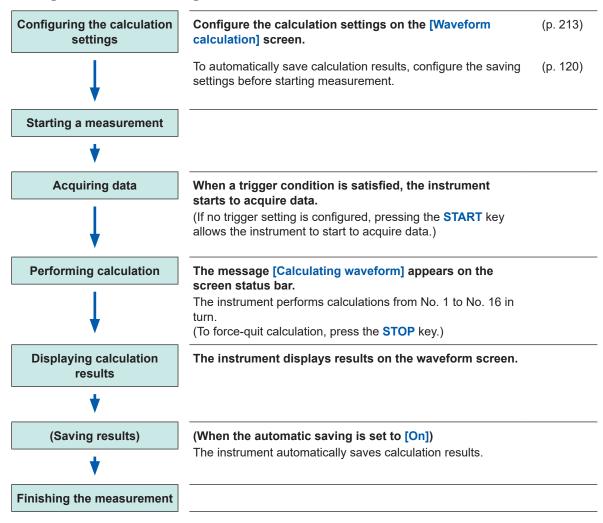

Performing calculations using existing data

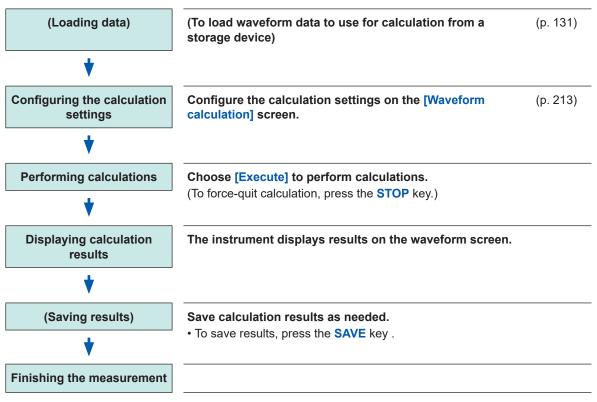

- The instrument can perform calculations using waveforms with a length of up to 5,000,000 points. To perform a calculation using a longer length of waveforms, partly save the waveforms with a length of less than 5,000,000 points and then reload the waveforms to perform another calculation.
- Using the memory division function allows the instrument to display calculation results of the last measured block.
- When the instrument perform a calculation using waveforms during measurement, force-quitting calculation prohibits the instrument from displaying calculation results.
- To restart the calculation, choose [Execute] in the [Waveform calculation] screen.


To specify a range for calculation

Before calculation, specify a calculation range using section cursors on the waveform screen. Set **[Area]** to **[Segment 1]** or **[Segment 2]** on the **[Waveform calculation]** screen. See "8.2 Configuring the Waveform Calculation Settings" (p. 213).

To automatically save waveform calculation results after measurement

See "Automatically saving waveform data" (p. 120).

8.2 Configuring the Waveform Calculation Settings

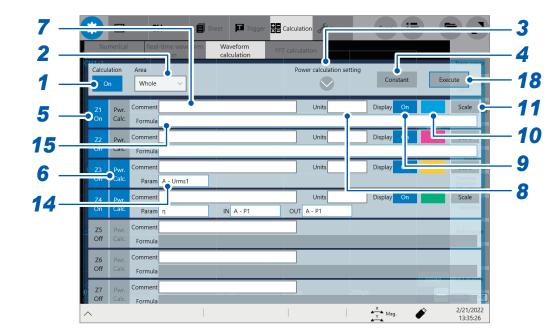

> [Calculation] > [Waveform calculation]

1 Tap the [Calculation] button to set it to [On].

2 Tap the [Area] box, and then from the list, choose an option for a waveform calculation range.

Whole [⊠]	Performs calculations using whole waveforms.
Segment 1	Performs calculations using waveform between cursors of Segment 1.
Segment 2	Performs calculations using waveform between cursors of Segment 2.

When choosing **[Segment 1]** or **[Segment 2]**, specify a calculation range with section cursors on the waveform screen. When the instrument has not acquired any waveforms, perform another measurement and specify a range. Doing so allows you to perform calculations using data acquired within the specified range from the next measurement.

3 (When configuring the power calculation settings) Tap the open mark under [Power calculation setting].

See "8.7 Setting Power Calculation Conditions" (p. 244).

- **4 Tap [Constant], and then specify constants to be used for calculation.** See "8.3 Defining Constants" (p. 220).
- **5** Tap any of the channels , [Z1] through [Z16], you want to specify a arithmetic calculation to set it to [On].
- **6** (When configuring the power calculation settings) Tap [Pwr. Calc.] to enable the power calculation.
- 7 Enter a comment in the [Comment] box.
- 8 Enter a unit symbol in the [Units] box.

9 Tap the [Display] button to set it to [On] or [Off].


On [⊠]	Displays a calculated waveform.
Off	Does not display any calculated waveform.

10 Tap the color button to the right of the [Display] button, and then choose a display color of the channel from the color pallet.

You can also choose the same color as lines acquired across other channels.

11 Tap [Scale] to the right of the color button.

The [Scale Settings] dialog box appears.




12 Tap the [Scale Settings] button to set the scale setting of calculation results to [Auto] or [Manual].

Auto ^ℤ	Automatically scales a calculation result.
Manual	Allows you to change the scale settings.

13 (When you choose [Manual] in the [Scale Settings] box.)

Tap the [Up] or [Low] box.

The numerical value entry dialog box appears.

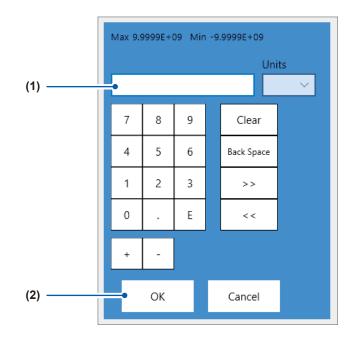

(1) Enter an upper and lower value in each box.

Use the numerical keypad, [+] button, and [-] button to enter.

```
-9.9999E+19 to 9.9999E+19
```

(2) Tap [OK].

The numerical value entry dialog box closes.

14 (When configuring the power calculation settings) Tap the [Param] box.

See "8.8 Types of Power Calculations and Explanations" (p. 252). This completes the power calculation settings. Follow the steps below to continue the waveform calculation settings.


15 Tap the [Formula] box.

The arithmetic expression setting dialog box appears.

16 Enter an arithmetic expression.

You can specify an arithmetic expression by combining numerical values, operators that includes the four arithmetic operations, calculation target channels, and constants

See "8.5 Examples of Configuring Waveform Calculation Settings" (p. 230).

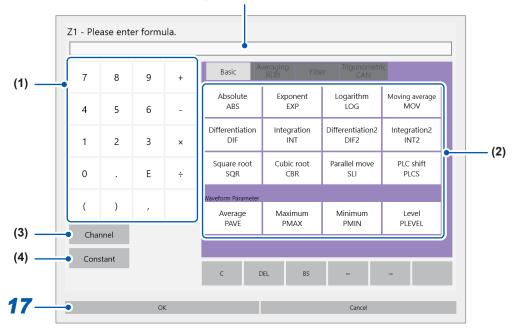

The arithmetic expression you have specified appears in the screen.

- (1) Numbers, four arithmetic operations
- (2) Operators
- (3) Allows you to choose calculation target channels.
- (4) Allows you to enter constants (5-digit numbers).

17 Tap [OK].

The arithmetic expression you have specified appears in the [Formula] box.

18 (To perform calculations using existing data) Tap [Execute].

(To perform calculations during measurement) START key

A measurement starts.

To automatically save waveform calculation results after measurement

See "Automatically saving waveform data" (p. 120).

To allocate a calculation result waveform on a sheet

See "1.4 Configuring the Sheet Settings" (p. 19).

To switch sheets on the waveform screen

See "Switching sheets on the waveform screen" (p. 24).

Arithmetic expressions

Name	Operator
Absolute value	ABS
Exponent	EXP
Common logarithm	LOG
Moving average	MOV
Differential	DIF
Integration	INT
2nd-order differential	DIF2
2nd-order integration	INT2
Square root	SQR
Cubic root	CBR
Parallel move	SLI
PLC shift	PLCS
Average value	PAVE
Maximum value	PMAX
Minimum value	PMIN
Level at time	PLEVEL
Simple average	AVESIM
Exponential average	AVEEXP
Half-wave average	AVEH
Half-wave period	PRDH
Half-wave frequency	FRQH
Half-wave RMS value	RMSH
Full-wave average	AVEF
Full-wave period	PRDF
Full-wave frequency	FRQF
Full-wave RMS value	RMSF
Polarity	POLE
Encoder	ABZ
Resolver	RSLV
Reminder	MOD

Name	Operator
FIR low-pass filter	LPFFIR
FIR high-pass filter	HPFFIR
FIR band-pass filter	BPFFIR
FIR band-stop filter	BSFFIR
IIR low-pass filter	LPFIIR
IIR high-pass filter	HPFIIR
IIR band-pass filter	BPFIIR
IIR band-stop filter	BSFIIR
Sine	SIN
Cosine	COS
Tangent	TAN
Arc sine	ASIN
Arc cosine	ACOS
Arc tangent	ATAN
2-argument arc tangent	ATAN2
CAN conversion	CAN

Arithmetic expression entry

- The length of each arithmetic expression is limited to 80 characters.
- You can directly enter a 30-digit numbers or less in arithmetic expressions (for constants, 5-digit number or less).
- If an expression you enter includes an error (its frame is filled with red), all calculation results become zero.
- Entering a complex, long arithmetic expression causes a red frame to enclose the entry box. Divide an expression into two or more.

 $\frac{\text{ABS}(\text{CH}(1,1))}{1} + \frac{\text{CH}(1,2) \times \text{CH}(1,3)}{2} - \frac{(\text{CH}(2,1) + \text{CH}(2,2)) \times \text{ABS}(\text{CH}(2,1))/\text{DIF}(\text{CH}(1,1),1)}{3}$

• You can use calculation result Zi in other arithmetic expressions. However, expression Zn can include only result Zn-1 or earlier.

Example: Expression Z4 can include result Z1 through Z3.

When an expression includes any one of the following operators: MOV, SLI, DIF, DIF2, PLEVEL, ATAN2, AVEEXP, and MOD.

The operators above require a comma and second parameter to follow the first parameter, which is enclosed in parentheses.

Operator	Setting	Setting example
MOV (moving average) SLI (parallel move)	Specify the number of points to be moved. Setting range MOV (moving average): 1 to 5000 SLI: -5000 to 5000 If you omit the second parameter, the instrument specifies [1] to perform calculations.	To calculate a 10-point moving average of the CH1-1 waveform MOV(CH(1,1),10)
DIF (Differential) DIF2 (2nd-order differential)	Specify a sampling interval for differentials Usually specify "1." To acquire amplitudes of a slowly fluctuating waveform, specify a greater number. Setting range DIF , DIF2 : 1 to 5000 If you omit the second parameter, the instrument specifies [1] to perform calculations.	To differentiate the CH1-2 waveform every 20 sampling points DIF(CH(1,2),20)
PLEVEL (level at time)	Specify a period of time from a trigger in second. If you omit the second parameter, the instrument specifies [0] to perform calculations.	To obtain a level 1 ms after a trigger yielded from CH1-3 PLEVEL(CH(1,3),0.001)
ATAN2 (2-argument arc tangent)	Entering "ATAN2(y,x)" allows the instrument to solve TAN(y/x). (p. 224) If you omit parameter x, the instrument specifies 1.0 to perform calculations. For parameter x, you cannot specify any functions or expressions, but CH, W, or Z.	To calculate 2-argument arc tangent of (CH1-1) / (CH1-2) ATAN2(CH(1,1),CH(1,2))
AVEEXP (exponential average)	Specify an attenuation constant for an exponential average calculation. Setting range: 2 to 1000 Omitting an attenuation constant causes an error.	To calculate an exponential average of the CH1-4 waveform using an attenuation constant of 40 AVEEXP(CH(1,4),40)
MOD (Reminder)	Specify a reminder. Omitting a reminder causes an error.	To obtain the remainder of the value of Z1 divided by 360 MOD(Z1,360)

When an expression includes any one of the following operators: AVEH, PRDH, FRQH, RMSH, AVEF, PRDF, FRQF, RMSF, and POLE.

Operator	Setting	Setting example
AVEH (half-wave average) RMSH (half-wave RMS value) AVEF (full-wave average) RMSF (full-wave RMS value)	Specify the reference channel, hysteresis threshold, the forcibly averaging time. If you omit to enter the forcibly averaging time, the instrument performs calculation without using the forcibly averaging. If you omit to enter the hysteresis threshold and the forcibly averaging time, the instrument performs calculation specifying zero for the hysteresis threshold without using the forcibly averaging. Omitting to enter the reference channel causes an error.	To calculate an average of the CH1-1 waveform every half cycle defined by the zero-crossings of the CH1-2 waveform with a hysteresis threshold of 100 mV and a forcibly average time of 500 ms AVEH(CH(1,1),CH(1,2),0.1,0.5)
PRDH (half-wave period) FRQH (half-wave frequency) PRDF (full-wave period) FRQF (full-wave frequency)	Specify the hysteresis threshold. If you omit to enter the hysteresis threshold, the instrument specifies zero for it and performs calculation.	To calculate the period of the CH1- 3 waveform on the basis of the zero- crossings that occur every half cycle with a hysteresis threshold of 100 mV PRDH(CH(1,3),0.1)
POLE (polarity)	Specify the reference channel and hysteresis threshold. Omitting to enter the reference channel causes an error. If you omit to enter the hysteresis threshold, the instrument performs calculation specifying zero for it.	To obtain the polarity of the CH1-1 waveform in reference to the CH1-2 waveform with a hysteresis threshold of 100 mV POLE(CH(1,1),CH(1,2),0.1)

When using the ABZ operator in equations

Operator	Setting	Setting example
ABZ (encoder)	Sets the A-phase channel, B-phase channel, Z-phase channel, low threshold value, and high threshold value. Omitting the channels and thresholds will result in an error.	To calculate the rotary encoder angle for a low threshold value of 0.5 V, a high threshold value of 4.5 V, and A-, B-, and Z-phase channels of CH1-1, CH1-2, and CH1-3, respectively: ABZ(CH(1,1),CH(1,2),CH(1,3),0.5,4.5)

When using the **RSLV** operator in equations

Operator	Setting	Setting example
RSLV (resolver)	Sets the excitation wave channel, cos wave channel, sin wave channel, hysteresis, and pole pairs. Omitting the channels and hysteresis will result in an error. If the number of pole pairs is omitted, a pole pair value of 1 will be used in calculations.	To calculate the resolver error with a hysteresis threshold value of 100 mV, 4 pole pairs, and an excitation wave, cos wave, and sin wave of CH1-1, CH1-2, and CH1-3, respectively: RSLV(CH(1,1),CH(1,2),CH(1,3),0.1,4)

Operator	Setting	Setting example
LPFFIR (FIR low-pass filter) HPFFIR (FIR high-pass filter)	Specify a cutoff frequency, the order of a filter, and a Kaiser window coefficient. Setting range Cutoff frequency: See p. 241. Order of a filter: 2 to 400 Kaiser window coefficient: 0 to 20	To pass the CH1-1 waveform through the 128th-order FIR low-pass filter with a cutoff frequency of 100 kHz and a Kaiser window coefficient of 10 LPFFIR(CH(1,1),100000,128,10)
BPFFIR (FIR band-pass filter) BSFFIR (FIR band-stop filter)	Specify a lower and higher cutoff frequencies, the order of a filter, and a Kaiser window coefficient. Setting range Cutoff frequency: See p. 241. Order of a filter: 2 to 400 Kaiser window coefficient: 0 to 20	To pass the CH1-1 waveform through the 128th-order FIR band-pass filter with a lower cutoff frequency of 100 kHz, a higher cutoff frequency of 200 kHz, and a Kaiser window coefficient of 10 BPFFIR(CH(1,1),100000,200000,128,10)
LPFIIR (IIR low-pass filter) HPFIIR (IIR high-pass filter)	Specify a cutoff frequency and the order of a filter. Setting range Cutoff frequency: See p. 241. Order of a filter: 1 to 64	To pass the CH1-1 waveform through the 2nd-order IIR high-pass filter with a cutoff frequency of 100 kHz HPFIIR(CH(1,1),100000,2)
BPFIIR (IIR band-pass filter) BSFIIR (IIR band-stop filter)	Specify a lower and higher cutoff frequencies, and the order of a filter. Setting range Cutoff frequency: See p. 241. Order of a filter: 1 to 64	To pass the CH1-1 waveform through the 2nd-order IIR band-stop filter with a lower cutoff frequency of 100 kHz and a higher cutoff frequency of 200 kHz BSFIIR(CH(1,1),100000,200000,2)
BIN (Binarization)	Specify a lower and a higher thresholds. Omitting to enter the thresholds causes an error.	To binarize the CH1-1 waveform using the lower thresholds of 1.5 V and higher of 3.5 V BIN(CH(1,1),1.5,3.5)

When a filter calculation is used in an arithmetic expression


If a calculation result overflows

- The instrument regards a calculation result that falls within the following range as an overflow. 1. Greater than +9.9999E+29
 - 2. Less than -9.9999E+29
- The instrument assigns +9.9999E+29 to positive overflows, and -9.9999E+29 to negative overflows.
- Trace cursors (A through H) read +9.9999E+29 at a positively overflowing point, and -9.9999E+29 at a negatively overflowing point.

8.3 Defining Constants

You can previously define constants to use in arithmetic expressions.



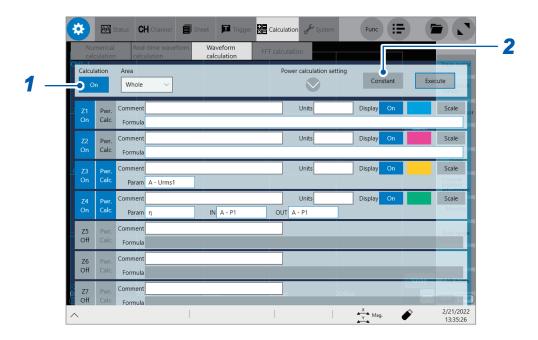


1 Tap the [Calculation] button to set it to [On].

2 Tap [Constant].


The constant entry dialog box appears.

3 Tap a box that has an alphabet you want to allocate a constant to.

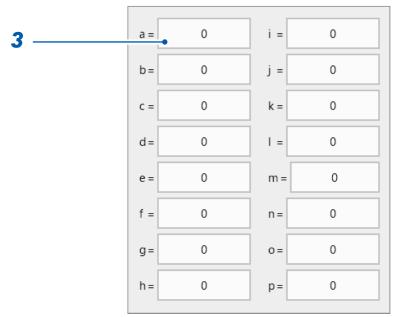

The numerical value entry dialog box appears.

4 Enter a constant.

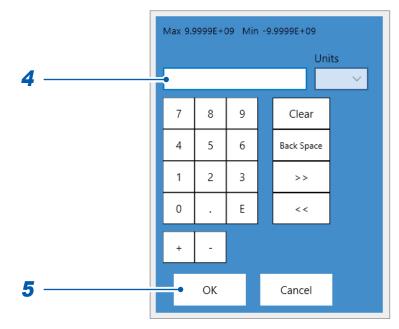

-9.9999E+29 to -1.0000E-29, 0, +1.0000E-29 to +9.9999E+29

You can specify a value to five or less significant figures.

Use the numerical keypad, [+] button, and [-] button to enter.

The instrument feeds constants you have defined to the constant display on the arithmetic expression setting dialog box.

5 Tap [OK].

The numerical value entry dialog box closes.

8.4 Operators of the Waveform Calculation and Calculation Results

Waveform calculation type	Description
Four arithmetic operations (+, −, ×, ÷)	Performs calculations using operators specified from the four arithmetic operations, which consists of addition (+), subtraction ($-$), multiplication (×), and division (\div). Multiplication signs (×) and division signs (\div) are represented as asterisks (*) and slashed (/), respectively.
Absolute value (ABS)	$b_i = d_i $ (<i>i</i> = 1, 2,, n)
Exponent (EXP)	$b_i = \exp(d_i)$ (<i>i</i> = 1, 2,, n)
Common logarithm (LOG)	For $d_i > 0$ $b_i = \log_{10} d_i$ For $d_i = 0$ $b_i = -\infty$ (Outputs overflowing values)For $d_i < 0$ $b_i = \log_{10} d_i \ (i = 1, 2,, n)$ Note: Using the following equations can convert a common logarithm into a naturallogarithm. $\ln X = \log_e X = \log_{10} X / \log_{10} e$ $1 / \log_{10} e \approx 2.30$
Square root (SQR)	For $d_i \ge 0$ $b_i = \sqrt{d_i}$ For $d_i < 0$ $b_i = -\sqrt{ d_i }$ $(i = 1, 2,, n)$
Cubic root (CBR)	$b_i = \sqrt[3]{d_i}$
Moving average (MOV)	This function requires the number of moving points to be specified in the second parameter <i>k</i> . When <i>k</i> is an odd number When <i>k</i> is an even number $b_i = \frac{1}{k} \sum_{\substack{t=i-\frac{k-1}{2}\\t=i-\frac{k}{2}}}^{i+\frac{k-1}{2}} d_t (i=1, 2,, n) \qquad b_i = \frac{1}{k} \sum_{\substack{t=i-\frac{k}{2}\\t=i-\frac{k}{2}+1}}^{i+\frac{k}{2}} d_t (i=1, 2,, n)$ $d_i: t$ th-point data acquired across the source channel <i>k</i> : Number of moving point (1 to 5000) Specify the constant <i>k</i> following a comma. Example: Calculating 100-point moving averages of the Z1 waveform MOV(Z1,100) For each <i>k</i> /2 points of data at the beginning and end of the calculation interval, the instrument performs calculations by plugging in zero for data-missing parts.
Parallel move in the time axis direction (SLI)	This function requires the number of moving points to be specified in the second parameter <i>k</i> . The instrument translates a waveform in the time-axis direction by the specified moving points. $b_i = d_{i-k}$ (<i>i</i> = 1, 2,, n) <i>k</i> : Number of moving points (-5000 to 5000) Specify the constant <i>k</i> following a comma. Example: Translating the Z1 waveform by 100 points SLI(Z1,100) Note: If the instrument finds non-data parts at the beginning or end of the calculation interval after translating a waveform, the instrument specifies zero-volt voltage there.

*b_i: i*th-point data in calculation results, *d_i: i*th-point data acquired across the source channel

*b_i: i*th-point data in calculation results, *d_i: i*th-point data acquired across the source channel

Waveform calculation type	Description	
Waveform shifting by a PLC delay time specified in a digital voltmeter module (PLCS)	The instrument shifts a waveform by a frequency (PLC) and delay time of PLCS, which are configured in the setting for Model MR8990 Digital Voltmeter Unit. Since digital voltmeter modules calculate averages of data acquired during periods specified in the NPLC setting, an observed waveform will lag behind waveforms acquired with Model 8966 Analog Unit by a half of the NPLC setting. The PLCS calculation advances a waveform acquired with the digital voltmeter module by the delay time to compensate for the lag behind a waveform acquired with Model 8966. Note If the instrument find non-data part at the end of the calculation result, the instrument specifies zero volt there.	
Sine (SIN)	$b_i = \sin(d_i)$ (<i>i</i> = 1, 2,, n) For the trigonometric and inverse trigonometric functions, specify numbers in radians (rad).	
Cosine (COS)	$b_i = \cos(d_i)$ (<i>i</i> = 1, 2,, n) For the trigonometric and inverse trigonometric functions, specify numbers in radians (rad).	
Tangent (TAN)	$b_i = \tan(d_i)$ (<i>i</i> = 1, 2,, n) For the trigonometric and inverse trigonometric functions, specify numbers in radians (rad).	
Arc sine (ASIN)	For $d_i > l$ $b_i = \pi/2$ For $-1 \le d_i \le 1$ $b_i = \arcsin(d_i)$ For $d_i < -1$ $b_i = -\pi/2$ $(i = 1, 2,, n)$ For the trigonometric and inverse trigonometric functions, specify numbers in radians (rad).	
Arc cosine (ACOS)	For $d_i > 1$ $b_i = 0$ For $-1 \le d_i \le 1$ $b_i = \arccos(d_i)$ For $d_i < -1$ $b_i = \pi$ ($i = 1, 2,, n$)For the trigonometric and inverse trigonometric functions, specify numbers in radians (rad).	
Arc tangent (ATAN)	$b_i = \arctan(d_i)$ (<i>i</i> = 1, 2,, n) For the trigonometric and inverse trigonometric functions, specify numbers in radians (rad).	
2-argument arc tangent (ATAN2(y, x))	Responses arc tangent of (y/x) in the range of $[-\pi, \pi]$. Specify numbers in radians (rad).ATAN2 $(y, x) =$ For $x \ge 0$ ATAN (y/x) For $x < 0$ and $y \ge 0$ ATAN $(y/x) + \pi$ For $x < 0$ and $y < 0$ ATAN $(y/x) - \pi$	

Waveform calculation type	Description
	The instrument makes 1st-order differential and 2nd-order differential calculations using 5th-order Lagrange interpolation formula to obtain 1-point data from 5-point values that includes before and after the point. The instrument differentiates data d_1 to d_n considering them as the corresponding data for the sampling time t_1 to t_n . Note: Differentiating a slowly oscillating waveform causes an increase in calculation results variation. In such a case, raise the second parameter of the function. The following equations hold when the second parameter equals one. Arithmetic expressions of 1st-order differential Point $t_1 b_1 = (-25d_1 + 48d_2 - 36d_3 + 16d_4 - 3d_5) / 12h$ Point $t_2 b_2 = (-3d_1 - 10d_2 + 18d_3 - 6d_4 + d_5) / 12h$ Point $t_3 b_3 = (d_1 - 8d_2 + 8d_4 - d_5) / 12h$
1st-order differential (DIF) 2nd-order differential (DIF2)	↓ Point $t_i b_i = (d_{i-2} - 8d_{i-1} + 8d_{i+1} - d_{i+2}) / 12h$ ↓ Point $t_{n-2} b_{n-2} = (d_{n-4} - 8d_{n-3} + 8d_{n-1} - d_n) / 12h$ Point $t_{n-1} b_{n-1} = (-d_{n-4} + 6d_{n-3} - 18d_{n-2} + 10d_{n-1} + 3d_n) / 12h$ Point $t_n b_n = (3d_{n-4} - 16d_{n-3} + 36d_{n-2} - 48d_{n-1} + 25d_n) / 12h$ b_1 to b_n : Calculation result data $h = \Delta t$: Sampling period Arithmetic expressions of 2nd-order differential Point $t_1 b_1 = (35d_1 - 104d_2 + 114d_3 - 56d_4 + 11d_5) / 12h^2$ Point $t_2 b_2 = (11d_1 - 20d_2 + 6d_3 + 4d_4 - d_5) / 12h^2$ Point $t_3 b_3 = (-d_1 + 16d_2 - 30d_3 + 16d_4 - d_5) / 12h^2$ ↓ Point $t_i b_i = (-d_{i-2} + 16d_{i-1} - 30d_i + 16d_{i+1} - d_{i+2}) / 12h^2$ ↓ Point $t_{n-2} b_{n-2} = (-d_{n-4} + 16d_{n-3} - 30d_{n-2} + 16d_{n-1} - d_n) / 12h^2$ Point $t_{n-1} b_{n-1} = (-d_{n-4} + 4d_{n-3} + 6d_{n-2} - 20d_{n-1} + 11d_n) / 12h^2$ Point $t_n b_n = (11d_{n-4} - 56d_{n-3} + 114d_{n-2} - 104d_{n-1} + 35d_n) / 12h^2$

 b_i : *i*th-point data in calculation results, d_i : *i*th-point data acquired across the source channel

Waveform calculation type	Descriptio	n
	To calculate values of 1st-order and 2nd-order in trapezoidal formula. The instrument integrates data d_1 to d_n considering the sampling time t_1 to t_n .	-
	Arithmetic expressions of 1st-order integratic Point $t_1 I_1 = 0$ Point $t_2 I_2 = (d_1 + d_2) h / 2$ Point $t_3 I_3 = (d_1 + d_2) h / 2 + (d_2 + d_3) h / 2 = I_2 + (d_2 + d_3) h / 2 = I_2 + (d_2 + d_3) h / 2 = I_2 + (d_2 + d_3) h / 2 = I_2 + (d_3 + d_3) h / 2 = I_2 + (d_3 + d_3) h / 2 = I_3 + (d_3 + $	
1st-order integration (INT)	Point $t_n I_n = I_{n-1} + (d_{n-1} + d_n) h / 2$ I_1 to I_n : Calculation result data $h = \Delta t$: Sampling period	
2nd-order integration (INT2)	Arithmetic expressions of 1st-order integratic Point $t_1 II_1 = 0$ Point $t_2 II_2 = (I_1 + I_2) h / 2$ Point $t_3 II_3 = (I_1 + I_2) h / 2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_2 + I_3) h / 2 = II_2 + (I_3 + I_3) h / 2 = II_3 + (I_3 + I_$	
	Point $t_n II_n = II_{n-1} + (I_{n-1} + I_n) h / 2$ II_1 to II_n : Calculation result data Note Integration is susceptible to minor devia execute zero-adjustment before perform point offset correction may be required. Example: To adjust the zero point by 0.1 Z1 = INT (CH(1,1)-0.000124)	ning measurement. In addition, zero-
Average value (PAVE)	Calculates an average value of waveform data to for waveform calculations. $A VE = \frac{1}{n} \sum_{i=1}^{n} d_{i} \qquad \begin{array}{c} AVE: \text{ Average} \\ n: & \text{Number of data poin} \\ d_{i}: & i\text{th-point data acquire} \end{array}$	
Maximum value (PMAX)	Calculates the maximum value of waveform data to use this numerical calculation result for waveform calculations.	Maximum value
Minimum value (PMIN)	Calculates the minimum value of waveform data to use this numerical calculation result for waveform calculations.	Minimum value
Level at time (PLEVEL)	Calculates a measured value at the time a specified time has elapsed from a trigger point to use this numerical calculation result for waveform calculations.	
Simple average (AVESIM)	$d_{i,i}$: <i>i</i> th-point data acquire	measurements le average results of the <i>m</i> th grepeated measurements ed across a channel of the <i>j</i> th grepeated measurements ressions (two expressions immediately

8

Waveform calculation type	Description
	This function requires an attenuation constant to be specified in the second parameter k. Calculates an exponential average of repeatedly measured waveform data sets. (First of repeated measurements)
	$A_{1,i} = d_{1,i}$ $A_{1,i}: i$ th-point data in exponential average results of the first measurement among repeated measurements $d_{1,i}: i$ th-point data obtained across a channel of the first measurement among repeated measurements
	(Second or later of repeated measurements)
Exponential average (AVEEXP)	$A_{m,i} = (d_{m,i} + (k-1) A_{m-1,i}) / k$
	 m: Number of repeated measurements A_{m,i}: ith-point data in exponential average results of the <i>m</i>th measurement among repeated measurements d_{m,i}: ith-point data acquired across a channel of the <i>m</i>th measurement among repeated measurements k: Attenuation constant
	Use an exponential average independently.
	Concurrent use with other calculations causes an error.

 b_i : *i*th-point data in calculation results, d_i : *i*th-point data acquired across the source channel

Waveform calculation type	Description	n
.,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,	Detects the points where the signal acquired across the reference channel has no voltage (zero-crossings), and calculates averages or RMS values of the signal acquired across the target channel during each time period specified by the zero-crossings. During each time period, the displayed period or frequency remains unchanged.	
	Time period for half-wave average and half- wave RMS value Time periods are defined by the zero-crossings that occur while the signal is both rising and falling (● marks), thus consisting of two parts: one from when the signal crosses the zero-volt level while rising to when it crosses the zero- volt level while falling, and vice versa.	Caluculation Target channel 0 V Reference channel Half-wave average
Half-wave average (AVEH) Full-wave average (AVEF) Half-wave RMS value	Time period for full-wave average and full- wave RMS value Time periods are defined by the zero-crossings that occur while the signal is rising only (• marks).	0 V Full-wave average
(RMSH) Full-wave RMS value (RMSF)	Once a zero-crossing (● mark) has been detected, the instrument will not honor subsequent zero-crossings (○ marks) when the signal crosses the zero-volt level before exiting the threshold range, which is between the positive and negative threshold values.	Positive threshold 0 V Negative threshold value Half-wave average, half-wave RMS value
		Positive threshold value 0 V Negative threshold value Full-wave average,
	When the forced-average setting is enabled, the instrument calculates averages or RMS values of the signal acquired during the period until the user-specified forced-average time has elapsed after detecting zero-crossings (• marks).	full-wave RMS value Forced-average time

b_i: ith-point data in calculation results, d_i: ith-point data acquired across the source channel

Waveform calculation type	Descriptio	n
	Detects the points where the signal acquired across the reference channel has no voltage (zero-crossings), and calculates the periods and frequencies of a signal for each time period. During each time period, the displayed period or frequency remains unchanged.	
	Time periods for calculating half-wave periods and frequencies Time periods are defined by the zero-crossings that occur while the signal is both rising and falling (• marks), thus consisting of two parts: one from when the signal crosses the zero-volt level while rising to when it crosses the zero- volt level while falling, and vice versa.	0 V Half-wave period
Half-wave period (PRDH) Half-wave frequency (FRQH) Full-wave period (PRDF) Full-wave frequency	Time periods for calculating full-wave periods and frequencies Time periods are defined by the zero-crossings that occur while the signal is rising only (• marks).	0 V Full-wave period
(FRQF)	Once a zero-crossing (mark) has been detected, the instrument will not honor subsequent zero-crossings (marks) when the signal crosses the zero-volt level before exiting the threshold range, which is between the positive and negative threshold values.	Positive threshold value 0 V Negative threshold value Half-wave period, half-wave frequency
		Positive threshold value 0 V Negative threshold value Full-wave period, full-wave frequency
Polarity (POLE)	If the waveform acquired across the target channel leads that acquired across the reference channel, the instrument displays the figure +1; if lags, the figure -1 .	Lead (+1) Reference Target channel channel

*b_i: i*th-point data in calculation results, *d_i: i*th-point data acquired across the source channel

Waveform calculation type	Description
Encoder (ABZ)	Cumulatively adds the pulses of an incremental-type rotary encoder. Values cannot be converted for absolute-type rotary encoders. This function uses 4× operation in which both the rising and falling edges are counted for A-phase and B-phase channels. The angle is incremented (decremented) by 1 when the A-phase leads (lags) the B-phase. Values are interpolated linearly for each angle count. The angle is reset to 0 at the Z-phase channel pulse's rising edge. The value 0 is output until the first Z-phase pulse is detected.
Resolver (RSLV)	When RSLV(CH _{EXC} , CH _{COS} , CH _{SIN} , hys) is entered into an equation, the calculation shown below is performed to calculate the resolver angle (in degrees). The output range is 0 to 360. Z_{RSLV} is output to the waveform calculation channel. $Z_{COS} = AVEH(CH_{exc} * CH_{cos}, CH_{exc}, hys)$ $Z_{SIN} = AVEH(CH_{exc} * CH_{sin}, CH_{exc}, hys)$ $Z_{RSLV} = ATAN2(Z_{SIN}, Z_{COS}) * 180/\pi$ CH_{Exc} : Excitation wave channel CH_{cos} : cos wave channel CH_{cos} : is in wave channel CH_{siN} : sin wave channel hys: Hystersis threshold value AVEH: Half-cycle average operator ATAN2: Arc tangent operator
Remainder (MOD)	When $d_i \ge 0$ $b_i = d_i \mod m$ m: DivisorWhen $d_i < 0$ $b_i = m - (d_i \mod m)$ m: Divisor
Low-pass filter (FIRLPF)	Passes a waveform through an FIR low-pass filter.
High-pass filter (FIRHPF)	Passes a waveform through an FIR high-pass filter.
Band-pass filter (FIRBPF)	Passes a waveform through an FIR band-pass filter.
Band-stop filter (FIRBSF)	Passes a waveform through an FIR band-stop filter.
Low-pass filter (IIRLPF)	Passes a waveform through an IIR low-pass filter.
High-pass filter (IIRHPF)	Passes a waveform through an IIR high-pass filter.
Band-pass filter (IIRBPF)	Passes a waveform through an IIR band-pass filter.
Band-stop filter (IIRBSF)	Passes a waveform through an IIR band-stop filter.
Binarization (BIN)	If the signal crosses the higher threshold while rising, the instrument displays the figure +1; if the lower while falling, the figure -1 . Higher Lower
CAN	Converts CAN signals into waveforms on the basis of CAN definition data. See "12.7 Choosing Data To Be Displayed as Waveforms (When Using the Waveform Calculation Function)" (p. 339).

8


Waveform Calculation Function

8.5 Examples of Configuring Waveform Calculation Settings

Obtaining an RMS waveform from an instantaneous waveform

This section explains how to display a RMS waveform obtained through a calculation using a constantly oscillating waveform acquired across the analog channel (CH1-1). The instrument provides no calculations to obtain an RMS waveform from a waveform with a variable period. This example demonstrates a calculation for a waveform data with a period of 200 samples.



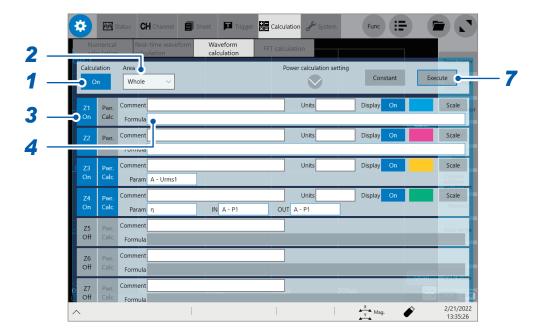

- **1** Tap the [Calculation] button to set it to [On].
- 2 Tap the [Area] box, and then choose [Whole].
- **3** Tap the channel to use for calculation, [Z1], to set it to [On].


Specify an arithmetic expression. Tap the [Formula] box of [Z1] to open the arithmetic expression setting dialog box.

5 Enter an arithmetic expression.

SQR(MOV(CH(1,1)*CH(1,1),200))

Number of sampling per period

(Specify 200 when measuring 50-Hz commercial power with a sampling rate of 10 kS/s)

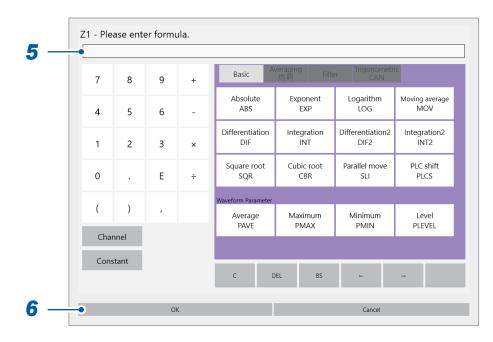

6 Tap [OK].

The arithmetic expression setting dialog box closes and the arithmetic expression you have entered appears.

	Status CH	Channel	Sheet Trigger	Calculatio	on 🖌 System	Func	
Numerica calculatio		time waveform lation	Waveform calculation	FFT calcula	ion		
Calculation On	Area Whole	~		Pow	er calculation setti	ng Constant	Execute Cursor
Z1 Pwr. On Calc		SQR(MOV(CH(1,1)*CH(1,1),200))		Units	Display On	Scale
Z2 Pwr. On Calc					Units	Display On	Scale
CZ3 Pwr. On Calc					Units	Display On	Scale
Z4 Pwr. On Calc					Units	Display On	Scale
Z5 Pwr. Off Calc							Auto rang
Z6 Pwr. Off Calc							
Z7 Pwr. Off Calc			roops	June	21	00µs	
^						Y Mag.	2/21/202 13:44:42

7 Tap [Execute] to execute the calculation.

8 Press the START key to start a measurement.

The instrument have acquired a waveform, then displaying the calculated waveform.

To perform calculations using previously acquired data

Tap **[Execute]** in the waveform calculation screen.

•	*	r	itatus Cl	Channel	Sheet	Trigger	Calcu	lation of System	m Func	-	
		merical culation		-time waveforn Ilation		eform ulation	FFT calc	ulation			
•	Calcul O		Area Whole	~			F	Power calculation s	etting Constant	Exe	cute
	Z1 On	Pwr. Calc.	Comment Formula					Units	Display On		Scale
	Z2 On	Pwr. Calc.	Comment Formula					Units	Display On		Scale
0	Z3 On	Pwr. Calc.	Comment Param	A - Urms1				Units	Display On		Scale Channel position
	Z4 On	Pwr. Calc.	Comment Param	η	IN	A - P1	OL	Units	Display On		Scale
- 1	Z5 Off	Pwr. Calc.	Comment Formula								Auto range
	Z6 Off	Pwr. Calc.	Comment Formula								
0	Z7 Off	Pwr. Calc.	Comment Formula					JS	200µs		SIDE SIDE
^	<								Y Mag.	é	2/21/2022 13:35:26

FIR filter

How to configure the FIR filter setting

For LPFFIR and HPFFIR, specify a channel number, cutoff frequency (default: 50 Hz), the order of a filter, and a Kaiser window coefficient in an arithmetic expression as follows. For LPFFIR: LPFFIR(CH(1,1),100000,128,10) For HPFFIR: HPFFIR(CH(1,1),200000,128,10)

For BPFFIR and BSFFIR, specify a channel number, a lower and higher cutoff frequencies (default: 40 Hz and 60 Hz, respectively), the order of a filter, and a Kaiser window coefficient in an arithmetic expression as follows.

For BPFFIR: BPFFIR(CH(1,1),100000,200000,128,10) For BSFFIR: BSFFIR(CH(1,1),100000,200000,128,10)

- See Table A (p. 241) for settable upper limits of cutoff frequencies (you can specify a value less than half a sampling frequency, which depends on the time-axis settings).
- For BPFFIR and BSFFIR, specify a lower cutoff frequency lower than higher cutoff frequency.
- Specify the order of the FIR filter in the range of 2 to 400 (default: 128). Higher-order filters exhibit steeper cutoff characteristics; however, calculation requires a longer time.
- Specify a Kaiser window coefficient in the range of 0.0 to 20.0 (default: 10.0). Specifying 0.0 exhibits no Kaiser window effect. A greater Kaiser window coefficient can reduce pass-band ripples due to filter amplitude characteristics, allowing a greater out-of-pass-band attenuation.

Example of an FIR low-pass filter (LPF) setting

This section explains how to configure the Z1 calculation setting to pass the CH1-1 data through a 128th-order FIR low-pass filter with a cutoff frequency of 100 kHz (100000 Hz) and a Kaiser window coefficient if 10.

(With a sampling rate of 500 kHz, which means a sampling period of 200 $\mu s)$

*

> [Calculation] > [Waveform calculation]




1 Tap the [Calculation] button to set it to [On].

2 Set [Area] to [Whole].

3 Tap the channel to use for calculation, [Z1], to set it to [On].

4 Specify an arithmetic expression.

Tap the [Formula] box of [Z1] to display the arithmetic expression setting dialog box.

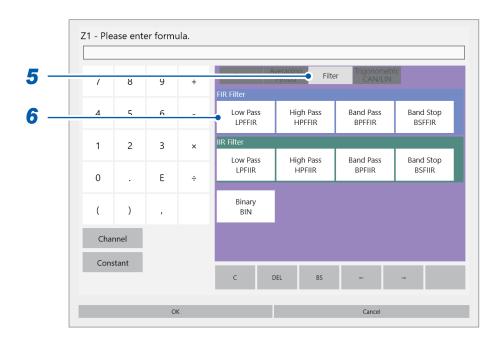


5 Tap the [Filter] tab.

The filter setting list appears.

6 Tap [Low Pass LPFFIR] of the calculation items.

The [FIR Low Pass Filter] setting dialog box appears.

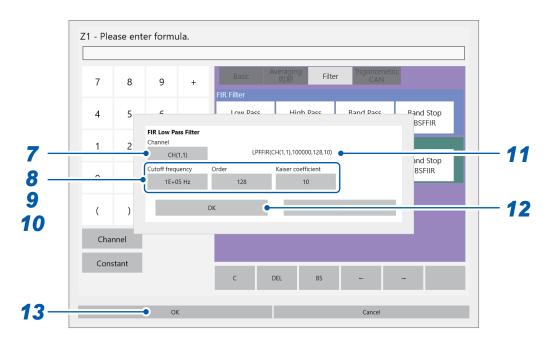

7 Tap the [Channel] box, and then choose a calculation target channel from the list (choose "UNIT1-CH1" of built-in modules).

	-in unit				
	CH1	CH2	СНЗ	CH4	
UNIT1 4ch ANALOG	Mode:Voltage	Mode:Voltage	Mode:Voltage	Mode:Voltage	
UNIT2 ANALOG	Mode:Voltage	Mode:Voltage			
UNIT3					
UNIT4					
JNIT5					
JNIT6					
JNIT7					
UNIT8					
UNIT8					
JNIT8					

- **8** Tap the [Cutoff frequency] box, and then specify "100E3" for a unit symbol.
- **9** Tap the [Order] box, and then specify "128." for a number and "k" for a unit symbol.

10 Tap the [Kaiser coefficient] box, and then specify "10."

11 Check the arithmetic expressions you entered.

12 Tap [OK].


The [FIR Low Pass Filter] setting dialog box closes.

The arithmetic expression you have specified appears in the screen.

13 Tap [OK].

The instrument closes the arithmetic expression setting dialog box, redisplaying the **[Waveform calculation]** screen.

The arithmetic expression you have specified appears in [Formula] box of [Z1].

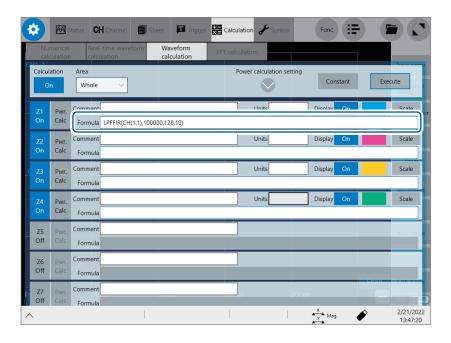

IIR filter

How to configure the IIR filter setting

For LPFIIR and HPFIIR, specify a channel number, cutoff frequency (default: 50 Hz), the order of a filter in an arithmetic expression as follows. For LPFIIR: LPFIIR(CH(1,1),100000,2) For HPFIIR: HPFIIR(CH(1,1),200000,2)

For BPFIIR and BSFIIR, specify a channel number, a lower and higher cutoff frequencies (default: 40 Hz and 60 Hz, respectively), the order of a filter in an arithmetic expression as follows. For BPFIIR: BPFIIR(CH(1,1),100000,200000,2) For BSFIIR: BSFIIR(CH(1,1),100000,200000,2)

- See Table A (p. 241) for settable upper limits of cutoff frequencies (you can specify a value less than half a sampling frequency, which depends on the time-axis settings).
- For BPFIIR and BSFIIR, specify a lower cutoff frequency lower than higher cutoff frequency.
- Specify the order of the IIR filter in the range of 1 to 64 (default: 2). Higher-order filters exhibit steeper cutoff characteristics.

Example of an IIR low-pass filter (LPF) setting

This section explains how to configure the Z1 calculation setting to pass the CH1-1 data through a 2nd-order IIR low-pass filter with a cutoff frequency of 100 kHz (100000 Hz). (With a sampling rate of 500 kHz, which means a sampling period of 2 μ s)






- **1** Tap the [Calculation] button to set it to [On].
- 2 Set [Area] to [Whole].
- **3** Tap the channel to use for calculation, [Z1], to set it to [On].

4 Specify an arithmetic expression.

Tap the [Formula] box of [Z1] to display the arithmetic expression setting dialog box.

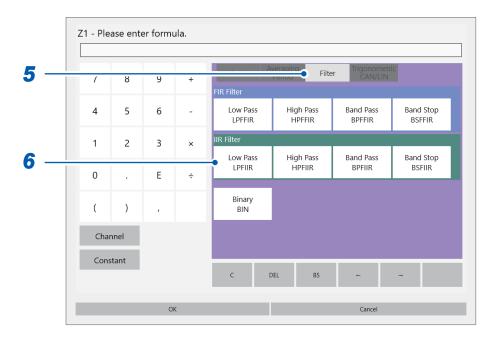


5 Tap the [Filter] tab.

The filter setting list appears.

6 Tap [Low Pass LPFIIR] of the calculation items.

The **[IIR Low Pass Filter]** setting dialog box appears.

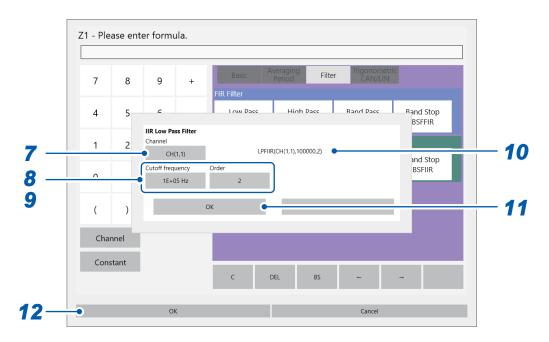

7 Tap the [Channel] box, and then choose a calculation target channel from the list (choose "UNIT1-CH1" of built-in modules).

	-in unit			
	CH1	CH2	СНЗ	CH4
JNIT1 Ich ANALOG	Mode:Voltage	Mode:Voltage	Mode:Voltage	Mode:Voltage
JNIT2 ANALOG	Mode:Voltage	Mode:Voltage		
JNIT3				
JNIT4				
JNIT5				
JNIT6				
JNIT7				
JNIT8				
JNIT8				
INIT8				

- **8** Tap the [Cutoff frequency] box, and then specify "100E3" for a unit symbol.
- **9** Tap the [Order] box, and then specify "2." for a number and "k" for a unit symbol.
- **10** Check the arithmetic expressions you entered.

8

11 Tap [OK].

The [IIR Low Pass Filter] setting dialog box closes.

The arithmetic expression you have specified appears in the screen.

12 Tap [OK].

The instrument closes the arithmetic expression setting dialog box, redisplaying the **[Waveform calculation]** screen.

The arithmetic expression you have specified appears in [Formula] box of [Z1].

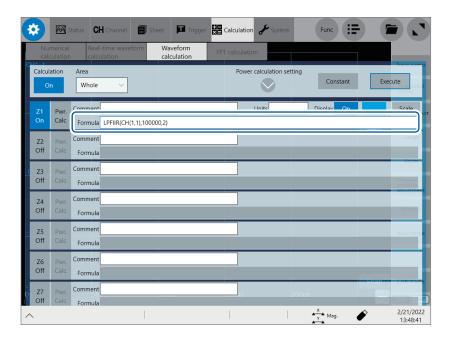


Table ARelationship among sampling rates, sampling frequencies, cutoff
frequencies, and setting resolutions of cutoff frequencies (for both
FIR and IIR filters)

Sampling rate	Sampling period	Sampling frequency	Upper limit of cutoff frequency (Value less than this frequency can be set)	Cutoff frequency setting resolution
200 MS/s	5 ns	200 MHz	100 MHz	200 kHz
100 MS/s	10 ns	100 MHz	50 MHz	100 kHz
50 MS/s	20 ns	50 MHz	25 MHz	50 kHz
20 MS/s	50 ns	20 MHz	10 MHz	20 kHz
10 MS/s	100 ns	10 MHz	5 MHz	10 kHz
5 MS/s	200 ns	5 MHz	2.5 MHz	5 kHz
2 MS/s	500 ns	2 MHz	1 MHz	2 kHz
1 MS/s	1 µs	1 MHz	500 kHz	1 kHz
500 kS/s	2 µs	500 kHz	250 kHz	500 Hz
200 kS/s	5 µs	200 kHz	100 kHz	200 Hz
100 kS/s	10 µs	100 kHz	50 kHz	100 Hz
50 kS/s	20 µs	50 kHz	25 kHz	50 Hz
20 kS/s	50 µs	20 kHz	10 kHz	20 Hz
10 kS/s	100 µs	10 kHz	5 kHz	10 Hz
5 kS/s	200 µs	5 kHz	2.5 kHz	5 Hz
2 kS/s	500 µs	2 kHz	1 kHz	2 Hz
1 kS/s	1 ms	1 kHz	500 Hz	1 Hz
500 S/s	2 ms	500 Hz	250 Hz	500 mHz
200 S/s	5 ms	200 Hz	100 Hz	200 mHz
100 S/s	10 ms	100 Hz	50 Hz	100 mHz
50 S/s	20 ms	50 Hz	25 Hz	50 mHz
20 S/s	50 ms	20 Hz	10 Hz	20 mHz
10 S/s	100 ms	10 Hz	5 Hz	10 mHz
5 S/s	200 ms	5 Hz	2.5 Hz	5 mHz
2 S/s	500 ms	2 Hz	1 Hz	2 mHz
1 S/s	1 s	1 Hz	0.5 Hz	1 mHz

• Stating a measurement and waveform calculation with the instrument having no waveform data allows the sampling rate setting on the measurement setting screen or the waveform screen to define a settable upper limit of a cutoff frequency.

• Tapping [Execute] on the waveform calculation screen to perform calculations using waveform data previously acquired in the instrument allows the sampling rate setting to define a settable upper limit of a cutoff frequency.

• The instrument with the external sampling clock setting performs calculations with one sample fixed at 1 Hz.

8.6 Explanations of Filter Calculation

Filter type

Filter name	Description	
FIRLPF (Finite impulse response low-pass filter) IIRLPF (Infinite impulse response low-pass filter)	Allows low-frequency components to pass, thus eliminating high-frequency-component noise.	
FIRHPF (Finite impulse response high-pass filter) IIRHPF (Infinite impulse response high-pass filter)	Allows high-frequency components to pass, thus eliminating low-frequency-component noise.	
FIRBPF (Finite impulse response band-pass filter) IIRBPF (Infinite impulse response band-pass filter)	Allows specified frequency-band components to pass, thus eliminating low- and high-frequency-component noise.	
FIRBSF (Finite impulse response band-stop filter) IIRBSF (Infinite impulse response band-stop filter)	Allows low- and high-frequency components to pass, thus eliminating specified-frequency-band-component noise.	

FIR filters (LPF, HPF, BPF, BSF)

The finite impulse response filter is a digital filter whose impulse response is of finite duration.

- Advantages: The filter has linear-phase characteristics (a phase difference is proportional to a frequency), reducing phase distortion (phase delay). Since input signals that have not been involved in any calculations are used for the filter calculation, calculated output signals do not diverge, resulting in stable output signals.
- Disadvantages: A higher order filter is required to obtain steep cutoff characteristics. However, calculation requires a longer time.


IIR filters (LPF, HPF, BPF, BSF)

The infinite impulse response filter is a digital filter whose impulse response continues indefinitely. The instrument uses a Butterworth IIR digital filter, which has flat pass-band characteristics, for calculation.


- Advantages: A lower-order filter is sufficient to obtain sharp cutoff characteristics. A lower-order filter requires a shorter period of calculation time.
- Disadvantages: A filter has non-linear phase characteristics (a phase difference is not proportional to a frequency), causing greater phase distortion (phase delay). Since input signals that have not been involved in any calculations are used for the filter calculation, calculated output signals may diverge, resulting in unstable output signals.

Filter configuration

FIR filter configuration (nth-order FIR filter)

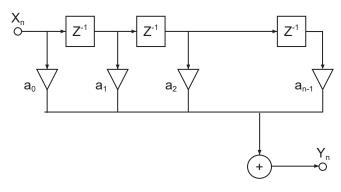

IIR filter configuration (4th-order IIR filter)

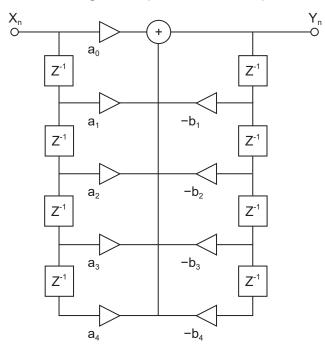

Delayer

A component that delays input signals by one sampling time

Adder A component that outputs the sum of two input signals


Multiplier A component that outputs multiplication of a input signal by constant a

8.7 Setting Power Calculation Conditions

Detailed power calculation settings

This section describes how to set calculation conditions for each of the four circuits.

>[Calculation] > [Waveform calculation] > [Power calculation setting]

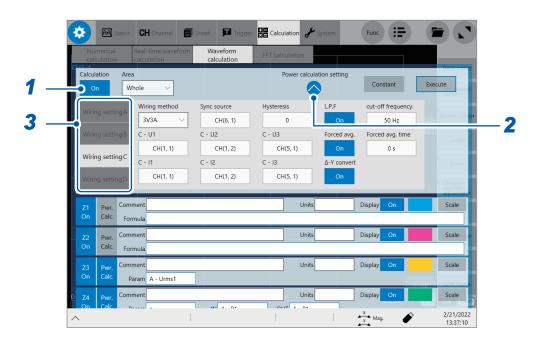


- **1** Tap the [Calculation] button and set it to [On].
- **2** Tap the "Open" mark underneath [Power Calculation Setting]. A screen of detailed power calculation settings will open.
- **3** Tap [Wiring setting A], [Wiring setting B], [Wiring setting C], or [Wiring setting D] and set the desired conditions.

The settings described below can be configured for [Wiring settingA], [Wiring settingB], [Wiring settingC], and [Wiring settingD].

Wiring method settings

This section describes how to set the wiring method.

> [Calculation] > [Waveform calculation] > [Power calculation setting]

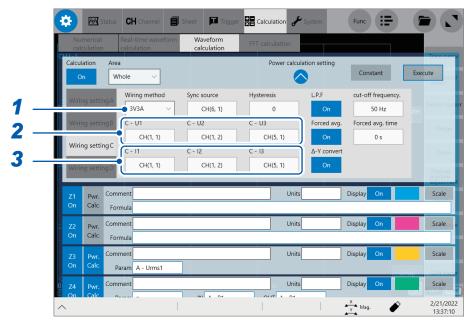

1 Tap the [Wiring method] box and select the wiring method.

Wiring method		Example settings	
1P2W	1-phase/2-wire	Configures the instrument for 1-phase/2-wire (1P2W) measurement and calculations.	
1P3W	1-phase/3-wire	Configures the instrument for 1-phase/3-wire (1P3W) measurement and calculations.	
3P3W	3-phase/3-wire	Configures the instrument for 3-phase/3-wire (3P3W) measurement and calculations. In this wiring method, the two channels of the 3-phase delta wiring line are used to perform two-power-meter measurement. It can be used to measure active power accurately even if the waveforms are distorted due to unbalance.	
3V3A	3-phase/3-wire	Configures the instrument for 3-phase/3-wire (3V3A) measurement and calculations. In this wiring method, the three channels of the 3-phase delta wiring line are used to perform two-power-meter measurement. It can be used to measure not only active power, but also apparent power, reactive power, and power factor accurately even if the lines are unbalanced.	
3P4W	3-phase/4-wire	Configures the instrument for 3-phase/4-wire (3P4W) measurement and calculations. In this wiring method, the three channels of the 3-phase Y (star) wiring line are used to perform three-power-meter measurement.	

See "16 Power Equations and Wiring Specifications" (p. 420).

2 Tap the voltage boxes ([U1] to [U3]) and set the voltage channel for each phase.

Set built-in unit and real-time calculation channels.

8

3 Tap the current boxes ([11] to [13]) and set the current channel for each phase.


Set built-in unit and real-time calculation channels.

Which voltage boxes ([U1] to [U3]) and current boxes ([I1] to [I3]) are displayed depends on the wiring method.

- Check the unit input and wiring method before measurement. Incorrect wiring will prevent proper measurement and calculation.
- Selecting either 3P3W or 3V3A when performing 3-phase/3-wire measurement will result in the same power waveform, since both methods use the same power waveform (P) measurement method.

Configuring zero-cross settings

A zero-cross event occurs when an input signal crosses the zero level. In power waveform calculations, the interval from one zero-cross to the next zero-cross when the signal crosses the zero level in the same direction is defined as 1 cycle, and calculations are performed for each cycle.

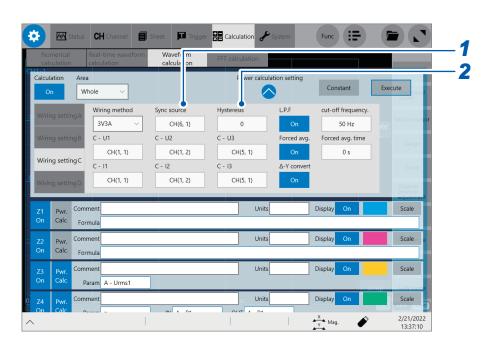

> [Calculation] > [Waveform calculation] > [Power calculation setting]

1 Tap the [Sync source] box and set the channel to use as the basis for cycles.

Set built-in unit and real-time calculation channels.

Set the source channel (zero-cross detection channel) to use in order to determine the cycle (zero-cross interval), which provides the basis for calculations.

Calculations will be performed from the first zero-cross point in captured waveforms to the last zero-cross point.

If specifying the interval with **[Area]**, the calculation scope will be defined as the interval from the first zerocross point that falls within the specified range to the last zero-cross point in that range.

2 Tap the [Hysteresis] box and set the threshold.

0 V^{III} to 9.9999E+29 V

Sync source

Set the source channel (zero-cross detection channel) to use in order to determine the cycle (zerocross interval), which provides the basis for calculations.


Calculations will be performed from the first zero-cross point in captured waveforms to the last zero-cross point.

If specifying the interval with **[Area]**, the calculation scope will be defined as the interval from the first zero-cross point that falls within the specified range to the last zero-cross point in that range.

Hysteresis

The cycle that provides the basis for calculations is the zero-cross interval for the sync source channel. If there is noise near this zero-cross, the instrument won't be able to detect one cycle accurately.

Hysteresis prevents erroneous calculations due to noise near the zero-cross by allowing you to set a threshold value.

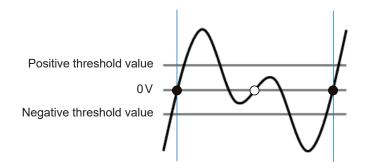

After a zero-cross point is detected (• mark), points at which 0 V is crossed (O mark) will not be treated as the next zero-cross point unless the signal has exceeded the hysteresis width (the range between the positive hysteresis threshold value and the negative hysteresis threshold value).

Low-pass filter settings

This section describes how to apply the IIR low-pass filter.

Calculation] > [Waveform calculation] > [Power calculation setting]

calculati		Real-time waveform calculation	Waveform calculation	FFT calc	ulation				
Calculation On		nole 🗸		F	Power calculat	tion set ng	Const it	Execu	ite Hori ontal
	etting A	Wiring method	Sync source	Hysteres	sis	L.P.F	cut-off frequency.		Section cursor
		3V3A 🗸	CH(6, 1)		0	On	50 Hz		Section curso
	etting B	C - U1	C - U2	C - U3		Forced avg.	Forced avg. time		Gauge
Wiring se	tting	CH(1, 1)	CH(1, 2)	CH	(5, 1)	On	0 s		
winng se	aunge	C - 11	C - 12	C - 13		∆-Y convert			Zoom
	tting D	CH(1, 1)	CH(1, 2)	CH	l(5, 1)	On			Channel
	_		_		_				position adjustment
Z1 Pw		nent			Units		Display On		Scale
On Cal	lc. Forr	nula							
Z2 Pw	r. Comr	nent			Units		Display On		Scale
On Cal	lc. Forr	nula							
	" Comn	nent			Units		Display On		Scale
72 Dur		aram A - Urms1							
Z3 Pw On Cal	lc. Pa	aram A - Urms I						inap	CAN frame
On Cal	Comp				Unite		Dicplay Op	E.	Scale
	r. Com				IS Units		Display On		Scale रा

1 Tap the [L.P.F] button and set it to [On].

2 (If the [L.P.F] button is set to [On])

Tap the low-pass filter's [cut-off frequency] box and set the frequency.

0 Hz^{II} to 1E+8 Hz

Low-pass filter

You can set an IIR low-pass filter to limit the frequency band.

This filter can be used to reject high-frequency components and unnecessary external noise components that exceed the set frequency.

For more information about the maximum cutoff frequencies that can be set, see Table A (p. 241). (The maximum cutoff frequency is half the sampling frequency, which is determined by the time width setting.)

Forced average time setting

This section describes how to force the instrument to perform calculations once a specified time elapses.

Func П Ċ CH Calculatio ā Waveform calculation 1 Constant Execute Whole 2 cut-off f quency Wiring method Sync source Hysteresis I.P. 3V3A CH(6, 1) 0 Hz C - U1 C - U2 C - U3 CH(1, 2) CH(5, 1) CH(1, 1) 0 s Wiring setting C C - 12 C - I1 C - 13 A-Y convert CH(1, 1) CH(1, 2) CH(5, 1) Units Display Scale Comment Pwr. Calc Formula Units Display Scale Comment Z2 On Pwr. Calc Formula Units Scale Comment Display Param A - Urms1 Units Display Scale mment 2/21/2022 13:37:10 Y Mag. Î

- **1** Tap the [Forced avg.] button and set it to [On].
- 2 (If the [Forced avg.] button is set to [On])Tap the [Forced avg. time] box and set the forced average time.


> [Calculation] > [Waveform calculation] > [Power calculation setting]

0 s[™] to 9.9999E+29 s

$\Delta\text{-}\mathbf{Y}$ conversion setting

This section describes how to convert Δ (delta) wiring to Y (star) wiring for a 3-phase measurement line.

This function is valid when the [Wiring method] is [3V3A].

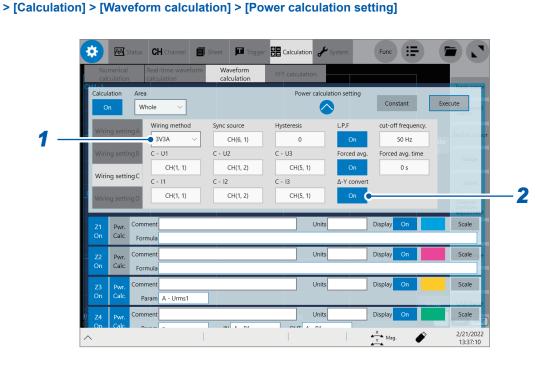


1 Tap the [Wiring method] box and select [3V3A].

2 Tap the [A-Y convert] button and set it to [On].

Δ -Y conversion

This function lets you perform measurement using the phase voltage applied to the motor coil as Y wiring even when using delta wiring when you can't access the neutral point in a motor that uses Y wiring internally.

Although voltage waveform, voltage measured value, and harmonic voltage input all use line-to-line voltages, calculations are made using phase voltages.

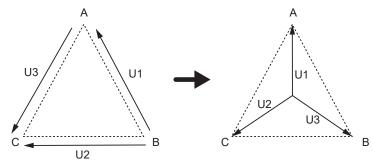


- With ∆–Y conversion, a virtual neutral point is used to convert voltage waveforms to vectors for use in analysis.
- Results may differ from actual phase voltages.
- Whereas active power for 3V3A wiring uses the two-power-meter method, after conversion the three-power-meter method will be used.

8.8 Types of Power Calculations and Explanations

This section describes how to set the types of power calculations to perform.

> [Calculation] > [Waveform calculation]

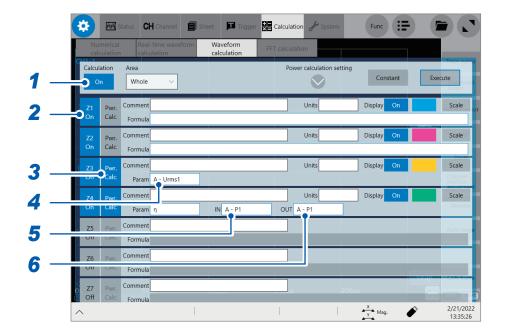

- **1** Tap the [Calculation] button and set it to [On].
- 2 Tap the calculation channel you wish to configure ([Z1] to [Z16]) and set it to [On].
- **3** (When setting a power calculation) Tap [Power Calc.] to enable power calculations.
- **4** Tap the [Param] box and select the type of calculation.

Parameter	Туреѕ
Voltage (U)	RMS value (Urms), mean value (Umn), simple average value (Udc)
Current (I)	RMS value (<i>Irms</i>), mean value (<i>Imn</i>), simple average value (<i>Idc</i>)
Power (P)	Active power (P), apparent power (S), reactive power (Q), power factor (λ), phase (ϕ)
Other	Efficiency (η), loss (loss)

- 5 (If [Param] is [ŋ] (efficiency) or [Loss])Tap the [IN] box and select the input-side power value.
- 6 (If [Param] is [η] (efficiency) or [Loss])Tap the [OUT] box and select the output-side power value.

.

U (voltage) and I (current)

These waveforms are generated by calculating the value each time voltage and current waveforms cross the zero level and then graphing the results.

.

A 1P2W		C 3V3A	D 3P4W	
U				
Voltage RMS val	lue		_	
D - Urms1	D - Urms2	D - Urms3	D - Urms12	D - Urms123
Voltage mean va	alue			
D - Umn1	D - Umn2	D - Umn3	D - Umn12	D - Umn123
Voltage simple a	average			
D - Udc1	D - Udc2	D - Udc3		
ouer	5 Odde	5 6445		

Voltage RMS value (Urms), current RMS value (Irms)

Calculates the true RMS value of the voltage or current.

$$Urms = \sqrt{\frac{1}{n} \sum_{i=1}^{n} (U_i)^2}$$

$$Irms = \sqrt{\frac{1}{n} \sum_{i=1}^{n} (I_i)^2}$$

$$n: \text{ Number of data points} \\ U_i: \text{ Voltage input waveform} \\ I_i: \text{ Current input waveform}$$

Voltage mean value (Umn), current mean value (Imn)

Calculates the average value of the voltage or current.

$$Umn = \frac{\pi}{2\sqrt{2}} \cdot \frac{1}{n} \sum_{i=1}^{n} |U_i|$$
$$Imn = \frac{\pi}{2\sqrt{2}} \cdot \frac{1}{n} \sum_{i=1}^{n} |I_i|$$

n: Number of data points

waveform waveform

- *U_i*: Voltage input waveform
- *Ii*: Current input waveform

Voltage simple average value (Udc), current simple average value (Idc)

Calculates the simple average value of the voltage or current.

$$Udc = \frac{1}{n} \sum_{i=1}^{n} U_i$$

$$Idc = \frac{1}{n} \sum_{i=1}^{n} I_i$$

$$i = 1$$

$$Idc = \frac{1}{n} \sum_{i=1}^{n} I_i$$

$$i = 1$$

$$I_i:$$
 Number of data points

$$U_i:$$
 Voltage input waveform

$$I_i:$$
 Current input waveform

P (power)

These waveforms are generated by detecting voltage and current zero-cross events, calculating values for each zero-cross event, and graphing the results.

A 1P2W	B 3P3W	C 3V3A	D 3P4W	
U	1	Р		
Active power				
D - P1	D - P2	D - P3	D - P12	D - P123
Apparent power	r			
D - S1	D - S2	D - S3	D - S12	D - S123
Reactive power				
D - Q1	D - Q2	D - Q3	D - Q12	D - Q123
Power factor				
D - λ1	D - λ2	D - λ3	D - λ12	D - λ123
Power phase an	gle			
D - Φ1	D - Ф2	D - Ф3	D - Φ12	D - Φ123

Active power (P)

Calculates the active power from the average product of the voltage and current waveforms.

$$P = \frac{1}{n} \sum_{i=1}^{n} (U_i \cdot I_i)$$

n: Number of data points

- *U*_{*i*}: Voltage input waveform
- *I_i*: Current input waveform

Apparent power (S)

Calculates the apparent power from voltage RMS values (Urms) and current RMS values (Irms).

 $S = Urms \cdot Irms$

Reactive power (Q)

Calculates the reactive power from the active power (P) and apparent power (S).

$$Q = \sqrt{(S^2 - P^2)}$$

Power factor (λ)

Calculates the reactive power from the active power (P) and apparent power (S).

$$\lambda = \left| \frac{P}{S} \right|$$

Power phase angle (ϕ)

Calculates the reactive power from the active power (P) and apparent power (S).

$$\phi = \cos^{-1}\left(\left|\frac{P}{S}\right|\right)$$

.

Others (efficiency, loss)

The instrument can calculate and display efficiency (η) [%] and loss [W] using the active power value and motor power value.

A 1P2W	B 3P3W	
		Others
Efficiency		
η		
Loss		
Loss		

Efficiency (η) and loss (loss)

Calculates the efficiency (η) and loss from the input-side power value (P_{in}) and the output-side power value (P_{out}).

Input side	[IN]:	$P_{\rm in}$
Output side	[OUT] :	$P_{\rm out}$
Efficiency	[ŋ]:	$100 imes P_{\mathrm{out}} / P_{\mathrm{in}} $
Loss	[Loss]:	$ P_{\rm in} - P_{\rm out} $

Types of Power Calculations and Explanations

FFT Calculation Function

Using the FFT function allows you to analyze input signal data with respect to frequency through the FFT calculation.

This function is useful to perform frequency analysis of a variety of signals, such as those from rotating objects, vibration, and sound.

See "16.2 FFT Definitions" (p. 409).

The instrument can perform FFT calculation using data previously obtained and processed through waveform calculation, as well as that being acquired concurrently with measurement. Using Model 8968 High Resolution Unit or Model 8979 Charge Unit, which are equipped with an anti-aliasing filter, allows a cutoff frequency to automatically be set in conjunction with the frequency range setting.

The FFT calculation function is not available in the following occasions:

- When the envelope is used
- When the real-time saving is set to [On]

Major features

- FFT calculation frequency range: 500 mHz to 100 MHz
- FFT calculation types (eight calculations)

FFT calculation type			
Linear spectrum	RMS spectrum		
Power spectrum	1CH Phase spectrum		
Cross power spectrum	Transfer function		
Coherence function	2CH Phase spectrum		

· For FFT calculation using signals outputted from a sound level or vibration meter connected with the instrument, you can directly read values in decibels processed through calibration by configuring the scaling setting in the channel setting screen.

See "3.2 Converting Input Values (Scaling Function)" (p. 56).

To perform FFT calculations without being affected by aliasing distortion due to sampling


- Using an input module equipped with a anti-aliasing filter is recommended.
- See "16.2 FFT Definitions" (p. 409), "Aliasing" (p. 411), and "Anti-aliasing filter" (p. 412).
- · For more information about the specifications of the FFT calculation function, refer to Quick Start Manual.

9.1 Operating Procedure


The following two methods are available:

Newly performing measurement before calculation.	You have to configure the FFT calculation settings before starting measurement.
Performing calculations using existing data	The instrument can perform calculations using waveform data that has already been acquired or that saved on storage devices.

Newly performing measurement and calculation

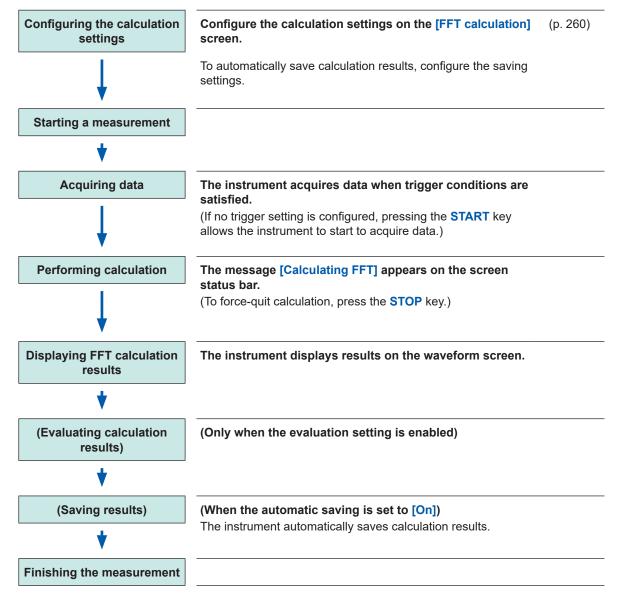

Performing calculations using existing data

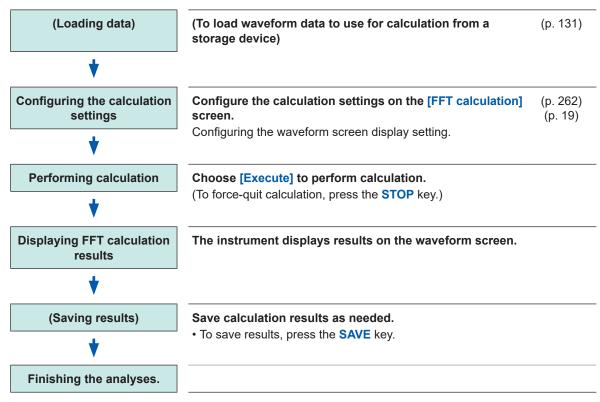

To specify a calculation range and perform calculation


You can specify a calculation range on the waveform screen. See "9.4 Performing Calculations on the Waveform Screen" (p. 276).

To automatically save waveform calculation results after measurement

See "Automatically saving waveform data" (p. 120).

9.2 Enabling the FFT Calculation Settings

> [Calculation] > [FFT calculation]

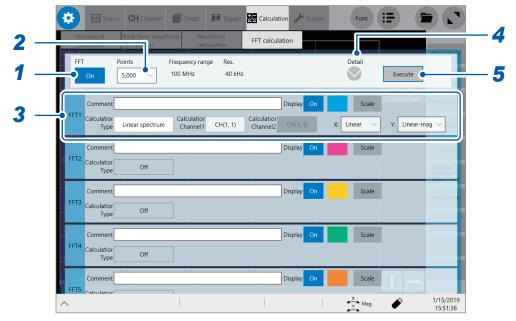

- **1** Tap the [FFT] button to set it to [On].
- **2** Tap the [Points] box, and then from the list, choose an option for the number of calculation points.

See "Specifying the number of calculation points" (p. 262).

3 Configure the basic FFT calculation settings.

The settings includes an FFT calculation type, channels, vertical- and horizontal-axes display preference, and display color.

See "FFT calculation advanced settings" (p. 272).

4 Configure the advanced FFT calculation settings.

The settings includes an averaging method, the number of acquisitions for averaging, window function, attenuation rate, correction method, correction factor, and peak value display method. See "Averaging calculation results" (p. 268).

See Averaging calculation results (p. 200).

See "Configuring the window function settings" (p. 265).

See "Configuring the calculation result peak value settings" (p. 267).

5 (To newly preform measurement before calculation)

Press the START key

The instrument starts a measurement to acquire data that contains the number of calculation points specified in the **[Points]** box (p. 262), and performs an FFT calculation.

(To perform calculations using existing data)

Tap [Execute].

The instrument performs a calculation using data displayed on the waveform screen (previously measured data stored in the internal buffer memory or data loaded from storage devices) that contains the number of calculation points specified in the **[Points]** box (p. 262).

You cannot change a frequency range. The instrument automatically set a frequency range according to a time-axis range and the point count setting.

See "Relationship among frequency ranges, frequency resolutions, and the number of calculation points" (p. 263).

To automatically save waveform calculation results after measurement

See "Automatically saving waveform data" (p. 120).

To allocate a calculation result waveform on a sheet

See "1.4 Configuring the Sheet Settings" (p. 19).

To toggle sheets on the waveform screen

See "Switching sheets on the waveform screen" (p. 24).


9.3 Setting FFT Calculation Conditions

This section describes how to configure the calculation condition setting.

Specifying the number of calculation points

You can specify the number of samples to be used for an FFT calculation.

> [Calculation] > [FFT calculation]

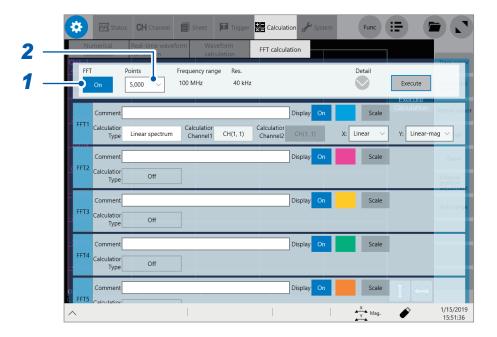

- This calculation point setting automatically decides the frequency range and frequency resolution, See "Relationship among frequency ranges, frequency resolutions, and the number of calculation points" (p. 263).
- Increasing the number of calculation points enhances the frequency resolution; however, it also increases the time required for calculation.

To perform calculation with the external sampling

Set the external sampling to [On]. (p. 6)

- **1** Tap the [FFT] button to set it to [On].
- **2** Tap the [Points] box, and then from the list, choose an option for the number of calculation points.

1000[™], 2000, 5000, 10000, 20000, 50000, 100000

Relationship among frequency ranges, frequency resolutions, and the number of calculation points

(1000 points to 10000 points)

		_		Number of FFT calculation points						
Sampling rate	Sampling period	Frequency range	10	00	20	00	50	00	100	000
(S/s)	penod	(Hz)	Resolution (Hz)	Acquisition period	Resolution (Hz)	Acquisition period	Resolution (Hz)	Acquisition period	Resolution (Hz)	Acquisition period
200 M	5 ns	100 M* ¹	200 k	5 µs	100 k	10 µs	40 k	25 µs	20 k	50 µs
100 M	10 ns	50 M* ¹	100 k	10 µs	50 k	20 µs	20 k	50 µs	10 k	100 µs
50 M	20 ns	25 M*1	50 k	20 µs	25 k	40 µs	10 k	100 µs	5 k	200 µs
20 M	50 ns	10 M* ¹	20 k	50 µs	10 k	100 µs	4 k	250 µs	2 k	500 µs
10 M	100 ns	5 M* ¹	10 k	100 µs	5 k	200 µs	2 k	500 µs	1 k	1 ms
5 M	200 ns	2.5 M*1	5 k	200 µs	2.5 k	400 µs	1 k	1 ms	500	2 ms
2 M	500 ns	1 M* ¹	2 k	500 µs	1 k	1 ms	400	2.5 ms	200	5 ms
1 M	1 µs	500 k*1	1 k	1 ms	500	2 ms	200	5 ms	100	10 ms
500 k	2 µs	250 k*1	500	2 ms	250	4 ms	100	10 ms	50	20 ms
200 k	5 µs	100 k*1	200	5 ms	100	10 ms	40	25 ms	20	50 ms
100 k	10 µs	50 k	100	10 ms	50	20 ms	20	50 ms	10	100 ms
50 k	20 µs	25 k	50	20 ms	25	40 ms	10	100 ms	5	200 ms
20 k	50 µs	10 k	20	50 ms	10	100 ms	4	250 ms	2	500 ms
10 k	100 µs	5 k	10	100 ms	5	200 ms	2	500 ms	1	1 s
5 k	200 µs	2.5 k	5	200 ms	2.5	400 ms	1	1 s	500 m	2 s
2 k	500 µs	1 k	2	500 ms	1	1 s	400 m	2.5 s	200 m	5 s
1 k	1 ms	500	1	1 s	500 m	2 s	200 m	5 s	100 m	10 s
500	2 ms	250	500 m	2 s	250 m	4 s	100 m	10 s	50 m	20 s
200	5 ms	100	200 m	5 s	100 m	10 s	40 m	25 s	20 m	50 s
100	10 ms	50	100 m	10 s	50 m	20 s	20 m	50 s	10 m	100 s
50	20 ms	25	50 m	20 s	25 m	40 s	10 m	100 s	5 m	200 s
20	50 ms	10* ²	20 m	50 s	10 m	100 s	4 m	250 s	2 m	500 s
10	100 ms	5* ²	10 m	100 s	5 m	200 s	2 m	500 s	1 m	1 ks
5	200 ms	2.5* ²	5 m	200 s	2.5 m	400 s	1 m	1 ks	500 µ	2 ks
2	500 ms	1* ²	2 m	500 s	1 m	1 ks	400 µ	2.5 ks	200 µ	5 ks
1	1 s	500 m* ²	1 m	1 ks	500 µ	2 ks	200 µ	5 ks	100 µ	10 ks

*1: The anti-aliasing filter of a module is set to off.

*2: The anti-aliasing filter cutoff frequency of a module is set at 20 Hz.

Relationship among frequency ranges, frequency resolutions, and the number of calculation points

(20000 points to 100000 points)

		_		Nur	nber of FFT calculation points				
Sampling rate	Sampling period	Frequency range	200	000	500	000	100	000	
(S/s)	penod	(Hz)	Resolution (Hz)	Acquisition period	Resolution (Hz)	Acquisition period	Resolution (Hz)	Acquisition period	
200 M	5 ns	100 M* ¹	10 k	100 µs	4 k	250 µs	2 k	500 µs	
100 M	10 ns	50 M* ¹	5 k	200 µs	2 k	500 µs	1 k	1 ms	
50 M	20 ns	25 M* ¹	2.5 k	400 µs	1 k	1 ms	500	2 ms	
20 M	50 ns	10 M* ¹	1 k	1 ms	400	2.5 ms	200	5 ms	
10 M	100 ns	5 M* ¹	500	2 ms	200	5 ms	100	10 ms	
5 M	200 ns	2.5 M* ¹	250	4 ms	100	10 ms	50	20 ms	
2 M	500 ns	1 M* ¹	100	10 ms	40	25 ms	20	50 ms	
1 M	1 µs	500 k*1	50	20 ms	20	50 ms	10	100 ms	
500 k	2 µs	250 k*1	25	40 ms	10	100 ms	5	200 ms	
200 k	5 µs	100 k* ¹	10	100 ms	4	250 ms	2	500 ms	
100 k	10 µs	50 k	5	200 ms	2	500 ms	1	1 s	
50 k	20 µs	25 k	2.5	400 ms	1	1 s	500 m	2 s	
20 k	50 µs	10 k	1	1 s	400 m	2.5 s	200 m	5 s	
10 k	100 µs	5 k	500 m	2 s	200 m	5 s	100 m	10 s	
5 k	200 µs	2.5 k	250 m	4 s	100 m	10 s	50 m	20 s	
2 k	500 µs	1 k	100 m	10 s	40 m	25 s	20 m	50 s	
1 k	1 ms	500	50 m	20 s	20 m	50 s	10 m	100 s	
500	2 ms	250	25 m	40 s	10 m	100 s	5 m	200 s	
200	5 ms	100	10 m	100 s	4 m	250 s	2 m	500 s	
100	10 ms	50	5 m	200 s	2 m	500 s	1 m	1 ks	
50	20 ms	25	2.5 m	400 s	1 m	1 ks	500 µ	2 ks	
20	50 ms	10* ²	1 m	1 ks	400 µ	2.5 ks	200 µ	5 ks	
10	100 ms	5* ²	500 µ	2 ks	200 µ	5 ks	100 µ	10 ks	
5	200 ms	2.5* ²	250 µ	4 ks	100 µ	10 ks	50 µ	20 ks	
2	500 ms	1* ²	100 µ	10 ks	40 µ	25 ks	20 µ	50 ks	
1	1 s	500 m ^{*2}	50 µ	20 ks	20 µ	50 ks	10 µ	100 ks	

*1 The anti-aliasing filter of a module is set to off.

*2 The anti-aliasing filter cutoff frequency of a module is set at 20 Hz.

Configuring the window function settings

You can choose a window function by which the instrument multiplies an acquired input signal. Using a window function reduces a leakage error. See "Window function" (p. 415).

The window functions fall into three major groups.





Rectangular window


Hann windowHamming windowBlackman window



- Exponential window
- Blackman Harris window
 Flat-top window

Using a non-rectangular window function generally attenuates FFT calculation results. Compensating this attenuation for effect of the use of a non-rectangular window function can correct calculation results to an equivalent level of those multiplied by a rectangular window.



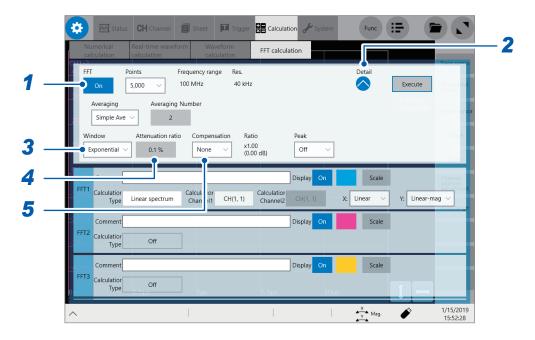

1 Tap the [FFT] button to set it to [On].

2 Tap the open mark under [Detail].

The FFT calculation advanced setting window appears.

3 Tap the [Window] box, and then choose a window function from the list.

Rectangular^Ø, Hanning, Hamming, Blackman, Blackman Harris, Flat-top, Exponential


See "Window function" (p. 415).

4 (When you choose [Exponential] in the [Window] box)

Tap the [Attenuation ratio] box, and then enter an attenuation rate.

0.1%[⊠] to 99.9%

Noise superimposing on attenuating waveform is mitigated.



Attenuation rate: 10%

5 Tap the [Compensation] box, and then choose a compensation method for an attenuation from the list.

The instrument compensates an attenuation of a calculation result for effect of the use of a non-rectangular window function.

None [⊠]	Does not compensate any attenuation for effect of the use of a window function.
Power	Compensates an attenuation for effect to correct energy of time-domain waveform to an equivalent level of energy generated when multiplied by a rectangular window.
Average	Compensates an attenuation for effect to correct an average of a time-domain waveform to an equivalent level of an average calculated when multiplied by a rectangular window.


Choosing [Rectangular] in the [Window] box fixes a correction value to a factor of one (0 dB).

Configuring the calculation result peak value settings

The instrument can display global or local maximum values of input signals and calculation results on the waveform screen.



> [Calculation] > [FFT calculation]

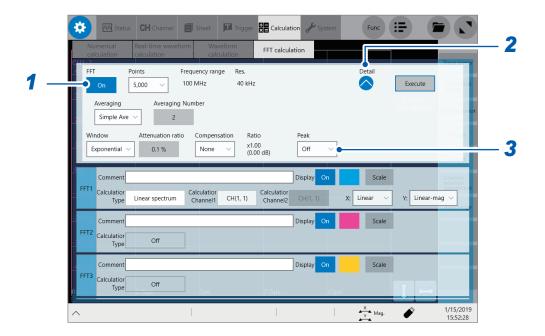

1 Tap the [FFT] button to set it to [On].

2 Tap the open mark under [Detail].

The FFT calculation advanced setting window appears.

3 Tap the [Peak] box, and then from the list, choose a peak value type to be displayed.

Off	Does not display any peak values.	Maximal value 1
Maximal	Displays the ten greatest values among maximal values. When a value of a data point is greater than values of both the adjacent points, the instrument determines that the point is a local maximum.	Maximum value
Maximum	Displays the ten greatest values.	4 5 6

- When the instrument does not find any peak values, it displays no values.
- The instrument can display peak values on the waveform screen, but no peak values can be stored in text-form files.
- Some split screens does not always display ten peak values. Such a screen displays as many values as possible in decreasing order.


Averaging calculation results

The averaging is a series of processes that include repeatedly acquiring waveforms, and then averaging them to perform calculations using the averaged waveform.

Using this function mitigates the effect of noise superimposed on waveforms and unstable factors.



> [Calculation] > [FFT calculation]

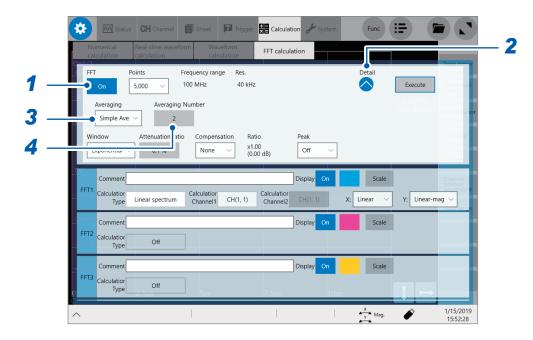

1 Tap the [FFT] button to set it to [On].

2 Tap the open mark under [Detail].

The FFT calculation advanced setting window appears.

3 Tap the [Averaging] box, and then choose a averaging method from the list.

Off [⊠]	Does not perform any averaging.
Simple Ave	Calculates an simple average of a frequency-domain waveform to output a calculation result.
Exp Ave	Calculates an exponential average of a frequency-domain waveform to output a calculation result.
Freq-peak hold	Continues to display the maximum value of a frequency-domain waveforms.

See "Averaging" (p. 414).

See "Relationship between recording modes and averaging types" (p. 270).

4 Tap the [Averaging Number] box, and then enter the number of times the instrument acquires a waveforms used for an averaging process.

2[™] to 10,000

Relationship between FFT calculation types and averaging types


✓: Enable, –: Disable

Coloulation type	Averaging		
Calculation type	Simple	Exponential	Peak hold
Off	_	_	_
Linear spectrum	✓	~	~
RMS spectrum	✓	~	~
Power spectrum	✓	~	~
1CH Phase spectrum	_	_	_
Cross power spectrum	✓	~	~
Transfer function	✓	~	~
Coherence function	✓	~	_
2CH Phase spectrum	_	-	_

Relationship between recording modes and averaging types

When the recording mode is set to [Single]


Repeatedly measures a waveform until the waveform acquisition count reaches the number specified in the **[Averaging Number]** box.

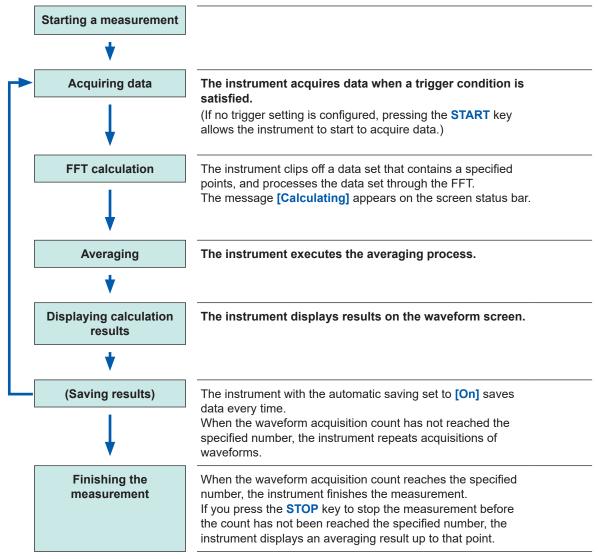

When the recording mode is set to [Repeat]

The instrument continues the measurement even if the waveform acquisition count has reached the number specified in the **[Averaging Number]** box.


When the waveform acquisition count reaches, the instrument re-executes the averaging process and repeats measurements until you press the **STOP** key.

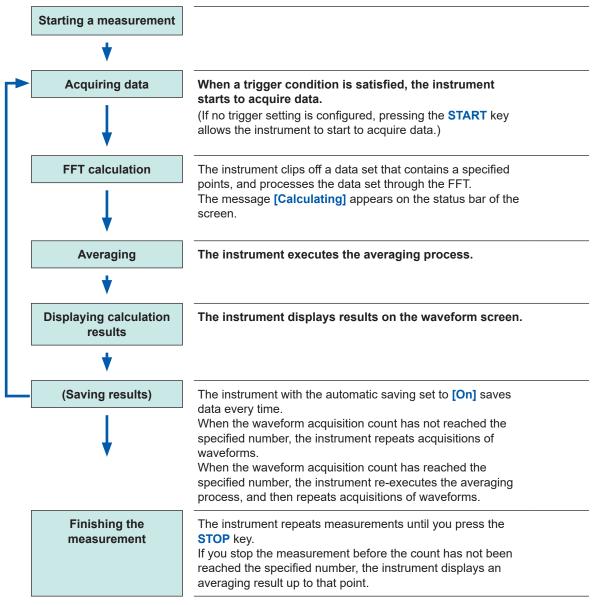

FFT calculation advanced settings

You can configure the FFT analysis setting that includes a type, channels, a waveform display color, and X- and Y-axes.

> [Calculation] > [FFT calculation]

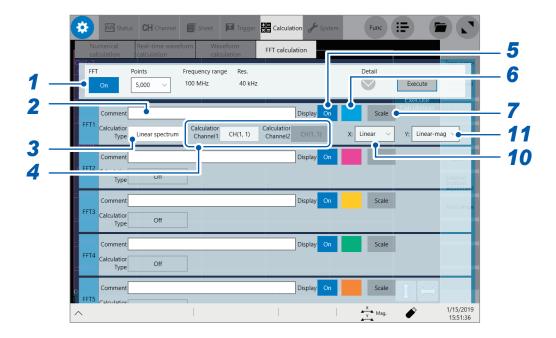

1 Tap the [FFT] button to set it to [On].

2 Enter a comment in the [Comment] box.

Number of characters that can be entered: up to 40

3 Tap the [Calculation Type] box, and then choose a calculation type from the list.

Off [∞]	Does not perform any calculations.
Linear spectrum	(p. 279)
RMS spectrum	(p. 281)
Power spectrum	(p. 283)
1CH Phase spectrum	(p. 284)
Cross power spectrum	(p. 285)
Transfer function	(p. 286)
Coherence	(p. 287)
2CH Phase spectrum	(p. 284)


See "Calculation types and internal calculation formulas" (p. 288).

- 4 Tap the [Calculation Channel 1] and [Calculation Channel 2] boxes in turn, and then from the list, choose channels to use for a calculation. Target: built-in modules, calculations
- 5 Tap the [Display] button of the FFT calculation results to set it to [On].

6 Tap the color button to the right of the [Display] button, and then choose a display color of the channel from the color pallet.

7 Tap [Scale] to the right of the color button.

The [Scale Settings] dialog box appears.




8 Tap the [Scale Settings] button to choose a Y-axis scale setting method.

Auto [⊠]	Automatically set the Y-axis (vertical axis) scale from a calculation result.
Manual	Allows you to set the Y-axis (vertical axis) scale depending on your purpose. This is useful to enlarge or reduce an amplitude and to shift the waveform upward or downward.

9 (When you choose [Manual] in the [Scale Settings] box.)

Tap the [Up] or [Low] box.

The numerical value entry dialog box appears.

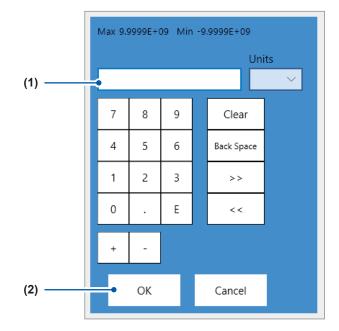

(1) Enter an upper and lower value in each box.

Use the numerical keypad, [+] button, and [-] button to enter.

-9.9999E+19 to 9.9999E+19

(2) Tap [OK].

The numerical value entry dialog box closes.

Q

10 Tap the [X:] box, and then choose a X-axis scale from the list.

Linear [⊠]	Indicates a frequency on the linear-scaled horizontal axis.	
Log	Indicates a frequency on the logarithmic-scaled horizontal axis. You can observe signals, such as sound and vibration, with the emphasis on a lower frequency range.	

When the instrument performs calculations using the external sampling, it displays the x-axis in terms with the number of samples.

11 Tap the [Y:] box, and then from the list, choose an option for calculation data the Y-axis indicates.

Selectable contents vary depending on calculation types. See "Calculation types and settable items on the X- and Y-axes" (p. 274).

Linear-mag [⊠]	Plots analyzed data on a linear scale.	
Log-magPlots a level of analyzed data (a logarithm of the ratio of a value to a reference in decibels. The reference value is 1 eV. Example: For voltage, the level of 1 V is 0 dB.		
Linear-real	Plots the real part of analyzed data on a linear scale.	
Linear-imag	Plots the imaginary part of analyzed data on a linear scale.	

Calculation types and settable items on the X- and Y-axes

✓: Enable, –: Disable

	X-axis		Y-axis			
Calculation type	Linear	Logarithmic	Amplitude (Linear)	Amplitude (dB)	Real (Linear)	lmaginary (linear)
Off	_	_	-	_	_	-
Linear spectrum	~	~	\checkmark	~	~	~
RMS spectrum	~	~	\checkmark	~	~	~
Power spectrum	~	~	\checkmark	~	_	-
Phase spectrum	~	~	\checkmark	_	_	-
Cross power spectrum	~	~	\checkmark	~	~	~
Transfer function	~	~	\checkmark	~	~	~
Coherence function	~	~	✓	_	_	_

Total harmonic distortion factor (THD)

When the calculation is set to one of the following types and the cursors are enabled, the distortion factor is calculated.

(Linear spectrum, RMS spectrum, power spectrum)

The distortion factor is calculated regarding the cursor position as the fundamental wave. When displaying the two cursors, the instrument regards the A cursor as the fundamental wave to calculate the distortion factor.

When no results are have been obtained, the instrument displays the string [---%].

Incidentally, the total harmonic distortion factor may significantly vary depending on the window function setting.

THD =
$$\sqrt{\frac{\sum (V_n)^2}{(V_0)}} \times 100$$
 [%]

 V_0 = Fundamental wave V_n = *n*th harmonic

9.4 Performing Calculations on the Waveform Screen

To specify a range before calculation

You can specify an FFT calculation range on acquired data.

The default calculation range is the number of the FFT calculation points from the start of measurement.



1	T-Y waveform	Acquired time series waveform
2	FFT waveform	FFT calculation result
3	FFT calculation selection cursor	Specifies an FFT calculation range on the displayed T-Y waveform.

You can specify a calculation range using the display format and split settings. See "1.4 Configuring the Sheet Settings" (p. 19).


✓: Enable, –: Disable

Display format	Split number	Range specification
Time series waveform	T-Y waveform on single screen	_ * ¹
	T-Y waveform on 2-split screen	_ * ¹
	T-Y waveform on 4-split screen	_ * ¹
	T-Y waveform on 8-split screen	_ * ¹
	T-Y waveform on 16-split screen	_ * ¹
FFT waveform	FFT waveform on single screen	_ * ¹
	FFT waveform on 2-split screen	_ * ¹
	FFT waveform on 4-split screen	_ * ¹
	T-Y and FFT waveforms on single screen	✓ * ²
	T-Y and FFT waveforms on 2-split screen	✓ * ²
	T-Y and FFT waveforms on 4-split screen	✓ * ²

*1: An FFT calculation starts at a measurement starting position.

*2: When you choose the "T-Y and FFT waveforms on single screen," "T-Y and FFT waveforms on 2-split screen," or "T-Y and FFT waveforms on 4-split single screen" for the split number setting and specify a calculation range on any sheet, the specified range also applies to FFT calculations on other sheet.


1 Tap the FFT calculation selection cursor displayed on T-Y waveform.

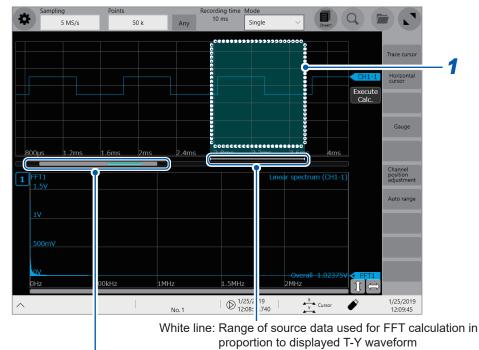

Bar indicating the range being displayed in proportion to whole acquired data Gray bar: T-Y waveform position

Blue bar: FFT calculation selection cursor position

White line: Range of source data used for FFT calculation

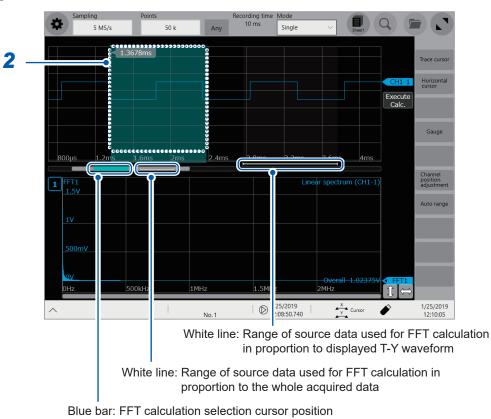

2 Drag the FFT calculation selection cursor.

- **3** Perform an FFT calculation within a range specified wit the FFT calculation selection cursor. Any one of the following actions allows the instrument to perform an FFT calculation within a range newly specified with the FFT calculation selection cursor.
 - Tap [Execute] on the waveform screen.
 - Tap [Execute] on the FFT calculation screen.
 - Press the START key

9.5 FFT Calculation Types

Calculation types and display examples

Linear spectrum

The instrument performs a calculation using strength of input signals within each frequency band to plot it on a frequency-domain graph.

Main uses:

To analyze peaks of frequency components of a waveform


See "Calculation types and internal calculation formulas" (p. 288).

Axis	Display type	Description
Horizontal axis	Linear	Indicates a frequency on a linear scale.
(X-axis)	Logarithmic	Indicates a frequency on a logarithm scale.
Vertical axis	Amplitude (linear)	Indicates analyzed data on a linear scale.
(Y-axis)	Amplitude (decibel)	Indicates analyzed data in decibels. (Reference of 0 dB: 1 eu)*
	Real part (linear)	Indicates the real part of analyzed data.
	Imaginary (linear)	Indicates the imaginary part of analyzed data.

*(Eu: engineering unit) The level is calculated using a reference value in terms with an engineering unit presently set.

(For example, when the unit is set to volts, 0 dB is equivalent to 1 V.)

Examples of waveforms

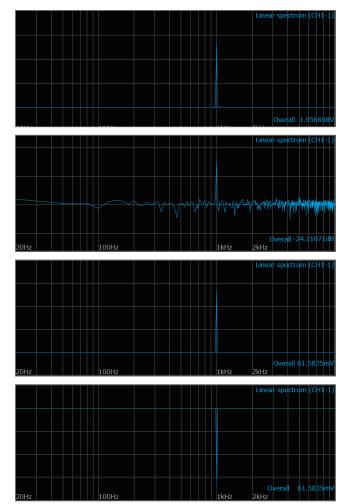

Normal display

Horizontal axis: logarithmic Vertical axis: amplitude (linear)

Normal display

Horizontal axis: logarithmic Vertical axis: amplitude (decibel)

Normal display

Horizontal axis: logarithmic Vertical axis: real part (linear)

Normal display

Horizontal axis: logarithmic Vertical axis: imaginary (linear)

- The instrument with a cursor enabled displays the total harmonic distortion factor (THD) regarding the cursor position as the fundamental wave. When displaying the two cursors, the instrument regards the A cursor as the fundamental wave. When no results have been obtained, the instrument displays the string [---%].
- When a sine wave is only inputted, the component level becomes approximately 1.4 times (3 dB) the overall value. To measure a signal using the same reference as the overall value, analyze it through the RMS spectrum or power spectrum.

See "RMS spectrum" (p. 281) and "Power spectrum" (p. 283).

RMS spectrum

The RMC spectrum calculates an input signal amplitude (RMS values) of each frequency band and plots the calculation results on a graph with a horizontal axis that indicates a frequency. The RMS spectrum shows the same calculation result as the power spectrum that logarithmically describes amplitudes in decibels.

Main uses:

To analyze an RMS value of each frequency component included in a waveform.


See "Calculation types and internal calculation formulas" (p. 288).

Axis	Display type	Description
Horizontal axis	Linear	Indicates a frequency on a linear scale.
(X-axis)	Logarithmic	Indicates a frequency on a logarithm scale.
Vertical axis	Amplitude (linear)	Indicates analyzed data on a linear scale.
(Y-axis)	Amplitude (decibel)	Indicates analyzed data in decibels. (Reference of 0 dB: 1 eu)*
	Real part (linear)	Indicates the real part of analyzed data.
	Imaginary (linear)	Indicates the imaginary part of analyzed data.

*(Eu: engineering unit) The level is calculated using a reference value in terms with an engineering unit presently set.

(For example, when the unit is set to volts, 0 dB is equivalent to 1 V.)

Examples of waveforms

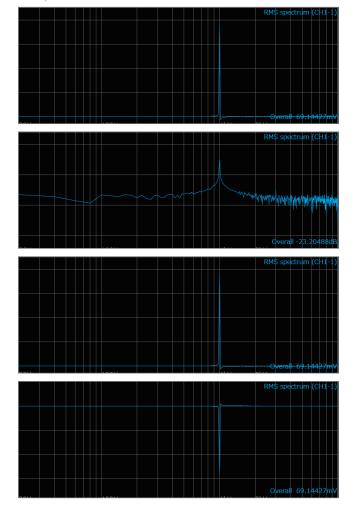

Horizontal axis: logarithmic Vertical axis: amplitude (linear)

Normal display Horizontal axis: logarithmic Vertical axis: amplitude (decibel)

Normal display

Normal display

Horizontal axis: logarithmic Vertical axis: real part (linear)

Normal display Horizontal axis: logarithmic Vertical axis: imaginary (linear)

The instrument with a cursor enabled displays the total harmonic distortion factor (THD) regarding the cursor position as the fundamental wave. When displaying the two cursors, the instrument regards the A cursor as the fundamental wave. When no results have been obtained, the instrument displays the string [---%].

Power spectrum

The power spectrum calculates an input signal power of each frequency band and plots the calculation results on a graph with a horizontal axis that indicates a frequency.

Main uses:

- To analyze peaks of frequency components of a waveform
- To analyze power levels of each frequency component


See "Calculation types and internal calculation formulas" (p. 288).

Axis	Display type	Description
Horizontal axis (X-axis)	Linear	Indicates a frequency on a linear scale.
	Logarithmic	Indicates a frequency on a logarithm scale.
Vertical axis (Y-axis)	Amplitude (linear)	Indicates a square of analyzed data. It represents power components.
	Amplitude (decibel)	Indicates analyzed data in decibels. (Reference of 0 dB: 1 eu ²)*

*(Eu: engineering unit) The level is calculated using a reference value in terms with an engineering unit presently set.

(For example, when the unit is set to volts, 0 dB is equivalent to 1 V².)

Examples of waveforms

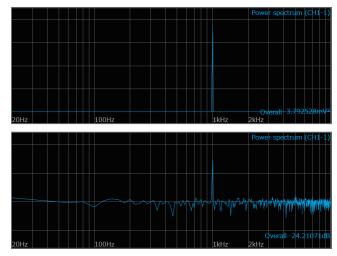

Normal display Horizontal axis: logarithmic Vertical axis: amplitude (linear)

Normal display Horizontal axis: logarithmic Vertical axis: amplitude (decibel)

The instrument with a cursor enabled displays the total harmonic distortion factor (THD) regarding the cursor position as the fundamental wave. When displaying the two cursors, the instrument regards the A cursor as the fundamental wave. When no results have been obtained, the instrument displays the string [---%].

Phase spectrum


The phase spectrum analyzes phase characteristics of an input signal.

Main uses:

- To analyze the phase spectrum of channel 1 The phase of a cosine waveform is indicated using a reference of 0°.
- To analyze the phase difference between channels 1 and 2 See "Calculation types and internal calculation formulas" (p. 288).
- 1ch FFT: The 1ch FFT displays the phase of a signal obtained across channel 1. The phase of a cosine waveform is indicated using a reference of 0°. A non-synchronized time-domain waveform causes phase values to be unstable.
- 2ch FFT: The 2ch FFT displays the phase difference between channels 1 and 2. Positive values indicate that the phase of channel 2 leads channel 1.

Axis	Display type	Description
Horizontal axis	Linear	Indicates a frequency on a linear scale.
(X-axis)	Logarithmic	Indicates a frequency on a logarithm scale.
Vertical axis (Y-axis)	Amplitude (linear)	Indicates analyzed data on a linear scale.

Examples of waveforms

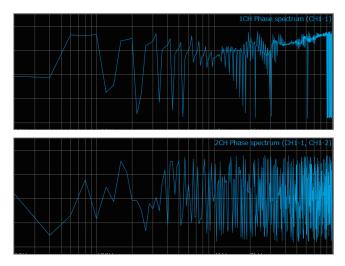

1ch FFT Horizontal axis: logarithmic Vertical axis: amplitude (linear)

2ch FFT Horizontal axis: logarithmic Vertical axis: amplitude (linear)

The instrument with a cursor enabled displays the total harmonic distortion factor (THD) regarding the cursor position as the fundamental wave. When displaying the two cursors, the instrument regards the A cursor as the fundamental wave. When no results have been obtained, the instrument displays the string [---%].

Cross power spectrum

The cross power spectrum finds a product of two input signal spectra. Common frequency components to both two signals can also be obtained.

You can input a voltage waveform and current waveform to calculate power (active power, reactive power, apparent power) of each frequency band.

Main uses:


To analyze common frequency components to two signals See "Calculation types and internal calculation formulas" (p. 288).

Axis	Display type	Description
Horizontal axis	Linear	Indicates a frequency on a linear scale.
(X-axis)	Logarithmic	Indicates a frequency on a logarithm scale.
Vertical axis (Y-axis)	Amplitude (linear)	Indicates a square of an amplitude component of analyzed data on a linear scale.
	Amplitude in decibels (logarithmic)	Indicates an amplitude component in decibels. (Reference of 0 dB: 1 eu ²)*
	Real part (linear)	Indicates a square of the real part of analysis data on a linear scale.
	Imaginary (linear)	Indicates a square of the imaginary part of analyzed data on a linear scale.

*(Eu: engineering unit) The level is calculated using a reference value in terms with an engineering unit presently set.

(For example, when the unit is set to volts, 0 dB is equivalent to $1 V^2$.)

Examples of waveforms

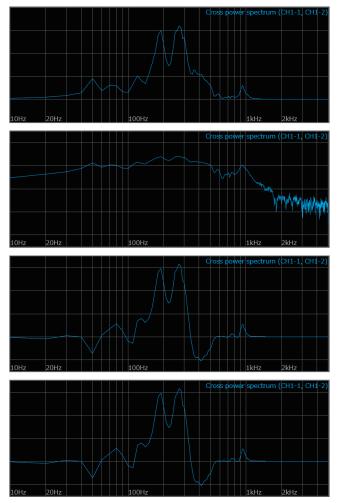

Normal display Horizontal axis: logarithmic Vertical axis: amplitude (linear)

Normal display Horizontal axis: logarithmic Vertical axis: amplitude (decibel)

Normal display

Horizontal axis: logarithmic Vertical axis: real part (linear)

Normal display

Horizontal axis: logarithmic Vertical axis: Imaginary (linear) 9

Transfer function

The instrument can obtain the transfer function (frequency characteristic) of a measurement system from an input and output signals.

Main uses:

- To analyze frequency characteristics of a filter
- · To analyze stability of a feedback control system

• To analyze a resonance frequency of an object using an impulse hammer and pick-up sensor See "Calculation types and internal calculation formulas" (p. 288) and "Linear time-invariant system" (p. 410).

Axis	Display type	Description
Horizontal axis	Linear	Indicates a frequency on a linear scale.
(X-axis)	Logarithmic	Indicates a frequency on a logarithm scale.
Vertical axis	Amplitude (linear)	Indicates an input-to-output ratio on a linear scale. (no units)
(Y-axis)	Amplitude in decibels (logarithmic)	Indicates an input-to-output ratio in decibels.
	Real part (linear)	Indicates the real part of an input-to-output ratio. (no units)
	Imaginary (linear)	Indicates the imaginary part of an input-to-output ratio. (no units)

Examples of waveforms

			Transfer	function (CH1-1, CH1-2)
10Hz 20Hz	100	Hz		ر بر المراجع Hz 2kHz

Normal display

Horizontal axis: logarithmic Vertical axis: amplitude (linear)


Normal display

Horizontal axis: logarithmic Vertical axis: amplitude (decibel)



Normal display

Horizontal axis: logarithmic Vertical axis: imaginary (linear)

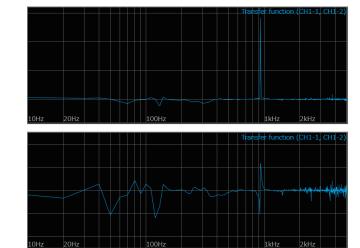

Coherence function

This function shows a ratio of components that have coherence with an input signal to whole components of an output signal. Values ranges zero to one. A coherence function of one shows that an input signal does not affect the frequency of an output signal.

Main uses:

• To analyze a transfer function

• To analyze effects of each input signal on an output signals for a multi-input system. See "Calculation types and internal calculation formulas" (p. 288).

Axis	Display type	Description
Horizontal axis	Linear	Indicates a frequency on a linear scale.
(X-axis)	Logarithmic	Indicates a frequency on a logarithm scale.
Vertical axis (Y-axis)	Amplitude (linear)	Indicates a cause-and-effect relationship of relevance ratio between two input signals, degree of which are presented by a numerical value that ranges zero to one. (non-dimensional)

Examples of waveforms

		Coherence (CH1-1, CH1-2)
1Hz	10Hz	1kHz

Normal display Horizontal axis: logarithmic Vertical axis: amplitude (linear)

- A single measurement causes the coherence function to be one across the entire frequency range. Always execute the averaging process of the FFT function before measurement.
- The coherence function has two general definition formulas. For the definition formulas, refer to "Calculation types and internal calculation formulas" (p. 288).

9

Calculation types and internal calculation formulas

Calculation type	Internal calculation formula (real: real part, imag: imaginary part, log: logarithm)		
Off	Does not perform any calculation.		
Linear spectrum	$X(k) = \sum_{n=0}^{N-1} x(n) W^{kn} \qquad F(k) = CX(k) \qquad C = \begin{cases} 1/N(DC) \\ 2/N(AC) \end{cases}$ linear = F(k) real = Re{F(k)} imag = Im{F(k)} log = 20log F(k)		
RMS spectrum	$F'(k) = C'F(k) \qquad C' = \begin{cases} 1 (DC) \\ 1/\sqrt{2}(AC) \end{cases}$ linear = F'(k) real = Re{F'(k)} imag = Im{F'(k)} log = 20log F'(k)		
Power spectrum	$P(k) = a F(k) ^{2} \qquad a = \begin{cases} 1 & (DC) \\ 1/2 & (AC) \end{cases}$ linear = P(k) $\log = 10\log P(k) $		
Phase spectrum	$\theta(k) = \frac{180}{\pi \times \tan^{-1}(\text{Im}(F'(k))/\text{Re}(F'(k)))}$ $\theta(k) = \frac{180}{\pi \times \tan^{-1}(\text{Im}(S_{yx}(k))/\text{Re}(S_{yx}(k)))}$		
Cross power spectrum	$\begin{split} S_{yx}(k) &= X^*(k)Y(k): \text{Cross spectrum} \\ X_{power}(k) &= AS_{yx}(k) \qquad A = \begin{cases} 1/N^2 (\text{DC}) \\ 2/N^2 (\text{AC}) \end{cases} \\ linear &= X_{power}(k) \qquad real = \text{Re}\{X_{power}(k)\} \\ imag &= \text{Im}\{X_{power}(k)\} \qquad log = 10 \text{log} X_{power}(k) \end{split}$		
Transfer function	$\begin{split} H(k) &= Y(k)/X(k)\\ linear &= H(k) real = \operatorname{Re}\{H(k)\} imag = \operatorname{Im}\{H(k)\} log = 20 \log H(k) \end{split}$		
Coherence function	$coh(k) = \sqrt{\frac{S_{yx}(k)S_{yx}^{*}(k)}{S_{xx}(k)S_{yy}(k)}}$		

• • • • • • • • • • • • • • • • • •


10 Memory Division Function

You can divide the internal memory into multiple blocks and store waveforms into them.

Start block:	Specifying a start block allows a waveform to be stored in other blocks without deleting previously measured waveforms.
Reference block:	You can overlay a newly acquired waveform with those retained in other blocks.
Blocks to be used:	Storing waveforms into multiple blocks can shorten dead times between blocks.


The memory can be divided into up to 1024 blocks (the more blocks you divide the memory into, the shorter the recording length is).

Normal



Recording length

Memory division

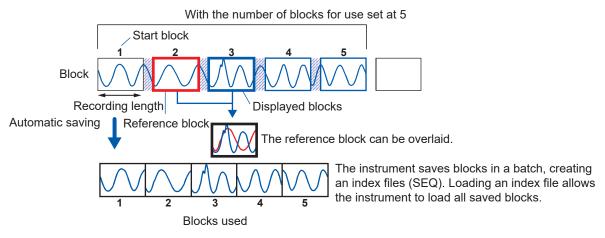

For manual save, you can choose whether to collectively save blocks used or to save only displayed blocks before saving data. (p. 127)

You cannot use the following functions concurrently with the memory division function.


- Real-time saving (See p. 124.)
- Stop trigger (See p. 140.)

During use of the memory division, the instrument may switch the trigger output (TRIG.OUT terminal) to a low level or irregularly output signals.

- The trigger output method is set to pulse.
- The recording length is set at 3 ms or less

10.1 Configuring the Memory Division Settings

> [Status] > [Condition]

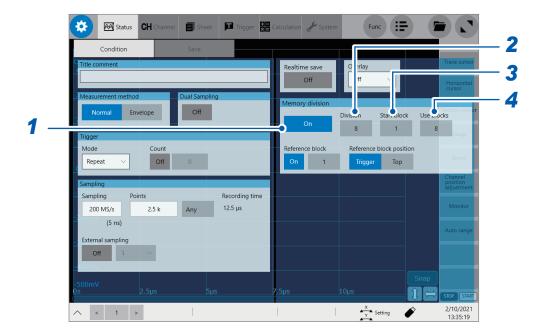

- **1** Tap the [Memory division] button to set it to [On].
- **2** Tap the [Division] box, and then enter the number of blocks the memory capacity is divided into.

Default setting: 2

3 Tap the [Start block] box, and then enter the start block number.

Default setting: 1

Figures you can set in [Start block] varies according to the settings in the [Division] box.

4 Tap the [Use blocks] box, and then enter the number of blocks to be used.

Default setting: 1 The maximum value that can be set is equivalent to a figure in the **[Division]** box.

The instrument defines a block to use for the next measurement according to the settings specified in the **[Start block]** and **[Use blocks]** boxes. The instrument clears a waveform in this block at the start of measurement if retained.

When the number of block for use is set at one

- The number of blocks for use is set at one.
- The recording mode is set to [Repeat].
- The trigger setting is enabled.

While the instrument is waiting for a trigger or filling the pre-trigger memory in the conditions above, halting measurement causes any waveform data to varnish.

Either of the following settings allows waveforms acquired before the instrument starts to wait for a trigger to remain in blocks the number of which, at a maximum, is the specified block number for use minus one.

The instrument can leave blocks, the number of which is one less than blocks used, that contains waveforms acquired before entering trigger standby mode with either one of the following settings:

- The recording mode is set to [Single] to perform measurement one after another.
- The recording mode is set to [Repeat] and the number of blocks to be used to two or more.

10.2 Configuring the Display Settings

> [Status] > [Condition]

🔅 🕅 Status CH 🗆	annel 🗐 Sheet 🏴 Trigger	Calculation System	Func III	
Condition	Save			
C Title comment		Realtime save	Overlay Off ~	Trace cursor Horizontal cursor
Measurement method Normal Envelope	Dual Sampling Off	Memory division On	Division Start block	Use blocks
Trigger Mode Cou	Int	Reference block	Reference block position Trigger Top	Gauge
Sampling				Channel position adjustment
200 MS/s 2.5 I	Any 12.5 μs			Monitor
Control Contro				Auto range
-500mV 0s 2.5µs		7.5µs	10µs	Snap) ⇔ STOP START
4			X Setting	> 2/10/2021 13:35:19

1 Tap the [Reference block] button to set it to [On].

You can overlay waveforms stored in other blocks with the waveform stored in the displayed block.

2 Tap the box to the right of the [Reference block] box, and then to choose a reference block number from the list.

Default setting: 1

You can choose a reference block number less than or equal to the figure specified in the [Division] box

3 Tap the [Reference block position] box, and then from the list, choose an option for the fiducial point to display the reference waveform.

Trigger	Arranges the reference waveform so that its trigger point is aligned with that of the displayed block waveform.
Тор	Arranges the reference waveform so that its start point is aligned with that of the displayed block waveform.

4 (When waveforms are stored in blocks after measurement)

Tap [<] and [>] or the number box to choose a block number to be displayed. You can also choose a block on the waveform screen.

10


Dead time (period during the instrument cannot sample data)

When the memory division set is [Off]

The instrument performs internal processes that include performing calculations, displaying waveforms, and saving data at every waveform acquisition.

These processes require a certain period of time as a dead time.

The instrument does not sample data during dead times even at any occurrences of unpredictable phenomena.




Dead time Period during which the instrument does not sample data to do internal and save processes

When the memory division set to [On]

The instrument acquires waveforms in blocks in a sequential order to save time the internal processes requires at every waveform acquisition.

Dead times can shorten because the instrument displays and saves waveforms after acquiring them.

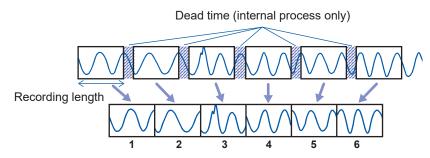

The instrument records a recording length of waveform data once per block.

• The relationships between dead times with the memory division setting and sampling rates are as follows.

10 MS/s to 200 MS/s: 1 to 4 samples

Sampling rate slower than 10 MS/s: 1 sample

- Measurement using Model 8970 Freq Unit in accumulation mode causes the last data set stored in the previous block to remain at the beginning of acquired data.
- When the instrument is frequently triggered, even pressing the **STOP** key may not stop measurement until the instrument has been acquired the specified number of blocks.
- Even the memory division is set to **[On]**, the following conditions require the instrument to perform processes that include performing calculations, displaying waveforms, and saving data at every waveform acquisition.
 - The numerical calculation is set to [On].
 - The waveform calculation is set to [On].
 - The FFT calculation is set to [On].

However, the instrument performs multiple-block measurement, it displays a calculation result of the last block after measurement. To display calculation results of other blocks, re-execute a calculation.

Automatic saving for the memory division setting

Measurement conditions	Automatic saving action
 The numerical calculation is set to [On]. The waveform calculation is set to [On]. The FFT calculation is set to [On]. 	Performs various calculations, automatically saves data, and displays waveforms at every 1-block measurement
• Sampling rate: 200 MS/s	Automatically saves data after a all-block measurement.
Other than above	Automatically saves data and displays waveforms during measurement.


Configuring the Display Settings

11 Dual Sampling

Dual sampling is a function that performs high-speed sampling in combination with low-speed sampling; the high-speed sampling can capture abnormal phenomena using triggers to record instantaneous waveforms while the low-speed sampling is continuously recording normal-state trend waveforms.


Multiple abnormal phenomena can be recorded using the memory division function.

Trend waveform

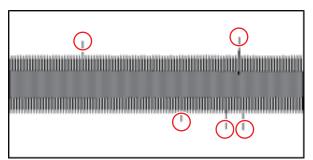

By observing trend waveforms, you can roughly check variation of waveforms under measurement. Instantaneous waveforms can be captured by configuring trigger settings, allowing you to examine abnormal phenomena (circled) closely.

Instantaneous waveform



By pressing the **START** key, you can start recording trend waveforms. When trigger conditions are met, instantaneous waveform recording can starts.


After measurement has finished, you can use instantaneous waveforms for numerical calculation, waveform calculation, and FFT calculation.

11.1 Dual Sampling Procedure

Configuring dual sampling settings	Enable the dual sampling function.	(p. 297)
*		
Configuring settings for capturing trend waveforms	Set the recording mode. Set the sampling speed and the number of points for the trend waveforms.	(p. 297) (p. 297)
*	waveloints.	
Configuring settings for acquiring instantaneous waveforms	Set the sampling speed and the number of points for instantaneous waveforms. Configure the memory division settings.	(p. 297) (p. 298)
*		
Configuring the input channel settings	Configure the analog and logic channels settings.	(p. 11)
*		
Configuring the trigger settings	Configure the timing settings for acquiring instantaneous waveforms	(p. 137)
*		
Configuring automatic saving settings	Configure the settings so that waveform data can be automatically stored while being acquired.	(p. 120)
*		
Starting measurement	Press the START key to start recording trend waveforms.	
*		
Measurement in progress	When a trigger activates, the instrument starts recording instantaneous waveforms. When the memory division is enabled, the instrument records instantaneous waveforms every time the trigger activates. When the automatic saving is enabled, the instrument automatically stores instantaneous waveforms every time it acquires waveforms.	
Finishing measurement	The instrument finishes measurement after it has acquired all the trend waveforms each of which contains set data points. When the automatic saving is enabled, the instrument stores instantaneous waveforms automatically. After measurement, you can perform various calculations using instantaneous waveforms.	(p. 306)

11.2 Configuring Dual Sampling Settings

> [Status] > [Condition]

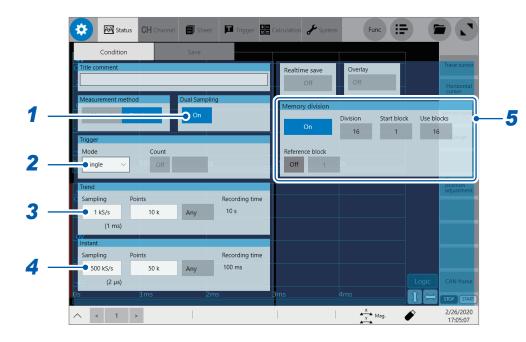

Dual Sampling

11

1 Tap the [Dual Sampling] box to set to [On].

The following settings change automatically.

Measurement method	Envelope
Realtime save	Off
Memory division	On
Overlay	Off

2

Tap the [Mode] box, and then from the list, choose a recording mode (behavior after finishing trend waveforms).

Single [∅]	Finishes recording after the set recording length of trend waveforms has been recorded.
Repeat	Clears waveforms after the recording length of trend waveforms have been recorded and records waveforms once again from the beginning. At this time, instantaneous waveforms are also recorded from the start block. You can stop recording by pressing the STOP key

3 Set the sampling speed and the number of points for the trend waveforms.

The instrument measures trend waveforms using the envelope method (records the maximum and minimum values per sample).

At this time, it performs oversampling of the input signals at the sampling speed specified for the instantaneous waveform recording.

See "Using the envelope" (p. 9).



Set the sampling speed and the number of points for instantaneous waveforms.

The instrument measures instantaneous waveforms using the normal method (acquiring one data point per sample). Choose a sampling rate faster than that chosen for trend waveforms. See the following page for the sampling speeds that can be set.


See "Linear time-invariant system" (p. 410).

5 Configure the memory division settings.

Instantaneous waveforms can be acquired into multiple blocks. By setting the dual sampling to **[On]**, the memory division is also set to **[On]** automatically, allowing you to set the number of blocks, start block number, and the number of blocks to be used. See "10 Memory Division Function" (p. 289).

6 Configure the input channel settings.


✿ > [Channel]

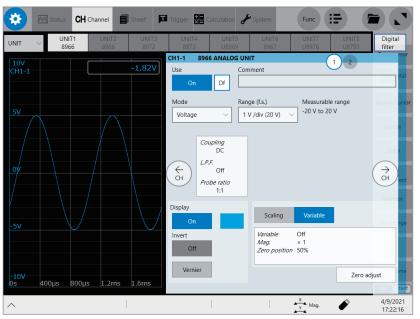

Configure the analog and logic channels settings. See "1.3 Configuring the Input Channel Settings" (p. 11).

7 Configure the trigger settings.



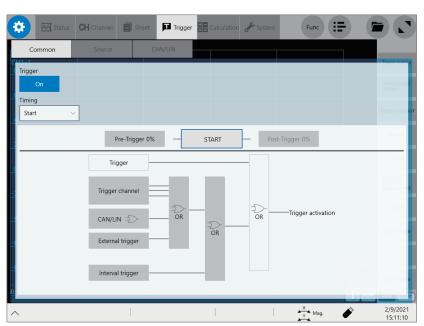

The instrument can record instantaneous waveforms using triggers under certain conditions only. See "5 Configuring the Trigger Settings" (p. 137).

IMPORTANT

The following trigger functions are disabled when the dual sampling is set to [Off].

- Trigger timing ([Stop], [Start/Stop])
- Post trigger

11


Trend waveform and instantaneous waveform

Recording trend waveforms can immediately start by pressing the START key.
 Instantaneous waveforms, which can use the memory division, are recorded into a different block one after another every time the instrument is triggered.

Even if blocks run out for recording instantaneous waveforms, the instrument continues to record waveforms until the recording length specified for trend waveforms elapses.

Example


When an instantaneous waveform is recorded with 2-memory-division setting The waveform is recorded into two or fewer blocks.

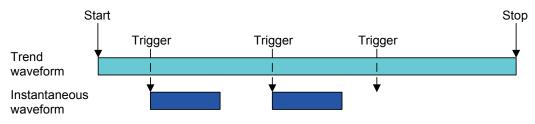

• Once the recording of trend waveforms finishes, recording of instantaneous waveforms is also finished.

Example


When an instantaneous waveform is recorded with 2-memory-division setting

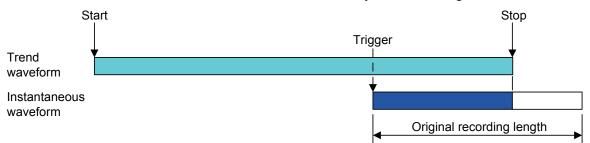

 For repetitive measurements, the instrument clears waveforms every time it finishes recording of trend waveforms, and then restarts recording waveforms from the beginning. At this time, instantaneous waveforms are also recorded from the start block. You can stop recording by pressing the STOP key

Example


When pressing the **STOP** key during the third measurement of instantaneous waveform recordings with the recording mode set to repeat and the number of the memory division set to four



11.3 Operating the Waveform Screen for Analyzing Waveforms

You can use the waveform screen to toggle between the trend waveform setting and the instantaneous setting, switch the display, and analyze waveforms with the trace cursors.

*

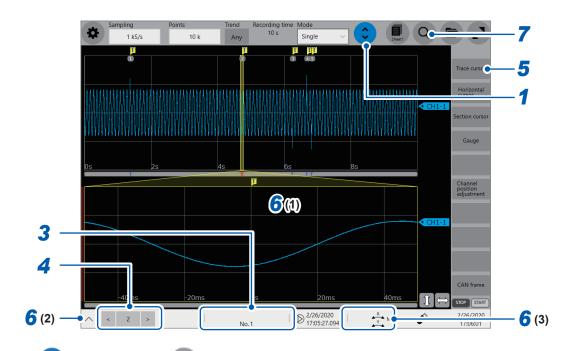

1 Tap 🗘 (blue) button or 🗘 (gray) button.

Every time you tap the button, it changes in color, and the settable items are toggled.

When the button color is blue 📿

The setting is of trend waveforms.


You can set the sampling speed, the number of measurement points, and the recording mode.



When the button color is gray 🤇

The setting is of instantaneous waveforms.

You can set the sampling speed, the number of measurement points, and the waveform type to be displayed on the screen,




2 Tap the [DisplayWaveform] box, and then from the list, choose a waveform type to be displayed on the waveform screen.

Dual	Displays trend waveforms on the upper split-screen and instantaneous waveforms on the lower split-screen.
Trend	Displays trend waveforms You can use the sheet setting to choose a screen spit setting.
Instantaneous	Displays Instantaneous waveforms. You can use the sheet setting to choose a screen spit setting.

See "1.4 Co	onfiguring the	Sheet Settings"	(p.	19).
-------------	----------------	-----------------	-----	------


When choosing [Dual]

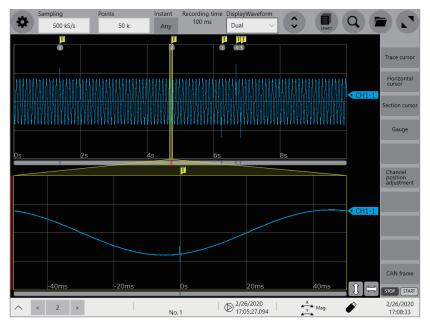

The trend waveforms (on the upper screen) have the trigger marks \mathbf{I} and block numbers that indicate the positions of the instantaneous waveforms.




The instantaneous waveforms (on the lower screen) have the trigger marks **I** that indicate the positions of the trigger positions.



ording 1 100 ms Ż Q <u>^</u> 500 kS/s 50 k Trend 3 45 Trace curs Horizontal cursor ection cu Gauge CH1-1 Channe position adjustn CAN frame (Ĵ ⇔ STOP START D 2/26/2020 17:05:26.971 2/26/2020 17:10:51 Y Mag. Ô < 2 > No.1


When choosing [Trend]

When choosing [Instantaneous]

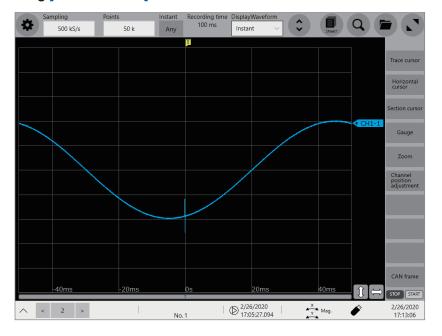


3 Check on the measurement state.

During measurement, the recording states of the trend waveforms and instantaneous waveforms are indicated using characters and the progress bar.

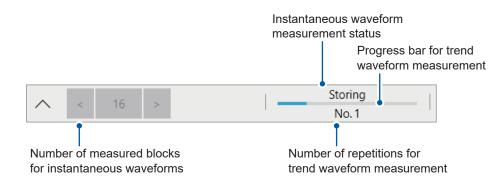

4 (When the displayed waveforms are set to [Dual] or [Instantaneous])

After measurement has finished, tap [<] and [>] to choose a block number of instantaneous waveforms to be displayed.



Tapping the number can display the block switching window.



Use the arrow keys, two-headed arrow keys, and slider to select a block number, and tap **[OK]** to display instantaneous waveforms contained in the selected-numbered block.

When the displayed waveforms are set to **[Dual]**, you can switch the block number to be displayed by tapping the number of the instantaneous waveform position mark.



5 Tap the [Trace cursor] button to display the cursor to read off measured values.

See "2.1 Reading Measured Values (Trace Cursors, Horizontal Cursors)" (p. 30).

Trace cursors retain their positions on both trend waveforms and instantaneous waveforms. When the displayed waveforms are set to **[Dual]**, the cursors for instantaneous waveforms are displayed, allowing you to operate the cursors.

6 Move and zoom in/out waveforms.

You can move and zooming in/out waveform using the following four ways:

- (1) Pinch in the waveform screen to zoom out waveforms, and pinch out to zoom in.
- (2) Use the quick access menu to zoom in/out waveforms.



See to "1.4 Supplying Power to the Instrument" in the Quick Start Manual.

(3) Press the rotary knob to choose an item you wish to operate and rotate the knob to change the display setting.



See "2.6 Operating the Rotary Knobs" (p. 45).


(4) Use the shortcut keys to zoom in/out waveforms.



See "13 Configuring the System Environment Settings" (p. 343).

When the displayed waveforms are set to [Dual], you can toggle waveforms to operate by tapping the screen.

You can operate waveforms that have the red bar at the left edge.

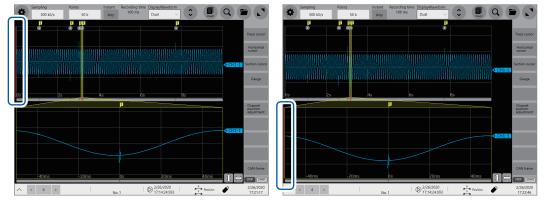

When the trend waveforms can be operated When the instantaneous waveforms can be operated

7 Search the instantaneous waveforms for the positions where the specified conditions are met.

Tap **[Search]** button to enter the conditions. The instrument searches the waveforms for the positions where the conditions are met.

See "6 Search Function" (p. 167).

You can jump to event marks on trend waveforms only. Other searches and jumps can be performed on instantaneous waveforms only regardless of the waveform display setting.

11.4 Calculation Function

After measurement has finished, you can preform various calculation using instantaneous waveforms.


1 Configure various calculation settings.

The following calculations are available:

- Numerical calculation See "7 Numerical Calculation Function" (p. 181).
- Waveform calculation See "8 Waveform Calculation Function" (p. 209).
- FFT calculation See "9 FFT Calculation Function" (p. 257).

2 Tap the 🔅 button.

The waveform screen is displayed.

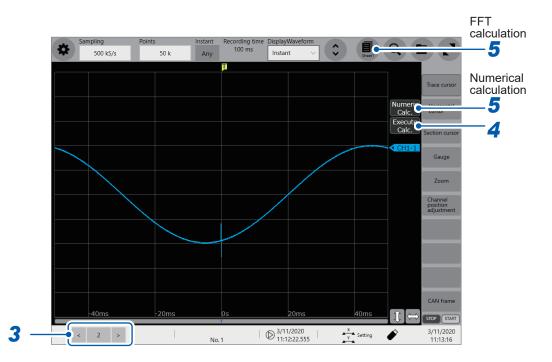

3 When the displayed waveforms are set to [Dual] or [Instantaneous]

Tap [<] and [>] to choose a block number of instantaneous waveforms to be used for calculation.


When the displayed waveforms are set to **[Dual]**, you can also choose a block number by tapping the position number of the instantaneous waveform position marks.

4 Tap [Execute Calc.].

The calculation is executed. When all calculations are set to **[Off]**, **[Execute Calc.]** does not appear.

5 For the numerical calculation

Tap [Numeric Calc.] to check on the calculation results displayed on the waveform screen.

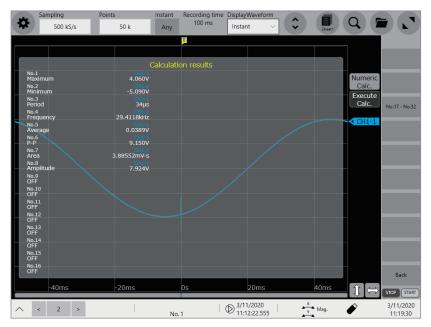

For waveform calculation

Check on the calculation results displayed as waveforms on the waveform screen.

For FFT calculation

Tap the [Sheet] button, which can switch over to the sheet with the display form set to FFT waveforms, to check on the calculation results.



IMPORTANT

Even if the calculation is set to **[On]**, no calculation is automatically performed during measurement.

After measurement has finished, tap [Execute Calc.] to perform calculation.

11.5 Files

You can save and load dual sampling waveform files.

Arranges the reference waveform so that its start point is aligned with that of the displayed block waveform.

The instrument saves instantaneous waveforms at the moment when finishing the measurement of each block, which is specified by the number of blocks you wish to use in the memory division settings.

When it has saved instantaneous waveforms of all blocks during measurement, it subsequently starts to save trend waveforms. When instantaneous waveforms of some blocks have been left unsaved on the completion of the measurement, the instrument starts to save trend waveforms at that moment.

The automatic saving function requires you to configure the settings, including save destinations and saving types, in advance of measurement.

See "4 Saving/Loading Data and Managing Files" (p. 115).

When the automatic saving function is enabled, the instrument saves trend waveforms and instantaneous waveforms of all blocks in a batch. An index file is also saved simultaneously.

Dual sampling waveform files you can save and load

✓: enabled, –: disabled File Automatic Manual Load onto Load onto File type **Extension** Content format saving **MR6000** computer save Instantaneous **√***¹ √ MEM waveform ⁄ 1 measured data Binary Trend Waveform **√***¹ ✓ REC waveform ~ 1 data measured data Text REC Text data √ ~ ~ _ Floating point Float CSV, TXT data Binary Management batch-save Index R_M 1 ~ 1 data*2 management data

*1 Loadable with Waveform Viewer (Wv)

*2 Automatically created when all binary files are collectively saved.

309

11


Dual Sampling

Hierarchical destination folders

The instrument automatically creates folders on recording media to save various files. One folder can contain up to 5000 files and folders, collectively.

Example of the folder hierarchy when the waveform file is named MRDAT

The shaded folders are created when recording media is inserted; the filled folders are created depending on a saving state.

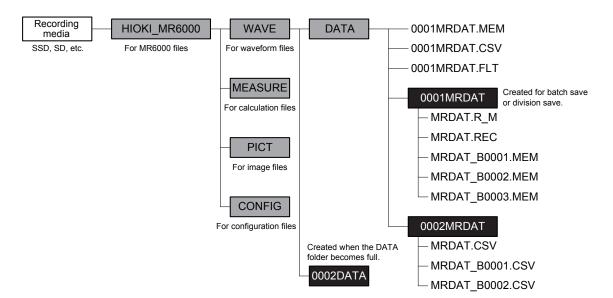

When dual-sampling waveforms are collectively saved or divided before saved into display blocks, the instrument newly creates the folder with the name of the waveform file name preceded by a running number and saves all the files in the folder.

For instantaneous waveform files, a block number is added to file names.

Automatically saving waveform data

The instrument automatically saves waveform data while being acquired. You have to specify a destination to save and a file type before starting measurement. See "Automatically saving waveform data" (p. 120).

All blocks containing trend waveforms and instantaneous waveforms are collectively saved. An index file is also saved simultaneously.

Freely choosing data items to be saved and save files (SAVE key)

You can save waveform data by pressing the **SAVE** key.

See "Freely choosing data items to be saved and save files (SAVE key)" (p. 127).

Manual save		
Media		
	TOSHIBA MQ01AAD0(D:) 286.2 GB / 298.1 GB	
File name		
DATA		
Туре	Save Block	
Waveform (Binary) $ \smallsetminus $	Display Block	
Channel	CAN	
Display \vee	Off	
Range		
All 🗸		
Divide		
Off 🗸 🗸		
Execute	Cancel	

1 Press the SAVE key.

The [Manual save] dialog box is displayed.

2 Tap the [Save Block] box, and then from the list, choose a block in which data is saved.

Display Block [⊠]	Saves waveforms included in displayed blocks.	
All Block	Saves waveforms included in the specified number of blocks being used counting from the start block.	

.

3 Tap [Execute].

Waveforms included in displayed blocks are saved.

Loading waveform data

You can load files saved in recording media onto the instrument. See "Loading Data" (p. 131).

Extension	Measurement target	
R_M	Loads trend waveforms and instantaneous waveforms included in all blocks to restore the waveforms to those measured with the dual sampling set to [On].	
REC	Loads trend waveforms only. The dual sampling setting is set to [Off].	
MEM	Loads instantaneous waveforms included in only one block. The dual sampling is set to [Off].	

12 CAN/LIN Measurement Function

Using the CAN/LIN measurement function, the instrument can record all CAN/LIN signals that transmit through a CAN/LIN bus and display user-selected signals as waveforms. To use this function, the Vector VN1600 interface is required.

The CAN/LIN measurement function cannot be used in the following conditions:

- When the memory division is set to [On]
- When the dual sampling is set to [On]
- When the external sampling is set to [On]

Up to 1,000,000 frames can be obtained through the CAN/LIN measurement. If the number of obtained frames reaches this number during measurement, the instrument will stop obtaining following frames, but continue the measurement until the set recording time has elapsed.

Main features


- All CAN signals transmitting through a CAN bus can be recorded.
- All LIN signals transmitting through a LIN bus can be recorded.
- · CAN FD, CAN, and LIN are supported.
- All of hardware configuration you have to do to record CAN/LIN signals is connecting the Vector VN1600 interface to the instrument's USB port. You do not need to change the existing input module configuration. The instrument becomes capable of recording CAN/LIN signals without removing inserted input modules.
- The instrument, which has four ports independent from one another, can connect to networks of various CAN/LIN bus types or baud rates.
- You can choose signals to be displayed as waveforms from recorded CAN/LIN signals. Up to 16 CAN/LIN signals can be simultaneously displayed as waveforms.
- Up to 300 CAN/LIN definition data sets can register for displaying CAN/LIN signals as waveforms.
- Files (DBC/LDF files) created with the Vector database CANdb can be directory loaded. Loaded definition data can be used without any process. You can also modify definition data contents.
- The instrument can send CAN messages and acknowledgments responding (ACK) to CAN messages, allowing you to perform a simple simulation.
- You can configure all the settings with the instrument.

12.1 CAN/LIN Measurement Procedure

Two methods are available for CAN/LIN measurement. You can choose an optimal method depending on your purpose (concurrent use is available).


Method	Advantage
Using waveform processing calculations	 Waveforms can be displayed after measurement. The waveform processing calculations are used. Waveforms can be computed. Up to 16 channels are available.
Displaying waveforms during measurement	 Waveforms can be displayed during measurement. The waveform display settings are used. Up to 64 channels are available. (Waveforms cannot be computed.)

Using waveform processing calculations

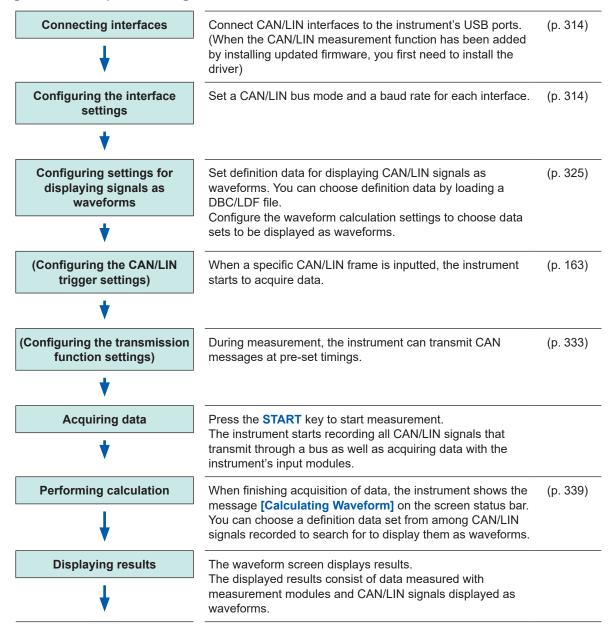

(Saving data)	(When the automatic saving is set to [On])	(p. 342)
¥	The instrument automatically saves data acquired with its input modules, CAN/LIN signals, and data displayed as waveforms in the storage device.	
(Displaying waveforms using different settings)	Configure the waveform calculation settings to choose data sets to be displayed as waveforms again.	
*	Perform calculation to display data sets lastly chosen as waveforms.	
Finishing measurement		

Displaying waveforms during measurement

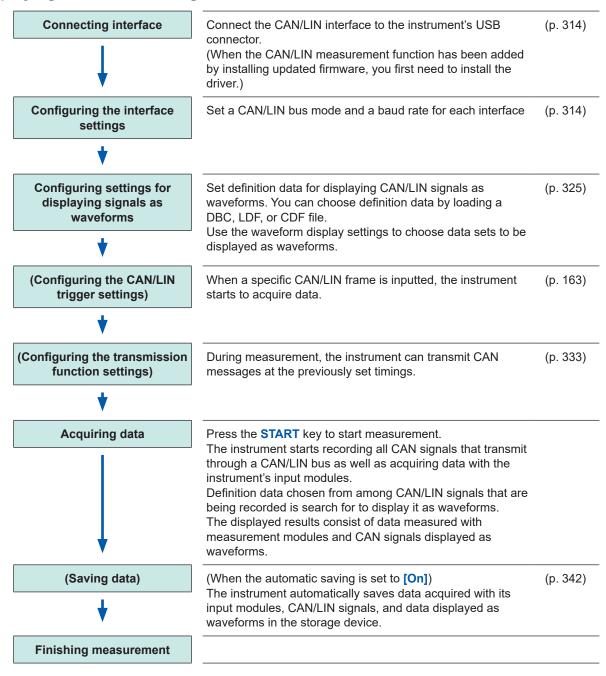

12.2 Connecting CAN/LIN Interfaces

1 Connect CAN/LIN interfaces to the instrument using a USB cable.

Any USB ports of the instrument are available to connect CAN/LIN interfaces. Only one CAN interface can be connected to the instrument. Do not connect more than one CAN interface. Some CAN interfaces can perform measurement involving up to four channels (C1 to C4). The CAN interfaces are assigned the channel numbers C1, C2, C3, and C4 to in the order in which they are detected.

Hioki has verified proper operation of the following CAN/LIN interfaces:

- VN1630, VN1640 (CANpiggy 1051cap/1057Gcap): CAN FD, High-speed CAN (up to 4 ports)
- VN1610: CAN FD, High-speed CAN (2 ports)
- VN1611: LIN, High-speed CAN

2 Turn on the instrument.

3 Disable the system protection function.

See "13 Configuring the System Environment Settings" (p. 343).


4 (Only when connecting CAN/LIN interfaces for the first time)
 Open Explorer and use the Vector Driver Disk, which came with the CAN/LIN interface (VN1600 interface), to install the CAN/LIN driver on the instrument.

See the instruction manual that came with the interface to install the driver.

5 Connect a USB mouse to the USB port.

From this time through step **17**, you can use the USB mouse for settings.

6 Tap 🔅 > [Channel] > [UNIT] > [CAN/LIN] > [Driver].

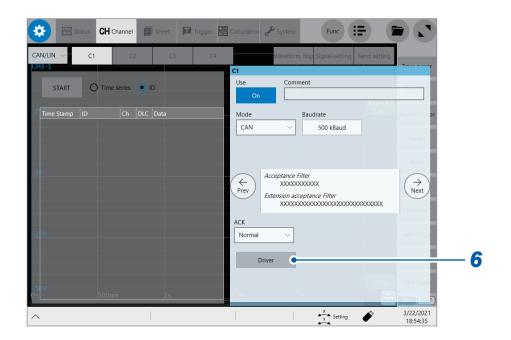


The [Vector Hardware Config] window appears.

If the **[Vector Hardware Config]** window does not appear, click the Windows button at the lower left corner of the screen with the mouse and choose **[Vector Hardware Configuration]** from the Start menu.


👼 Vector Hardware Config		_	×
Application License Support Help			
Hardware Vitual CAN Bus 1 Vitual CAN Bus 1 VI1610 1 VI1630A 1 (545423) Solution Global Settings Driver status License	Details		

7 Check if the connected CAN interface has detected.

Under **[Hardware]**, the connected CAN interface appears. If the instrument cannot correctly detect the CAN interface, an error mark appears on the icon,

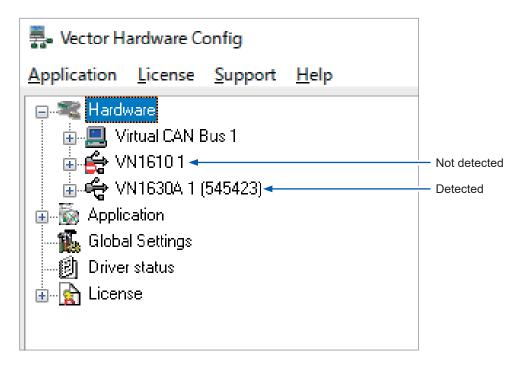

8 Right-click [Application], and then from the shortcut menu, select [Add application].

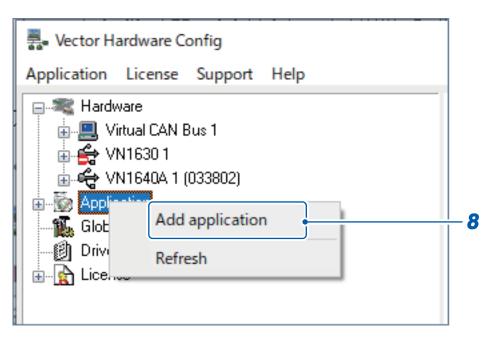

The [Application settings] appears.

9 In the [Application name] box, enter the string [hiokiCANcontrol].

Exercise care as the software won't be able to connect if even one character differs.

Application settings	×	
Application name hiokiCANcontrol		- 9
Channel Usage		
CAN: 2 V	-	- 10
J1708: 0 🗸 K-Line: 0 🗸 AFDX: 0 🗸 Ethernet: 0	~	
D/AIO: 0 - A429: 0 - GNSS: 0 - W11P: 0	\sim	
SENT: 0 🗸		
OK Curr		- 11

10 Click the [CAN:] box, and then from the list, choose the number of the connected CAN interfaces.

11 Click [OK].

The [Application settings] dialog box closes.

12 On the left pane of the [Vector Hardware Config] window, click the plus sign next to [Hardware].

The tree structure consisting of the connected CAN interfaces expands.


12 7 Vector Hardware Config Α plication License Support Help 📳 💐 Hardware 🛓 🛄 Virtual CAN Bus 1 🖕 🚓 VN1630A 1 (545423) 💼 🐵 On board CAN 1051cap(Highspeed) 🛓 🕘 Or CANalyzer > 🗄 – 🌧 Cł CANape > ⊞…, _ Cł ⊕..., _ Or CANoe hiokiCANcontrol > CAN 1 13 🗄 🖓 Application 🌇 Global Set CAN 2 Default CAN baud rate 😰 Driver stat 🗄 🖳 🏠 License Refresh

13 Right-click a CAN interface of your choice, click [hiokiCANcontrol] on the shortcut menu, and then choose a CAN channel number (such as [CAN 1]).

Assign channel numbers to all of the CAN interfaces actually connected. When you click a plus sign, the tree structure expands; a minus sign, collapses.

14 Click the plus sign next to [Application].

The node expands.

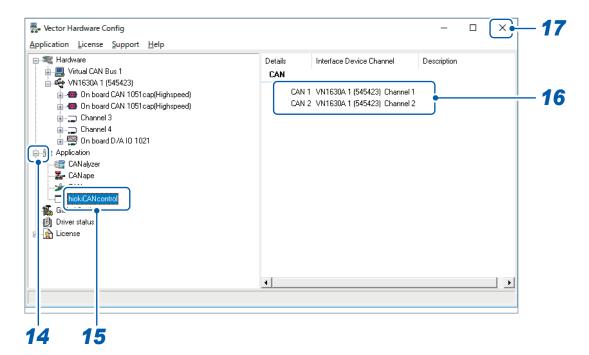

15 Click [hiokiCANcontrol].

On the right pane of the window, the state of assigned CAN channels is displayed. For channels not assigned correctly, the string **[Not assigned]** appears.

16 Check if channel numbers are assigned to the CAN interfaces as intended.

17 Tap the [Close] button.


The [Vector Hardware Config] window closes; the screen returns to the recorder application.

18 Cycle the instrument.

Refer to "2.9 Supplying Power to the Instrument" in the Quick Start Manual.

12.3 Configuring the CAN/LIN Interface Settings

This section describes how to configure condition settings required for measurement, such as the baud rate and packet filter.

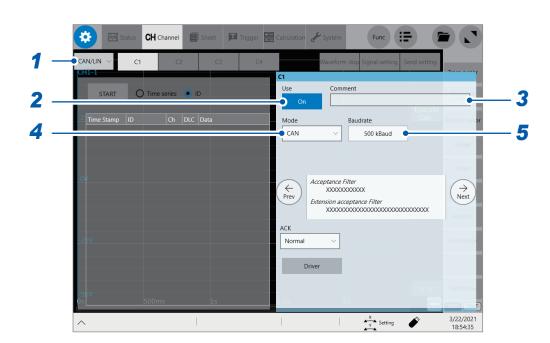

Channel] > [UNIT] > [CAN/LIN]

1 Tap the box that can toggle between [Unit] and [CAN/LIN] to select [CAN/LIN].

2 Tap the [Measurement] button to set it to [On] or [Off].

Off [⊠]	Does not designate the channel as a measuring target. The instrument does not acquire any data; nothing is displayed or saved.
On	Designates the channel as a measuring target.

3 Enter a comment in the [Comment] box.

Number of characters that can be entered: up to 40

4 Tap the [Mode] box, and then from the list, choose a CAN mode (setting common to C1 through C4).


CAN ^ℤ	Enters CAN mode.
CAN FD	Enters CAN FD mode.
LIN	Enters LIN mode.

5 Tap the [Baudrate] box, and then from the list, choose a baud rate.

CAN, CAN FD	33.3 k, 50 k, 83.3 k, 100 k, 125 k, 250 k, 500 k [⊠] , 1 M (Baud)
LIN	2.4 k [∞] , 9.6 k, 14.4 k, 19.2 k (Baud)

6




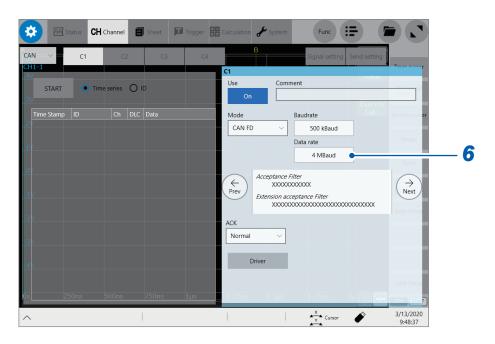

Tap the [Data rate] box, and then from the list, choose a baud rate used in the data phase.

33.3 k, 50 k, 83.3 k, 100 k, 125 k, 250 k, 500 k, 1 M^{2/}, 2 M, 4 M (Baud)


7 (When you set [Mode] to [LIN])

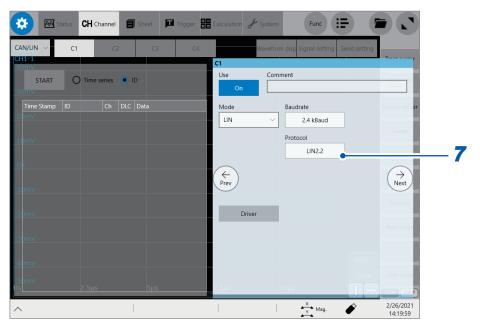

Tap the [Protocol] box, and then from the list, choose a protocol you wish to use.


LIN2.2^{III}, LIN2.1, LIN2.0, LIN1.3

8 (When you set [Mode] to [CAN] or [CAN FD])

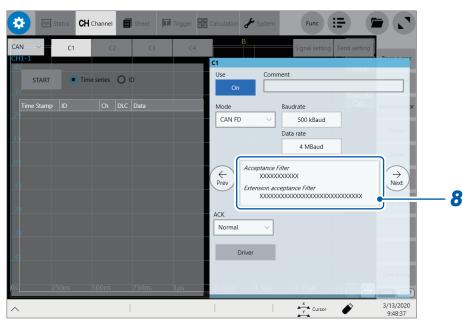

Tap the area that includes [Acceptance Filter].

The **[Acceptance Filter/Extension acceptance Filter]** dialog box appears. Use this dialog box to set which message is filtered to perform measurement.

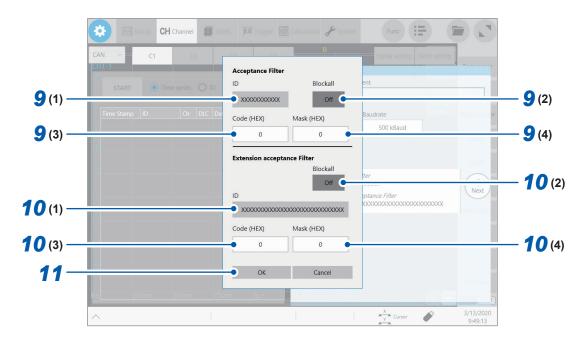

9 Configuring the receiving filter settings.

(1) Under [Acceptance Filter], tap the [ID] box, and then enter a filter ID.

The instrument blocks a message of a bit whose filter ID does not match the ID bit of each signal. Bits whose bit mask to which the character X has been set pass all messages. The bit mask automatically calculates a code and mask.

(2) Tap the [Blockall] button to set it to [On] or [Off].

Off [∅]	Passes all messages.
On	Blocks any messages. [Blockall] of [Extension acceptance Filter] is set to [Off].

(3) Tap the [Code (HEX)] box, and then enter a filter code.

(4) Tap the [Mask (HEX)] box, and then enter a filter mask.

Example 1 Code: arbitrary, Mask: 000 Passes all messages.
Example 2 Code: 001, Mask: 7FE Passes messages only with the ID whose first bit is one or zero (ID = 0, ID = 1).

10 Configuring the extended receiving filter settings.

(1) Under [Extension acceptance Filter], tap the [ID] box, and then enter a filter ID. The instrument blocks a message of a bit whose filter ID does not match the ID bit of each signal. Bits whose bit mask to which the character X has been set pass all messages. The bit mask automatically calculates a code and mask.


(2) Tap the [Blockall] button to set it to [On] or [Off].

Off [∅]	Passes all messages.			
On	Blocks any messages. [Blockall] of [Acceptance Filter] is set to [Off].			

- (3) Tap the [Code (HEX)] box, and then enter a filter code.
- (4) Tap the [Mask (HEX)] box, and then enter a filter mask.

11 Tap [OK].

The [Acceptance Filter/Extension acceptance Filter] dialog box appears.

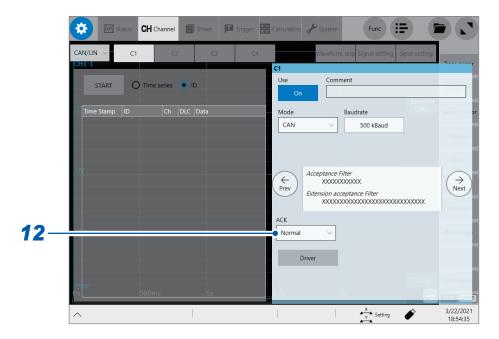


Normal [⊠]	The CAN controller participates in bus communication. The instrument sends acknowledgments.
ACK OFF	The bus is influenced by the measurement since the CAN controller on the interface card represents the interface between the analysis software and the CAN bus. Particularly the CAN controller sends its acknowledge for correctly recognized messages by sending a dominant level (on the bus) in the corresponding slot of the CAN message. To reduce the influence on the system you can switch off this functionality. Thereby the node is no longer visible on the bus. Please keep in mind that - when you switched off acknowledge - communication on the bus only may happen if at least one other network node sends an acknowledge.

12 Tap the [ACK] box, and then from the list, choose an ACK measurement setting.

Excerpt from CANoeCANlyzer.chm of Vector CANalyzer (Vector Infomatic)

When [ACK OFF] is selected, the CAN transmission function is disabled.

13 Monitor the state of the CAN/LIN bus.

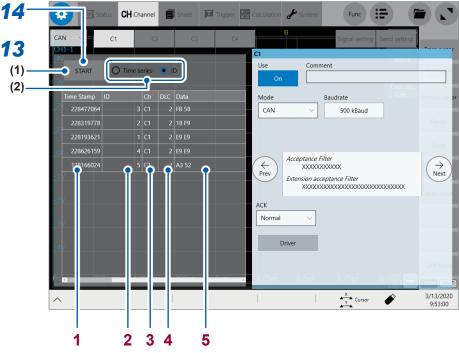

(1) Tap [START].

The monitor value table is displayed on the left half of the screen.


No.	Name	Function
1	Time Stamp	Displays time stamps.
2	ID	Displays message IDs in hexadecimal notation.
3	Ch	Displays channel numbers (C1 through C4).
4	DLC	Displays the numbers of bytes of the received data.
5	Data	Displays data in hexadecimal notation.

(2) Tap [Time series] or [ID] to change the order of monitor values.

Time seriesDisplays monitor values in the acquired order.	
ID	Displays monitor values in the order of IDs.

12

14 Tap [START] to hide the monitor values.

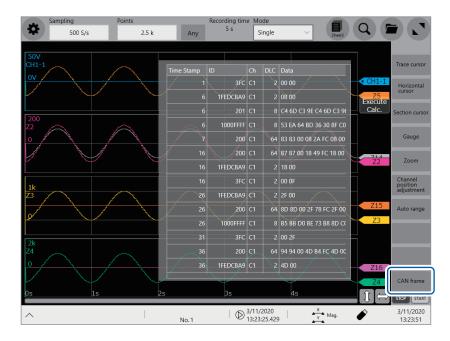

The monitor table can be displayed on the waveform screen.

If you tap **[CAN frame]** on the waveform screen, the monitor table appears, allowing you to check monitor values during measurement.

Tapping [CAN frame] once more closes the monitor table.

12.4 Configuring the CAN/LIN Definition Data Settings

> [Channel] > [UNIT] > [CAN/LIN] > [Signal setting]

This chapter describes how to set definition data for displaying CAN/LIN signals as waveforms. In CAN measurement mode, loading a DBC file or a CDF file can choose CAN definition data. In LIN measurement mode, loading a LDF file, which stands for LIN description file, can choose LIN definition data.

10 141516 11 12 13 2 3 Δ 8 9 6 ۵ CAN/LIN elect num File Edit Calc <u>م</u> آ 8 Little Signed 0 Classic ~ Ō 8 Little Signed 0 Classic ^ ~ Ē 0 Classic v 8 Little Signed ^ 8 Little 0 Classic Ō ^ ~ Signed 0 Classic Ō 8 Little Signed ~ 8 Little Signed 0 Classic Ŵ ~ Ŵ 8 Little Signed 0 Classic ~ Ō 8 Little 0 Classic Signed ~ 9 8 Little Signed 0 Classic Ō ^ 10 8 Little Signed 0 Classic Ŵ ^ v 11 0 Classic 8 Little <u>م</u> ا ~ Signed 12 0 Classic 8 Little <u>م</u> ق ~ Signed 8 Little Signed 0 Classic <u>ت</u> ^ ~ 3/10/2021 13:53:12 Y Mag. Î

No.	Name	Function					
1	SignalAllows you to enter a signal name for the data concerned. Number of characters that can be entered: up to 32						
2	2IDAllows you to enter a message ID, in hexadecimal notation (p. 33 message that includes data you wish to allocate to a channel. Both 11-bit base IDs and 29-bit extended IDs are supported.						
		0 to 1FFFFFFF					
3	Start bit	Allows you to enter the data starting address on the message frame. Specify the least significant bit (LSB) of a signal you wish to capture.					
		0 [⊠] to 63					
		See "To find out the data starting address ([Start bit])" (p. 329).					
4	Bit length	Allows you to enter the data size, in bits, of a signal you wish to capture.					
		1 to 64, default setting: 8 [⊠]					

No.	Name	Function						
5	Byte order	Allows you to choose between big-endian ordering and little-endian ordering for the data concerned,						
		Big ^ℤ	Sends the most significant byte first (Motorola order).					
		Little	Sends the least significant byte first (Intel order).					
		See "Data allocation	([Byte order])" (p. 330).					
6	Data type	Allows you to choose	a data type for the data concerned.					
		Signed [⊠]	Signed integral type					
		Unsigned	Unsigned integral type					
		Float	Single-precision floating-point data type					
		Double Double-precision floating-point data type						
7	Ratio	Allows you to enter a conversion ratio						
8	Offset	(Physical value) = (Co	be obtained from the following expression. Conversion ratio) × (Data value [bit]) + (Offset) atio: 1.0, default offset value: 0.0)					
9	Check sum	Allows you to choose a checksum concept for every frame ID when performing LIN measurement.						
		Classic [⊠]	Standard checksum					
		Enhanced Enhanced checksum						
10	DLC	Allows you to enter a data length code (DLC) for every frame ID when performing LIN measurement. (Default: 1)						

Data manipulations

No.	Name	Function							
11	File	Select the rows where you wish to add data, and then tap [File] to display the file selection dialog box. You can add data to multiple rows in a batch. Choose items you wish to add, and then tap [OK]. The chosen columns are overwritten in ascending order. See "Choosing CAN definition data" (p. 331).							
12	Edit	Select the rows you wish to edit, and then tap [Edit] to display the [Signal setting] dialog box. You can add data to multiple rows in a batch. Enter items you wish to edit, and then tap [OK]. The edited items are overwritten.							

No.	Name		Function					
13	Calc.	Tap [Calc.] to display the [CAN calculation] setting dialog box. Enter arithmetic expressions, and then tap [OK] . The arithmetic expressions will be confirmed.						
		Waveform calculation list	CAN calculation Channel Signal No. Calc. number C1 S1 Z2 Calculation Formula Set formula On CAN(C1,S1) SET to Z2 Tab the formula to move to the wavef rm calc. displav To Z2 Tab the formula to move to the wavef rm calc. displav Comment On Calc. Formula CH(1,1) Z2 Pwr. Comment On Calc. Formula Z3 Pwr. Comment On Calc. Param A - Urms1 Z4 Pwr. Comment Param n IN A - P1					
		Channel	Allows you to choose a channel number (C1 to C4).					
		Signal No.	Allows you to choose a signal number (S1 to S300).					
		Calc. number	Allows you to choose a calculation number (Z1 t Z16).					
		Calculation	Tap to set to [On] to display the waveform calculation list. See "12.7 Choosing Data To Be Displayed as Waveforms (When Using the Waveform Calculation Function)" (p. 339).					
		Formula	Displays the formula set in [Channel] and [Signal No.] .					
		Set formula	Assigns the formula to the calculation number chosen in [Calc.number] .					
		Waveform calculation list	You can scroll the list upward and downward. Tapping the [Formula] box can display the formula setting dialog box.					
14	Delete	Tap the tion in default values.	the row you wish to delete. The values return to the					
15	Up	Tap the 🔨 icon in	the row you wish to move upward.					
16	Down	Tap the 🔽 icon in	the row you wish to move downward.					


Bit addressing

- 1. Configure the least significant bit (LSB) of the first byte data in the data frame at address 0. Allocate addresses to every bit toward the most significant bit (MSB), incrementing by one.
- 2. When the MSB is addressed, allocate the following addresses to the next byte data beginning from the LSB toward the MSB, incrementing by one as with the first byte (byte 0).
- 3. A data frame can have a size of eight bytes (64 bits) at most. The MSB of the eighth byte (byte 7) is configured at address 63.

	MSB 🔫								
		Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0
First	Byte 0	7	6	5	4	3	2	1	0
	Byte 1	15	14	13	12	11	10	9	8
	Byte 2	23	22	21	20	19	18	17	16
	Byte 3	31	30	29	28	27	26	25	24
	Byte 4	39	38	37	36	35	34	33	32
	Byte 5	47	46	45	44	43	42	41	40
Ļ	Byte 6	55	54	53	52	51	50	49	48
Last	Byte 7	63	62	61	60	59	58	57	56

To find out the data starting address ([Start bit])

When you wish to capture 8-bit data of the second byte from the first (byte 1), configure the LSB at address 8.

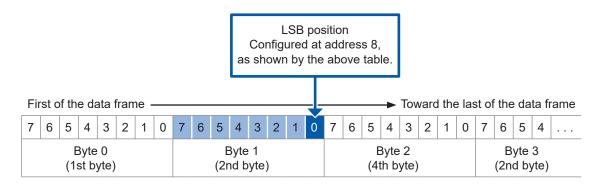

Data allocation ([Byte order])

Captured data using a big-endian ordering differs from those using a little-endian ordering although the same data starting address ([Start bit]) and the same bit length ([Bit length]) are uses. In the following figure, the shaded cells indicate the pieces of data to be captured when a bit length of 10 and a data starting address (LSB position) of bit 16 are configured.

Big-endian ordering The MSB is configured at address 9								
	Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0
Byte 0	7	6	5	4	3	2	1	0
Byte 1	15	14	13	12	11	10	9	8
Byte 2	23	22	21	20	19	18	17	16
Byte 3	31	30	29	28	27	26	25	24

Little-endian ordering

The MSB is configured at address 25.

	Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0
Byte 0	7	6	5	4	3	2	1	0
Byte 1	15	14	13	12	11	10	9	8
Byte 2	23	22	21	20	19	18	17	16
Byte 3	31	30	29	28	27	26	25	24

In the following figure, assuming that byte 0 and byte 1 have 16-bit data of FF and 00, respectively. The following 16-bit data sets are captured:

Big-endian ordering (MSB first): FF00 (Data starting address: 8)

Little-endian ordering (LSB first): 00FF (Data starting address: 0)

Fi	First of the data frame ————————————————————————————————————															-	Tov	varc	the	e las	st of	the	e da	ta fi	rame			
7	6	5	4	3	2	1	0	7	7 6 5 4 3 2 1 0						7 6 5 4 3 2 1 0						0	7	6	5	4			
			Byte st b								3yte nd b)						Byte th b							yte d b		

1

Choosing CAN definition data

Loading a DBC file can set CAN definition data.

> [Channel] > [UNIT] > [CAN/LIN] > [Signal setting]

CAN/LIN	C1 C2	C3				Waveform	disp Signal s	ettir 📥				
4 Selec	t number File	Edit		Calc.							Hor	izon sor
	Signal ID	Start bit	Bit length	Byte order	Data type	Ratio	Offset	Check sum	DLC	Delate	Up D	own
2		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
2		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
1 ³		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
4		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
0 5		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
6		0 0	8	Little	Signed	1	0	Classic	1	Ô	^	~
-1 7	(0 0	8	Little	Signed	1	0	Classic	1	Ô	^	~
8		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
9		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
-3 10	(0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
11		0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~
-4 12		0 0	8	Little	Signed	1	o	Classic	1	Ō	^	~
_ 13	(0 0	8	Little	Signed	1	0	Classic	1	Ō	^	~

1 Tap [Signal setting].


2 Tap [File].

The file selection dialog box is displayed.

Signal	ID	Start bit	Bit length	Byte order	Data type	Ratio	Offset	Check :
Sig1Bit	0	0	1	Little	Unsigned	1	0	
Sig8Bit	0	0	8	Little	Unsigned	1	0	
Sig7Bit	0	0	7	Little	Unsigned	1	0	
Discrete	66	0	3	Little	Unsigned	1	0	
Line	65	0	10	Little	Unsigned	1	0	
State	64	23	1	Little	Unsigned	1	0	
Curve	64	0	16	Little	Unsigned	0.1	0	
Counter	64	16	7	Little	Unsigned	1	0	
SineJitter	11	16	16	Little	Unsigned	0.0001	-1	
Sine	11	0	16	Little	Unsigned	0.0001	-1	
		-						
Peak2	12	8	2	Little	Unsigned	1	0	
Peak1	12	0	2	Little	Unsigned	1	0	

3 Tap [File selection].

The file selection dialog box is displayed.

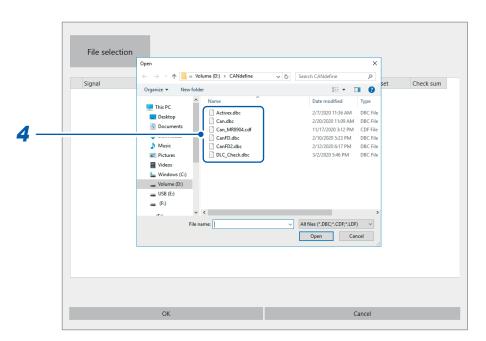

4 Select a file and tap [Open].

The contents of the file you chose are displayed.

5 Tap data sets (rows) to be analyzed.


The chosen rows turn blue. You can choose multiple rows. Tap a chose data again to put it into unselected.

6 Tap [OK].

The file selection dialog box closes, and the chosen data (rows) appear on the [Signal setting] screen.

12.5 Configuring the Transmission Function Settings (Creating a Transmission List)

This section describes how to set data to be transmitted from the instrument to a CAN bus and transmission timing.

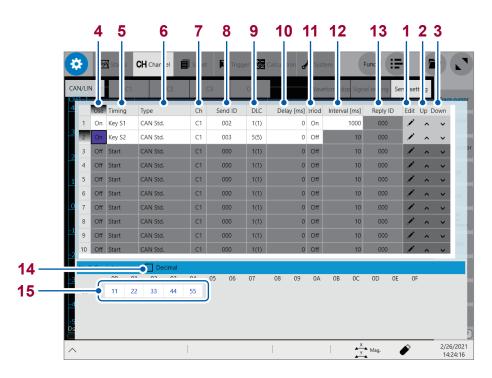

> [Channel] > [CAN/LIN] > [Send setting]

Operation of the transmission list

No.	Name	Function
1	Edit	Tap the selection icon in a row you wish to edit. The DBC file selection dialog box appears. Enter items you wish to edit, and then tap [OK] . The edited items are overwritten.
2	Up	Tap the icon in the row you wish to move upward.
3	Down	Tap the 🔽 icon in the row you wish to move downward.

Tapping the transmission list displays the data, at the bottom, to be transmitted of the number you tapped.

Settings of the transmission list

No.	Name		Function
4	Use	Allows you to choose	whether to transmit the data concerned.
		Off [⊠]	Does not transmit the data.
		On	Transmit the data.
5	Timing	Allows you to set whe	en to transmit the data concerned.
		Key S1	When you press the S1 key
		Key S2	When you press the S2 key
		Start [∅]	When you press the START key Otherwise, when you send the :START command to start measurement
		Trigger	When the trigger activates
		Reply	When the instrument receives a message ID set in [Reply ID] during measurement. (The instrument does not reply any response while no measurement is being performed.)
		Pass	When a pass judgment is yielded for the numerical calculation
		Fail	When a fail judgment is yielded for the numerical calculation
		Error	When an error occurs or a warning is issued
6	Туре	Allows you to choose	a data type to be transmitted.
		CAN Std. [⊠]	CAN data frame in the base format
		CAN Ext.	CAN data frame in the extended format
		CAN Remote Std.	CAN remote frame in the base format
		CAN Remote Ext.	CAN remote frame in the extended format
		CAN FD Std.	CAN FD data frame in the base format
		CAN FD Ext.	CAN FD data frame in the extended format
		(p. 319). • In CAN mode, data sent.	annot be sent depending on the CAN mode-setting set to [CAN FD Std.] or [CAN FD Ext.] cannot be ata set to [CAN Remote Std.] or [CAN Remote Ext.]
7	Ch	Allows you to specify	a CAN channel for use in transmission.
		C1 ^{II} , C2, C3, C4, AI	I
		When you choose [A channels.	II], the instrument transmits the same data for all
8	Send ID	Allows you to enter a hexadecimal notation	message ID of the data to be transmitted. Use
		For the base format	
		0 to 7FF	
		For the extended for	rmat
		0 to 1FFFFFF	

DLC		Function								
	Allows you to enter the DLC and the number of bytes of the data to transmitted.									
	For CAN									
	0(0) to 8(8)									
	For CAN FD									
	0(0) to 8(8), 9(12), 1	0(16), 11(20), 12(24), 13(32), 14(48), 15(64)								
Delay [ms]		delay time, a period of time from when the condition to when the data is transmitted (unit: ms).								
	0 to 10000									
Period	Allows you to choose whether to transmit data only once or at regular intervals. This setting is available when you chose [Key S1], [Key S2], or [Start] i [Timing].									
	Off [∅]	Transmits data only once.								
	On Transmits data at regular intervals.									
	 When [Timing] is set to [Key S1] or [Key S2] Pressing the same key again can stop transmission. When [Timing] is set to [Start] Transmission stops once measurement has finished, and the START key indication has been turned off. 									
		ve measurement, pressing the STOP key can stop s well as measurement.								
nterval [ms]	Allows you to enter a t to [On] .	ransmission interval (unit: ms) when you set [Period]								
	0 to 10000									
Reply ID	Allows you to enter a [Timing] .to [Reply] .	message ID in hexadecimal notation when you set								
	For the base format									
	0 to 7FF									
	For the extended for	mat								
	0 to 1FFFFFF									
	Period	0(0) to 8(8) For CAN FD 0(0) to 8(8), 9(12), 1 Allows you to enter a set in [Timing] is met 0 to 10000 When [Timing] is set Pressing the s When [Timing] is set Pressing the s When [Timing] is set Transmission s START key inc During repetitive transmission a nterval [ms] Allows you to enter a for 0 to 10000 Reply ID Allows you to enter a [Timing].to [Reply]. For the base format 0 to 7FF For the extended for								

Editing data to be transmitted

No.	Name		Function
14	Decimal	Allows you to choose notation.	whether to display data in decimal or hexadecimal
			Displays it in hexadecimal notation.
			Displays it in decimal notation.
15	Editing data	Allows you to edit dat	a. (p. 336)


How to edit data to be transmitted

40	J	Use	Timing	Туре		Ch	Send I	D DLC	Delay [ms]	eriod	Interval [ms]	Reply ID	Edit	Up D	Dow
	1	On	Key S1	CAN Std.		C1	002	1(1)	0	On	1000	000	1	^	~
30	2	On	Key S2	CAN Std.		C1	003	5(5)	0	Off	10	000	1	^	~
20	3	Off	Start	CAN Std.		C1	000	1(1)	0	Off	10	000	1	^	~
	4	Off	Start	CAN Std.		C1	000	1(1)	0	Off	10	000	1	^	`
10	5	Off	Start	CAN Std.		C1	000	1(1)	0	Off	10	000	/	^	`
	6		Start	CAN Std.		C1	000	1(1)	0	Off	10	000		^	`
0	7		Start	CAN Std.		C1	000	1(1)	0		10	000	/	^	`
-10	8		Start	CAN Std.		C1	000	1(1)	0		10	000		^	`
	9		Start	CAN Std.		C1	000	1(1)	0		10	000		^	`
-20	10	Off	Start	CAN Std.		C1	000	1(1)	0	Off	10	000		^	
	No.2	Send	l data		imal										
-3		6	0.00		03	04	05 06	6 07	08 09	0A	OB OC	OD OE	E OF		
		-0	11 22	2 33	44	55									

1 Tap data item you wish to modify.

1

The tapped data item tunes red, and the editing dialog box appears.

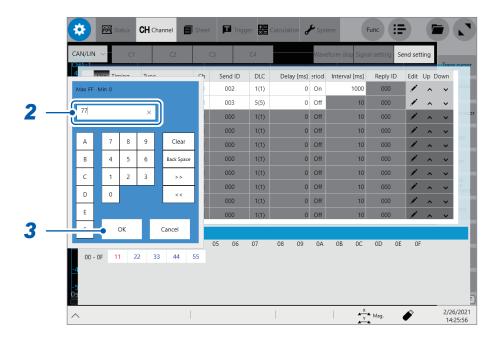

2 Enter values in the editing dialog box. For hexadecimal notation

0 to FF

For decimal notation

0 to 255

3 Tap [OK].

The editing dialog box closes. The edited data is displayed.


	Use	Timing	Туре		Ch	Ser	nd ID	DLC	Delay	/ [ms]	Priod	Interval	[ms]	Reply	/ ID	Edit	Up D) Own	
1		Key S1	CAN Std.		C1		02	1(1)	D Citaj	0			000	000		1	^	~	
2	On	Key S2	CAN Std.		C1	0	03	5(5)		0	Off		10	000	D	1	^	~	
3	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	D	1	^	~	
4	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	D	1	^	~	
5	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	D	1	^	~	
6	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	D	1	^	~	
7	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	D	1	^	~	
8	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	D	1	^	~	
9	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	D	/	^	~	
10	Off	Start	CAN Std.		C1	0	00	1(1)		0	Off		10	000	0	1	^	~	
No.2	Send	d data	_	imal															
00 -	OF	77 01		03 44	04 55	05	06	07	08	09	0A	OB	0C	0D	OE	OF			

12.6 Choosing Data Sets to Be Displayed as Waveforms (When Displaying Waveforms During Measurement)

This section describes how to use the waveform display settings to display CAN/LIN waveforms during measurement.

The instrument converts CAN signals based on CAN definition data before displaying waveforms.

Channel] > [UNIT] > [CAN/LIN] > [Waveform disp]

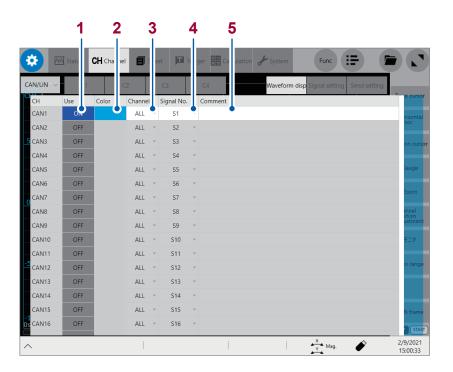


No.	Element	Function
1	Use	Set the column to [On] or [Off].
2	Color	Set a waveform color.
3	Channel	Tap the button to choose a channel. If you choose [ALL] , all channels' signals are converted.
4	Signal No.	Choose a signal number.
5	Comment	Displays the signal name entered in [Signal setting].

12.7 Choosing Data To Be Displayed as Waveforms (When Using the Waveform Calculation Function)

You can use the waveform calculation function to convert CAN signals on the basis of CAN definition data.

This section describes how to perform calculation for CAN channel C1 on the basis of definition data S1.


> [Calculation] > [Waveform calculation]

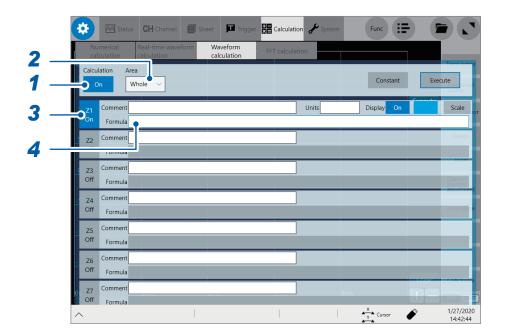

- **1** Tap the [Calculation] button to set it to [On].
- **2** Tap the [Area] button, and then from the list, select [Whole].
- **3** Tap [Z1], which you wish to set, to set to [On].

4 Tap the [Formula] box of [Z1].


The expression setting dialog box is displayed.

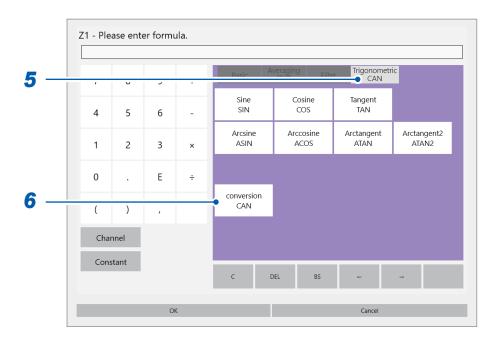

5 Tap the [Trigonometric/CAN] tab.

6 Tap [conversion CAN].


The [setting CAN] dialog box appears.

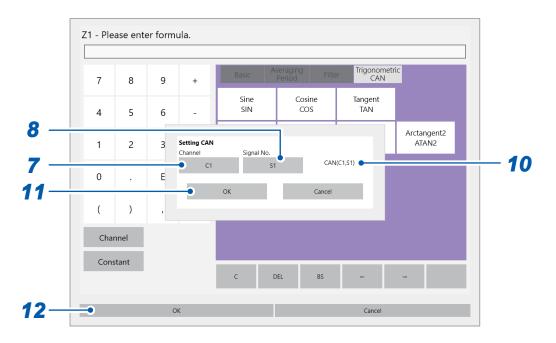

7 Tap the [Channel] box, and then from the list, select [C1].

8 Tap the [Signal No.] box.

The definition data list is displayed.

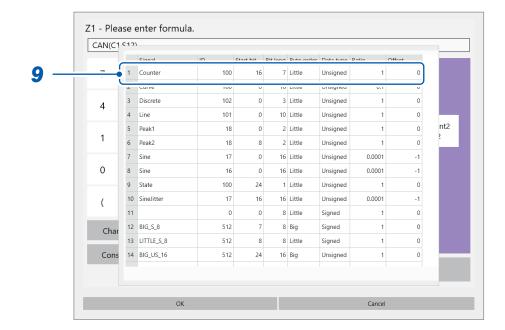

9 Tap the definition data set you wish to use from the list (choose the first row, definition data S1).

The definition data list closes.

10 Check if the selected expression is displayed.

11 Tap [OK] in the [Setting CAN] dialog box.

The **[Setting CAN]** dialog box closes. The selected expression is displayed.

12 Tap [OK] in the expression setting dialog box.

The expression setting dialog box closes. The selected expression is displayed in the **[Formula]** box of **[Z1]**.

	And State	us CH Channel	Sheet 🎞 Trigger	Calculation 🖌 System	m Func	
	imerical culation	Real-time waveform calculation	Waveform calculation	FFT calculation		
Calcul		rea Whole ~			Constant	Execute Cursor
Z1	Comment			Units	Display On	Scale
On	Formula	CAN(C1,S1)				_
SOZ2 Off	Comment Formula					Gauge
0 √Z3	Comment					200m
Off	Formula					Channel
-50Z41	Comment					a justice of
Off	Formula					Auto range
Z5	Comment					
Off	Formula					
Z6	Comment					
Off	Formula					CAN trame
05 Z7	Comment		Ling			
Off	Formula				×	▲ 1/27/2020
\sim					Y Cursor	1/2//2020

12.8 Saving Data

You can save all CAN frame data measured.

File format

CAN frame data is saved as files different from waveform files. Data can be saved in binary form or text form.

Туре	Form	Extension	Description
CAN binary	Binary	CLG	CAN frame data is saved as a binary file.
CAN text	Text	CSV, TXT	CAN frame data is saved as a text file. Only manually saving is available.
CAN index	Index	IXC	These files are used to manage waveform binary files and CAN binary files. They are saved along with CAN binary files. When a CAN index file is loaded, the waveform and CAN frame data are read into the instrument's internal memory at the same time.

CAN binary file

(1) Saving by pressing the SAVE key (manual save)

When a CAN binary file is saved, a CAN binary file can be simultaneously saved. Tap the **[CAN]** button to specify the file to be saved.

Off	Saves the waveform file only.
On	When the CAN frame data exists, the CAN binary file and CAN index file, as well as the waveform binary file, are saved.

(2) Automatic saving, real-time saving

When CAN frame data exists, a CAN binary file and CAN index file are automatically saved along with the waveform binary file.

CAN text file

CAN text files can be saved by pressing the **SAVE** key (manual save) only. Tap the **[Type]** button, and choose **[CAN(Text)]**.


13 Configuring the System Environment Settings

You can configure the system environment settings for the instrument.

IMPORTANT

Do not change any Windows[®] setting unless otherwise indicated in this document. Doing so may cause unstable system operation.

> [System] > [Env.]

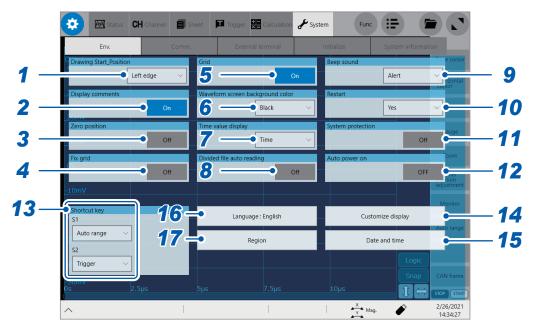

1 Tap the [Drawing Start_Position] box, and then choose a start position of the scrolling display from the list.

Left edge [⊠]	Starts scrolling through waveforms from the left side of the waveform screen.
Right edge	Starts scrolling through waveforms from the right side of the waveform screen.

2 Tap the [Display comments] button to choose a comment display setting.

You can display a title comment and each channel comment on the waveform screen. Each channel comment appears along with each input-channel marker.

On ^ℤ	Displays comments.
Off	Does not display any comments.

3 Tap the [Zero position] button to choose a zero-position marker display setting.

You can display markers at the zero position of each input channel on the time-axis waveform display.

Off [⊠]	Does not display any markers.
On	Displays markers at the zero positions on the left side of the waveform screen.

4 Tap the [Fix grid] button to choose waveform operation mode.

Entering this mode prohibits you from using the touch panel to scroll, enlarge, or compress waveforms in the voltage-axis direction by anchoring the waveform display position.

Off	Allows you to scroll, enlarge, and compress waveforms in the voltage-axis direction.
On	Prohibits you from scrolling, enlarging, and compressing wave-forms in the voltage- axis direction.

5 Tap the [Grid] button to choose a grid display setting of the waveform screen.

On [⊠]	Displays the solid-line grid.	
Off	Does not display any grids.	

6 Tap the [Waveform screen background color] box, and then from the list, choose a background color of the waveform screen.

Black [⊠]	Sets the background color of the waveform screen to black.
White	Sets the background color of the waveform screen to white.

7 Tap the [Time value display] box, and then from the list, choose a display format for the lapse time from a trigger point.

Time [⊠]	Displays the lapse time from the trigger point (the unit is fixed).
Mod 60	Displays the lapse time from the trigger point (in the sexagesimal [base 60] system).
Date	Displays the time when the instrument acquired a waveform.
Samples	Displays the number of samples acquired during the period from the trigger point.

• During the external sampling, this setting is fixed to [Samples].

• These settings also apply to values of the trace cursors.

8 Tap the [Divided file auto reading] button to choose a operation mode for loading divided files.

Off [∅]	Clears the instrument's internal memory and loads the specified file only. To load divided files consecutively, load an IDX file.
On	When you choose the file adjacent to the end of a waveform saved in the instrument's internal memory, the instrument will additionally load files while leaving the waveforms in the internal memory (The waveform's portion of loaded length at the other end is deleted). If you specify files other than those adjacent, the instrument clears the internal memory and consecutively loads the divided files adjacent to the specified file until the internal memory becomes full.

Example of automatic loading of divided files

1. If the storage media contains eight divided individual files 512 MB in size.

| Data in |
|----------|----------|----------|----------|----------|----------|----------|----------|
| file 1 | file 2 | file 3 | file 4 | file 5 | file 6 | file 7 | file 8 |
| (512 MB) |

If the instrument loads file 3 with its internal memory (2 GB) containing no waveforms, the files until file 6 are loaded.

1					r,
	Data in	Data in	Data in	Data in	
	file 3	file 4	file 5	file 6	
	(512 MB)	(512 MB)	(512 MB)	(512 MB)	
	(3.1_1)	(((i i

3. If the instrument loads file 7 in this state, it is additionally loaded and the data potion of file 3 is deleted from the internal memory.

	1				
1	I	Data in	Data in	Data in	Data in
1	1	Batam	Data m	Data III	Data III
		file 4	file 5	file 6	file 7
			nie J	ille 0	IIIE /
i i		(512 MB)	(512 MB)	(512 MB)	(512 MB)
1	I				
1 1	1		· ,	· ,	,

4. If the instrument loads file 2 in this state furthermore, the internal memory is cleared and file 2 through file 6 are automatically loaded.

file 2 file 3 file 4 file 5	r	Data in file 5	
(512 MB) (512 MB) (512 MB) (512 MB)		(512 MB)	

9 Tap the [Beep sound] box, and then choose a beep setting from the list.

Off	Does not allow the instrument to beep.
Alert [∞]	Allows the instrument to beep in the following cases: • If an error message or warning appears • If a fail judgment is given
Alert+Action	Allows the instrument to beep when the instrument starts a measurement, is triggered, stops the measurement, and completes auto-saving, in addition to the cases described above.

10 Tap the [Restart] box, and then from the list, choose whether to immediately restart the measurement after changing a setting that affects measurement during the measurement.

No	Does not restart any measurement. You cannot change any settings during measurement.
Yes [⊠]	If you change a setting during measurement, the instrument confirms the changes and then restart the measurement.

11 Tap the [System protection] box to choose a system protection function setting for power outrage.

On [⊠]	Protects the system from unexpected power interruptions.
Off	Does not protect the system from unexpected power interruptions.

This system protection function uses the UWF (unified write filter) feature installed in Windows[®]. If the system is continuously running for one month or more, we recommend you to turn off this function and prepare an external UPS.

IMPORTANT

If the instrument is shut down while saving files onto an external storage device, it cannot save data correctly.

See "2.9 Supplying Power to the Instrument" in the Quick Start Manual.

13

12 Tap the [Auto power on] button to set whether or not to use the automatic startup function.

Off [∅]	Does not use the automatic startup function.
On	Uses the automatic startup function. Supplying power to the instrument can automatically start running Windows [®] , allowing you to start measurement. You do not need to use the power key.

In the [Shortcut key] area, tap the [S1] and [S2] boxes in turn, and then from the list, choose an action allocated to each of the S1 and S2 keys.

Off	Does not execute any action.
Auto range [⊠]	Executes the automatic ranging. (Default setting for the S1 key)
Trigger [⊠]	Executes the forcible trigger. (Default setting for the S2 key)
See entire waveform	Displays the recording length of waveforms so that they fit the single screen width. A relatively long recording length may require a lot of time for displaying waveforms.
Reset zoom	Displays waveforms at the default display magnification.
Execute	Performing calculation using existing data.
Send CAN data	Sends data whose the CAN transmission [Timing] setting configured to [Key S1] or [Key S2]. When the [Period] setting is configured to [On], pressing S1 or S2 key can start regular transmission. Pressing the same key can stop periodic transmission.
Undo	Cancels the previous action, which restores the instrument to the previous setting.
Redo	Performs the action canceled by tapping [Undo].

13

Configuring the System Environment Settings

14 Tap [Customize display].

The settings screen appears.


To adjust the brightness

(1) Drag the [Adjust brightness level] slider to adjust the brightness.

 Home Customize your display Find a setting System Display Apps & features Default apps Notifications & actions Identify Detect Power & sleep Change the size of text, apps, and other items: 100% (Recommended) Storage Orientation Offline maps Landscape Apply Cancel Apply Cancel About 		
Find a setting Find a setting System Display If Apps & features If Apps & for websites Apps for websites Apply Cancel Apply Cancel	Settings	- 0 >
System Display Image: Display Image: Display <	Home	Customize your display
 Display If Apps & features Default apps Notifications & actions Identify Detect Power & sleep Change the size of text, apps, and other items: 100% (Recommended) Storage Orfine maps Cinentation Offline maps Landscape Multitasking Apps for websites Apps for websites About 	Find a setting ρ	
Image: Apps & features Image: Default apps Image: Default apps <	System	
 Default apps Notifications & actions Identify Detect Power & sleep Change the size of text, apps, and other items: 100% (Recommended) Storage Orientation Offline maps Landscape Adjust brightness level Multitasking Apply Cancel About 	🖵 Display	1
 Notifications & actions Identify Detect Power & sleep Change the size of text, apps, and other items: 100% (Recommended) Storage Orientation Offline maps Iandscape Tablet mode Adjust brightness level Multitasking Apps for websites About 	iΞ Apps & features	
Identify Detect Orientation Change the size of text, apps, and other items: 100% (Recommended) Storage Orientation Offline maps Landscape Tablet mode Adjust brightness level Multitasking Apply Cancel About	⊟ Default apps	
 Storage Orientation Offline maps Tablet mode Adjust brightness level Multitasking Apps for websites About 	Notifications & actions	Identify Detect
Image: Contraction Image: C	O Power & sleep	Change the size of text, apps, and other items: 100% (Recommended)
M Offline maps Landscape Iablet mode Adjust brightness level Multitasking Apps for websites Apps for websites Adpuly Cancel Advanced display settings	📼 Storage	Orientation
Adjust brightness level Apps for websites About Advanced display settings	따 Offline maps	
Apps for websites Apply Cancel ① About Advanced display settings	Tablet mode	Adjust brightness level
Apps for websites Advanced display settings	D Multitasking	
U About	Apps for websites	Apply Cancel
	① About	Advanced display settings
🛨 🕞 📴 📴 🏟 🐘 🔿 🖓 💭	# 🗇 🐂 🛱 🔤 🛊	n Matiat 📰 🙀 🥎

To automatically turn off the display (to blank the screen)

- (2) Tap [Power & sleep].
- (3) In the [Screen] area, tap the list box to choose a length of time after which the screen is blanked.

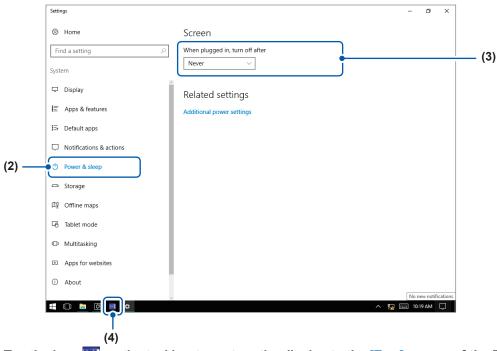

(4) Tap the icon 🚾 on the taskbar to restore the display to the [Env.] screen of the Recorder.

15 Tap [Date and time] ,and then set the clock.

See "2.10 Setting the Clock" in the Quick Start Manual.

16 Change the user interface languages.

- (1) Tap [Language: English].
 - The setting dialog box appears.

Image: Splay comments Maveform screen background color Restart Con Black Yes in co ero position Off Black Yes in co Image: Delease celert language ystem protection stage Nortcut key Shut down this MR6000 and change the display language. OK? Customize display the display 1 Auto range OK Cancel Date and time stage	zontal or n cursor uge
On Black Yes No ero position Off Language ystem protection up Date and time Off Customize display to	
off Language Please select language Please select language the display language. OK? ystem protection urg Off Shut down this MR6000 and change the display language. OK? Customize display urg 1 OK Cancel Date and time urg	
Off Disase calert Iannuane, Off Off Nortcut key hortcut key Shut down this MR6000 and change the display language. OK? Customize display Nortcut key 11 Auto range OK Cancel Date and time Provide 52 Date and time Provide Provide Provide Provide	uge
hortcut key the display language. OK? Customize display disp	
Auto range 52	
Auto range V 52 Date and time Date and time	ion
²²	range
Trigger V	-
2.5µs 5µs 7.5µs 10µs 🖬 🚐	
2.5µs 5µs 7.5µs 10µs 👔 🚗	

(2) Tap the [Language] box, and then choose a user interface language from the list.



(3) Tap [OK].

The instrument is turned off.

(4) Press the power key.

The instrument starts up with the display in the chosen language.

17 Tap [Region].

Choose characters that represent the decimal symbol and the separator used in data included in waveform files (text format) and numerical calculation result files.

Tap the [Decimal point], and then from the list, choose a character that represents the decimal symbol.

Period . ^{III}	Designates the period (.) as the decimal point.
Comma ,	Designates the comma (,) as the decimal point.

Tap the [Decimal point], and then from the list, choose a character that represents the separator.

Comma , [⊠]	Designates the comma (,) as the separator.
Space	Designates the space symbol as the separator.
Tab	Designates the tab symbol as the separator.
Semicolon ;	Designates the semicolon (;) as the separator.

• Either the decimal symbol or separator, but not both, can be set to [Comma ,].


• Filenames have the .CSV extension with the [Comma ,] separator setting; the .TXT extension with a separator settings other than [Comma ,] .

14 Connecting the Instrument to Computers


Familiarize yourself with the section "Before connecting to an external device" in "Operation Precautions" in the Quick Start Manual.

This instrument is equipped with the Ethernet 1000BASE-T interface for LAN communications. You can control the instrument using computers or other devices connected to your network with 10BASE-T or 100BASE-TX or 1000BASE-T cable.

> [System] > [Comm.]

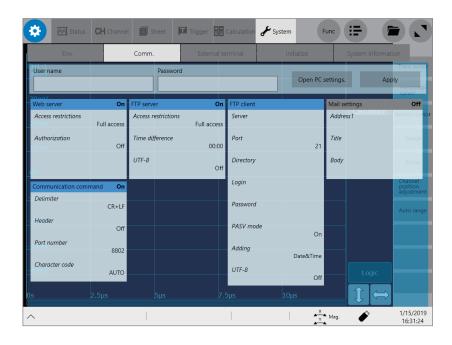

Operation available on the [Comm.] screen

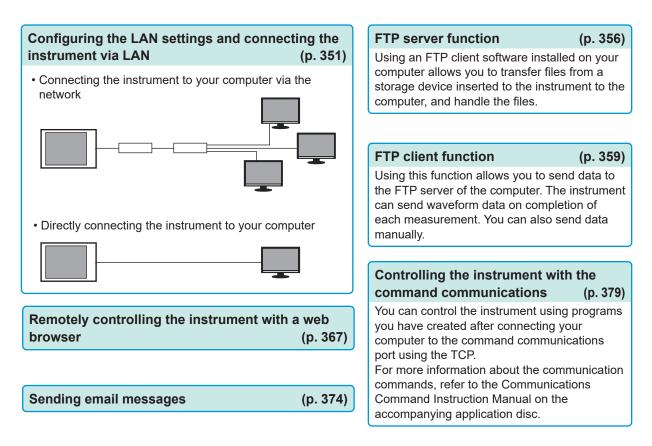

14.1 Configuring the LAN Settings and Connecting the Instrument to the Network

This section describes how to configure the LAN settings of the instrument and how to connect the instrument to your computer with a LAN cable before using the FTP or web browser with a computer or command-communicating.

Be sure to configure the LAN settings before connecting the instrument to the network. When you change the settings while the instrument is connecting to the network, the IP addresses may fail to be unique or invalid address data may be transmitted over the network.

For more information on how to connect the instrument to computers, refer to "2.6 Connecting the Instrument With Computers" in the Quick Start Manual.

When the system protection function (p. 345) is enabled, you cannot change the LAN settings.

IMPORTANT

Do not change any Windows[®] setting unless otherwise indicated in this document. Doing so may cause unstable system operation.

Configuring the LAN settings with the instrument

Items to be checked before configuring the LAN settings

The required settings are different depending on whether to connect the instrument to an existing network or whether to establish a new network consisting of only the instrument and a computer.

When connecting the instrument to the existing network

Ask your network administrator to assign the following items in advance. Be sure that there is no conflict with other devices.

The computer name and address of the instrument
Computer name (up to 15 characters):
IP address:
Subnet mask:
Gateway
Whether to use a gateway: Yes/No
IP address (When used):

When establishing a new network consisting of the instrument and a computer

(Using the instrument on the local network not connect to any external networks)


When no administrator exists for your network or you are entrusted with the settings, the following addresses are recommended.

Setting example:

IP Address Computer: 192.168.0.1 Recorder 1: 192.168.0.2 Recorder 2: 192.168.0.3 . . . Assign numbers in a sequential order. Computer name......Any name (must be unique) Subnet mask......255.255.255.0 GatewayOff

Setting items


> [System] > [Comm.]

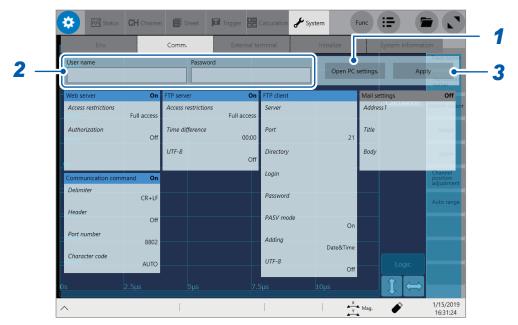

1 Tap [Open PC settings.].

The Ethernet settings screen appears.

- (1) Tap [Ethernet Properties]. The [Network Connections] window appears.
- (2) Tap [Ethernet].
- (3) Tap [Change settings of this connection]. The [Ethernet Properties] window appears.

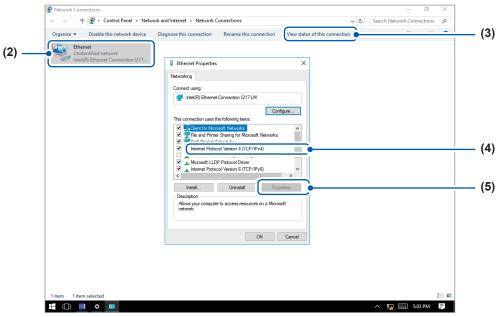

- (4) Tap [Internet Protocol Version 4 (TCP/IPv4)].
- (5) Tap [Properties]. The [Internet Protocol Version 4 (TCP/IPv4) Properties].

(6) Enter the necessary information.

IP address	The IP addresses identify individual devices on the network. Assign a unique address different from that of other devices.
Subnet mask	The subnet mask divides the IP address into the network address and the host address. Configure the subnet mask settings in the same way as those of other devices on the network.
Default gateway	For network connection When your computer to be used (host device) connects to another network than the instrument, specify a gateway device. When your computer connects to the same network, usually assign the same address as the default gateway in the computer communications settings.

(7) Tap [OK].

- (8) In the [Ethernet Properties] window, tap [OK].
- (9) Tap the [Close] ([×]) button to close the [Network Connections] window.
- (10) Tap the icon 💹 on the taskbar to restore the display to the [Comm.] screen of the Recorder.
- **2** Tap the [User name] and [Password] boxes in turn, and then enter your authorization user name and password in each box

These are used when you log in to the FTP of the instrument or use the web browser installed in the computer (When the authorization setting is set to **[On]**).

With the authorization setting configured, you can log in only when you enter the user name and password same as those specified. Configuring this setting is recommended when you would like to limit the users.

The password entered in the [Password] box is hidden behind the asterisks (*).

Characters you can use: Alphabetic characters and symbols (however, the colon [:] is prohibited.)

When you would like to allow anyone to access the network or log in as an "anonymous" FTP client, leave the **[User name]** box and **[Password]** boxes blank.


3 Tap [Apply].

Tap **[OK]** to confirm the settings.

Renaming the computer

This name in the **[Current PC name]** box identifies the instrument on the network. If necessary, change the computer name to a unique one among the network devices.

> [System] > [Comm.]

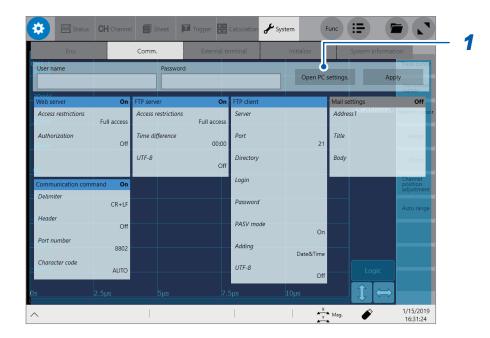

1 Tap [Open PC settings.].

The Ethernet settings screen appears.

2 Tap [Home].

The Windows[®] settings screen appears.


3 Tap [System].

- **4** Tap [About] under System.
- **5** Tap [Rename PC], and then enter another name in the [Current PC name] box.
- **6 Tap [Next].** Restarting the instrument is required.
- 7 Tap [Restart now].

How to configure the LAN settings

Follow this procedure in accordance with the intended usage. For details on each setting, refer to "Setting items" (p. 352).

For details on your network including the IP address, contact your network administrator.

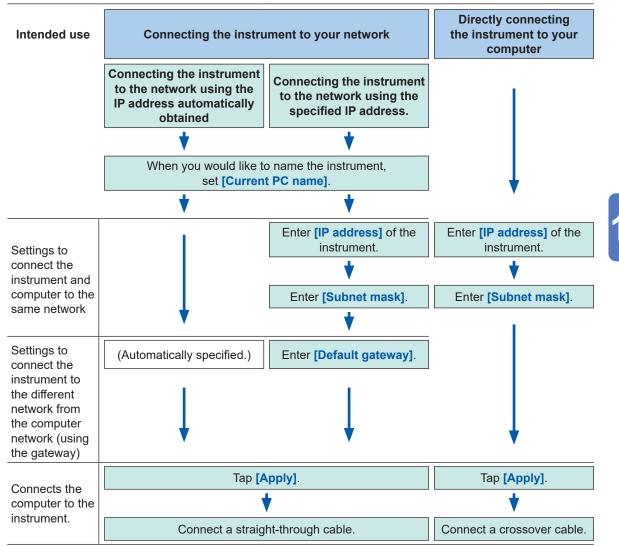

14.2 Managing Data in the Instrument With the FTP Server Function

Using the FTP client software installed in your computer allows you to transfer files from storage devices in the instrument to the computer, and manage the files with the computer.

- The instrument is equipped with an FTP server.
- · You can operate the instrument using Explorer or various free software.

Precautions when the FTP is used

- The FTP server of the instrument allows only one connection. Multiple computers cannot simultaneously access the server.
- If no command is sent from the computer for more than one minute after the FTP connection has been established, the FTP session may time out. If a timeout occurs, reconnect the computer via the FTP.
- The instrument interrupts an FTP session during real-time saving (during measurement).
- Before inserting or removing an SD memory card or a USB flash drive, terminate the FTP connection first.
- Do not handle any files during an FTP session.
- With Internet Explorer®, updated dates of files may not match those saved in the instrument.
- With Internet Explorer[®], temporary Internet files created during the previous access are retained;

thus, the previous data may be acquired instead of the latest data.

- If you cancel the transfer of selected files or folders before its completion, some FTP client/ browser programs may delete all of them from the source regardless of whether they have been transferred. Avoid moving files and folders. Download files and folders using the copy function, and then delete them.
- Be careful that the user name and password themselves will get transmitted via the network when the FTP server is used.
- When you upload a file, the time stamp on the file will change to the uploading time.
- Each storage device appears as a directory on the FTP server.

/STORAGE	Waveform data written in the instrument (Writing data is prohibited.)
/D through /Z	Storage devices serving as drives


Configuring the FTP sever setting with the instrument



1

Tap [FTP server].

The setting dialog box appears.

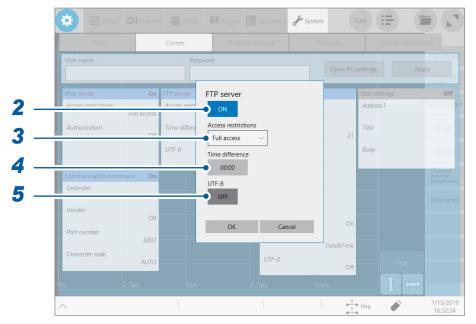

- **2** Tap the [FTP server] button to set it to [On].
- **3** Tap the [Access restrictions] box, and then from the list, choose an access restriction setting.

Read only	Enables you to read files only. Choosing this option prevents files from being deleted or changed from outside the instrument.
Full access [⊠]	Enables you to write (upload) files on storage devices, as well as delete and rename files.

4 Tap the [Time difference] box, and then enter a time correction.

In general, leave it at [00:00].


Setting the time difference between files

With some versions of Internet Explorer[®], time stamps may differ between those on files in your computer and the instrument to a certain extent. In this case, you can correct the time stamps by specifying the time difference. However, the corrected time stamps will differ from those on files in any FTP clients other than Internet Explorer[®]. Example: -9:00

5 Tap the [UTF-8] button to choose an UFT-8 support setting.

Operating the instrument with your computer (FTP server function)

The following example shows how to operate the instrument with File Explorer on Windows 10.

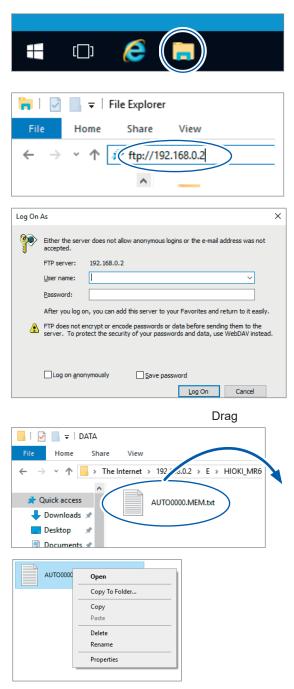

 Run File Explorer on your computer. Click the File Explorer icon on the Windows 10 taskbar to start File Explorer.

2 Enter an IP address.

Click the address bar in File Explorer and enter an IP address. Enter the character string **[ftp://]** followed by the IP address.

3 Log on to the FTP server.

The Log On As screen appears when you have been registered your authentication user name and password in the communication screen or the instrument. Enter your user name and password to log on,

4 Download a file.

Choose a file you would like to download from the file list. Drag the file to the download destination (press and hold the mouse left button on the file, move it to the intended location while pressing the button, and then release the button).

5

Delete or rename a file.

Right-click a file in the FTP folder list, and select **[Delete]** or **[Rename]** from the shortcut menu.

14.3 Sending Data to a Computer With the FTP Client Function

The instrument is equipped with the FTP transmission function (FTP client). You can send data to the FTP server on the network.

FTP transmission method

Real-time saving data transmission	Automatically sends waveform data during measurement. Configure the real-time saving settings and specify the save destination to [FTP] .
Automatic saving data transmission	Automatically sends save target data on completion of the measurement, according to the automatic saving settings. Configure the automatic saving settings and specify the save destination to [FTP] .
Transmission with the SAVE key	Press the SAVE key automatically sends save target data. With the manual save settings, specify the save destination to [FTP].

• The date of a file sent to the computer is set at when the file was sent.

- Transmission to all FTP servers is not necessarily guaranteed due to differences among servers.
- If a file with the same name exists in the destination, the file is overwritten.

To turn a feature on, select its check box. To turn a feature off, clear its check box. A filled box means that only part of the feature is turned on.

Internet Explorer 11
Internet Information Services

FTP Extensibility

🕞 🔳 📕 Web Management Tools

⊞ IIS 6 Management Compatibility

Internet Information Services Hostable Web Core

OK

Cancel

IIS Management Console

■ IIS Management Service World Wide Web Services


🖃 🔳 📑 FTP Server

Configuring an FTP server setting on a computer

The following example shows how to configure the FTP server settings on Windows 10. The Microsoft[®] Windows[®] Home Edition does not include any FTP server. Use free software such as the FileZilla (trademark of another company) Server.

- The setting contents may vary with environment. When necessary, refer to the help topics of the FTP server or consult your network administrator.
- Microsoft[®] Windows[®] administrator privileges are required for setup.

Enabling the FTP

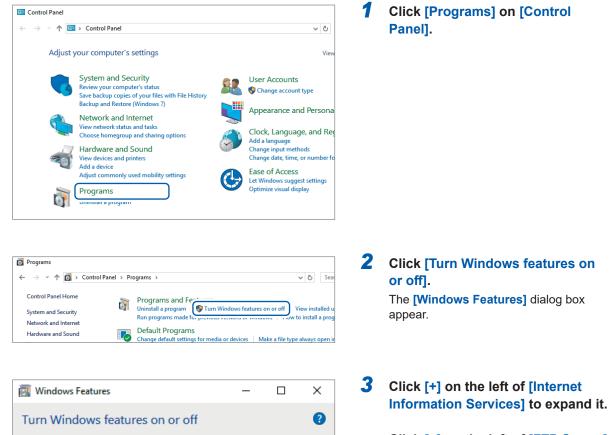


Click [+] on the left of [FTP Server] to expand it, and then select [FTP Service].

Click [+] on the left of [Web Management Tools] to expand it, and then select [IIS Management Console].

Click [OK].


Configuring the FTP settings

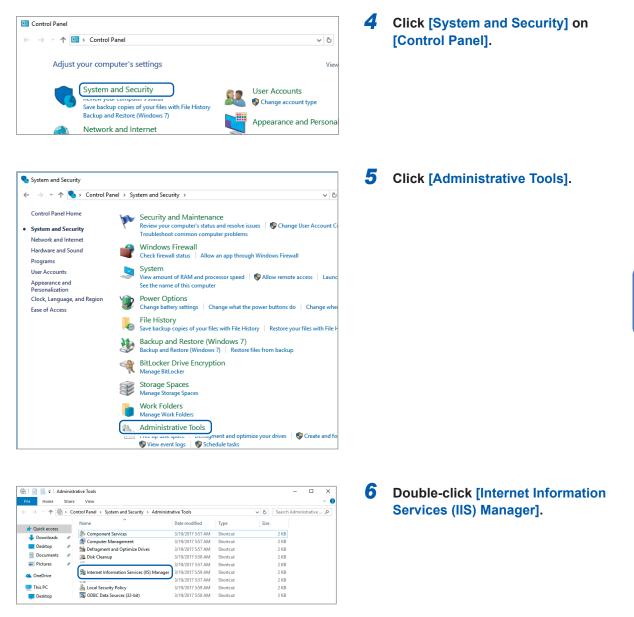


📬 Internet Information Se	rvices (IIS) Manager
← → € ► EMC	1KA7 🕨
File View Help	
Connections	EMC1
> 4 EMC1KA7 (eme¹Le³2)	Refresh Add Website Start Stop Add FTP Site Rename
	Switch to Content View

7 Right-click on the item displayed under [Connections] on the left side of the screen to display the shortcut menu, and then click [Add FTP Site].

Communication may be blocked depending on the settings of the computer protecting software (example: firewall).

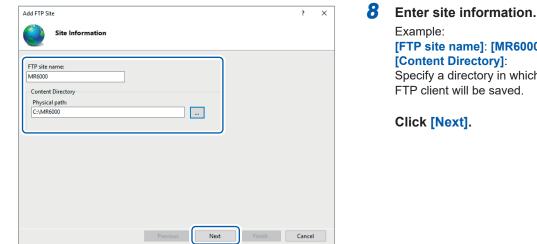

Add FTP Site				?	×
Binding and SSL Settings					
Binding					
IP Address:	Port:				
All Unassigned	~ 21				
Enable Virtual Host Names:					
Virtual Host (example: ftp.contoso.c	om):				
Start FTP site automatically					
SSL	$ \rightarrow$				
No SSL					
O Allow SSL					
O Require SSL					
SSL Certificate:					
Not Selected	~	Select	View		

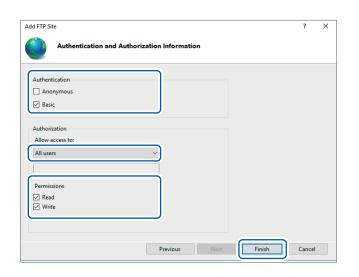

[FTP site name]: [MR6000] Specify a directory in which data from the FTP client will be saved.

9 Specify the [Binding] and [SSL] settings as follows:

[IP Address]	[All Unassigned]
[Port]	[21]
[Start FTP site automatically]	Select
[SSL]	[No SSL]

Click [Next].

10 Specify [Authentication and Authorization Information] as follows:

[Authentication]	Select [Basic].
[Authorization]	[All users]
[Permissions]	Select both [Read] and [Write].

Click [Finish].

Configure the access user setting


Enter an FTP user name and password.

Enter the user name and password specified here in the [Login] and [Password] boxes,

respectively, of the FTP client setting screen of the instrument (see step **4** "Enter a login name and password to use for logging in to the FTP server in the **[Login]** and **[Password]** box, respectively." in p. 365).

j i 🛃 🔜 ≂ i Adi File Home	mini: Shai	strative Tools re View			-	>
- → · ↑ 檣			strative Tools		マ ひ Search Ac	ې م Iministrative ۵
# Quick access		Name	Date modified	Туре	Size	
			3/19/2017 5:57 AM	Shortcut	2 KB	
Downloads	1	🔚 Computer Management	3/19/2017 5:57 AM	Shortcut	2 KB	
Desktop	1	······································	3/19/2017 5:57 AM	Shortcut	2 KB	
🔮 Documents	1	📜 Disk Cleanup	3/19/2017 5:58 AM	Shortcut	2 KB	
Pictures	*	🛃 Event Viewer	3/19/2017 5:57 AM	Shortcut	2 KB	
ConeDrive		🎇 Internet Information Services (IIS) Manage	er 3/19/2017 5:59 AM	Shortcut	2 KB	
Chebrive		👧 iSCSI Initiator	3/19/2017 5:57 AM	Shortcut	2 KB	
💻 This PC		http://www.com/comments/action	3/19/2017 5:59 AM	Shortcut	2 KB	
Desktop		ODBC Data Sources (32-bit)	3/19/2017 5:58 AM	Shortcut	2 KB	

11 Select [Computer Management] in [Administrative Tools] mentioned in step 5 (p. 361).

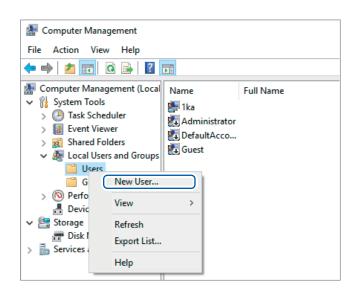


12 Right-click [Users] under [Local Users and Groups], then select [New User].

New User	?	Х
User name: MR6000		
Full name:		
Description:		
Password:		
Confirm password:		
User must change password at next logon		
User cannot change password		
Password never expires		
Account is disabled		
Help	Clos	e

13 Enter your user name, password, and the same password entered in the [User name], [Password], and [Confirm password] boxes, respectively, then select [Password never expires].

14 Click [Create].

Configuring the Windows[®] firewall settings

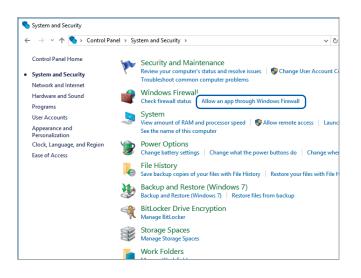

 Follow step 4 (p. 361), and then select [System and Security] > [Allow an app through Window Firewall].

16 Select [FTP Server].

Select private or public, whichever connects with Model MR6000.

Allowed apps			- 0	
$ ightarrow ~ \uparrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \$	Search	Control P	anel	
Allow apps to communicate through Windows Firewall				
To add, change, or remove allowed apps and ports, click Change settings.				
What are the risks of allowing an app to communicate?		- 😯 Cha	nge settir	ngs
Allowed apps and features:				
Name		Private	Public	^
☑ DIAL protocol server				
Distributed Transaction Coordinator				
✓ Email and accounts				
File and Printer Sharing				
FTP Server				
I Get Office		M	M	
✓ Get started			✓	
☐ HomeGroup				
□ iSCSI Service				
Key Management Service				
☑ Mail and Calendar			✓	
Media Center Extenders				\mathbf{v}
	Deta	ai <u>l</u> s	Re <u>m</u> ov	e
		Allow an	othe <u>r</u> ap	p


Configuring the FTP client setting with the instrument



1

Tap [FTP Client].

The setting dialog box appears.

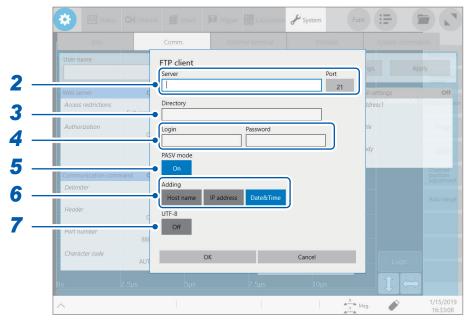

2 Tap the [Server] box and the [Port] button in turn.

The key pad and numerical value entry dialog box appears.

Enter a computer name or an IP address in the [Server] box. In the [Port] box, enter a port number with which the FTP server is operating if the number is not the standard number of 21.

3 Enter a directory name in the [Directory] box.

When the directory is left blank, the instrument stores the file in the contents directory of the FTP site specified in step **8** on p. 362.

If you wish to specify a directory of the contents directory to store files, enter the directory path in the [Directory] box.

Setting example

If you have specified the C:\MR6000 folder as the contents directory in step 8 on p. 362 and have left the directory name blank in this step, the file is stored in the C:\MR6000 folder.

If you enter WAVE for the contents directory, the file is stored in the C:\MR6000\wave folder. Do not enter an absolute path beginning with a drive letter.

4 Enter a login name and password to use for logging in to the FTP server in the [Login] and [Password] box, respectively.

Enter the user name and password specified for the FTP server of the computer. See "Configure the access user setting" (p. 363).

5 Tap the [PASV Mode].button to choose a PASV mode setting.

To establish communications in PASV mode, set it to [On].

6 Tap any of the buttons in the [Adding] area,

Tap a button to add identifiers to file names.

- No identifies is added when you choose a file on the file screen to send it. Files with the same name are overwritten.
- When you have configured the setting to append numerical calculation results to existing files (when you set the [Calculation result] button to [On] or choose [Append] in the [File] box), no identifiers representing time of day are added. Moreover, if a file with the same name exists, the instrument attempts to append data to the file.
- No button in the **[Adding]** area is enabled, a file with the same name is overwritten when it exists. Note that all files with the same name will be overwritten if **[Date&Time]** is disabled with the continuous measurement setting and some others.

7 Tap the [UTF-8] button to choose an UFT-8 support setting.

14.4 Operating the Instrument With a Browser Installed in a Computer

You can configure the instrument settings, operate the instrument, and acquire data from a computer with a web browser. Internet Explorer[®] Version 8 or later or Microsoft Edge[®] is recommended.




1

> [System] > [Comm.]

Tap [Web server].

The setting dialog box appears.

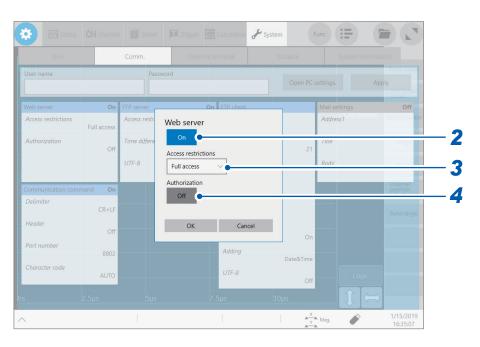

2 Tap the [Web server] button to set it to [On].

3 Tap the [Access restrictions] box, and then from the list, choose an access restriction setting.

Monitor onlyAllows you to browse only the screen and waveform data).		Allows you to browse only the screen and status from the browser (you can obtain waveform data).
	Full access [™]	Allows you to operate the instrument and configure settings from the browser.

4 Tap the [Authentication] button to choose a web-server authentication setting.

Off	Allows you to operate the instrument without the web server authentication.
On	Allows you to operate the instrument with the web server authentication.


14

Connecting your computer to the instrument with a web browser

The following example describes how to connect your computer to the instrument with Internet Explorer[®] on Windows 10.

Start Internet Explorer[®] on the computer and enter the character string [http://] followed by the IP address or the computer name in the address bar.

When the IP address of the instrument is "192.168.0.3"

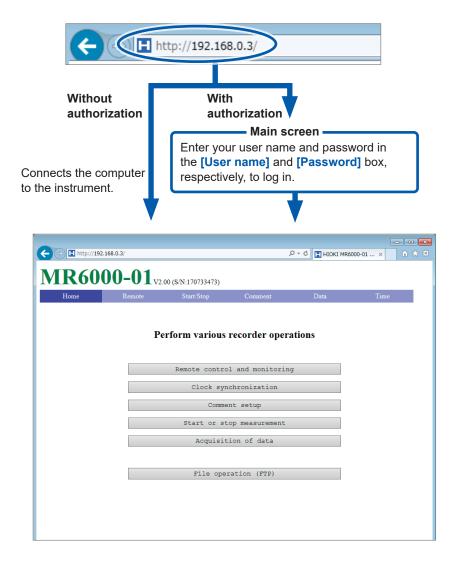

Remotely operating the instrument



1 Click [Remote] on the menu.

The screen switches to the remote operation screen, and the screen displayed on the instrument appears as it is on the browser.

The operation panel buttons conform to the buttons on the instrument. Clicking the screen with a mouse (same as tapping the screen of the instrument) allows you to remotely operate the instrument.

MR60 Home		emote	Start/Stop		Comment	Data	1	Гіте
Update Speed: Norm	al 🗸							Screen Cop
		I Sheet	Trigger	Calculation	System F			SAVE
Env.		Comm.	External te		Initialize	System inf	ormation	H
2User name		Pass			_		Trace curso	S1 S2
1					Open PC s	settings. Nume Calcula	Apply ric Horizontal tion	XL XR
Web server	On	FTP server	On	FTP client		Mail settings	Off	
Access restrictions	Full access	Access restrict	ions Full access	Server		Address 1	Section curso	хс
Authorization	Off	Time differenc	e 00:00	Port	21	Title	Gauge	
- 2mV		UTF-8		Directory		Body	Zoom	YL YR
-			Off	Login			Channel	
Communication comm	nand On						position adjustment	YC
-4mV	CR+LF			Password			Auto range	START
Header	Off			PASV mode	On			
Port number	8802			Adding				STOP
Character code				UTF-8	Date&Time			
-/mV	AUTO			011-8	Off			

- **2** Choose a screen update speed from the [Update Speed] list box.
- **3** To save a screenshot, click [Screen Copy].

Starting/Stopping measurement

You can start and stop measurement

(C)			P - C 王 HIOKI MRC	5000-01 × n 📩
Home	Remote Start/St		Data ations	Time
		control and monitorin ck synchronization	g	
		Comment setup or stop measurement quisition of data		
		Le operation (FTP)		

. . .

1 Click [Start/Stop] on the menu.

The [Measurement Start/Stop] screen appears.



2 Choose an action.

START	Starts a measurement.	
STOP	Stops the measurement.	
ABORT	Forcibly stops the measurement.	

No post-measurement processes such as numerical calculations and automatic saving are performed.


Configuring the comment setting

You can configure the comment setting.

H http://192.1	168.0.3/		۶	HIOKI M	16000-01 × fit ☆ 🕸
MR60)0-01 V2.00 (S/N:1)	70733473)			
Home	Remote Sta	rt/Stop	Comment	Data	Time
			-•		
	Daufaum		 	4	
	Perform	various rec	order opera	itions	
	Remo	te control ar	nd monitoring	J	
		Clock synchro	nization		
		Comment s	etup		
	St	art or stop m	neasurement		
		Acquisition	of data		
		-			
		File operati	on (FTP)		
		1110 Operadi	(111)		
	MR60	Home Remote Star	NR6000-01 V2.00 (S.N:170733473) Home Remote Start/Stop Perform various reco Remote control ar Clock synchro Comment s Start or stop m Acquisition	Home Remote Start/Stop Comment Perform various recorder opera	NR60000-01 V2.00 (S/N:170733473) Home Remote Start/Stop Comment Date Perform various recorder operations Remote control and monitoring Clock synchronization Clock synchronization Comment setup Start or stop measurement Acquisition of data

1 Click [Comment] on the menu.

The [Comment setup] screen appears.

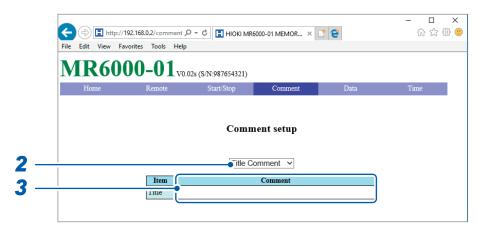

2 From the [Comment setup] list box, choose a comment type. You can enter the following comments:

Title Comment[⊠], Analog Channel, Logic Channel, Real-time Waveform Calculation, Waveform Calculation Comment, FFT Calculation Comment

3 Enter a comment in the [Comment] box.

Acquiring data from the instrument


Data written in the memory of the instrument can be acquired.

	← → Http://192.	168.0.3/			P - C H HIOKI MR6000-01 × 命☆ 3
	MR60	DO-01 _{V2}	.00 (S/N:170733473)		
	Home	Remote	Start/Stop	Comment	Data Time
1					
•		Р	erform various	recorder op	erations
			Remote contro	l and monitor	ring
			Clock syn	chronization	
			Comme	nt setup	
			Start or st	op measuremer	nt
			Acquisit	ion of data	
			File oper	ation (FTP)	

. .

1 Click [Data] on the menu.

The [Acquisition of measurement data] screen appears.

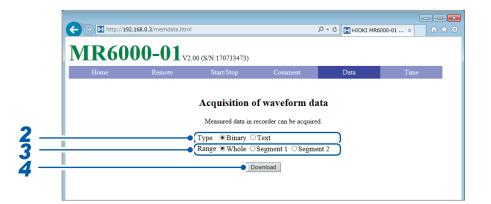

2 Choose a data type.

Binary, Text

3 Choose a data range ([Section cursor]).

Whole, Segment 1, Segment 2

4 Click [Download].

.


Setting the clock

The time of the clock on your computer can be set by that in the instrument. You cannot the clock during measurement.

← → H http://192	168.0.3/			P - C 🖪 HIOKI MR	5000-01 ×
MR60	00_01				
Home	Remote		<i>a</i>	Data	Time
Home	Kemote	Start/Stop	Comment	Data	Lime
	Р	erform various	recorder oper	ations	
		Remote contro	l and monitorin	g	
		Clock svr	chronization		
		Comme	nt setup		
		Start or st	op measurement		
		Acquisit	ion of data		
		File ope	ration (FTP)		

1 Click [Time] on the menu.

The **[Synchronization]** screen appears, and the time of the clock on the computer and the recorder (instrument) appear.

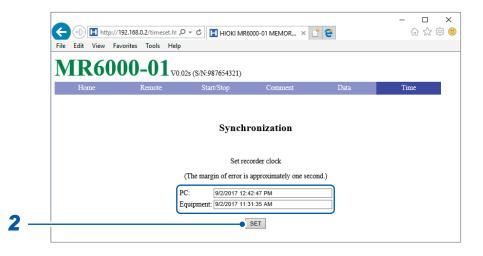

2 Click [SET].

The time of the clock on the computer is set by that in the recorder (instrument). However, an error of one second may occur.

Handling files

You can transfer files in the instrument. See "14.2 Managing Data in the Instrument With the FTP Server Function" (p. 356).

.

14.5 Sending Email messages

The instrument is equipped with the email transmission function. You can send email messages to computers in the network or to those installed in remote locations via the SMTP server. Moreover, you can install the instrument in a remote location and collect waveform data through an email attachment.

How to send email messages

Automatic saving email message	Automatically sends an email message with data saved on completion of measurement attached, according to the automatic saving settings. Set [Auto save settings] to [On] and choose [Mail] in the [Media] box in advance. (p. 120)
Manual email transmission with the SAVE key	Pressing the SAVE key automatically allows an email message to be sent with saved data attached. Set the [Media] box of the manual save setting to [Mail] in advance. (p. 127)
Test email message	Checks if an email message is successfully sent.

Encryption of email attachments

You can encrypt email attachments, such as screen data and waveform data, to prevent it from getting into outsiders.

- · If transmission conditions are frequently satisfied, email messages will also be sent frequently.
- Data size of an email attachment may get extremely large. Depending on the communication environment, an email message cannot correctly be sent if the size is extremely large.
- Email attachment data is encrypted in ZIP format by WinZip 128-bit AE-2 / AES encryption. Encrypted files can be unzipped by Corel WinZip (trademark of another company) or free software such as 7z. (The WinZip AES encryption is stronger and securer than the standard ZIP encryption; however, supporting software is limited. The built-in ZIP feature of Microsoft[®] Windows[®] cannot unzip encrypted files in this format.)
- Files are encrypted by 128-bit AES encryption. Presently, this encryption method is sufficiently strong; however, Hioki does not guarantee that files are never decrypted.
- Handle your encryption password so that outsiders could know. Note that you cannot decrypt any files if you forget your password or enter an invalid password.
- When you have set or changed the password, send a test email message first to check whether you can unzip an attachment before actual use.
- Encrypted ZIP files are not compressed.
- When files are encrypted and zipped, sending email messages require a long time due to conversion time.
- The instrument supports pop-before-smtp and smtp-auth (PLAIN, LOGIN, CRAM-MD5) as the SMTP authentication (since the instrument does not support IMAP, SSL, or STARTTLS, you cannot send email messages to some mail servers, such as Gmail).
- We cannot guarantee transmission to all SMTP servers due to differences among servers.
- AES is the encryption standard specified in the U.S. Federal Information Processing Standard (FIPS) PUB 197.
- The instrument have no email reception function but the transmission function.
- You cannot load any compressed and encrypted data as it is on the instrument or on the Wave Viewer (Wv).

Configuring the basic setting for sending email messages




1

> [System] > [Comm.]

Tap [Mail settings].

The setting dialog box appears.

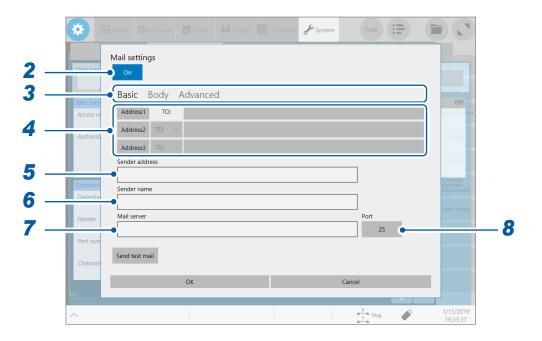

- **2** Tap the [Mail settings] button to set it to [On].
- **3** Tap [Basic].
- 4 Tap [Address1] to choose it, and then enter an email address in the blank box. To send email messages to multiple destinations, enter other email addresses in the [Address2] and [Address3] boxes in the same manner. Specify a recipient type ([To] or [Bcc]) for [Address2] and [Address3].
- **5** Tap the [Sender address] box, and then enter a sender address.
- **6** Tap the [Sender name] box, and then enter a name so that the recipients identify email messages received from the instrument.
- 7 Tap the [Server] box, and then enter a computer name or computer address.
- 8 (When the SMTP server is operating with the number other than the standard number, 25.) Tap [Port] button, and then enter a port number.

Configuring the email contents settings

			Calculation	System Func	
User na	Mail settings On				n France
Web se Access	Title	vanced			
Author	Body]	
Commu Delimi Headeu Port nu					Chan posit adjus Auto
Charac Os	Send test mail	K	_	Cancel	
~			Ĩ	X Mag.	× 1/15


- **1** Tap [Body].
- **2** Tap the [Title] box, and then enter a mail title.
- **3** Tap the [Body] box, and then enter an email body.
- **4** Tap the [Maximum attachment size] button, and then enter the maximum attachment size.

1^{II} to **2048**

Specify the maximum file size so that no large-size data is sent to the mail server. If a measured data size automatically saved is larger than the specified size, the instrument does not send email messages.

- Data with the specified file size or less may also not be sent due to server restrictions.
- Data is converted (encoded by Base64, compressed, encrypted) for attachment; however, the maximum file size is determined in terms of the size before conversion. Thus, the actually sent data may be larger (approximately 1.3 times) than the size limitation.

Configuring the authentication, compression, and encryption settings for email messages to be sent

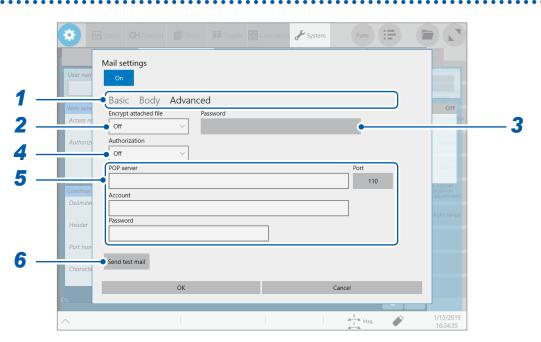

1 Tap [Advanced].

2 Tap the [Encrypt attached file] box, and then choose an attachment setting from the list.

Off [⊠]	Attaches files in original format.
ZIP	Attaches ZIP-compressed files.
ZIP+AES	Attaches files in encrypted ZIP format. The instrument does not compress files.

3 (To encrypt attachments)

Enter an encryption password in the [Password] box.

Number of characters: up to 16

4 (When a user authentication is required)

Tap the [Authentication] box, and then choose a authentication method from the list.

Off [∞]	Sends mails with no user authentication.
РОР	Sends mails using POP (APOP) before SMTP.
SMTP	Sends mails using SMTP (supports CRAM-MD5, PLAIN, and LOGIN).

5 Configure the authorization information settings.

• When using POP authentication

Tap the **[POP server]** box and the **[Port]** button in turn, and then enter a POP server name and its port number, respectively.

When the **[POP server]** is left blank, the instrument uses the figure entered in the **[Mail server]** box. Tap the **[Account]** and **[Password]** boxes in turn, and then enter an authentication user name and password, respectively.

When using SMTP authentication

Tap the **[SMTP Server]** box and the **[Port]** button in turn, and then enter a POP server name and its port number, respectively.

Tap the [Account] and [Password] boxes in turn, and then enter an authentication user name and password, respectively.

6 Check if an email message can normally be sent.

Tap [Send test mail].

The instrument send a test email message that contains specified contents.

Check if the specified destination can correctly receive the email message. If the specified destination cannot receive the email message, review your settings.

If the attachment encryption setting is enabled, the instrument encrypts the test email image.

Be sure to decompress the attachment to check whether the password is correctly set.

14.6 Controlling the Instrument With Command Communications (LAN)

You can externally control the instrument using commands via the communication interface. Communications can be established with a LAN connection.


For details, refer to the Communication Command Instruction Manual on the accompanying application disc.

Configure the LAN settings and connect the instrument before using the command communications. See "14.1 Configuring the LAN Settings and Connecting the Instrument to the Network" (p. 351).

> [System] > [Comm.]

1 Tap [Communication command].

The setting dialog box appears.

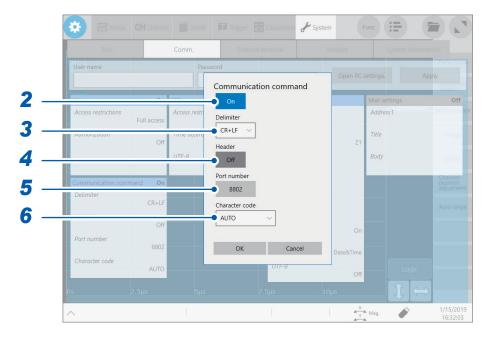

- **2** Tap the [Communication command] button to set it to [On].
- **3** Tap the [Delimiter] box, and then choose a character code (line feed code) that represents the data delimiter.

CR+LF [∅]	Sends the character codes 0x0d and 0x0a.
LF	Sends the character code 0x0a.

4 Tap the [Header] to choose whether to prefix a header to command responses.

Off [⊄]	Does not prefix any header to response data.
On	Prefixes a header to response data.

UTF-8

5 Tap the [Port number] box, and enter a port number in the range of 1002 to 49002. The last digit is fixed at [2].


Sets the character code to UTF-8.

6 AUTO[∅] Automatically sets the character code. SJIS Sets the character code to SJIS.

Tap the [Character code] box, and then choose a character code setting from the list.

14.7 Connecting to a Network Drive

This section describes how to allocate a folder on a networked PC as a network drive and use it as if it were connected to the instrument. First, it's necessary to share the folder on the host PC.

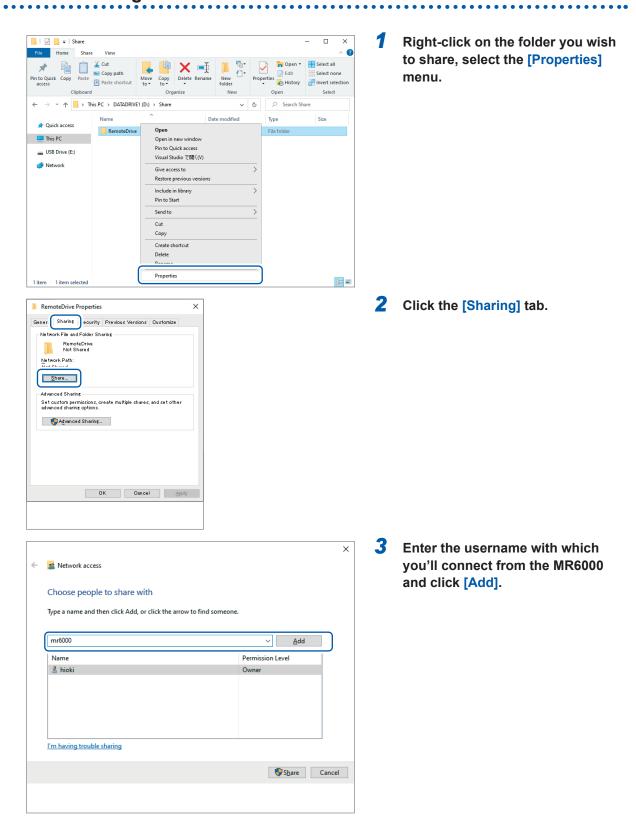


Host PC settings

Connecting the Instrument to Computers

÷	Retwork access Choose people to share with	×	4	Set the access privileges for the newly added user to [Read/Write] and click [Share].
	Type a name and then click Add, or click the arrow to find some	one.		
		∼ <u>A</u> dd		
	Name	Permission Level		
	💄 hioki			
	3 mr6000	Read/Write 🔻		
	I'm having trouble sharing			
		Share Cancel		
			5	Olioly [Donal
		×	9	Click [Done].
←	a Network access			
	Your folder is shared.			
	You can e-mail someone links to these shared items, or copy and	naste the links into another app.		
	······································			
	In dividual Dense			
	Individual Items	^		
	RemoteDrive \\HAEUMR100\RemoteDrive			
	Show me all the network shares on this computer.			
		Done		

MR6000 settings

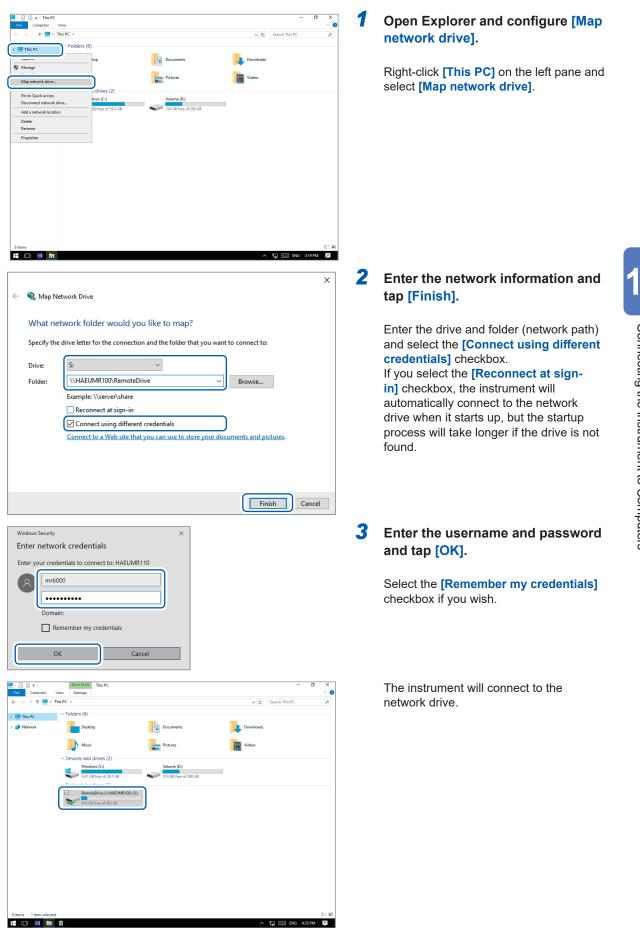

Connecting to a Network Drive

15 Externally Controlling the Instrument

Read the section "Before connecting to an external device" in "Operation Precautions" in the Quick Start Manual carefully.

Connecting the external control terminals with external devices allows the instrument to start and stop measurement.

This section describes the procedure and the external control terminal function to externally control the instrument.

The terminals are referred to collectively as "external control terminals."

Signals inputted into the external control terminals can operate the instrument even when the key lock function is enabled.

For more information about the specifications of the FFT calculation function, refer to Quick Start Manual.

15.1 External Input and Output

External input (IN1), (IN2)


Externally inputting signals can start and stop measurement as well as save data. In factory default settings, the START signal is assigned to the IN1 terminal, and the STOP signal to the IN2 terminal.

How to input signals

1 Connect each of the IN1, IN2, and GND terminals to an external signal-outputting device with wires.

See "2.5 Connecting the External Control Terminals" in the Quick Start Manual.

2 > [System] > [External terminal]

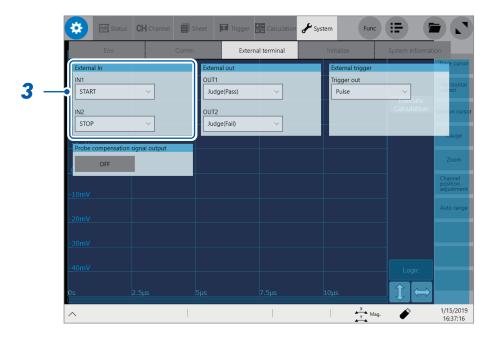


3 Tap the [IN1] and [IN2] boxes in the [External In] area in turn, and then from the list, choose an action performed when an input signal is inputted.

START Starts a measurement.		
STOP	Stops the measurement (post-measurement processes such as numerical calculations and automatic saving are performed).	
START/STOP	Starts a measurement when the low-level signal is inputted; stops the measurement when the high-level signal is inputted.	
SAVE	Saves data on the specified conditions into a storage device that is specified in ([Status] > [Save] > [Save key operation] >) [Quick].	
ABORT	Forcibly terminates the measurement. (No post-measurement processes such as numerical calculation or automatic saving are performed. However, the instrument automatically saves a waveform file that contains data acquired until the forcible termination).	
EVENT	Puts on an event mark. The event marks are put on the waveform screen. You can put event marks by pressing the START key during measurement.	

4 Connect the terminal and the GND terminal with each other, or input pulse waves or square waves to the terminal. The signal have to be with a high-level voltage of between 2.5 V and 10 V, and a low-level voltage of between 0 V and 0.8 V.

The low level of the input waveform controls the instrument.

Available voltage range	High level: 2.5 V to 10 V; low level: 0 V to 0.8 V	
Pulse width	High-level period: 50 ms or more; low-level period: 50 ms or more	
Pulse interval	200 ms or more	
Maximum input voltage	10 V DC	

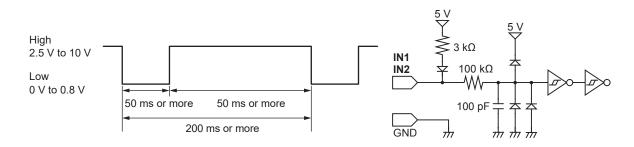

External output (OUT1), (OUT2)


The instrument can output various signals depending on its state.

How to output signals

1 Connect each of the OUT1, OUT2, and GND terminals to an external signal-inputting device with wires.

See "2.5 Connecting the External Control Terminals" in the Quick Start Manual.

2 > [System] > [External terminal]

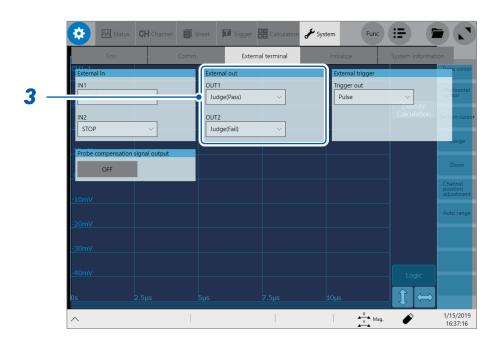

3 Tap the [OUT1] and [OUT2] boxes in the [External out] area in turn, and then from the list, choose a signal output action.


Choose a condition under which the instrument outputs a signal.

Judge(Pass)	Outputs a low-level signal when a pass judgment is given for the numerical calculation result.	
Judge(Fail)	Outputs a low-level signal when a fail judgment is given for the numerical calculation result.	
Error	Outputs a low-level signal when some kind of error or warning occurs.	
Busy	Outputs a low-level signal while rejecting a START signal because the instrument is in the busy state such as performing a measurement and saving data.	
[Waiting for Trigger] Outputs a low-level signal while waiting for a trigger.		

The instrument continues outputting the signal for a pass/fail judgment (low-level output) until it starts the next measurement.

The instrument can output various signals depending on its state.

Output signal	Open-drain ou	Open-drain output (with voltage output), active low	
Output voltage	High level:	4.0 V to 5.0 V	
range	Low level:	0 V to 0.5 V	
Maximum input voltage	50 V DC, 50 m	50 V DC, 50 mA, 200 mW	

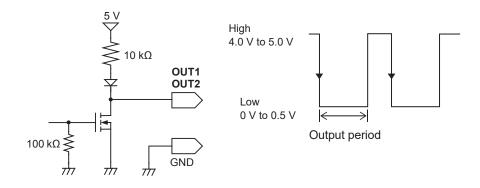

Trigger output (TRIG.OUT)


The instrument outputs a signal when it is triggered. You can use this signal to control multiple instruments, achieving synchronous operation.

How to output signals

1 Connect each of the TRIG OUT and GND terminals to an external signal-inputting device with wires.

See "2.5 Connecting the External Control Terminals" in the Quick Start Manual.

2 (System] > [External terminal]

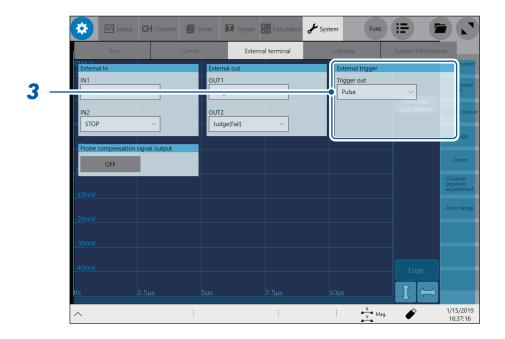


3 In the [External trigger] area, tap the [Trigger out] box, and then from the list, choose a signal output method (the signal is outputted through the trigger output terminal).

Pulse [⊠]	Outputs a low-level signal, and then switches it to the high level after the specified time has elapsed.
Level	Continuously outputs a low-level signal after triggered during the measurement

When triggered, the instrument outputs a pulse wave, which switches from the high level (4.0 V to 5.0 V) to the low level (0 V to 0.5 V).

Output signal	Open-drain output (with voltage output), active low*		
Output voltage range	High level:	4.0 V to 5.0 V	
	Low level:	0 V to 0.5 V	
Pulse width	With the pulse setting:	2 ms ± 1 ms	
	When the level setting:	(Sampling rate) × (Number of data points after trigger) or longer	
Maximum input voltage	50 V DC, 50 mA, 200 mW		

*: The instrument is triggered when the signal voltage level switches from the high level to the low level.

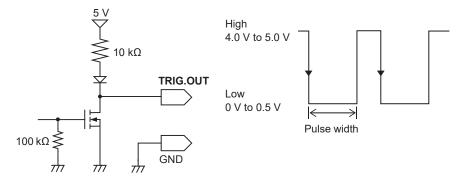

When the auto-range function is used, the instrument is triggered, outputting the TRIG.OUT signal. Be careful when performing auto-range measurement while using the TRIG.OUT signals.

During use of the memory division, the instrument may switch the trigger output (output signal from the TRIG_OUT terminal) to the low level, or irregularly output signals.

- Sampling rate: 200 MS/s to 1 MS/s
- · Recording (measuring) length: 5 ms or less

External trigger terminal (EXT.TRIG)

Externally inputting the trigger signal can trigger the instrument. You can use this signal to control multiple instruments, achieving synchronous operation.


How to an input signal

1 Connect each of the EXT.TRIG and GND terminals to an external signal-outputting device with wires.

See "2.5 Connecting the External Control Terminals" in the Quick Start Manual.


2 > [Trigger] > [Common]

3 Tap the [Trigger] button to set it to [On].

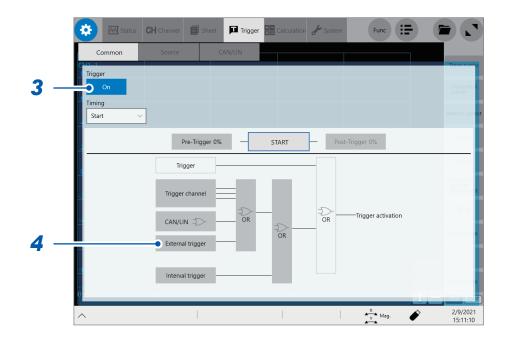

4 Tap [External trigger].

The setting dialog box appears.

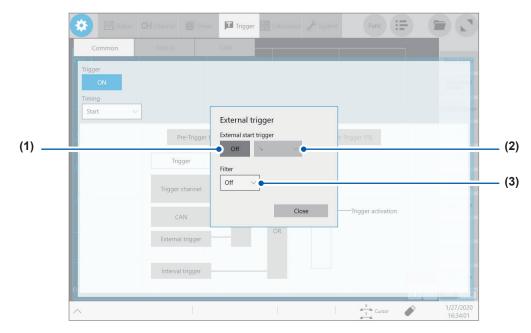

- (1) Tap the [External start trigger] button to set it to [On].
- (2) Tap the box to the right of the **[External start trigger]** box, and then from the list, choose which direction to used for reception of the external trigger.
 - To accept a rising edge: $[/]^*$ To accept a falling edge: $[\backslash]^*$ To accept both a rising edge and falling edge: $[/ \& \backslash]^*$
 - *: When the trigger satisfaction condition is set to [AND], the instrument displays [HIGH] or [LOW] instead of them. You cannot set the trigger satisfaction condition to [High or Low].
- (3) Tap the [Filter] box, and then from the list, choose a filter setting.


This setting can prevent noise and chattering from triggering the instrument unintentionally. Always set this setting to **[Off]** to synchronize multiple instruments using the external trigger.

Off⊄	Enables the chattering prevention filter.				
On	Disables the chattering prevention filter.				

5 Connect the EXT.TRIG terminal and GND terminal with each other, or input pulse waves or square waves to the EXT.TRIG terminal. The wave have to be with a high-level voltage of between 2.5 V and 10 V and a low-level voltage of between 0 V and 0.8 V.

Available voltage range	High level: 2.5 V	2.5 V to 10 V; low level: 0 V to 0.8 V					
Pulse width	Whit the filter disabled	High level: 1 ms or more; Low level: 2 μs or more					
	With the filter enabled	High and low level: 2.5 ms or more					
Maximum input voltage	10 V DC						

The instrument accepts an external trigger on the rising or falling edge of the input waveform.

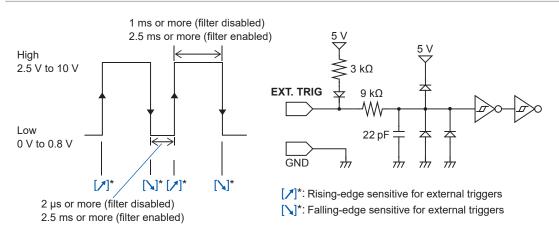

15.2 External Sampling (EXT.SMPL)

Externally inputting the signal allows you to set the sampling rate at any value.

How to an input signal

1 Connect the external sampling terminal of the instrument and the sampling signal-outputting device with the SMB cable.

See "2.4 External Sampling (EXT.SMPL)" in the Quick Start Manual.


2 > [Status] > [Condition]

- **3** Tap the [External sampling] button to set it to [On].
- **4** Tap the box to the right of the [External sampling] box, and then from the list, choose which direction to used for reception of the external sampling signal.

To accept a rising edge: [1] To accept a falling edge: [1] To accept both a rising edge and falling edge: [1&]

5 Input pulse waves or square waves to the EXT.SMPL terminal. The waves have to be with a high-level voltage of between 2.5 V and 10 V and a low-level voltage of between 0 V and 0.8 V.

Available voltage range	High level: 2.5 V to 10 V; low level: 0 V to 0.8 V
Pulse width	High and low level: 50 ns or more
Response frequency	10 MHz or less
Maximum input voltage	10 V DC

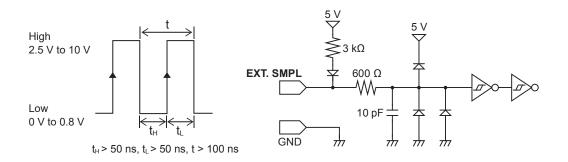

• If a sampling signal with 5 MHz or more is inputted, trigger points are delayed by one sample.

• Using Model 8968 High Resolution Unit disables the anti-aliasing filter even when you set [A.A.F.] to [On].

16 Appendix

16.1 Information for Reference Purposes

Waveform file size (values for reference purposes)

MEM file size (waveforms acquired without using the envelope)

(MEM file size) = (Setting part size) + (Data part size)

(Setting part size) = 187392 + 512 × [(Number of analog channels) + 4 × (Number of logic channels) + (Number of real-time calculation channels)]

(Data part size) = $\{2 \times [(Number of analog channels other than Model MR8990)\}$

+ (Number of logic modules)] + 4 × [(Number of Model MR8990 channels)

+ (Number of real-time calculation channels)]} × (Number of data points)

Recording	Number of channels used							
length (Points)	1	2	4	8	16	32		
2.5 k	192 KB	198 KB	209 KB	231 KB	275 KB	363 KB		
5 k	197 KB	208 KB	229 KB	271 KB	355 KB	523 KB		
10 k	207 KB	228 KB	269 KB	351 KB	515 KB	843 KB		
20 k	227 KB	268 KB	349 KB	511 KB	835 KB	1.5 MB		
50 k	287 KB	388 KB	589 KB	991 KB	1.8 MB	3.4 MB		
100 k	387 KB	588 KB	989 KB	1.8 MB	3.4 MB	6.6 MB		
200 k	587 KB	988 KB	1.8 MB	3.4 MB	6.6 MB	13 MB		
500 k	1.2 MB	2.2 MB	4.2 MB	8.2 MB	16.2 MB	32.2 MB		
1 M	2.2 MB	4.2 MB	8.2 MB	16.2 MB	32.2 MB	64.2 MB		
2 M	4.2 MB	8.2 MB	16.2 MB	32.2 MB	64.2 MB	128.2 MB		
5 M	10.2 MB	20.2 MB	40.2 MB	80.2 MB	160.2 MB	320.2 MB		
10 M	20.2 MB	40.2 MB	80.2 MB	160.2 MB	320.2 MB	640.2 MB		
20 M	40.2 MB	80.2 MB	160.2 MB	320.2 MB	640.2 MB	1.28 GB		
50 M	100.2 MB	200.2 MB	400.2 MB	800.2 MB	1.6 GB	_		
100 M	200.2 MB	400.2 MB	800.2 MB	1.6 GB	_	_		
200 M	400.2 MB	800.2 MB	1.6 GB	_	-	_		
500 M	1 GB	2 GB	_	_	_	_		
1 G	2 GB	-	-	_				

• These sizes are of files that contain data acquired using analog channels (other than Model MR8990) and can be used only as a reference. Any number of logic channels on one module occupies one channel; one analog channel (Model MR8990) and one real-time calculation channel occupies two channels each.

 The instrument divides files with a size that exceeds 512 MB into multiple files of about 512 MB each to save them (except when the memory division is enabled).

REC file size (waveforms acquired by using the envelope)

(REC file size) = (Setting part size) + (Data part size)

(Setting part size) = 187392 + 512 × [(Number of analog channels) + 4 × (Number of logic channels) + (Number of real-time calculation channels)]

(Data part size) = $\{2 \times [(Number of analog channels other than Model MR8990)\}$

+ (Number of logic modules)] + 4 × [(Number of Model MR8990 channels)

+ (Number of real-time calculation channels)]] × (Number of data points) × 2

Recording	Number of channels used								
length (Points)	1	2	4	8	16	32			
2.5 k	197 KB	208 KB	229 KB	271 KB	355 KB	523 KB			
5 k	207 KB	228 KB	269 KB	351 KB	515 KB	843 KB			
10 k	227 KB	268 KB	349 KB	511 KB	835 KB	1.5 MB			
20 k	267 KB	348 KB	509 KB	831 KB	1.5 MB	2.8 MB			
50 k	387 KB	588 KB	989 KB	1.8 MB	3.4 MB	6.6 MB			
100 k	587 KB	988 KB	1.8 MB	3.4 MB	6.6 MB	13 MB			
200 k	987 KB	1.8 MB	34 MB	6.6 MB	13 MB	25.8 MB			
500 k	2.2 MB	4.2 MB	8.2 MB	16.2 MB	32.2 MB	64.2 MB			
1 M	4.2 MB	8.2 MB	16.2 MB	32.2 MB	64.2 MB	128.2 MB			
2 M	8.2 MB	16.2 MB	32.2 MB	64.2 MB	128.2 MB	256.2 MB			
5 M	20.2 MB	40.2 MB	80.2 MB	160.2 MB	320.2 MB	640.2 MB			
10 M	40.2 MB	80.2 MB	160.2 MB	320.2 MB	640.2 MB	1.28 GB			
20 M	80.2 MB	160.2 MB	320.2 MB	640.2 MB	1.28 GB	_			
50 M	200.2 MB	400.2 MB	800.2 MB	1.6 GB	_	_			
100 M	400.2 MB	800.2 MB	1.6 GB	_	-	-			
200 M	800.2 MB	1.6 GB	_	_	_	-			
500 M	2 GB	_	_	_	_	-			

• These sizes are of files that contain data acquired using analog channels (other than Model MR8990) and can be used only as a reference. Any number of logic channels on one module occupies one channel; one analog channel (Model MR8990) and one real-time calculation channel occupies two channels each.

• The instrument divides files with a size that exceeds 512 MB into multiple files of about 512 MB each to save them (except when the memory division is enabled).

Waveform (text) file size

Size of files that contain data acquired without using the envelope

(Text file size) = (Header part size) + (Data part size) (Header part size) = (About 14 KB at a maximum) (varies depending on the setting condition) (Data part size) = [24 + 14 × (Number of analog channels) + 32 × (Number of logic modules) + 14 × (Number of real-time calculation channels)] × (Number of data points)

Recording	Number of channels used							
length (Points)	1	2	4	8	16	32		
2.5 k	235 KB	270 KB	340 KB	480 KB	760 KB	1.4 MB		
5 k	330 KB	400 KB	540 KB	820 KB	1.4 MB	2.5 MB		
10 k	520 KB	660 KB	940 KB	1.5 MB	2.7 MB	4.9 MB		
20 k	900 KB	1.2 MB	1.8 MB	2.9 MB	5.1 MB	9.6 MB		
50 k	2 MB	2.8 MB	4.2 MB	7 MB	12.6 MB	23.8 MB		
100 k	4 MB	5.4 MB	8.2 MB	13.8 MB	25 MB	47.4 MB		
200 k	7.8 MB	10.6 MB	16.2 MB	27.4 MB	49.8 MB	94.6 MB		
500 k	19.2 MB	26.2 MB	40.2 MB	68.2 MB	124.2 MB	236.2 MB		
1 M	38.2 MB	52.2 MB	80.2 MB	136.2 MB	248.2 MB	472.2 MB		
2 M	76.2 MB	104.2 MB	160.2 MB	272.2 MB	496.2 MB	944.2 MB		
5 M	190.2 MB	260.2 MB	400.2 MB	680.2 MB	1.24 GB	2.36 GB		
10 M	380.2 MB	520.2 MB	800.2 MB	1.36 GB	2.48 GB	4.72 GB		
20 M	760.2 MB	1.04 GB	1.6 GB	2.72 GB	4.96 GB	9.44 GB		
50 M	1.9 GB	2.6 GB	4 GB	6.8 GB	12.4 GB	_		
100 M	3.8 GB	5.2 GB	8 GB	13.6 GB	_	_		
200 M	7.6 GB	10.4 GB	16 GB	_	_	_		
500 M	19 GB	26 GB	_	_	_	_		
1 G	38 GB	_	_	_	_	_		

• These sizes are of files that contain data acquired using analog channels (other than Model MR8990) and can be used only as a reference.

• Depending on the setting conditions, the size may slightly differ from those provided in the above table. Allow 20% of the size provided in the above table for margin.

• The instrument divides files with a size that exceeds 512 MB into multiple files of about 512 MB each to save them.

Size of files that contain acquired by using the envelope

(Text file size) = (Header part size) + (Data part size)

(Header part size) = (About 14 KB at a maximum) (varies depending on the setting condition) (Data part size) = 24 + [14 × (Number of analog channels) + 32 × (Number of logic modules) + 14 × (Number of real-time calculation channels) × 2] × (Number of data points)

Recording	Number of channels used							
length (Points)	1	2	4	8	16	32		
2.5 k	270 KB	340 KB	480 KB	760 KB	1.4 MB	2.5 MB		
5 k	400 KB	540 KB	820 KB	1.4 MB	2.5 MB	4.8 MB		
10 k	660 KB	940 KB	1.5 MB	2.7 MB	4.9 MB	9.4 MB		
20 k	1.2 MB	1.8 MB	2.9 MB	5.1 MB	9.6 MB	18.6 MB		
50 k	2.8 MB	4.2 MB	7 MB	12.6 MB	23.8 MB	46.2 MB		
100 k	5.4 MB	8.2 MB	13.8 MB	25 MB	47.4 MB	92.2 MB		
200 k	10.6 MB	16.2 MB	27.4 MB	49.8 MB	94.6 MB	184.2 MB		
500 k	26.2 MB	40.2 MB	68.2 MB	124.2 MB	236.2 MB	460.2 MB		
1 M	52.2 MB	80.2 MB	136.2 MB	248.2 MB	472.2 MB	920.2 MB		
2 M	104.2 MB	160.2 MB	272.2 MB	496.2 MB	944.2 MB	1.84 GB		
5 M	260.2 MB	400.2 MB	680.2 MB	1.24 GB	2.36 GB	4.6 GB		
10 M	520.2 MB	800.2 MB	1.36 GB	2.48 GB	4.72 GB	9.2 GB		
20 M	1.04 GB	1.6 GB	2.72 GB	4.96 GB	9.44 GB	_		
50 M	2.6 GB	4 GB	6.8 GB	12.4 GB	-	_		
100 M	5.2 GB	8 GB	13.6 GB	_	-	_		
200 M	10.4 GB	16 GB	-	-	-	-		
500 M	26 GB	-	-	-	-	-		

• These sizes are of files that contain data acquired using analog channels (other than Model MR8990) and can be used only as a reference.

• Depending on the setting conditions, the size may slightly differ from those provided in the above table. Allow 20% of the size provided in the above table for margin.

 The instrument divides files with a size that exceeds 512 MB into multiple files of about 512 MB each to save them.

Maximum recordable time when the real-time saving is enabled (values for reference purposes)

The maximum recordable time is expressed in the following equation.

(Maximum recordable time) = [(Recording capacity) × (Sampling time)] ÷
[(Number of channels used) × 2]
(Number of channels used) = [(Number of analog channels other than Model MR8990)
+ (Number of logic modules) + (Number of Model MR8990 channels)] × 2
+ (Number of real-time calculation channels) × 2

The maximum recordable times for saving data to each storage device are shown in the following table (assume that each storage device is empty). Since no capacity of the header of a waveform file is included, use about 90% of the recordable time provided in the table as a reference. Some conditions allow a long-term recordable time (1 year or more, shaded areas in the tables) to be set; however, the operation cannot be guaranteed because the warranty period or product life may disturb it.

For saving data acquired without using the envelope on Model U8332 SSD Unit

Sampling	Number of channels used							
rate	2	4	8	16	32			
20 MS/s	53 min 20 s	-	-	-	-			
10 MS/s	1 h 46 min 40 s	53 min 20 s	-	-	-			
5 MS/s	3 h 33 min 20 s	1 h 46 min 40 s	53 min 20 s	-	-			
2 MS/s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s	1 h 6 min 40 s	-			
1 MS/s	17 h 46 min 40 s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s	1 h 6 min 40 s			
500 kS/s	1 d 11 h 33 min 20 s	17 h 46 min 40 s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s			
200 kS/s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s	11 h 6 min 40 s	5 h 33 min 20 s			
100 kS/s	7 d 9 h 46 min 40 s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s	11 h 6 min 40 s			
50 kS/s	14 d 19 h 33 min 20 s	7 d 9 h 46 min 40 s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s			
20 kS/s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9 d 6 h 13 min 20 s	4 d 15 h 6 min 40 s	2 d 7 h 33 min 20 s			
10 kS/s	74 d 1 h 46 min 40 s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9 d 6 h 13 min 20 s	4 d 15 h 6 min 40 s			
5 kS/s	148 d 3 h 33 min 20 s	74 d 1 h 46 min 40 s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9 d 6 h 13 min 20 s			
2 kS/s	370 d 8 h 53 min 20 s	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s	46 d 7 h 6 min 40 s	23 d 3 h 33 min 20 s			
1 kS/s	740 d 17 h 46 min 40 s	370 d 8 h 53 min 20 s	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s	46 d 7 h 6 min 40 s			
500 S/s	1481 d 11 h 33 min 20 s	740 d 17 h 46 min 40 s	370 d 8 h 53 min 20 s	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s			
200 S/s	3703 d 16 h 53 min 20 s	1851 d 20 h 26 min 40 s	925 d 22 h 13 min 20 s	462 d 23 h 6 min 40 s	231 d 11 h 33 min 20 s			
100 S/s	7407 d 9 h 46 min 40 s	3703 d 16 h 53 min 20 s	1851 d 20 h 26 min 40 s	925 d 22 h 13 min 20 s	462 d 23 h 6 min 40 s			
50 S/s	10000 d	7407 d 9 h 46 min 40 s	3703 d 16 h 53 min 20 s	1851 d 20 h 26 min 40 s	925 d 22 h 13 min 20 s			
20 S/s	10000 d	10000 d	9259 d 6 h 13 min 20 s	4629 d 15 h 6 min 40 s	2314 d 19 h 33 min 20 s			
10 S/s	10000 d	10000 d	10000 d	9259 d 6 h 13 min 20 s	4629 d 15 h 6 min 40 s			
5 S/s	10000 d	10000 d	10000 d	10000 d	9259 d 6 h 13 min 20 s			
2 S/s	10000 d							
1 S/s	10000 d							

d: days, h: hours, min: minutes, s: seconds

For saving data acquired without using the envelope on Model U8333 HD Unit

d: days, h: hours, min: minutes, s: seconds

Sampling	Number of channels used							
rate	2	4	8	16	32			
10 MS/s	2 h 12 min 48 s	_	-	-	-			
5 MS/s	4 h 25 min 36 s	2 h 12 min 48 s	_	_	-			
2 MS/s	11 h 4 min 0 s	5 h 32 min 0 s	2 h 46 min 0 s	-	-			
1 MS/s	22 h 8 min 1 s	11 h 4 min 0 s	5 h 32 min 0 s	2 h 46 min 0 s	-			
500 kS/s	1 d 20 h 16 min 3 s	22 h 8 min 1 s	11 h 4 min 0 s	5 h 32 min 0 s	2 h 46 min 0 s			
200 kS/s	4 d 14 h 40 min 8 s	2 d 7 h 20 min 4 s	1 d 3 h 40 min 2 s	13 h 50 min 1 s	6 h 55 min 0 s			
100 kS/s	9 d 5 h 20 min 17 s	4 d 14 h 40 min 8 s	2 d 7 h 20 min 4 s	1 d 3 h 40 min 2 s	13 h 50 min 1 s			
50 kS/s	18 d 10 h 40 min 35 s	9 h 20 min 17 s	4 d 14 h 40 min 8 s	2 d 7 h 20 min 4 s	1 d 3 h 40 min 2 s			
20 kS/s	46 d 2 h 41 min 29 s	23 d 1 h 20 min 44 s	11 d 12 h 40 min 22 s	5 d 18 h 20 min 11 s	2 d 21 h 10 min 5 s			
10 kS/s	92 d 5 h 22 min 59 s	46 d 2 h 41 min 29 s	23 d 1 h 20 min 44 s	11 d 12 h 40 min 22 s	5 d 18 h 20 min 11 s			
5 kS/s	184 d 10 h 45 min 59 s	92 d 5 h 22 min 59 s	46 d 2 h 41 min 29 s	23 d 1 h 20 min 44 s	11 d 12 h 40 min 22 s			
2 kS/s	461 d 2 h 54 min 57 s	230 d 13 h 27 min 28 s	115 d 6 h 43 min 44 s	57 d 15 h 21 min 52 s	28 d 19 h 40 min 56 s			
1 kS/s	922 d 5 h 49 min 55 s	461 d 2 h 54 min 57 s	230 d 13 h 27 min 28 s	115 d 6 h 43 min 44 s	57 d 15 h 21 min 52 s			
500 S/s	1844 d 11 h 39 min 50 s	922 d 5 h 49 min 55 s	461 d 2 h 54 min 57 s	230 d 13 h 27 min 28 s	115 d 6 h 43 min 44 s			
200 S/s	4611 d 5 h 9 min 35 s	2305 d 14 h 34 min 47 s	1152 d 19 h 17 min 23 s	576 d 9 h 38 min 41 s	288 d 4 h 49 min 20 s			
100 S/s	9222 d 10 h 19 min 10 s	4611 d 5 h 9 min 35 s	2305 d 14 h 34 min 47 s	1152 d 19 h 17 min 23 s	576 d 9 h 38 min 41 s			
50 S/s	10000 d	9222 d 10 h 19 min 10 s	4611 d 5 h 9 min 35 s	2305 d 14 h 34 min 47 s	1152 d 19 h 17 min 23 s			
20 S/s	10000 d	10000 d	10000 d	5764 d 0 h 26 min 59 s	2882 d 0 h 13 min 29 s			
10 S/s	10000 d	10000 d	10000 d	10000 d	5764 d 0 h 26 min 59 s			
5 S/s	10000 d							
2 S/s	10000 d							
1 S/s	10000 d							

For saving data acquired without using the envelope on Model Z4006 USB Drive

d: days, h: hours, min: minutes, s: seconds

Sampling	Number of channels used							
rate	2	4	8	16	32			
5 MS/s	13 min 25 s	-	-	_	-			
2 MS/s	33 min 32 s	16 min 46 s	_	_	-			
1 MS/s	1 h 7 min 5 s	33 min 32 s	16 min 46 s	_	-			
500 kS/s	2 h 14 min 10 s	1 h 7 min 5 s	33 min 32 s	16 min 46 s	_			
200 kS/s	5 h 35 min 26 s	2 h 47 min 43 s	1 h 23 min 51 s	41 min 55 s	20 min 57 s			
100 kS/s	11 h 10 min 53 s	5 h 35 min 26 s	2 h 47 min 43 s	1 h 23 min 51 s	41 min 55 s			
50 kS/s	22 h 21 min 47 s	11 h 10 min 53 s	5 h 35 min 26 s	2 h 47 min 43 s	1 h 23 min 51 s			
20 kS/s	2 d 7 h 54 min 28 s	1 d 3 h 57 min 14 s	13 h 58 min 37 s	6 h 59 min 18 s	3 h 29 min 39 s			
10 kS/s	4 d 15 h 48 min 57 s	2 d 7 h 54 min 28 s	1 d 3 h 57 min 14 s	13 h 58 min 37 s	6 h 59 min 18 s			
5 kS/s	9 d 7 h 37 min 55 s	4 d 15 h 48 min 57 s	2 d 7 h 54 min 28 s	1 d 3 h 57 min 14 s	13 h 58 min 37 s			
2 kS/s	23 d 7 h 4 min 49 s	11 d 15 h 32 min 24 s	5 d 19 h 46 min 12 s	2 d 21 h 53 min 6 s	1 d 10 h 56 min 33 s			
1 kS/s	46 d 14 h 9 min 38 s	23 d 7 h 4 min 49 s	11 d 15 h 32 min 24 s	5 d 19 h 46 min 12 s	2 d 21 h 53 min 6 s			
500 S/s	93 d 4 h 19 min 17 s	46 d 14 h 9 min 38 s	23 d 7 h 4 min 49 s	11 d 15 h 32 min 24 s	5 d 19 h 46 min 12 s			
200 S/s	232 d 22 h 48 min 14 s	116 d 11 h 24 min 7 s	58 d 5 h 42 min 3 s	29 d 2 h 51 min 1 s	14 d 13 h 25 min 30 s			
100 S/s	465 d 21 h 36 min 28 s	232 d 22 h 48 min 14 s	116 d 11 h 24 min 7 s	58 d 5 h 42 min 3 s	29 d 2 h 51 min 1 s			
50 S/s	931 d 19 h 12 min 56 s	465 d 21 h 36 min 28 s	232 d 22 h 48 min 14 s	116 d 11 h 24 min 7 s	58 d 5 h 42 min 3 s			
20 S/s	2329 d 12 h 2 min 20 s	1164 d 18 h 1 min 10 s	582 d 9 h 0 min 35 s	291 d 4 h 30 min 17 s	145 d 14 h 15 min 8 s			
10 S/s	4659 d 0 h 4 min 41 s	2329 d 12 h 2 min 20 s	1164 d 18 h 1 min 10 s	582 d 9 h 0 min 35 s	291 d 4 h 30 min 17 s			
5 S/s	9318 d 0 h 9 min 23 s	4659 d 0 h 4 min 41 s	2329 d 12 h 2 min 20 s	1164 d 18 h 1 min 10 s	582 d 9 h 0 min 35 s			
2 S/s	10000 d	10000 d	5823 d 18 h 5 min 52 s	2911 d 21 h 2 min 56 s	1455 d 22 h 31 min 28 s			
1 S/s	10000 d	10000 d	10000 d	5823 d 18 h 5 min 52 s	2911 d 21 h 2 min 56 s			

• When saving data in Model Z4003 SD memory card, consider the recordable time to be about half the time provided in the above table as a reference.

• When saving data in Model Z4001 SD memory card, consider the recording to be about 1/8 of the time provided in the above table as a reference.

For saving data acquired by using the envelope on Model U8332 SSD Unit

d: days, h: hours, min: minutes, s: seconds

Sampling	Number of channels used						
rate	2	4	8	16	32		
10 MS/s	53 min 20 s	-	_	-	-		
5 MS/s	1 h 46 min 40 s	53 min 20 s	_	-	-		
2 MS/s	4 h 26 min 40 s	2 h 13 min 20 s	1 h 6 min 40 s	-	-		
1 MS/s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s	1 h 6 min 40 s	-		
500 kS/s	17 h 46 min 40 s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s	1 h 6 min 40 s		
200 kS/s	1 d 20 h 26 min 40 s	22 h 13 min 20 s	11 h 6 min 40 s	5 h 33 min 20 s	2 h 46 min 40 s		
100 kS/s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s	11 h 6 min 40 s	5 h 33 min 20 s		
50 kS/s	7 d 9 h 46 min 40 s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s	11 h 6 min 40 s		
20 kS/s	18 d 12 h 26 min 40 s	9 d 6 h 13 min 20 s	4 d 15 h 6 min 40 s	2 d 7 h 33 min 20 s	1 d 3 h 46 min 40 s		
10 kS/s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9 d 6 h 13 min 20 s	4 d 15 h 6 min 40 s	2 d 7 h 33 min 20 s		
5 kS/s	74 d 1 h 46 min 40 s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9 d 6 h 13 min 20 s	4 d 15 h 6 min 40 s		
2 kS/s	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s	46 d 7 h 6 min 40 s	23 d 3 h 33 min 20 s	11 d 13 h 46 min 40 s		
1 kS/s	370 d 8 h 53 min 20 s	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s	46 d 7 h 6 min 40 s	23 d 3 h 33 min 20 s		
500 S/s	740 d 17 h 46 min 40 s	370 d 8 h 53 min 20 s	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s	46 d 7 h 6 min 40 s		
200 S/s	1851 d 20 h 26 min 40 s	925 d 22 h 13 min 20 s	462 d 23 h 6 min 40 s	231 d 11 h 33 min 20 s	115 d 17 h 46 min 40 s		
100 S/s	3703 d 16 h 53 min 20 s	1851 d 20 h 26 min 40 s	925 d 22 h 13 min 20 s	462 d 23 h 6 min 40 s	231 d 11 h 33 min 20 s		
50 S/s	7407 d 9 h 46 min 40 s	3703 d 16 h 53 min 20 s	1851 d 20 h 26 min 40 s	925 d 22 h 13 min 20 s	462 d 23 h 6 min 40 s		
20 S/s	10000 d	9259 d 6 h 13 min 20 s	4629 d 15 h 6 min 40 s	2314 d 19 h 33 min 20 s	1157 d 9 h 46 min 40 s		
10 S/s	10000 d	10000 d	9259 d 6 h 13 min 20 s	4629 d 15 h 6 min 40 s	2314 d 19 h 33 min 20 s		
5 S/s	10000 d	10000 d	10000 d	9259 d 6 h 13 min 20 s	4629 d 15 h 6 min 40 s		
2 S/s	10000 d						
1 S/s	10000 d						
30 S/min	10000 d						
12 S/min	10000 d						
6 S/min	10000 d						
2 S/min	10000 d						
1 S/min	10000 d						

For saving data acquired by using the envelope on Model U8333 HD Unit

d: days, h: hours, min: minutes, s: seconds

Sampling		Nui	nber of channels us	ed	
rate	2	4	8	16	32
5 MS/s	2 h 12 min 48 s	-	-	-	-
2 MS/s	5 h 32 min 0 s	2 h 46 min 0 s	_	_	-
1 MS/s	11 h 4 min 0 s	5 h 32 min 0 s	2 h 46 min 0 s	-	-
500 kS/s	22 h 8 min 1 s	11 h 4 min 0 s	5 h 32 min 0 s	2 h 46 min 0 s	-
200 kS/s	2 d 7 h 20 min 4 s	1 d 3 h 40 min 2 s	13 h 50 min 1 s	6 h 55 min 0 s	3 h 27 min 30 s
100 kS/s	4 d 14 h 40 min 8 s	2 d 7 h 20 min 4 s	1 d 3 h 40 min 2 s	13 h 50 min 1 s	6 h 55 min 0 s
50 kS/s	9 d 5 h 20 min 17 s	4 d 14 h 40 min 8 s	2 d 7 h 20 min 4 s	1 d 3 h 40 min 2 s	13 h 50 min 1 s
20 kS/s	23 d 1 h 20 min 44 s	11 d 12 h 40 min 22 s	5 d 18 h 20 min 11 s	2 d 21 h 10 min 5 s	1 d 10 h 35 min 2 s
10 kS/s	46 d 2 h 41 min 29 s	23 d 1 h 20 min 44 s	11 d 12 h 40 min 22 s	5 d 18 h 20 min 11 s	2 d 21 h 10 min 5 s
5 kS/s	92 d 5 h 22 min 59 s	46 d 2 h 41 min 29 s	23 d 1 h 20 min 44 s	11 d 12 h 40 min 22 s	5 d 18 h 20 min 11 s
2 kS/s	230 d 13 h 27 min 28 s	115 d 6 h 43 min 44 s	57 d 15 h 21 min 52 s	28 d 19 h 40 min 56 s	14 d 9 h 50 min 28 s
1 kS/s	461 d 2 h 54 min 57 s	230 d 13 h 27 min 28 s	115 d 6 h 43 min 44 s	57 d 15 h 21 min 52 s	28 d 19 h 40 min 56 s
500 S/s	922 d 5 h 49 min 55 s	461 d 2 h 54 min 57 s	230 d 13 h 27 min 28 s	115 d 6 h 43 min 44 s	57 d 15 h 21 min 52 s
200 S/s	2305 d 14 h 34 min 47 s	1152 d 19 h 17 min 23 s	576 d 9 h 38 min 41 s	288 d 4 h 49 min 20 s	144 d 2 h 24 min 40 s
100 S/s	4611 d 5 h 9 min 35 s	2305 d 14 h 34 min 47 s	1152 d 19 h 17 min 23 s	576 d 9 h 38 min 41 s	288 d 4 h 49 min 20 s
50 S/s	9222 d 10 h 19 min 10 s	4611 d 5 h 9 min 35 s	2305 d 14 h 34 min 47 s	1152 d 19 h 17 min 23 s	576 d 9 h 38 min 41 s
20 S/s	10000 d	10000 d	5764 d 0 h 26 min 59 s	2882 d 0 h 13 min 29 s	1441 d 0 h 6 min 44 s
10 S/s	10000 d	10000 d	10000 d	5764 d 0 h 26 min 59 s	2882 d 0 h 13 min 29 s
5 S/s	10000 d	10000 d	10000 d	10000 d	5764 d 0 h 26 min 59 s
2 S/s	10000 d	10000 d	10000 d	10000 d	10000 d
1 S/s	10000 d	10000 d	10000 d	10000 d	10000 d
30 S/min	10000 d	10000 d	10000 d	10000 d	10000 d
12 S/min	10000 d	10000 d	10000 d	10000 d	10000 d
6 S/min	10000 d	10000 d	10000 d	10000 d	10000 d
2 S/min	10000 d	10000 d	10000 d	10000 d	10000 d
1 S/min	10000 d	10000 d	10000 d	10000 d	10000 d

For saving data acquired by using the envelope on Model Z4006 USB Drive

d: days, h: hours, min: minutes, s: seconds

Sampling	pling Number of channels used									
rate	2	4	8	16	32					
2 MS/s	17 m 53 s	-	-	-	_					
1 MS/s	35 m 47 s	17 m 53 s	-	-	-					
500 kS/s	1 h 11 m 34 s	53 m 47 s	17 m 53 s	-	_					
200 kS/s	2 h 58 m 57 s	1 h 29 m 28 s	44 m 44 s	22 m 22 s	-					
100 kS/s	5 h 57 m 54 s	2 h 58 m 57 s	1 h 29 m 28 s	44 m 44 s	22 m 22 s					
50 kS/s	11 h 55 m 49 s	5 h 57 m 54 s	2 h 58 m 57 s	1 h 29 m 28s	44 m 44 s					
20 kS/s	1 d 5 h 49 m 34 s	14 h 54 m 47 s	7 h 27 m 23 s	3 h 43 m 41 s	1 h 51 m 50 s					
10 kS/s	2 d 11 h 39 m 8 s	1 d 5 h 49 m 34 s	14 h 54 m 47 s	7 h 27 m 23 s	3h 43 m 41 s					
5 kS/s	4d23h18m16s	2 d 11 h 39 m 8 s	1 d 5 h 49 m 34 s	14 h 54 m 47 s	7 h 27 m 23 s					
2 kS/s	12d10h15m41s	6 d 5 h 7 m 50 s	3 d 2 h 33 m 55 s	1 d 13 h 16 m 57 s	18 h 38 m 28 s					
1 kS/s	24 d 20 h 31 m 23 s	12 d 10 h 15 m 41 s	6 d 5 h 7 m 50 s	3 d 2 h 33 m 55 s	1 d 13 h 16 m 57 s					
500 S/s	49 d 17 h 2 m 47 s	24 d 20 h 31 m 23 s	12d10h15m41s	6 d 5 h 7 m 50 s	3 d 2 h 33 m 55 s					
200 S/s	124 d 6 h 36 m 58 s	62 d 3 h 18 m 29 s	31 d 1 h 39 m 14 s	15 d 12 h 49 m 37 s	7 d 18 h 24 m 48 s					
100 S/s	248 d 13 h 13 m 56 s	124 d 6 h 36 m 58 s	62 d 3 h 18 m 29 s	31 d 1 h 39 m 14 s	15 d 12 h 49 m 37 s					
50 S/s	497 d 2 h 27 m 52 s	248 d 13 h 13 m 56 s	124 d 6 h 36 m 58 s	62 d 3 h 18 m 29 s	31 d 1 h 39 m 14 s					
20 S/s	1242 d 18 h 9 m 42 s	621 d 9 h 4 m 51 s	310 d 16 h 32 m 25 s	155 d 8 h 16 m 12 s	77 d 16 h 8 m 6 s					
10 S/s	2485 d 12 h 19 m 24 s	1242 d 18 h 9 m 42 s	621 d 9 h 4 m 51 s	310 d 16 h 32 m 25 s	155 d 8 h 16 m 12 s					
5 S/s	4971 d 0 h 38 m 49 s	2485 d 12 h 19 m 24 s	1242 d 18 h 9 m 42 s	621 d 9 h 4 m 51 s	310 d 16 h 32 m 25 s					
2 S/s	10000 d	6213 d 18 h 48 m 32 s	3106 d 21 h 24 m 16 s	1553 d 10 h 42 m 8 s	776 d 17 h 21 m 4 s					
1 S/s	10000 d	10000 d	6213 d 18 h 48 m 32 s	3106 d 21 h 24 m 16 s	1553 d 10 h 42 m 8 s					
30 S/min	10000 d	10000 d	10000 d	6213 d 18 h 48 m 32 s	3106 d 21 h 24 m 16 s					
12 S/min	10000 d	10000 d	10000 d	10000 d	7767 d 5 h 30 m 40 s					
6 S/min	10000 d	10000 d	10000 d	10000 d	10000 d					
2 S/min	10000 d	10000 d	10000 d	10000 d	10000 d					
1 S/min	10000 d	10000 d	10000 d	10000 d	10000 d					

• When saving data in Model Z4003 SD memory card, consider the recordable time to be about 1/2 of the time provided in the above table as a reference.

• When saving data in Model Z4001 SD memory card, consider the recording to be about 1/8 of the time provided in the above table as a reference.

Scaling method for strain gauges

This section describes how to determine the scaling conversion ratio when measurement is performed with strain gauges and Model U8969 Strain Unit.

The appropriate conversion equation into stress varies depending on how the strain gauges are used.

Three methods are available: the 1-gauge (for a gauge), 2-gauge (for two gauges), and 4-gauge methods (for four gauges). The 2-gauge method is used for strain measurement involving temperature compensation.

E: Young's modulus, v: Poisson's ratio, ɛ: Measured strain value

Measuring tensile and compressive stress: Stress (σ) = E × ϵ

When 2- or 4-gauge method measurement is performed involving temperature compensation, position the gauges perpendicularly to each other.

The stress (σ) is multiplied by 1 / (1 + ν) for the 2-gauge method, and 1 / [2 (1 + ν)] for the 4-gauge method.

Measuring bending stress: Stress (σ) = E × ϵ

When 2- or 4-gauge measurement is performed involving temperature compensation, the stress (σ) is multiplied by 1/2 or 1/4, respectively.

Measuring torsional stress: Stress (σ) = E / [2 (1 + v)] × ϵ (2-gauge method)

When the 4-gauge method is used, the stress is halved.

See the instruction manual of the strain gauge for how to combine strain gauges for each measurement.

Example: Measuring compressive stress Using the 1-gauge method, material of measured object: aluminum, Young's modulus: 73 (GPa) (See the table below.)

- $\sigma = 73 \times 10^9 \times$ (Measured value) × 10⁻⁶ (unit of measured value: $\mu\epsilon$)
- = 73 × (Measured value) (unit: kPa)

= $7.44^* \times (Measured value) (unit: gf/mm^2)$

*: 1 Pa = $1.01971621 \times 10^{-7}$ kgf/mm² = 1 N/m²

Conversion ratio: 7.44, unit: gf/mm² Enter this value as the scaling conversion ratio.

Mechanical properties of industrial materials

Material	Modulus of longitudinal elasticity (Young's modulus)	Poisson's ratio					
	E (GPa)	ν					
Carbon steel (Carbon content: 0.1% to 0.25%)	205	0.28 to 0.3					
Carbon steel (Carbon content: 0.25% or more)	206	0.28 to 0.3					
Spring steel (Quenched)	206 to 211	0.28 to 0.3					
Nickel steel	205	0.28 to 0.3					
Cast iron	98	0.2 to 0.29					
Brass (Cast)	78	0.34					
Phosphor bronze	118	0.38					
Aluminum	73	0.34					
Concrete	20 to 29	0.1					

See "3.2 Converting Input Values (Scaling Function)" (p. 56).

Example of a waveform text file

The waveform text file consists of a header and data. The header includes the following information:

- (1) Title comment
- (2) Recording length, sampling rate, trigger time
- (3) Channel number, module type, measurement range, LPF, channel comment, scaling (setting, conversion ratio, offset), invert

Example of a saved file (data acquired without using the envelope)

"Title comment"(1)
"Rec length","Sampling","Trigger Time"
"2500 sample","1MS/s","17/09/20 16:42:07.044"
"Channel","Mode","Range(f.s.)","L.P.F.","Comment","Scaling","Ratio","Offset","Invert"
"CH1-1","VOLTAGE","10V","OFF","Analog 1-1","OFF","-","OFF"(3)
"CH1-2","VOLTAGE","100mV","OFF","Analog 1-2","OFF","-","-","OFF"
"CH2-1","K","200^cC","","Temperature 1","ON(SCI)","2.1568E+00","4.9874E+00","OFF"
"CH2-2","K","200^cC","","Temperature 2","OFF","-","-","ON"
"CH3-1","VOLTAGE","10V","","Digital Voltmeter Unit 3-1","ON(ENG)","2.4178E+00","1.0254E+01","OFF"
"CH3-2","VOLTAGE","10V","","Digital Voltmeter Unit 3-2","OFF","-","-","ON"
"L4 A1","-","-","4LA1","-","-","-","-"
"L4 A2","-","-","4LA2","-","-","-","-"
"L4 A3","-","-","4LA3","-","-","-","-"
"L4 A4","-","-","4LA4","-","-","-","-"
"Time[s]","CH1-1[V]","CH1-2[V]","CH2-1[^cC]","CH2-2[^cC]","CH3-1[V]","CH3-2[V]","L4A1","L4A2","L4A3","L4A4"
+0.00000000E+00,+1.510000E+00,-3.000000E-04,+3.997600E+02,+3.997600E+02,-9.997559E-03,-9.340576E-02,1,1,1,1
+1.00000000E-06,+1.510000E+00,-2.500000E-04,+3.997600E+02,+3.997600E+02,-9.997559E-03,-9.340576E-02,1,1,1,1
0.00000000E-06,+1.510000E+00,-3.000000E-04,+3.997600E+02,+3.997600E+02,-9.997559E-03,-9.340576E-02,1,1,1,1
+3.00000000E-06,+1.440000E+00,+3.500000E-04,+3.997600E+02,+3.997600E+02,-9.997559E-03,-9.340576E-02,1,1,1,1
+4.00000000E-06,+1.430000E+00,+2.000000E-04,+3.997600E+02,+3.997600E+02,-9.997559E-03,-9.340576E-02,1,1,1,1

File saving rates (values for reference purposes)

The instruments can save waveform binary files onto either of Hioki's optional storage devices or through LAN at the following saving rates:

. . .

Storage device	Saving rate (value for reference purposes)
Model U8332 SSD Unit	40 MB/s
Model U8333 HD Unit	20 MB/s
Model Z4006 USB Drive (using USB 3.0 connector)	12 MB/s
Model Z4006 USB Drive (using USB 2.0 connector)	10 MB/s
Z4001 SD Memory Card (2 GB)	12 MB/s
Z4003 SD Memory Card (8 GB)	20 MB/s
LAN (FTP client)	8 MB/s

• When saved files containing two channels of data, the instrument can save them at the rates on the table. As the number of channels increases, the size of a data set increases. Although saving the data set requires longer, the saving rate will increase because a more extensive data set can be transferred at once.


• When LAN is used, the saving rate is greatly impacted by connection conditions.

16.2 FFT Definitions

The FFT, which stands for fast Fourier transform, is an efficient method to compute the DFT (discrete Fourier transform) from a time-domain waveform. The reverse process of transforming frequency data obtained through the FFT into its original time-domain waveform is called the IFFT (Inverse FFT). The FFT function performs various analyses using FFT and IFFT.

Time and frequency domain considerations

All signals inputted to the instrument are functions of time. These functions can be considered as a combination of sine waves at various frequencies, such as in the following diagram. Although observing a signal only as a the time-domain waveform may be difficult to analyze, you can easily understand its characteristics by transforming it into a frequency-domain graph.

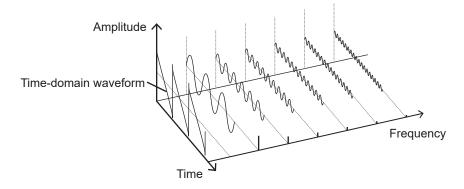

Discrete Fourier transform and inverse discrete Fourier transform

Let x(n) denote a discrete signal, X(k) denote its discrete Fourier transform (DFT), and N denote the number of calculation points. The relationships among them are as follows:


$$X(k) = DFT\{x(n)\} = \sum_{n=0}^{N-1} x(n)W_N^{kn} \qquad (1)$$
$$x(n) = IDFT\{X(k)\} = \frac{1}{N} \sum_{k=0}^{N-1} X(k)W_N^{-kn} \qquad (2)$$
$$W_N = \exp\left(-j\frac{2\pi}{N}\right) \qquad (3)$$

The discrete signal X(k) is typically a complex number, thus expression (1) can be transformed again and written as follows:

$$\phi(k) = \tan^{-1} \frac{\text{Im}\{X(k)\}}{\text{Re}\{X(k)\}} \dots (5)$$

|F(k)| : Altitude spectrum, $\phi(k)$: Phase spectrum

The above relationships are represented on the following complex plane.



Linear time-invariant system

Consider a linear time-invariant (LTI) system that produces a response y(n) to a discrete timedomain signal x(n).

The linear time-invariant system (hereafter referred to as LTI system) is a system in which the following expression holds for any integer *Ai* where the equation $y_i(n) = L[x_i(n)]$ is the response to $x_i(n)$.

 $L[A_1x_1(n) + A_2x_2(n)] = A_1y_1(n) + A_2y_2(n)....(6)$

Let h(n) denote a system function of the LTI system, the relationship between an input and output is given by the following expression.

$$y(n) = \sum_{m=0}^{\infty} h(m)x(n-m) = \sum_{m=-\infty}^{\infty} h(n-m)x(m) \dots (7)$$

Assign a unit impulse $\delta(n)$ (1 for n = 0, 0 for other numbers) to x(n), and the following expression holds.

y(n) = h(n).....(8)


Thus, applying the unit impulse to the input signal allows the LTI system characteristics to absolutely outputs. The response waveform of a system to a unit impulse is called the impulse response.

On the other hand, where the discrete Fourier transforms of x(n), y(n), and h(n) are X(k), Y(k), and H(k), respectively, expression (7) can be written as follows:

Y(k) = X(k)H(k).(9)

The function H(k) is also called the transfer function, which is calculated from X(k) and Y(k). Also, the inverse discrete Fourier transform function of H(k) is the unit impulse response h(n) of the LTI system.

The instrument calculates an impulse response and a transfer function using the relationships of expression (9).



Aliasing

When a measured signal oscillates at a higher frequency compared to the sampling rate you have chosen, the instrument may plot a false waveform oscillating lower than the actual signal with respect to a frequency once the signal frequency reaches a certain level. This phenomena, which occurs when a signal is sampled at a lower frequency than that defined by the Nyquist-Shannon sampling theorem, is called aliasing.


Let f_{max} denote the highest frequency component of an input signal, and f_s denote a sampling frequency. The following expression have to stand.


Thus, if the input includes frequency components higher than $f_s/2$, a lower frequency component folds higher frequency components, resulting in an occurrence of false frequency components.

The following figures show the results of spectrum analysis of composite waveforms that have components of 1 kHz and 3 kHz, and of 1 kHz and 7 kHz.

If the instrument samples a signal that has frequency components of above 5 kHz (in this case, 7 kHz) at the sampling frequency f_s of 10 kHz, folded spectral components of 5 kHz or lower are observed.

This example demonstrates that the difference between the 3 kHz and 7 kHz components is indistinguishable from one anther.

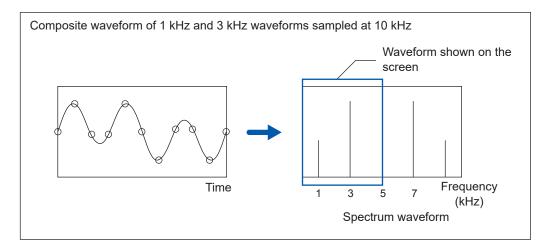


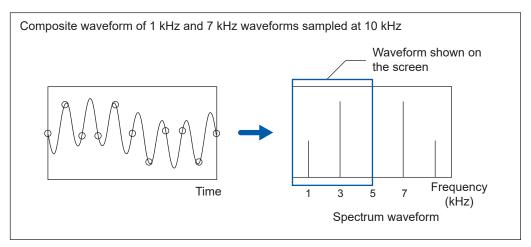


Anti-aliasing filter

An input signal causes aliasing if it includes the maximum frequency component higher than half the sampling frequency. Countermeasures against aliasing includes using a low-pass filter that eliminates frequency components higher than half the sampling frequency. This low-pass filter is called the anti-aliasing filter.

The figures below shows the effect of use of an anti-aliasing filter for a square wave input waveform.

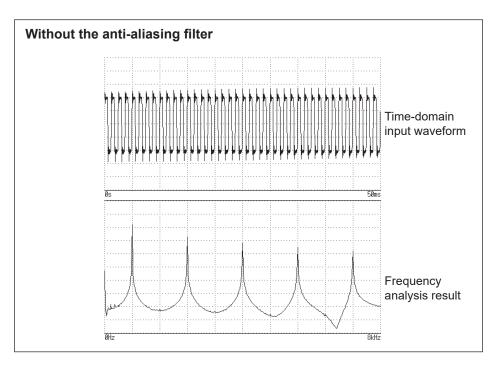


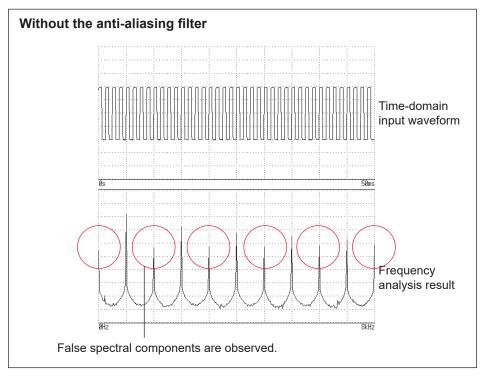


Imaging

If the instrument is configured with a frequency range that exceeds the maximum sampling frequency defined for each unit, multiple sampled data points will be arrayed and interpolated by creating intermediate data. In this case, the time-axis waveform will exhibit a stepped shape. If FFT analysis is performed under these conditions, spectra that do not actually exist will be observed at high frequencies. This phenomenon, known as imaging, is caused by 0-order hold characteristics.

The figure below depicts the time-axis waveform and spectra when a sine wave is applied to the 8968 High Resolution Unit.

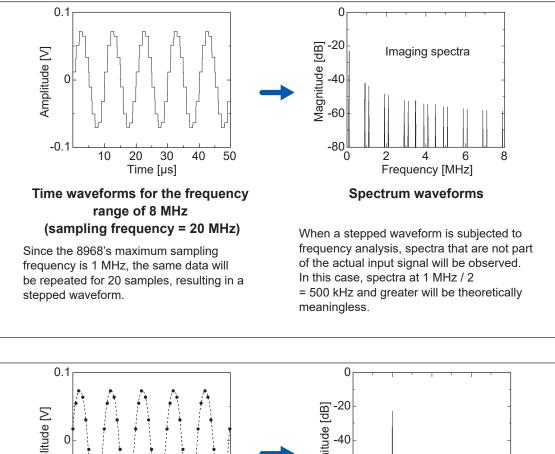

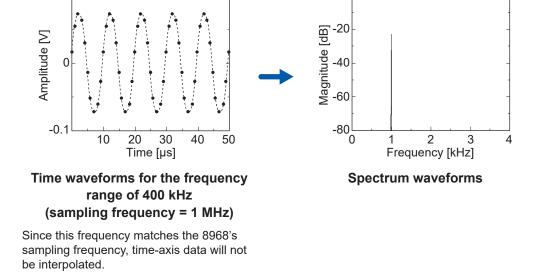

To prevent the imaging phenomenon when analyzing waveforms using the FFT function, be sure to check the unit's maximum sampling frequency prior to measurement.

16

Averaging

With the FFT function, averaging used the following expressions.

(1) Simple average

Add acquired data sets in series and divides the sum by a acquisition count.

 $A_n = \frac{(n-1)A_{n-1} + Z_n}{n}....(11)$

n: Acquisition count for averaging A_n : *n*th averaging result Z_n : *n*th waveform data set

(2) Exponential average

Calculates an weighted average such that newer data points contribute more than others.

N: Specified number of acquisition for averaging

n: Acquisition count for averaging $(n \ge 2)$

 A_n : *n*th averaging result ($A_1 = Z_1$)

 Z_n : *n*th waveform data set

Overall value

The overall value shows the sum of power spectra of each frequency. This value is nearly equal to the sum of the squares of an input signal (square of RMS value)(except when frequency averaging is performed). With the FFT function, the instrument displays RMS values for stored waveforms, or overall values for frequency-domain waveforms calculated using the sum of power spectra. Any FFT analysis modes other than the power spectrum, however, take the root square of the overall value to match the unit.

With the FFT analysis mode set to the power spectrum

$$(Over all) = \sum_{i=0} P_i$$
(13-1)

With the FFT analysis mode set to the histogram, linear spectrum, RMS spectrum, impulse response, 1/1 octave analysis, or 1/3 octave analysis

$$(Over all) = \sqrt{\sum_{i=0} P_i}$$
 (13-2)

 P_i : *i*th power spectrum

Total harmonic distortion factor (THD)

The total harmonic distortion factor (THD) indicates a percentage of the total harmonic to the fundamental.

The more severely the waveform distorts, the larger the value becomes.

THD =
$$\sqrt{\frac{\sum (V_n)^2}{(V_o)}} \times 100$$
 [%].....(14)


 V_0 : Fundamental wave V_n : *n*th order harmonic

Window function


The Fourier transform of a continuous system is defined to be the integral from negative infinity to positive infinity with respect to time as expression (15) provides.


$$X(f) = \int_{-\infty}^{\infty} x(t) \,\varepsilon^{-2\pi f t} dt \qquad (15)$$


However, since expression (15) cannot apply to actual measurement, a certain finite interval is used for calculation. Extracting a segment of a waveform is called window processing. The FFT function performs a calculation assuming that this finite interval of a waveform segment repeats periodically (as shown below).

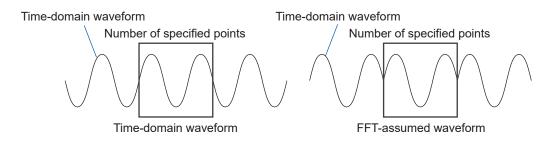

When the number of FFT calculation points is equal to an integer multiple of the input signal frequency, a single line spectrum is obtained. However, if the number is unequal to an integer multiple of the frequency (with the result that the FFT-assumed waveform has discontinuous points), spectral lines spread, resulting in failure of production of a line spectrum. This phenomenon is called the leakage error (as shown below).

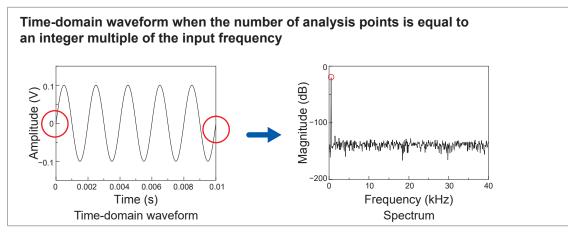



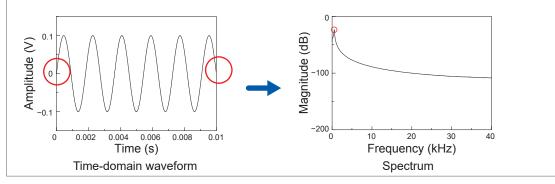


The window function has been created to suppress such leakage errors. The window function smoothly connects each cropped end of a time-domain waveform.

The following figure presents an example of spectral analysis of a time-domain waveform multiplied by a window function.

Multiplying the time-domain waveform by the window function eliminates discontinuous points on the waveform, obtaining the spectrum with a lobe similar to the line spectrum.


Waveform obtained by multiplying the above-described waveform ("Time-domain waveform when the number of analysis points is unequal to an integer multiple of the input frequency" (p. 415)) by Blackman Harris window

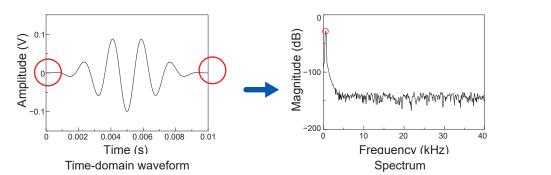


The following figure illustrate the time-domain waveform multiplied by the window function and its spectrum.

Each spectrum shows a highest peak at a low frequency, and many lower peaks at higher frequencies. The highest peak is called the main lobe, and the smaller peaks are the side lobes. A narrower width of the main lobe and lower lobes lead to accurate results of FFT analyses; however, the conditions are incompatible with one another. Thus, if you wish to emphasize altitudes, use a window function that has a wider main lobe. If you wish to observe spectra adjacent to each other, use a window function that has a narrower main lobe. If you wish to eliminate the effect of the adjacent spectra, use a window function that has smaller side lobe values.


Since the main lobe width is proportional to the width of the window (1/W), increasing the number of analysis points increases the frequency resolution.

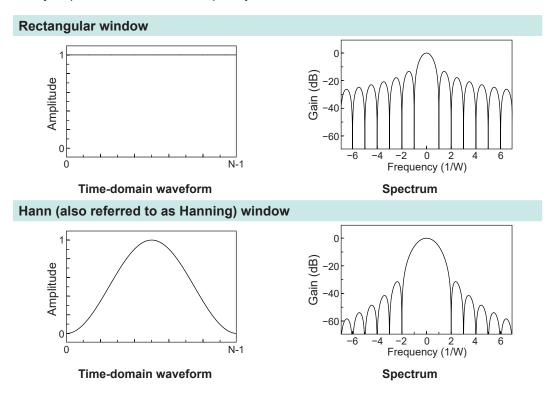

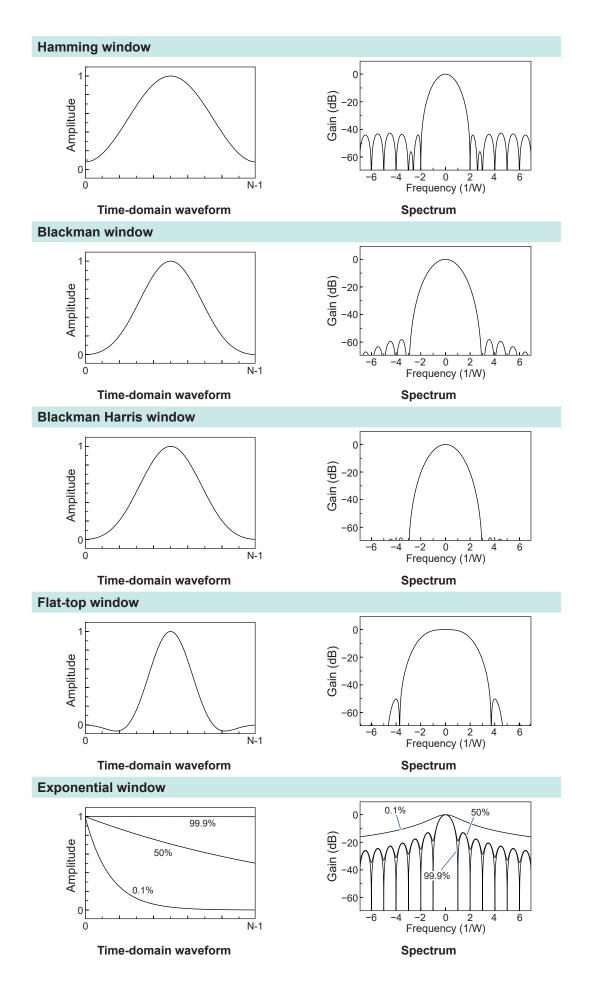

The following example shows the analyses of input sine waves, which has a frequency of 1050 Hz and 1150 Hz, with different window functions.

In this example, since the frequencies are close to each other, the rectangular window, which can yield a narrow main lobe, can separately display both frequencies; the Hann (also referred to as Hanning) window, however, which yields a wide main lobe, displays the two frequency component as a single component.

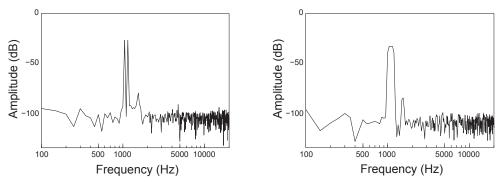

Analysis using the rectangular window

Analysis using the Hann window

16.3 Dual Sampling

Sampling speed combination that can be set

✓: Selectable, –: Not selectable

			Sampling speed for trend waveforms																									
		10 MS/s	5 MS/s	2 MS/s	1 MS/s	500 kS/s	200 kS/s	100 kS/s	50 kS/s	20 kS/s	10 kS/s	5 kS/s	2 kS/s	1 kS/s	500 S/s	200 S/s	100 S/s	50 S/s	20 S/s	10 S/s	5 S/s	2 S/s	1 S/s	30 S/min	12 S/min	6 S/min	2 S/min	1 S/min
	100 MS/s	✓	✓	✓	✓	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	✓	~
	50 MS/s	-	✓	_	✓	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	\checkmark
	20 MS/s	-	_	✓	✓	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	\checkmark
	10 MS/s	-	_	_	✓	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	✓	\checkmark
	5 MS/s	-	_	-	-	~	-	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	\checkmark
	2 MS/s	-	_	-	-	-	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	✓	✓	✓
	1 MS/s	-	_	_	_	-	-	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	✓	✓	\checkmark
ms	500 kS/s	-	_	-	-	-	-	-	~	_	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	✓	✓
efori	200 kS/s	-	_	_	_	-	-	-	-	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~
wav	100 kS/s	-	_	_	_	-	-	-	-	_	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	~	✓	✓
snoe	50 kS/s	-	_	-	-	-	-	-	-	_	-	~	-	~	~	~	~	~	~	~	~	~	~	~	~	✓	✓	✓
ltan€	20 kS/s	-	_	-	-	-	-	-	-	_	-	_	~	~	~	~	~	~	~	~	~	~	~	~	~	✓	✓	✓
ıstar	10 kS/s	-	_	-	_	-	-	-	-	_	-	-	-	~	~	~	~	~	~	~	~	~	~	~	~	✓	✓	~
Sampling speed for instantaneous waveforms	5 kS/s	-	_	_	_	-	-	-	-	_	-	_	_	-	~	-	~	~	~	~	~	~	~	~	~	~	~	\checkmark
eed	2 kS/s	-	_	_	_	-	-	-	-	_	-	_	_	-	_	~	~	~	~	~	~	~	~	~	~	~	~	\checkmark
ds bi	1 kS/s	-	_	_	_	-	-	-	-	_	-	_	_	-	_	_	~	~	~	~	~	~	~	~	~	~	✓	~
nplir	500 S/s	-	_	_	_	-	-	-	-	_	-	_	_	-	-	-	-	~	-	~	~	~	~	~	~	~	~	\checkmark
Sar	200 S/s	-	_	_	_	-	-	-	-	_	-	_	_	-	-	-	-	-	~	~	~	~	~	~	~	~	~	\checkmark
	100 S/s	-	_	_	_	-	-	-	-	_	-	_	_	-	-	-	-	-	-	~	~	~	~	~	~	✓	~	~
	50 S/s	-	_	_	_	-	-	-	-	_	-	_	_	-	-	-	-	-	-	-	~	_	~	~	~	~	~	\checkmark
	20 S/s	-	_	_	_	-	-	-	-	_	-	_	_	-	_	_	-	-	-	-	-	~	~	~	~	~	~	\checkmark
	10 S/s	-	_	_	_	-	-	-	-	_	-	_	_	-	_	_	-	-	-	-	-	_	~	~	~	~	~	✓
	5 S/s	-	_	_	_	-	-	-	-	_	-	_	_	-	_	-	-	-	-	-	-	_	_	~	~	~	~	~
	2 S/s	-	_	_	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	_	-	-	~	~	~	✓
	1 S/s	-	_	-	_	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	~	~	✓

Trend waveforms are measured using the envelop method (the maximum and minimum values are recorded per sample).

At this time, the instrument performs oversampling at a sampling speed set for instantaneous waveform recording.

Although the sampling speed for trend waveform recording has been fixed at a specific value, measurement results of trend waveforms differ according to the sampling speed for instantaneous waveform recording.

16.4 Power Equations and Wiring Specifications

.


Power equation

Wiring setting Item	1P2W	1P3W	3P3W	3V3A	3P4W				
Voltage RMS value	$Urms_1 = \sqrt{\frac{1}{n} \sum_{i=1}^{n} (U_{1i})^2}$	$Urms_{12} = \frac{1}{2}$	$(Urms_1 + Urms_2)$	$Urms_{123} = \frac{1}{3} (Urms_1 + Urms_2 + Urms_3)$					
Voltage mean value	$Umn_1 = \frac{\pi}{2\sqrt{2}} \frac{1}{n} \sum_{i=1}^{n} U_{1i} $	$Umn_{12} = \frac{1}{2}$	$(Umn_1 + Umn_2)$	$Umn_{123} = \frac{1}{3} (Umn_1 + Umn_2 + Umn_3)$					
Voltage simple average value	$Udc = \frac{1}{n} \sum_{i=1}^{n} U_i$								
Current RMS value	$Irms_1 = \sqrt{\frac{1}{n} \sum_{i=1}^{n} (I_{1i})^2}$	$Irms_{12} = \frac{1}{2}$	$(Irms_1 + Irms_2)$	$Irms_{123} = \frac{1}{3} \left(Irms_1 + \frac{1}{3} \right)$	$-Irms_2 + Irms_3$)				
Current mean value	$Imn_{1} = \frac{\pi}{2\sqrt{2}} \frac{1}{n} \sum_{i=1}^{n} I_{1i} $	$Imn_{12} = \frac{1}{2}$	$Imn_{123} = \frac{1}{3} (Imn_1 + Imn_2 + Imn_3)$						
Current simple average value	$Idc = \frac{1}{n} \sum_{i=1}^{n} I_i$								
Active power	$P_1 = \frac{1}{n} \sum_{i=1}^{n} \left(U_{1i} \times I_{1i} \right)$	P ₁₂ =	$= P_1 + P_2$	$P_{123} = P_1 + P_2$	$P_{123} = P_1 + P_2 + P_3$				
Apparent power	$S_1 = Urms_1 \times Irms_1$	$S_{12} = S_1 + S_2$	$S_{12} = \frac{\sqrt{3}}{2} \left(S_1 + S_2 \right)$	$S_{123} = \frac{\sqrt{3}}{3} \left(S_1 + S_2 + S_3 \right)$	$S_{123} = S_1 + S_2 + S_3$				
Reactive power	$Q_1 = \sqrt{S_1^2 - P_1^2}$	$Q_{12} = $	$S_{12}^{2} - P_{12}^{2}$	$Q_{123} = \sqrt{S_{123}^2}$	$-P_{123}^{2}$				
Power factor	$\lambda_1 = \frac{ P_1 }{ S_1 }$	λ ₁₂	$= \frac{P_{12}}{S_{12}}$	$\lambda_{123} = \frac{P_{123}}{S_{123}}$					
Power phase angle	$\phi_1 = \cos^{-1} \lambda_1 $	$\phi_{12} =$	$\cos^{-1} \lambda_{12} $	$\phi_{123} = \cos^{-1} \lambda_{123} $					
	a points; <i>i</i> : <i>i</i> th data point A wiring, 3P4W equatior		∆-Y conversion.						


. .

Wiring specifications

1-phase/2-wire (1P2W)

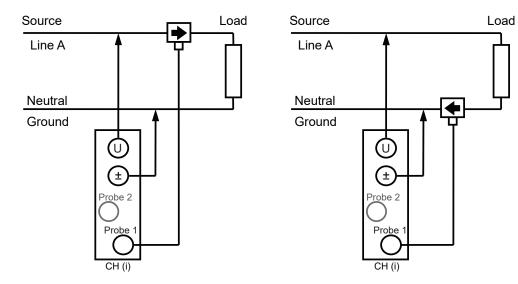


1-phase/3-wire (1P3W)

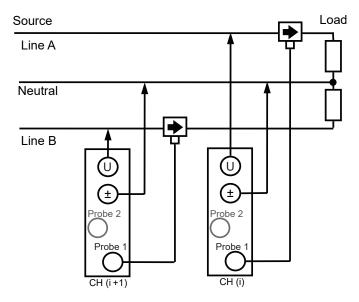


16 Appendix


3-phase/3-wire (3P3W)

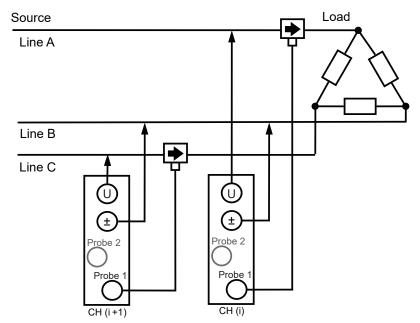

3-phase/3-wire (3V3A)

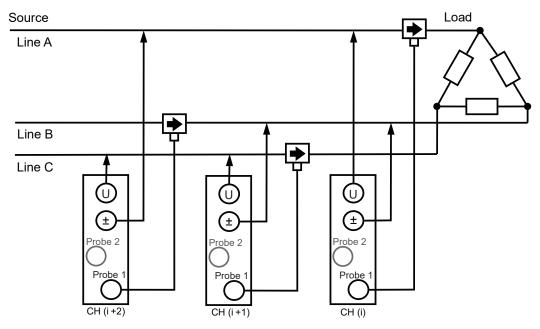

4-phase/3-wire (3P4W)

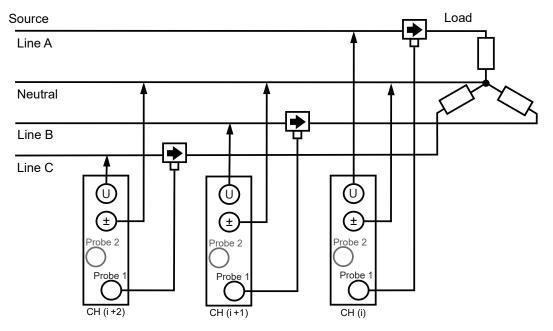

Power Equations and Wiring Specifications

Index

When the reference pages of an index entry include "Quick," please also see the Index pages of the Quick Start Manual.

Symbol

+Width	185, 191, 206
-Width	185, 191, 206
∆-Y conversion	251

0-9

2-point setting	58
2 point ootting	00

<u>A</u>

A.A.F	67, 84
Accumulation	. 185, 187, 206
Acquisition period	263, 264
Aliasing	7, 411
Amplitude	. 185, 187, 206
Analog channel	13
Analog trigger	149
Angle of XY waveform	. 185, 189, 207
Anti-aliasing filter	67, 84, 412
Area	. 185, 187, 202
Absolute value	202
Only the negative-amplitude part	203
Only the positive-amplitude part	203
Total	202
Attenuation rate	266
Automatic balancing	70
Automatic ranging	Quick
Automatic saving	118, 120
Automatic setup	135
Automatic startup function	
Average	. 185, 187, 201
Averaging	268, 414

В

Веер	345
Binary	116, 121
Blackman Harris window	265, 417
Blackman window	265, 417
Block to be used	290
BMP	116
Burst width	185, 192, 206

C

Calculation starting point	276
Calculation type	272, 274, 288
Calibration	79
CAN interface	319
CAN/LIN definition data	325
CAN/LIN measurement function	311

CAN statistics	185, 194, 207
CAN transmission function	333
CAN trigger	163
Character code	380
Clock	Quick
Coherence function	287
Command	379
Comment	5, 13, 17
Communications	349
Command communications	379
Computer name	354
Gateway	353
IP address	
Subnet mask	353
Computer name	354
Concierge	176
Conversion ratio	58
Copy function	
Cross power spectrum	
Cursor value	

D

DBC file	331
Dead time	292
Decibels (dB)	
Delimiter	
Display magnification	
Waveform	41
Zoom function	
Display position	
Waveform	41
Display setting	
Dual sampling	295
Duty ratio	185, 188, 205

E

Email transmission	374
Envelope	
Evaluation	197
Event count	152
Event mark	386
Explorer	136
Exponential average	
Exponential window	265, 417
External control	
External control terminal	385
External sampling	262, 394
External trigger	391
EXT.SMPL	394, Quick
EXT.TRIG	391, Quick

F

Fall time
FFT 409
FFT calculation function 257
FFT calculation type 279
FFT internal calculation formula 288
File
File type 116
File screen
File size
MEM file 395
REC file
Waveform (text) file
Filter 151, 153, 155, 158
Flat-top window
Forced average time 250
Forcible trigger
Format
Formatting storage devices 136, Quick
Four arithmetic operations 185, 194, 205
Fourier transform 409
Frequency 185, 188, 201
Frequency resolution
FTP

G

Gateway	3
Gauge (vertical scale) 3	7
Glitch trigger 15	7

н

Hamming window	265, 417
Hann window	265, 416
Header	379
High level	185, 187, 205
High-speed response	
Horizontal cursor	34
How to connect a computer	Quick
Hysteresis	248

I. .

Imaging 413
Impulse response 410
IN1 386, Quick
IN2
Initializing the instrument
Input coupling 15
Instantaneous waveform 295, 300
Intermediate value 185, 187, 205
Internal calculation formula 288
Interval trigger 160
In trigger 153
Invert

IP address	353
------------	-----

κ

Key check	Quick
Key lock	Quick

Ľ.

LAN	351, 379
Language	
Level at time	
Level trigger	151
Linear spectrum	
Linear time-invariant system	
Loading data	
File type	
Logical AND/OR operation	147
Logic channel	17
Logic trigger	
Low level	185, 187, 205
Low-pass filter	15, 249
L.P.F.	
LTI system	
,	

М

Managing files	136
Manual saving	127
Maximal value	168, 267
Maximum value	185, 187, 201, 267
Measurement mode	13
Measurement range	14
Memory HiConcierge	176
Minimal value	168
Minimum value	185, 187, 201
Module-specific setting	67, 86

N

Network drive	381
Normal	9
NPLC	. 78
Numerical calculation	181
Evaluation	197
Numerical calculation result	195
Setting	184

0

Offset	58
Option	Quick
OUT1	
OUT2	
Out trigger	
Overall value	414

Overlay		. 54
Overshoot	185, 187,	206

Ρ

)1
)1
55
55
)5
34
80
2
0
20
33
2
5
5
)5
)4

Q

R

Real-time saving	124
Recordable time	
Recording length	
Recording method	
Envelope	
Normal	
Recording mode	6, 297
Rectangular window	
Reference block	
Remote operation	
Response	
Response time	
Rise time	
RMS	185, 187, 201
RMS spectrum	
Rotary knob	45

S

S1 key S2 key	
Sampling rate	
SAVE key	118, 127
Saving data	115, 118
Automatic saving	118, 120
File type	116
Quick saving	118, 127
Selective saving	118, 127

Saving type	118, 121, 128
Scaling	56
Using Model U8969 Strain Unit	61
Using strain gauge	61, 405
Screenshot	116, 123
Saving data	127
Scrolling through waveforms	39
Search	167
Section cursor	35
Selective save	118, 127
Setting	
Automatically loading	
Input channel	11
Measurement condition	5
Numerical calculation	184
Saving data	118
Trigger	138
SF8000	110
Sheet	19
Shortcut key	346
Simple average	414
Standard deviation	185, 187, 202
Start block	290
Starting measurement	
STARTUP	135
Subnet mask	353
Sync source	247
System protection function	345

<u>т</u>____

Text		116,	121
Thermocouple			. 68
Time			
Time to maximum	. 185,	187,	201
Time to minimum	. 185,	187,	201
Time difference (Time lag)	. 185,	193,	205
Time to level			
Trace cursor			. 30
Transfer function			286
Trend waveform		295,	300
Trigger			137
CAN trigger			163
Glitch			157
In			153
Level			151
Out			153
Period-in			155
Period-out			155
Voltage drop			154
Trigger filter	. 151,	153,	155
Trigger output			389
Trigger priority			145
Trigger setting			138
Trigger source (AND/OR operation)			147
TRIG.OUT			389

U

V	
Vernier	1
Voltage drop trigger 154	1

W

Warning	Quick
Waveform	4.4
Display magnification	
Display position	41
Range specification	35
Zoom-in/zoom-out	46
Waveform calculation	210
Operator	222
Waveform file size	395
Waveform generation	. 86, Quick
Waveform image	116
Waveform screen	276
Wave marker software	110
Web browser	
Window function	265, 415
Wiring method	
Wiring specifications	
o 1	

<u>x</u>_____

XY area	185, 189, 203
Coordinate method	203
Trapezoidal approximation method	204
XY composite	25, 47

Ζ_____

Zero-cross	247
Zoom function	. 46

HIOKI

www.hioki.com/ **HIOKI E.E. CORPORATION** 81 Koizumi, Ueda, Nagano 386-1192 Japan



All regional contact information

2402 EN Printed in Japan

Edited and published by HIOKI E.E. CORPORATION •Contents subject to change without notice.

• It is prohibited to copy, reproduce, or modify the content of this document without permission. ·Company names, product names, etc. mentioned in this document are trademarks or

registered trademarks of their respective companies.

 Europe only

 •EU declaration of conformity can be downloaded from our website.

 •Contact in Europe:

 HIOKI EUROPE GmbH

 •Listfmann Park 2, 65760 Eschborn, Germann

Helfmann-Park 2, 65760 Eschborn, Germany

hioki@hioki.eu